
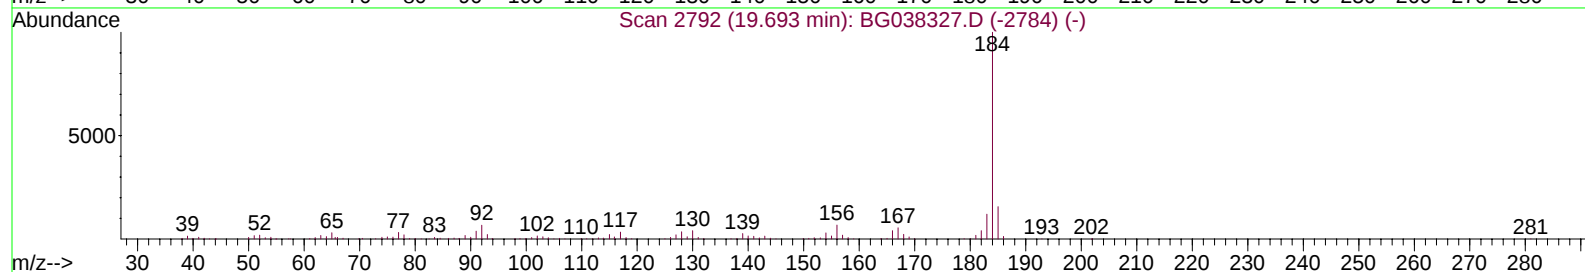
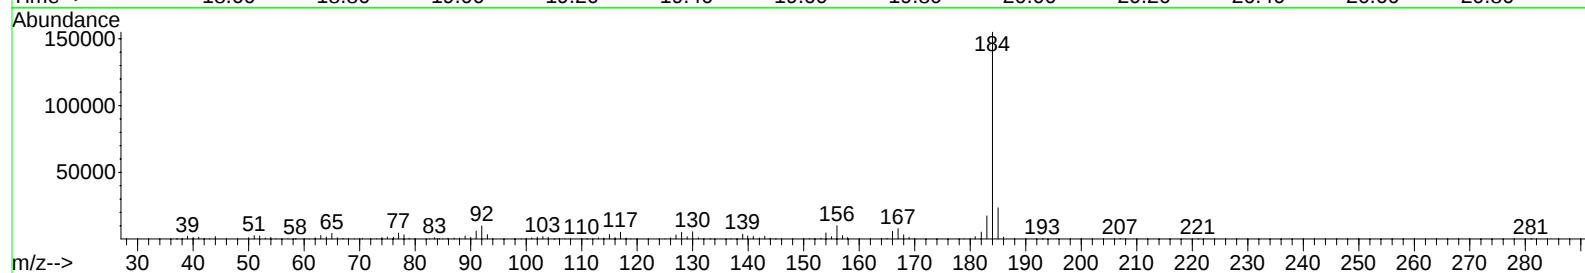


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120418\
 Data File : BG038323.D
 Acq On : 4 Dec 2018 10:45
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 13:53:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 04 17:15:40 2018
 Response via : Initial Calibration

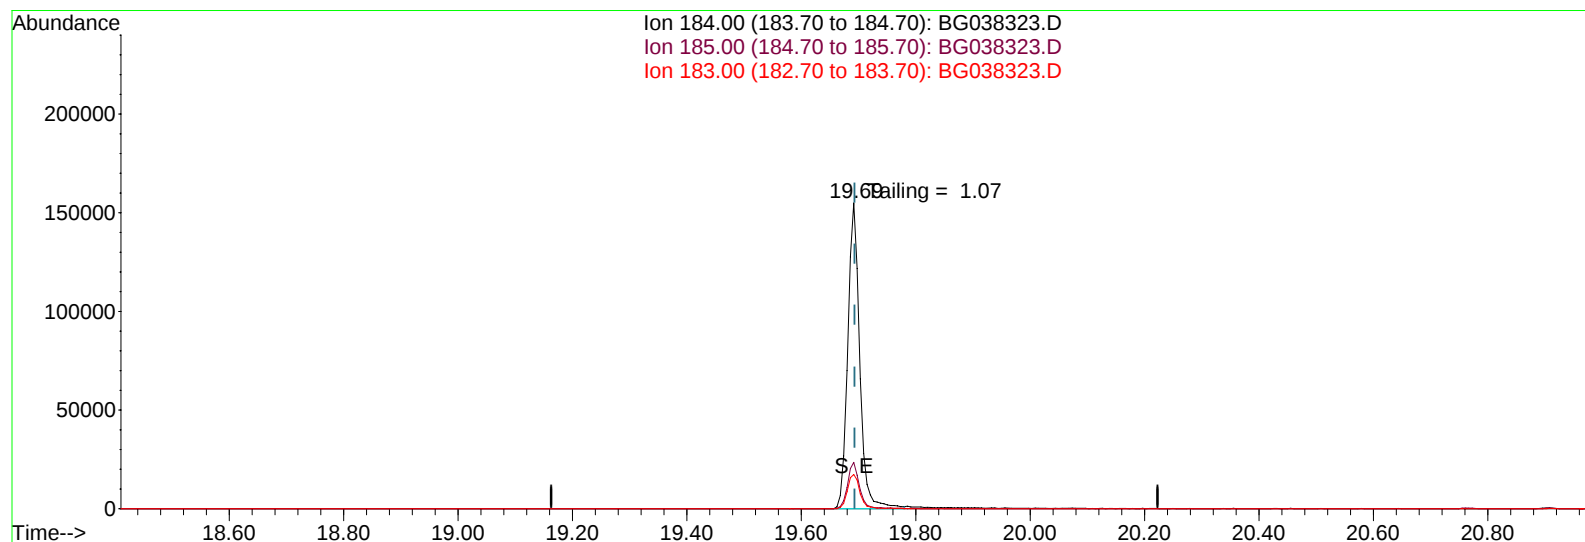

TIC: BG038323.D

(77) Benzidine




19.691min (-0.001) 11511.51ng

response 226856

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.16
183.00	12.70	11.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120418\
Data File : BG038323.D
Acq On : 4 Dec 2018 10:45
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 13:53:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

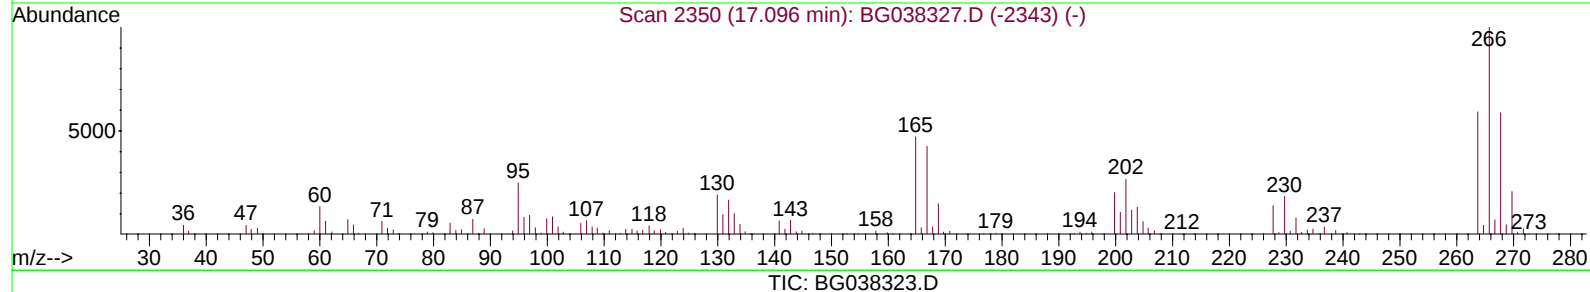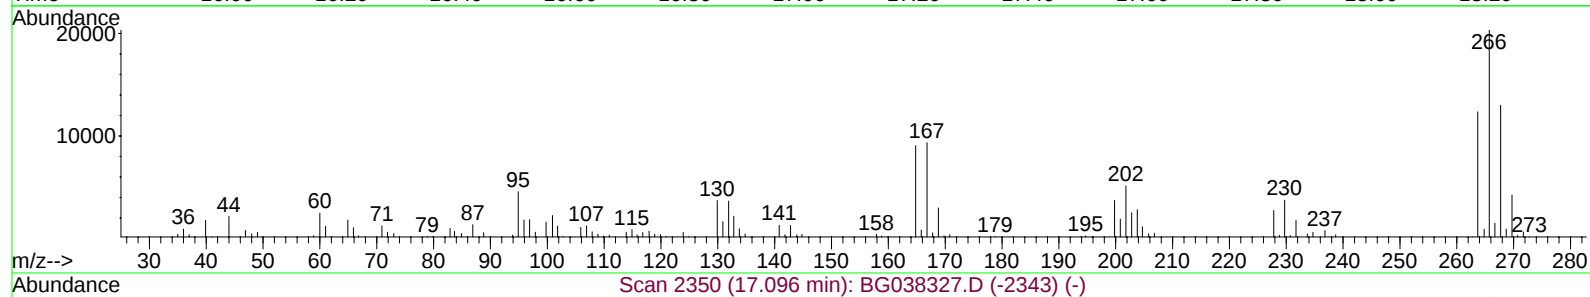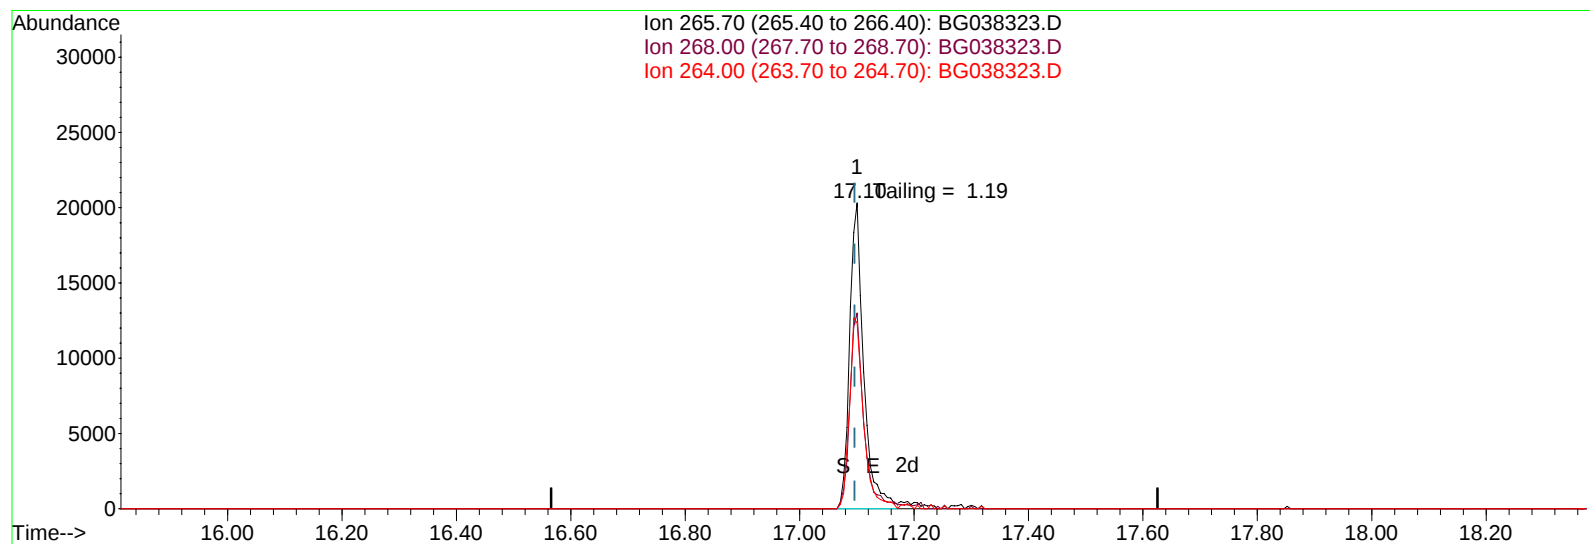

(70) Pentachlorophenol (C)

17.100min (+0.005) 35509.69ng

response 34948

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	68.47
264.00	73.60	60.83
0.00	0.00	0.00