
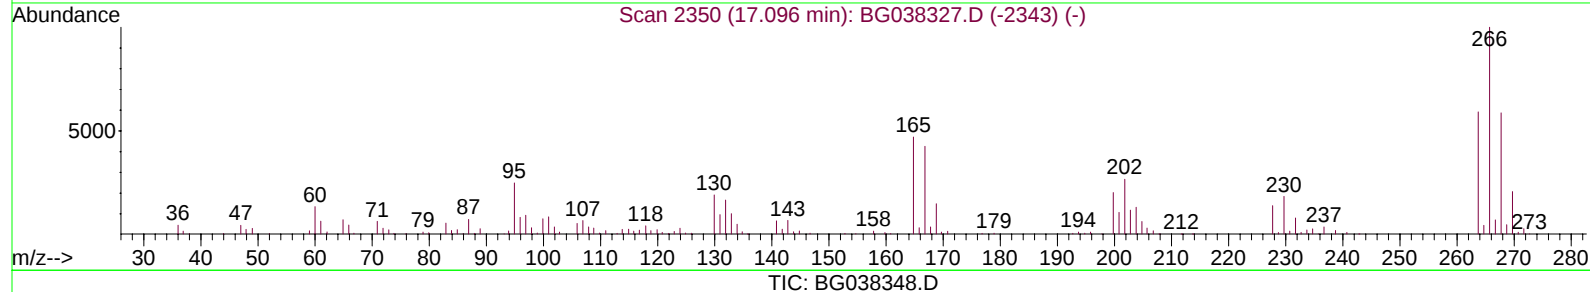
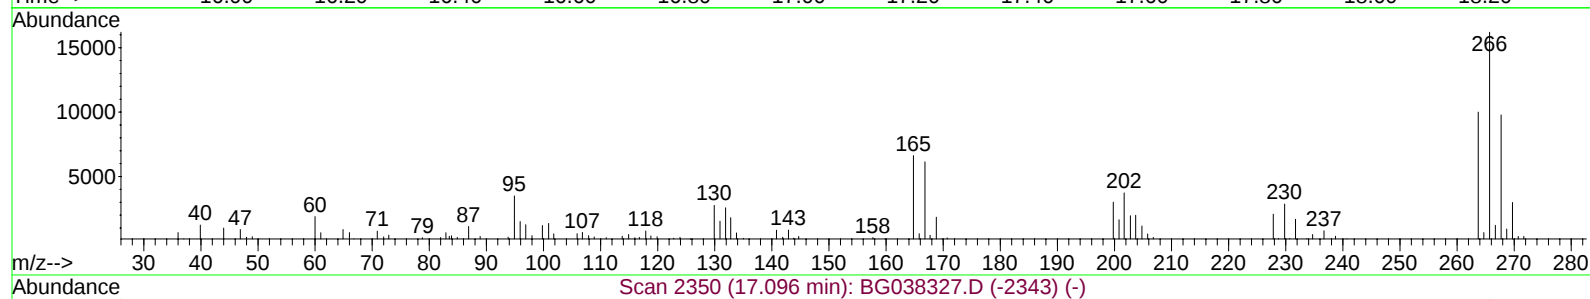


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120418\
Data File : BG038348.D
Acq On : 5 Dec 2018 7:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 13:22:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

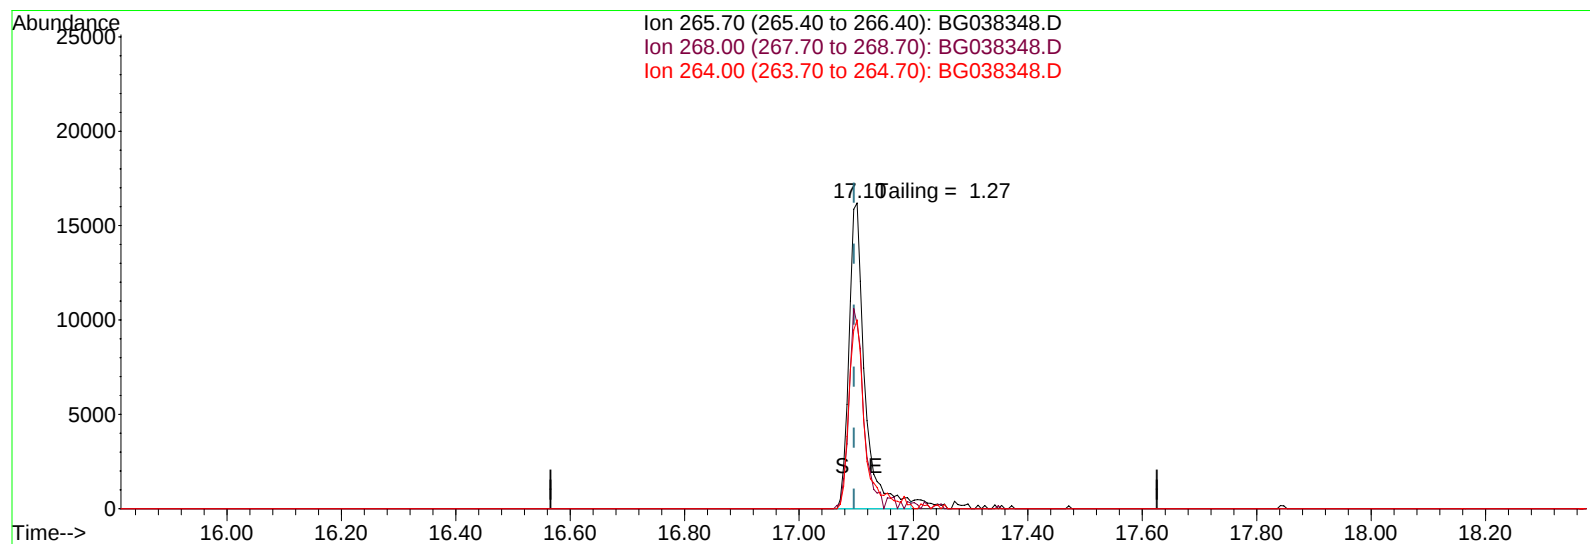

(70) Pentachlorophenol (C)




17.101min (+0.006) 72088.02ng

response 31349

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.08
264.00	73.60	65.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG120418\
Data File : BG038348.D
Acq On : 5 Dec 2018 7:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 05 13:22:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

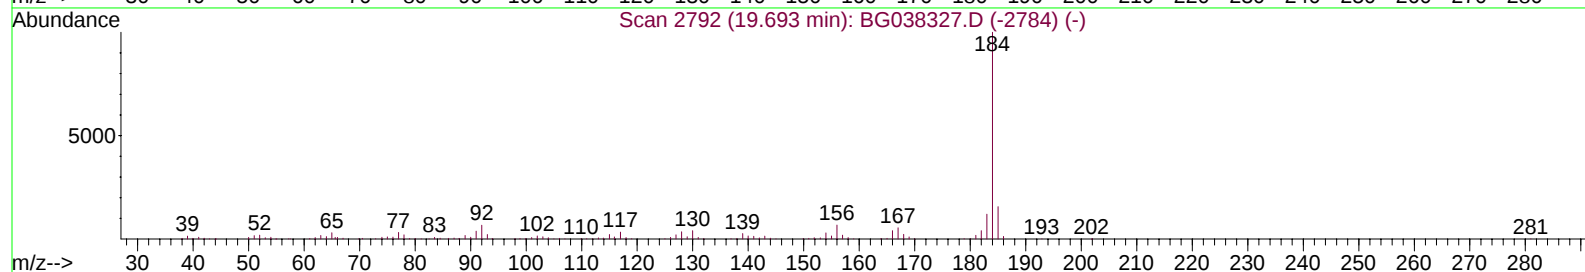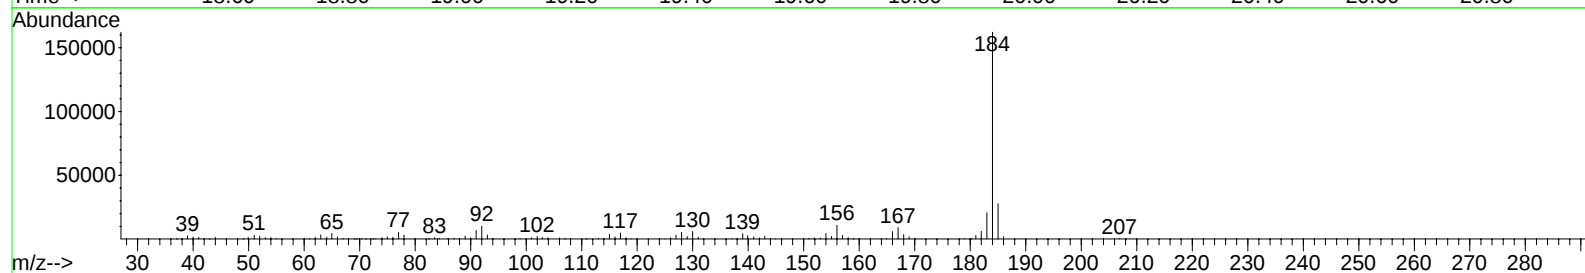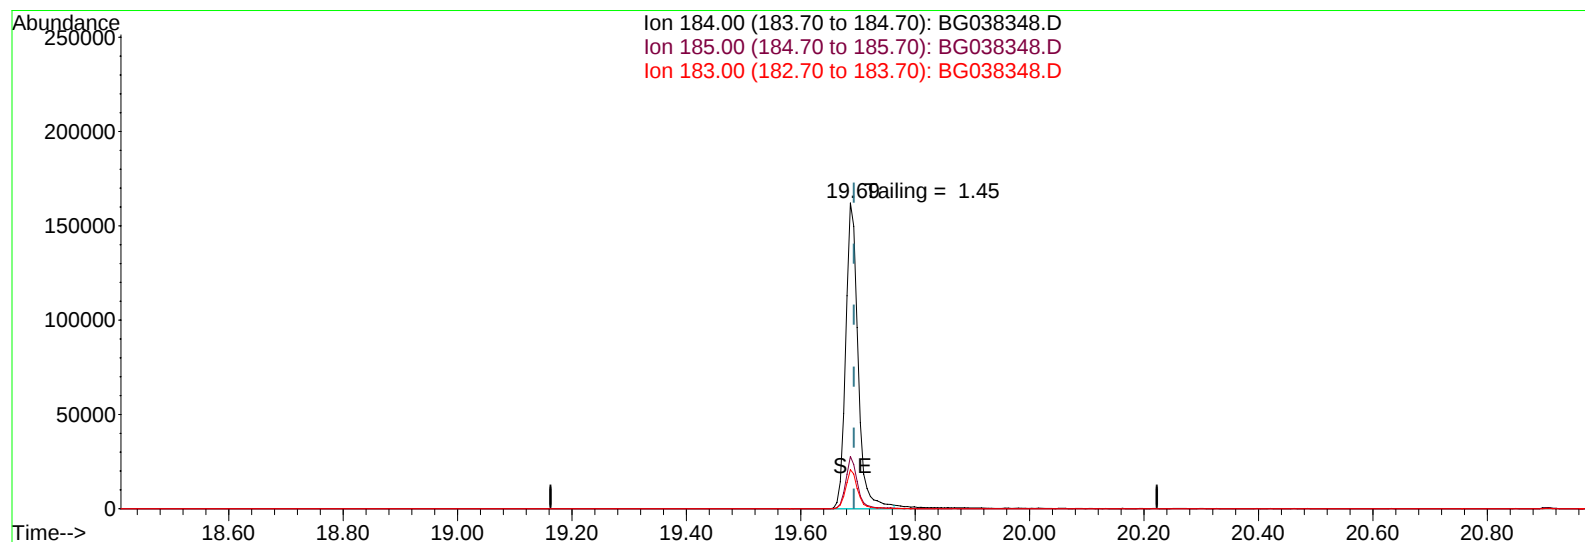

TIC: BG038348.D

(77) Benzidine

19.687min (-0.006) 0.00ng

response 248480

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	17.09
183.00	12.70	12.78
0.00	0.00	0.00