


Instrument :
BNA_G
ClientSampleId :

1,2-Dichlorobenzene

Response Ratio

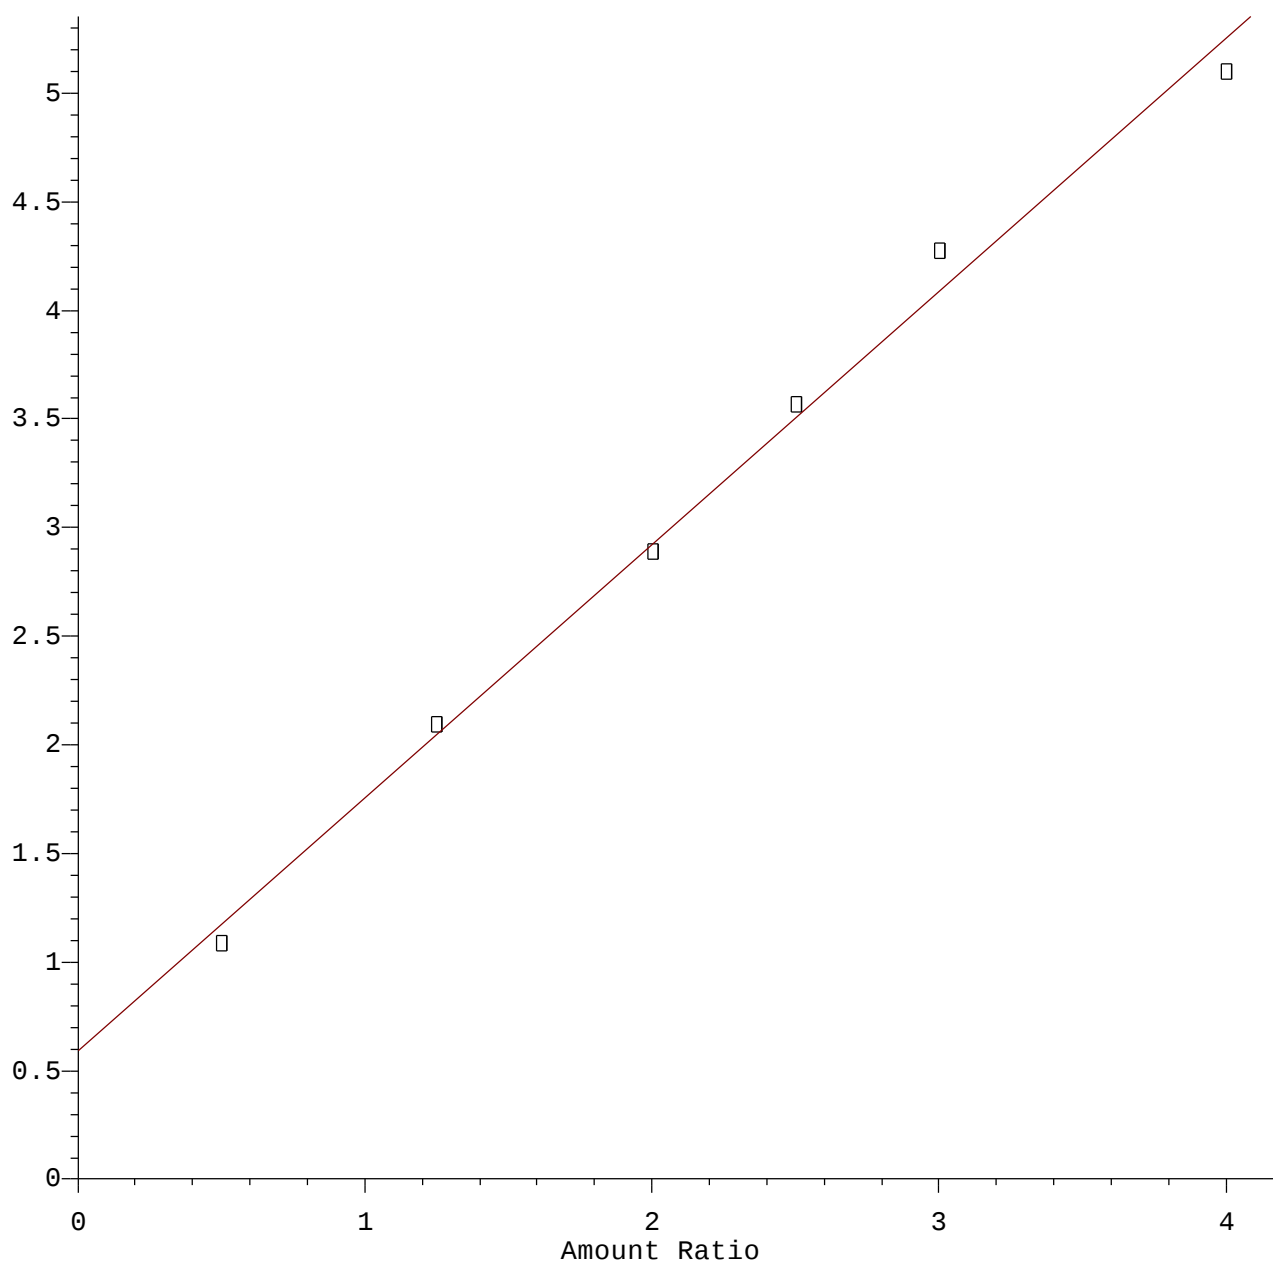


Resp Ratio = 1.17e+000 * Amt + 5.92e-001
Coef of Det (r²) = 0.993 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
Calibration Table Last Updated: Tue Dec 04 17:15:40 2018

Instrument :
BNA_G
ClientSampleId :

2-Methylphenol

Response Ratio

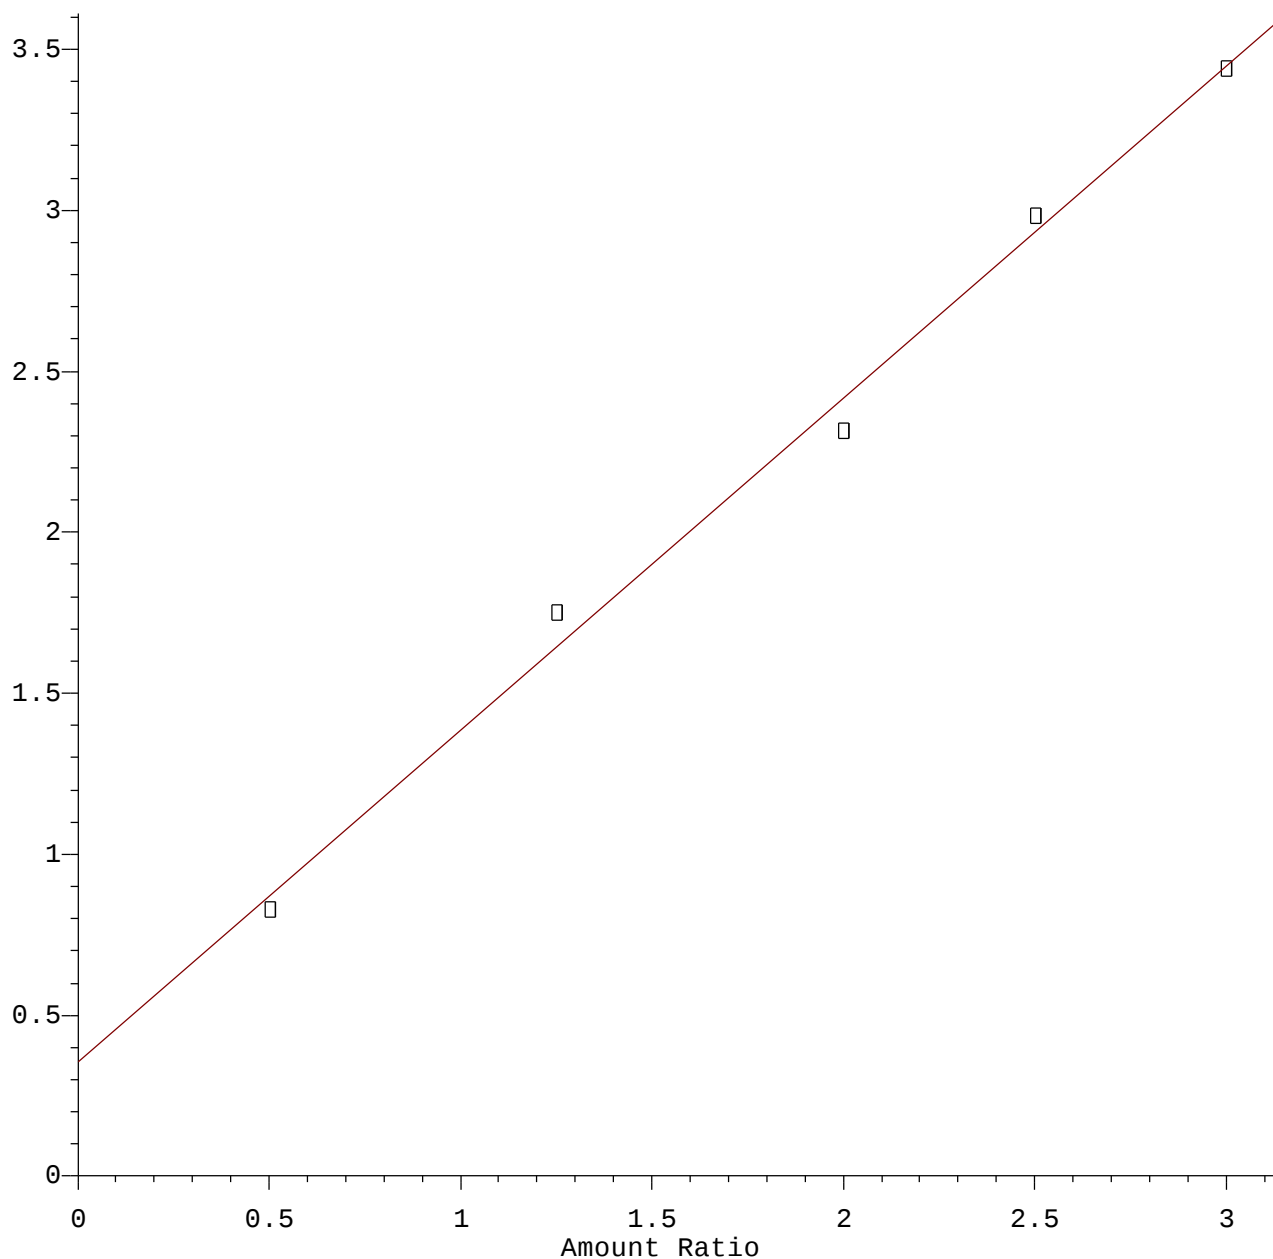


Resp Ratio = $1.03e+000 * \text{Amt} + 3.55e-001$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
Calibration Table Last Updated: Tue Dec 04 17:15:40 2018

Instrument :
BNA_G
ClientSampleId :

n-Nitroso-di-n-propylamine


Response Ratio

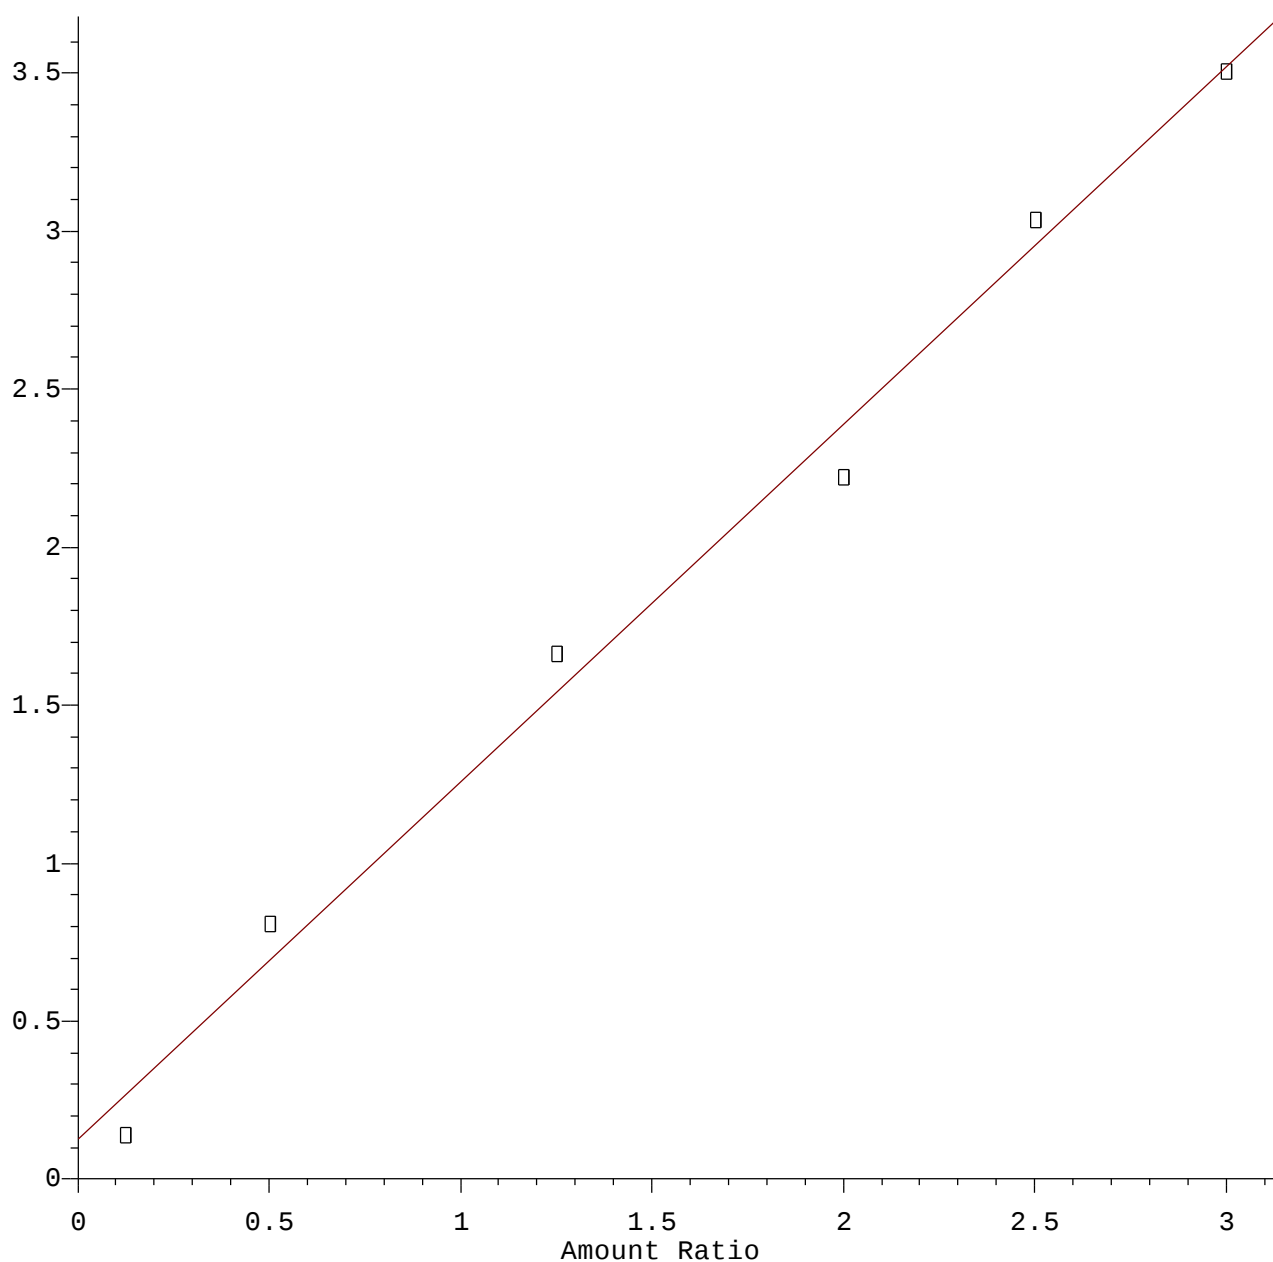

Resp Ratio = 1.13×10^0 * Amt + 1.26×10^{-1}
Coef of Det (r^2) = 0.990 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
Calibration Table Last Updated: Tue Dec 04 17:15:40 2018

Instrument :
BNA_G
ClientSampleId :

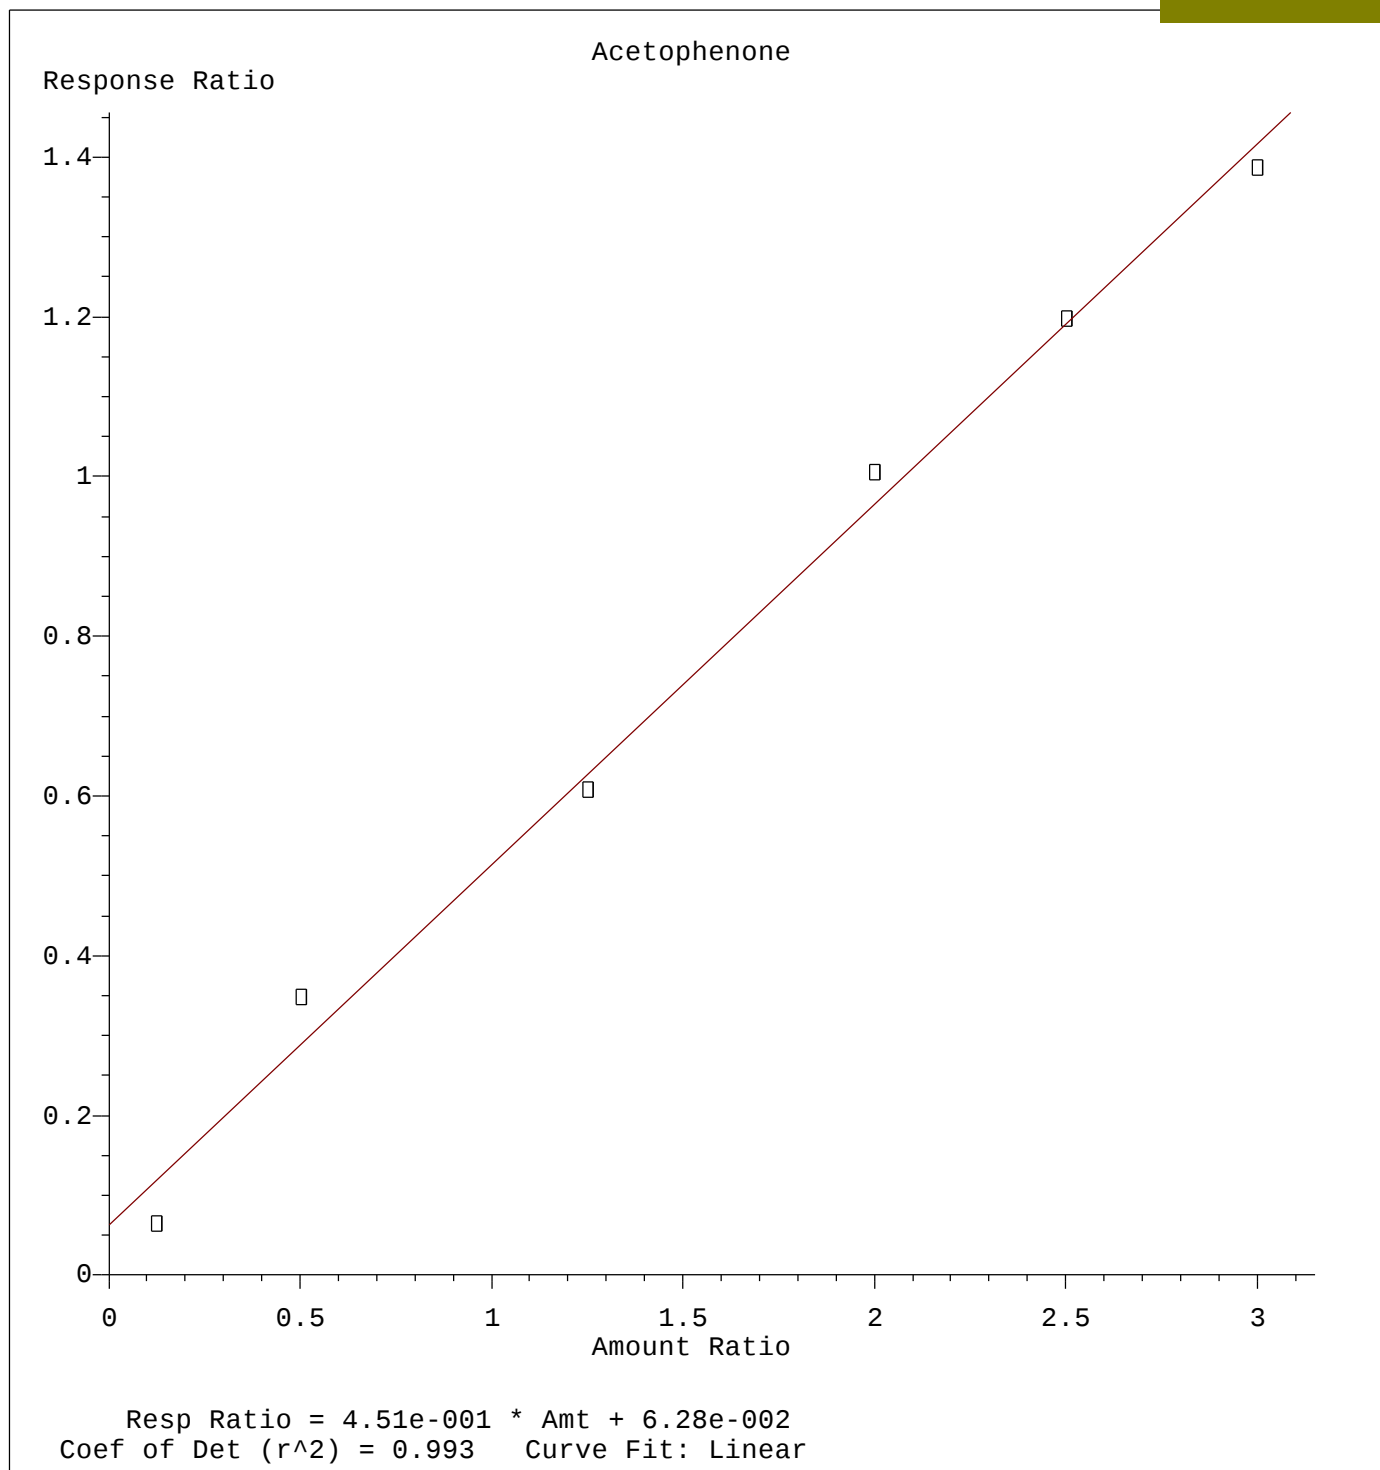

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
Calibration Table Last Updated: Tue Dec 04 17:15:40 2018

Instrument :
BNA_G
ClientSampleId :

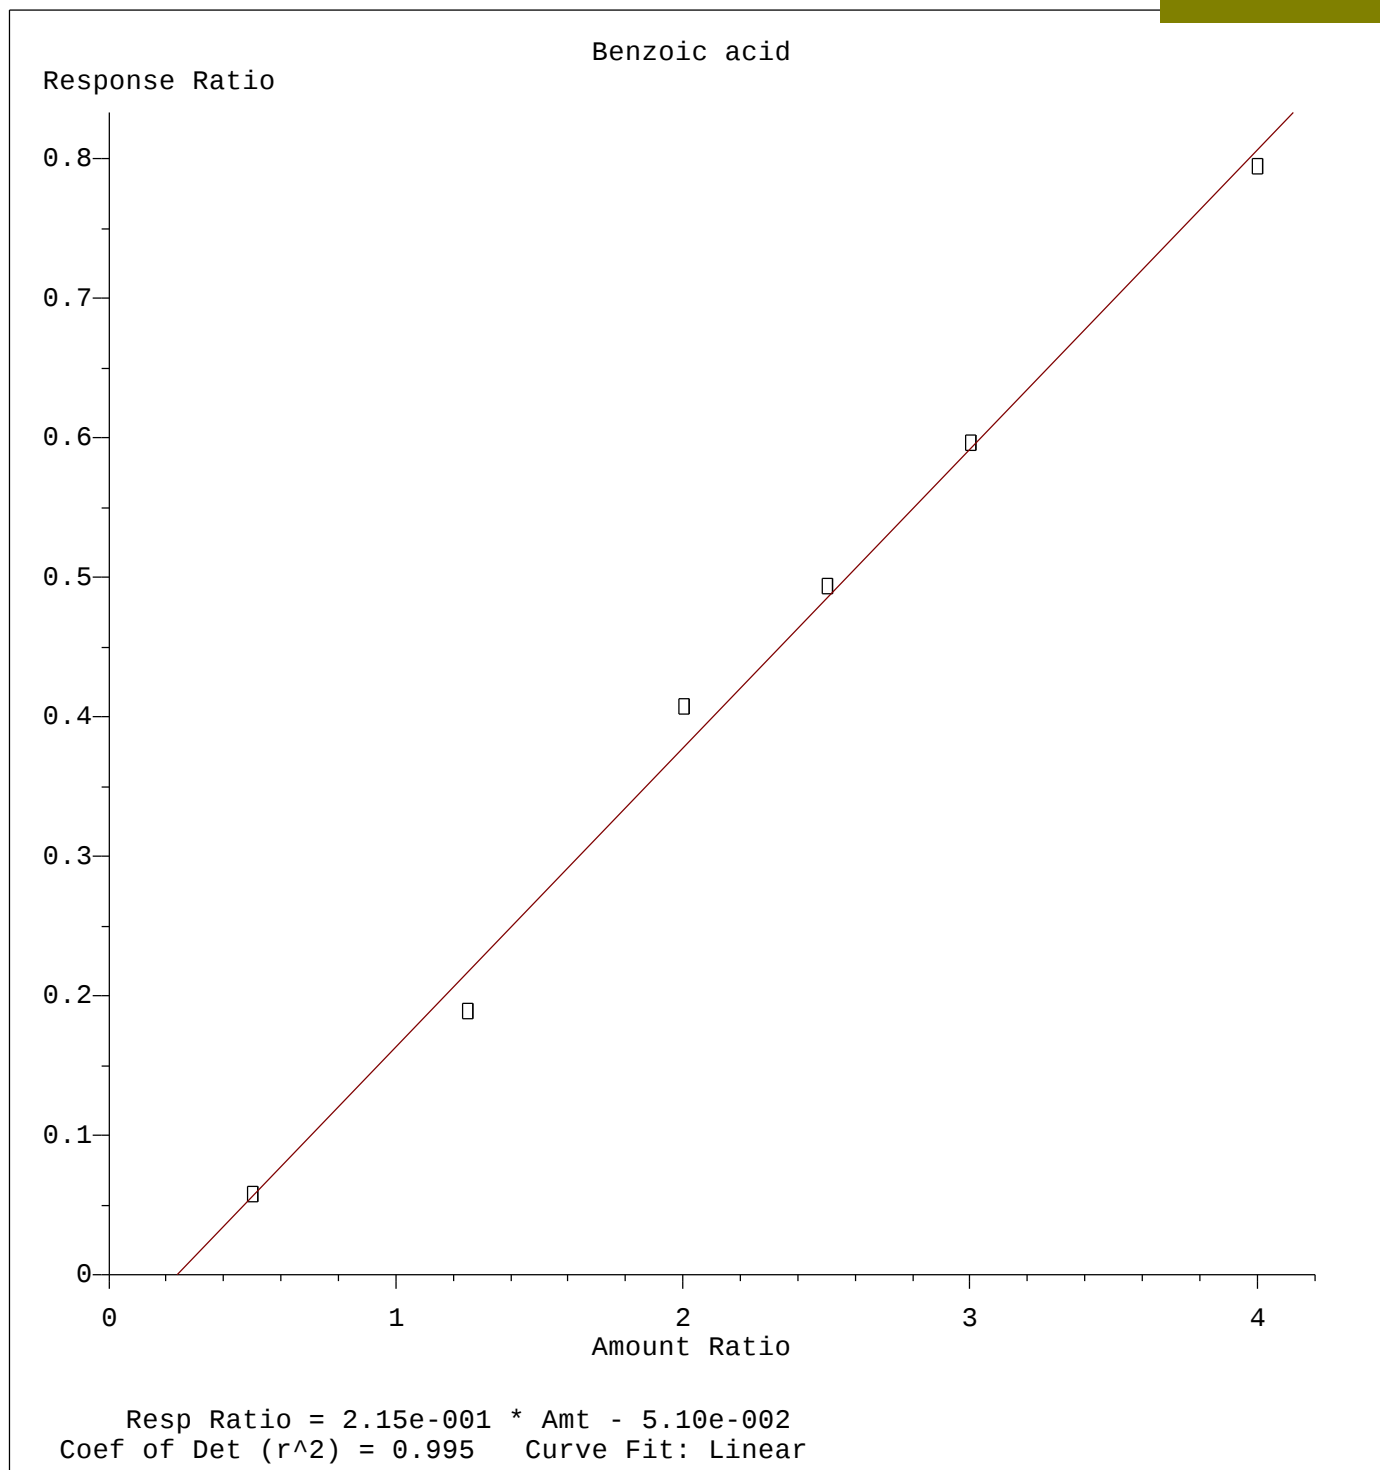

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
Calibration Table Last Updated: Tue Dec 04 17:15:40 2018