

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
 Data File : BG038356.D
 Acq On : 5 Dec 2018 12:22
 Operator : JU/SJ
 Sample : J6159-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB-1129-S-TCLP-GRID19

Quant Time: Dec 05 13:01:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 04 17:15:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	30264	20.00	ng	0.00
21) Naphthalene-d8	10.89	136	137423	20.00	ng	0.00
39) Acenaphthene-d10	14.71	164	84663	20.00	ng	0.00
64) Phenanthrene-d10	17.46	188	221558	20.00	ng	0.00
76) Chrysene-d12	21.73	240	222202	20.00	ng	0.00
87) Perylene-d12	25.04	264	229570	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	182523	106.73	ng	0.00
7) Phenol-d6	7.22	99	212856	86.11	ng	0.00
23) Nitrobenzene-d5	9.25	82	187414	67.71	ng	0.00
42) 2,4,6-Tribromophenol	16.20	330	133341	128.29	ng	0.00
45) 2-Fluorobiphenyl	13.33	172	433408	72.94	ng	0.00
79) Terphenyl-d14	20.06	244	851095	82.05	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
Data File : BG038356.D
Acq On : 5 Dec 2018 12:22
Operator : JU/SJ
Sample : J6159-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB-1129-S-TCLP-GRID19

Quant Time: Dec 05 13:01:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

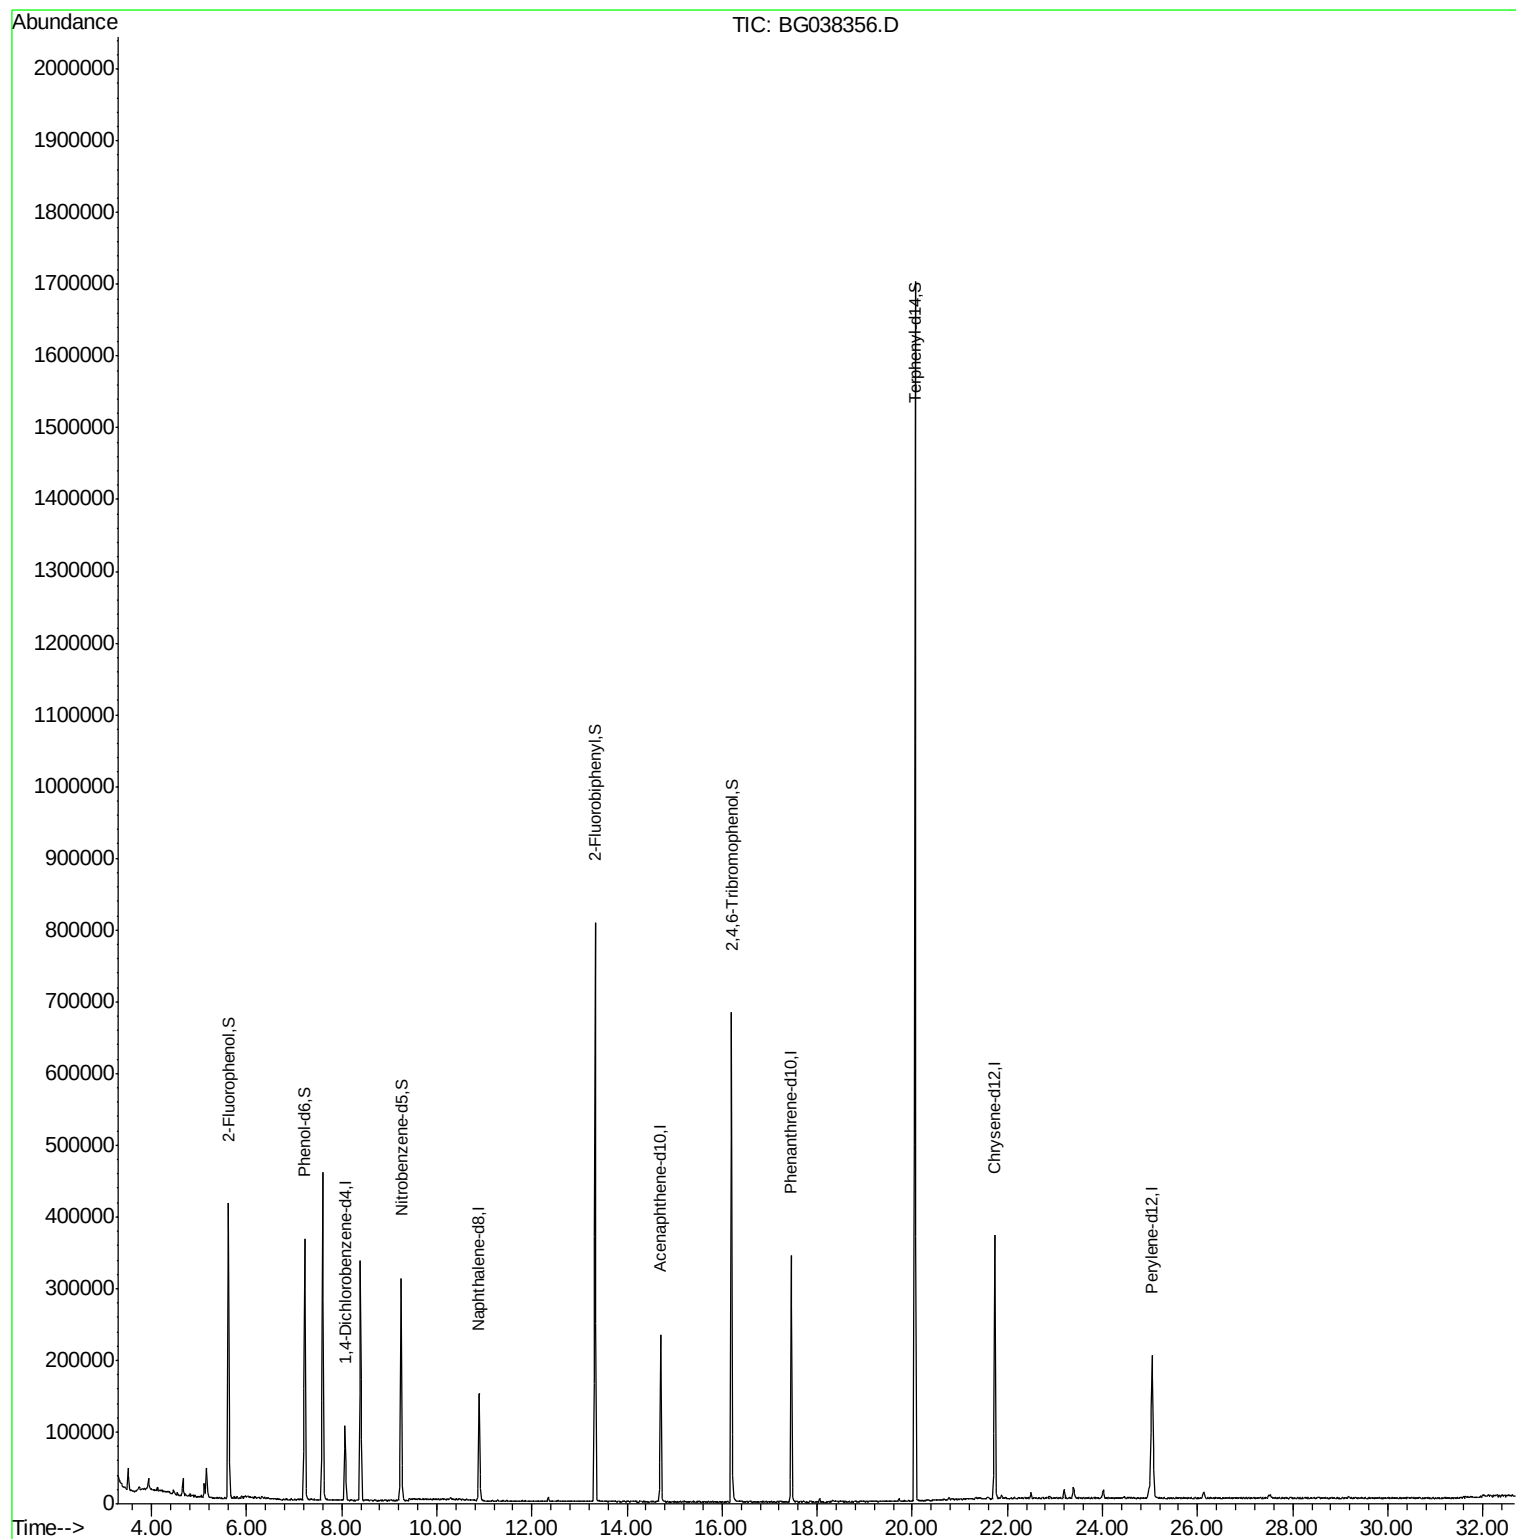

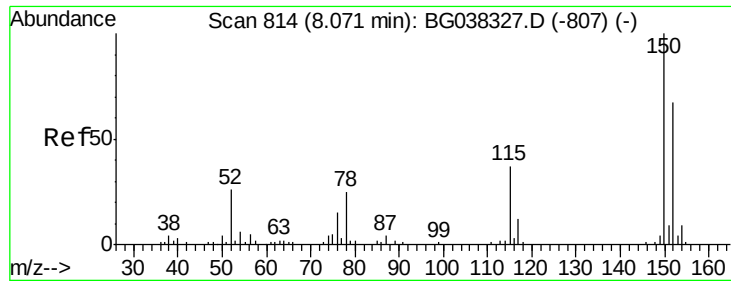


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 814
Delta R.T. 0.00 min
Lab File: BG038356.D
Acq: 5 Dec 2018 12:22

Instrument :
BNA_G
ClientSampleId :
CB-1129-S-TCLP-GRID19

Tot Ion:152 Resp: 30264
Ion Ratio Lower Upper
152 100
150 166.3 126.0 189.0
115 62.6 45.5 68.3

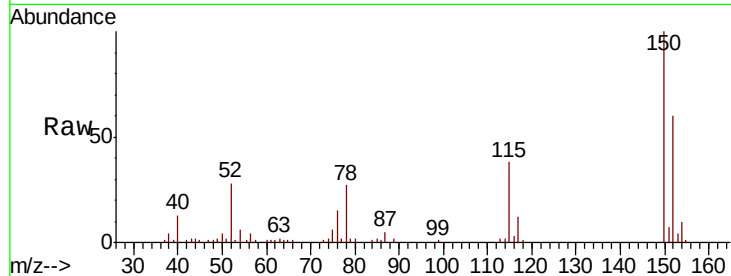


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

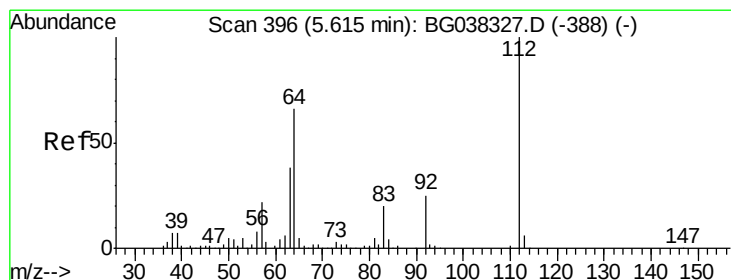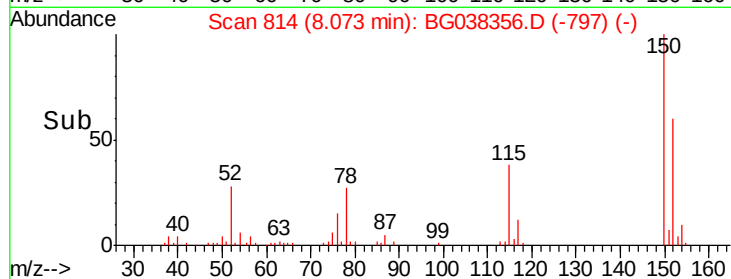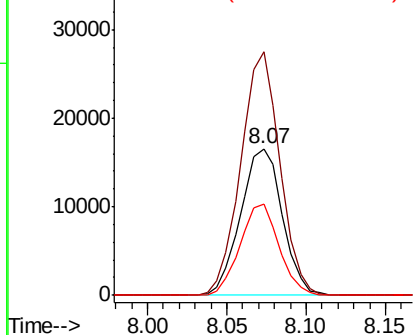



#5


2-Fluorophenol
Concen: 106.728 ng
RT: 5.62 min Scan# 396
Delta R.T. 0.00 min
Lab File: BG038356.D
Acq: 5 Dec 2018 12:22

Tgt Ion:112 Resp: 182523
Ion Ratio Lower Upper
112 100
64 68.9 53.1 79.7
63 38.0 27.3 40.9

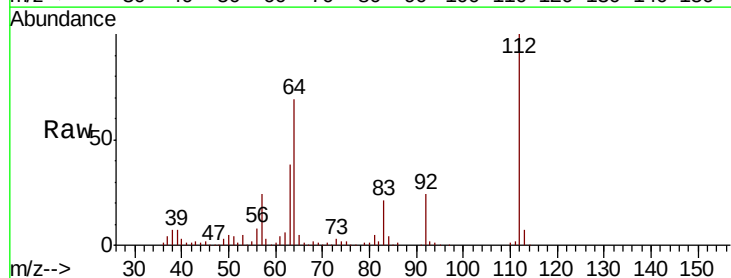

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

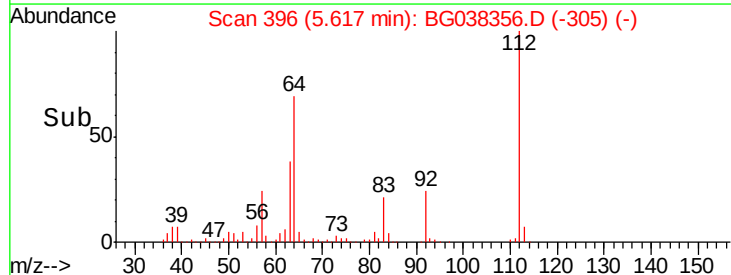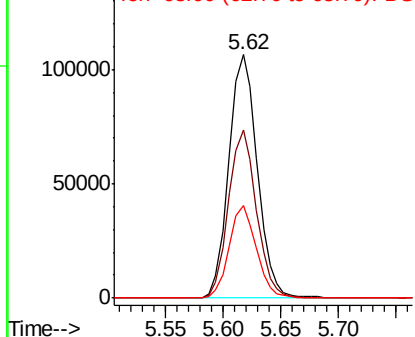

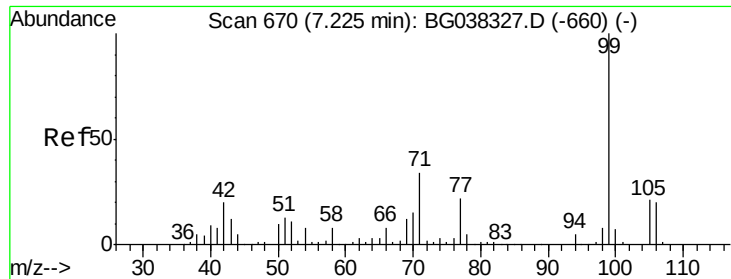

#7

Phenol-d6

Concen: 86.115 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.00 min

Lab File: BG038356.D

Acq: 5 Dec 2018 12:22

Instrument :

BNA_G

ClientSampleId :

CB-1129-S-TCLP-GRID19


Tot Ion: 99 Resp: 212856

Ion Ratio Lower Upper

99 100

42 22.6 15.0 22.4#

71 35.9 25.5 38.3



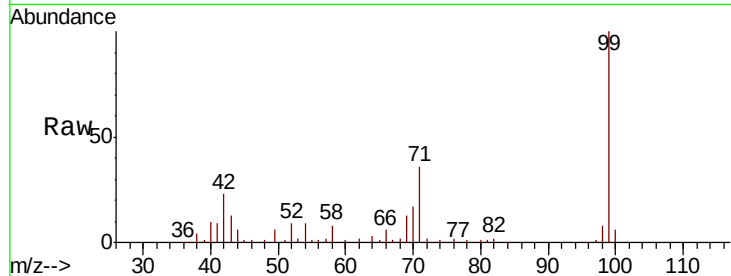


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

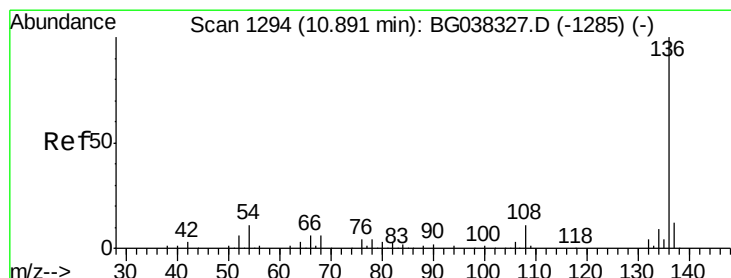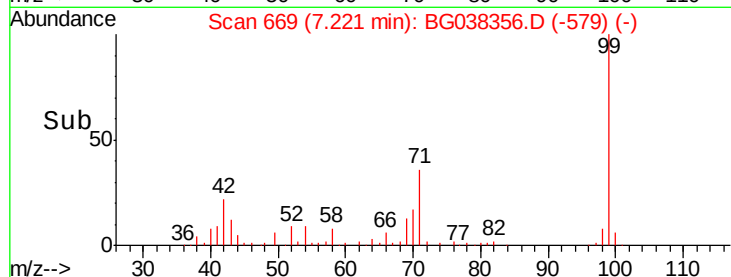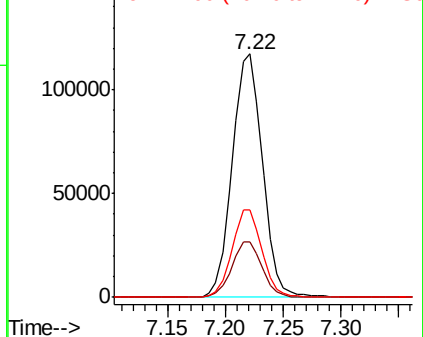

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.89 min Scan# 1293

Delta R.T. -0.00 min

Lab File: BG038356.D

Acq: 5 Dec 2018 12:22

Tgt Ion: 136 Resp: 137423


Ion Ratio Lower Upper

136 100

137 11.5 9.6 14.4

54 10.5 7.9 11.9

68 6.5 4.8 7.2

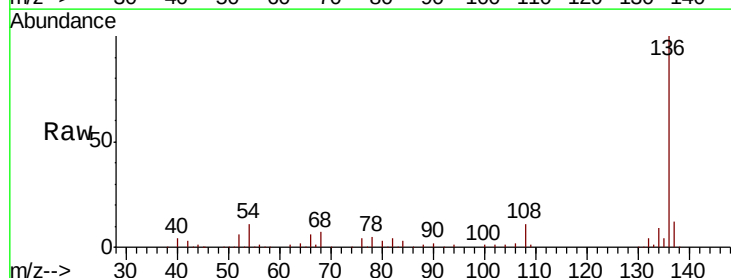



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



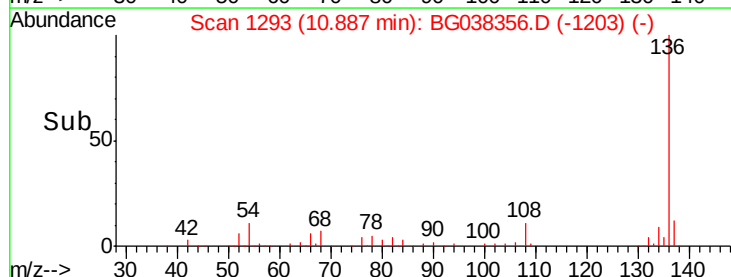
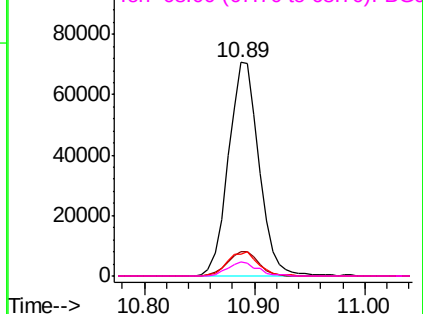


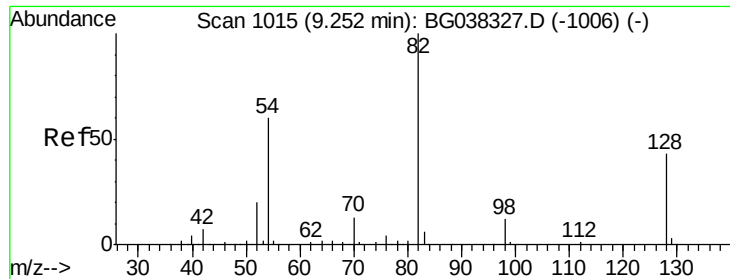

#23
Nitrobenzene-d5
Concen: 67.709 ng
RT: 9.25 min Scan# 1014
Delta R.T. -0.00 min
Lab File: BG038356.D
Acq: 5 Dec 2018 12:22




Instrument :
BNA_G
ClientSampleId :
CB-1129-S-TCLP-GRID19


Tot Ion: 82 Resp: 187414
Ion Ratio Lower Upper
82 100
128 43.2 34.6 51.8
54 61.8 45.3 67.9

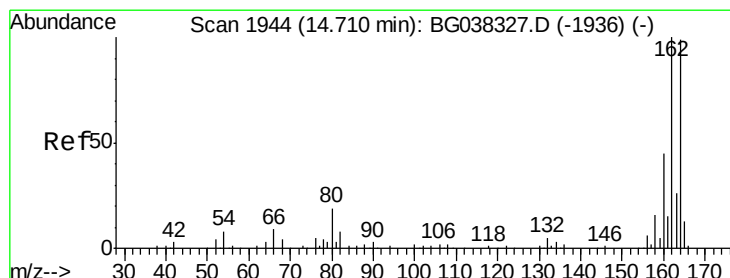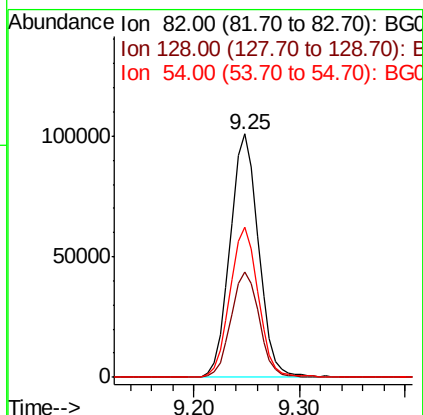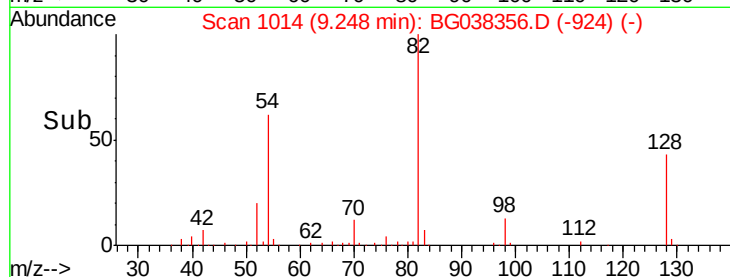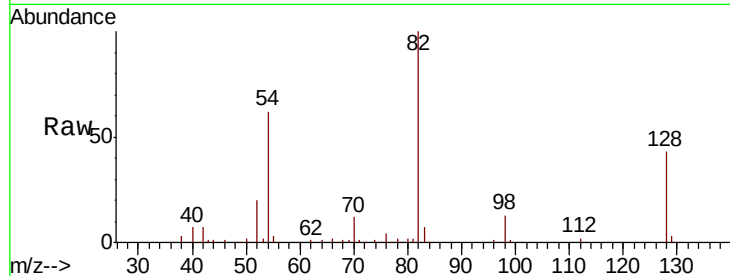

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.71 min Scan# 1943
Delta R.T. -0.00 min
Lab File: BG038356.D
Acq: 5 Dec 2018 12:22

Tgt Ion:164 Resp: 84663
Ion Ratio Lower Upper
164 100
162 106.5 81.3 121.9
160 44.6 36.3 54.5

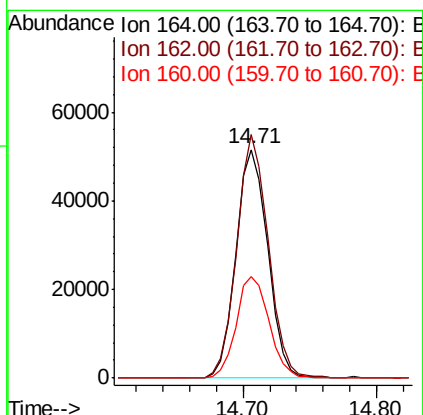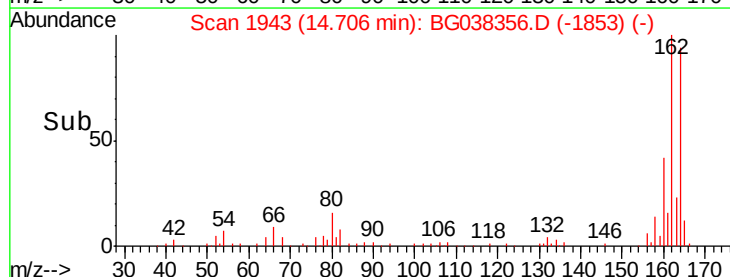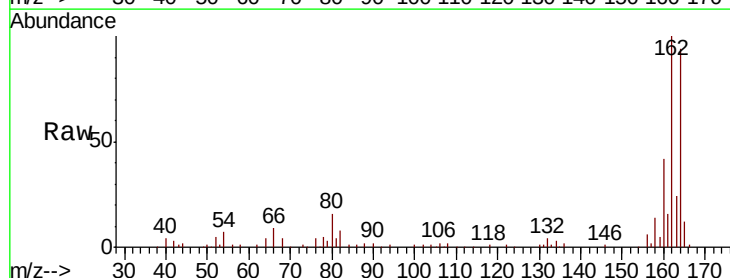


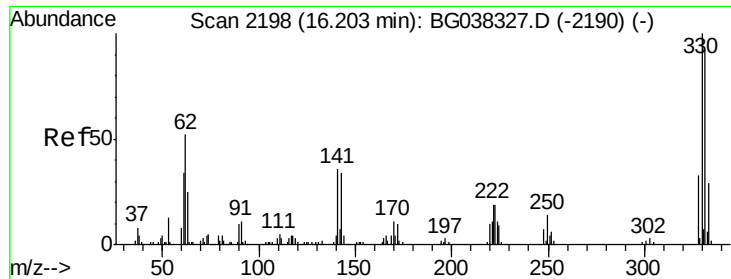




#42
 2,4,6-Tribromophenol
 Concen: 128.294 ng
 RT: 16.20 min Scan# 2197
 Delta R.T. -0.00 min
 Lab File: BG038356.D
 Acq: 5 Dec 2018 12:22

Instrument :
 BNA_G
 ClientSampleId :
 CB-1129-S-TCLP-GRID19

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	78.4	117.6
141	39.3	32.2	48.2

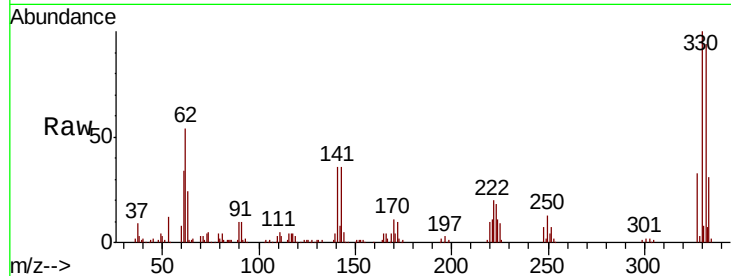


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

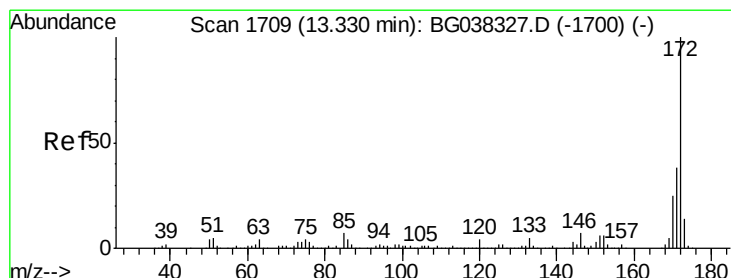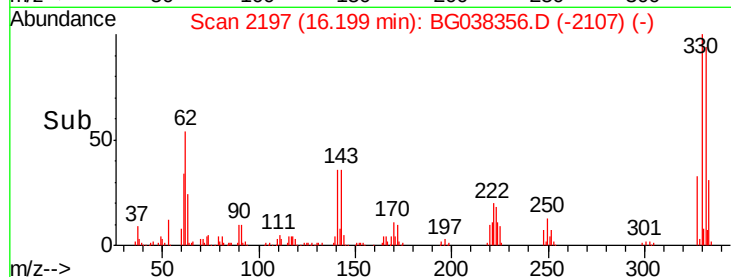
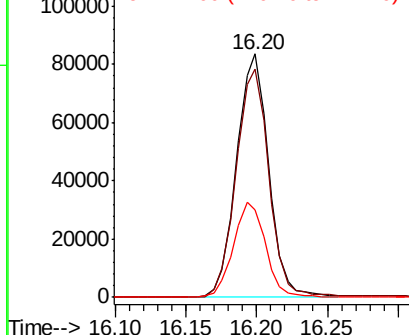



#45
 2-Fluorobiphenyl
 Concen: 72.944 ng
 RT: 13.33 min Scan# 1708
 Delta R.T. -0.00 min
 Lab File: BG038356.D
 Acq: 5 Dec 2018 12:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	31.0	46.4
170	24.6	20.2	30.2

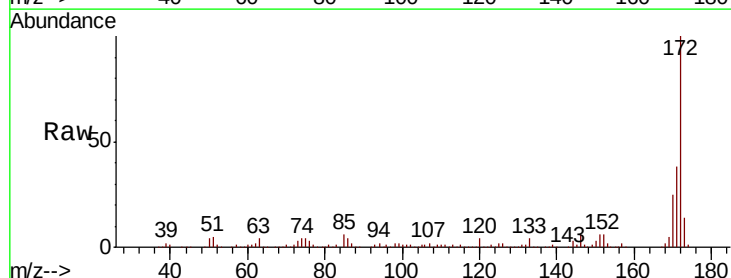

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

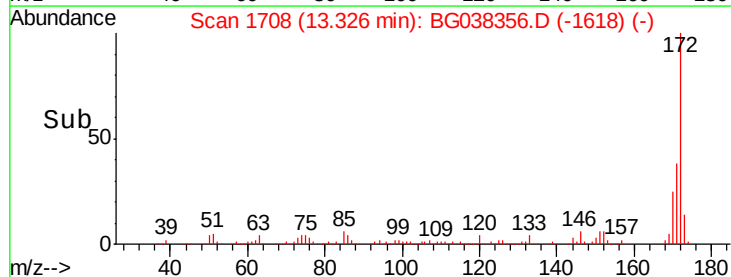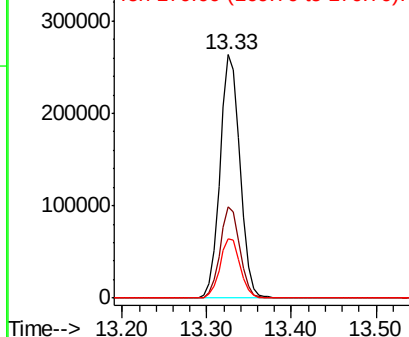

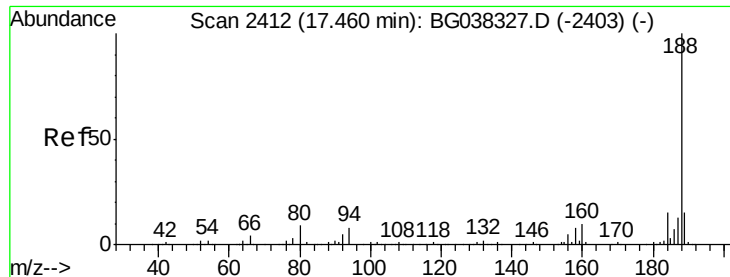

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.46 min Scan# 2411

Delta R.T. -0.00 min

Lab File: BG038356.D

Acq: 5 Dec 2018 12:22

Instrument :

BNA_G

ClientSampleId :

CB-1129-S-TCLP-GRID19


Tot Ion:188 Resp: 221558

Ion Ratio Lower Upper

188 100

94 7.8 7.2 10.8




80 8.5 7.7 11.5

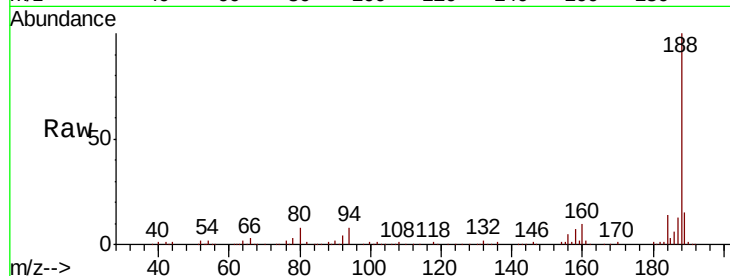

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0

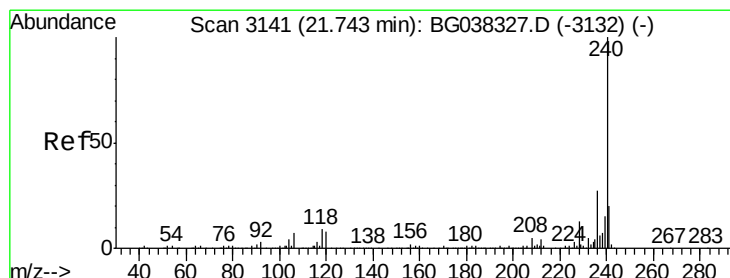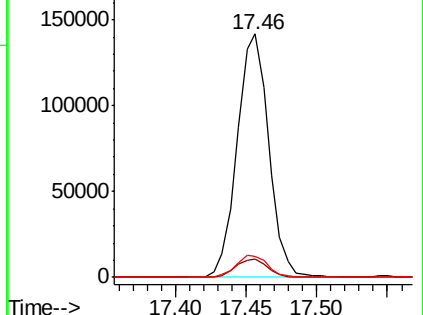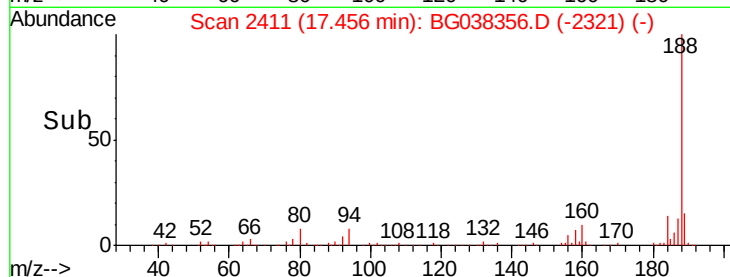

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.73 min Scan# 3139

Delta R.T. -0.01 min

Lab File: BG038356.D

Acq: 5 Dec 2018 12:22


Tgt Ion:240 Resp: 222202

Ion Ratio Lower Upper

240 100

120 9.3 8.1 12.1



236 25.6 21.4 32.0

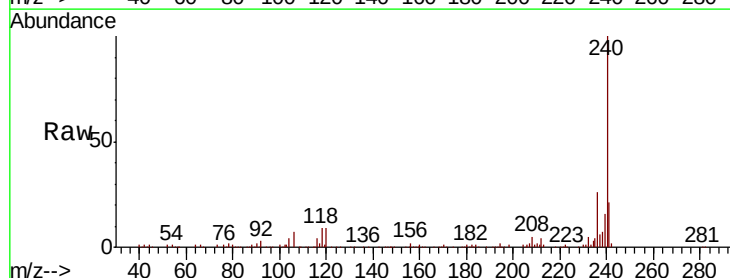


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

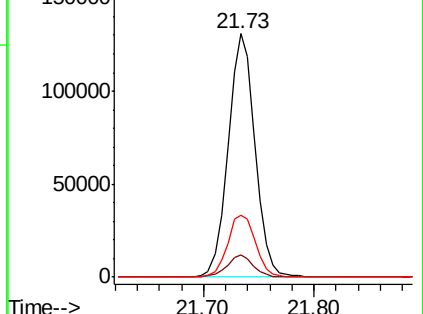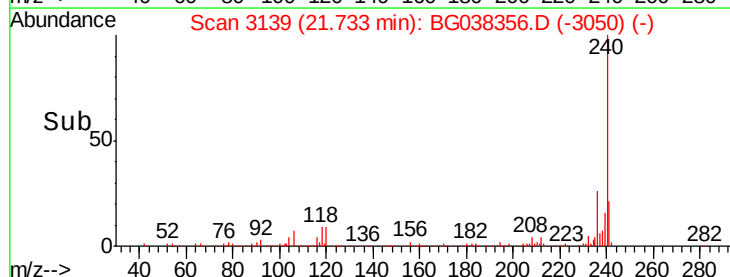

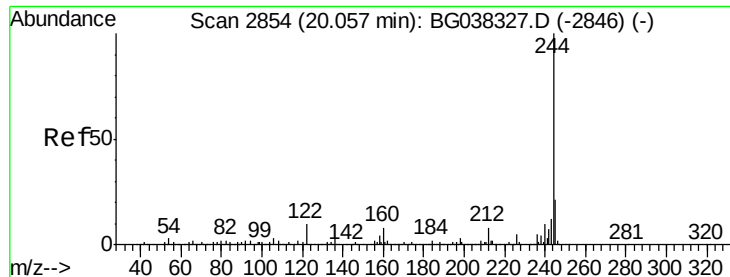

#79

Terphenyl-d14

Concen: 82.054 ng

RT: 20.06 min Scan# 2854

Delta R.T. 0.00 min

Lab File: BG038356.D

Acq: 5 Dec 2018 12:22

Instrument :

BNA_G

ClientSampleId :

CB-1129-S-TCLP-GRID19


Tot Ion:244 Resp: 851095

Ion Ratio Lower Upper

244 100

212 8.1 6.5 9.7




122 8.5 9.0 13.4#

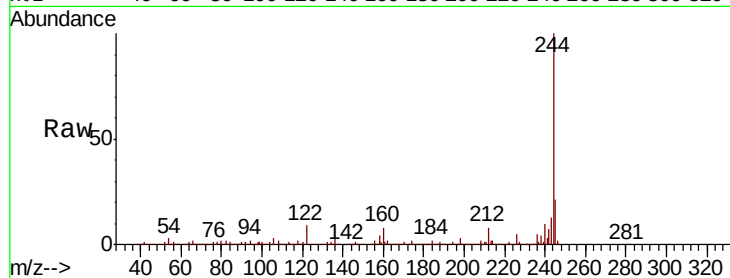

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

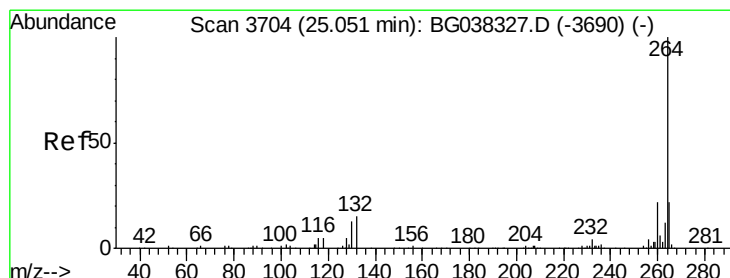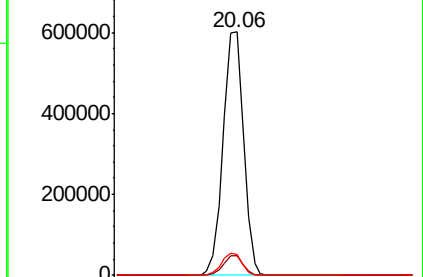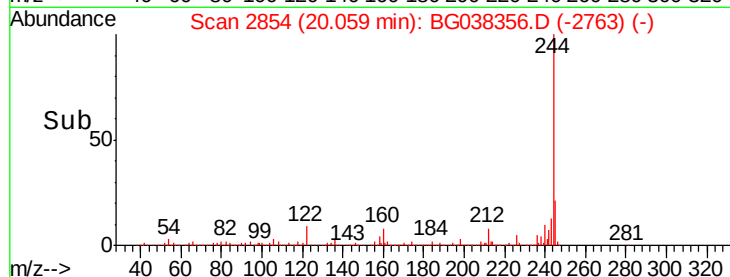

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.04 min Scan# 3702

Delta R.T. -0.01 min

Lab File: BG038356.D

Acq: 5 Dec 2018 12:22


Tgt Ion:264 Resp: 229570

Ion Ratio Lower Upper

264 100

260 23.2 18.2 27.4

265 21.4 17.9 26.9

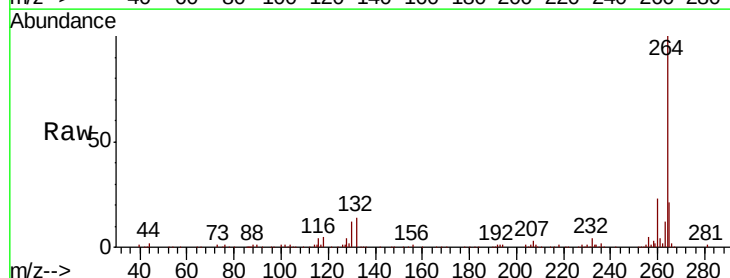

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

