

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
 Data File : BG038345.D
 Acq On : 5 Dec 2018 4:29
 Operator : JU/SJ
 Sample : J6003-23
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NON-UST-03R-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.219	153	158	166	rVB	26878	40278	1.85%	0.187%
2	5.153	310	317	326	rVB2	12374	23338	1.07%	0.108%
3	5.617	389	396	407	rBV	288359	481116	22.04%	2.233%
4	7.215	661	668	677	rBV	195948	353259	16.18%	1.639%
5	7.597	725	733	746	rBV	445343	797649	36.54%	3.702%
6	8.073	806	814	826	rVB	95387	173172	7.93%	0.804%
7	8.396	859	869	875	rBV	351456	662755	30.36%	3.076%
8	8.437	875	876	884	rVB	23586	30464	1.40%	0.141%
9	8.549	884	895	901	rBV2	15179	25578	1.17%	0.119%
10	9.166	993	1000	1007	rBV3	76174	137811	6.31%	0.640%
11	9.248	1007	1014	1024	rVB2	363947	704836	32.29%	3.271%
12	9.695	1084	1090	1096	rVB	55977	97273	4.46%	0.451%
13	10.059	1145	1152	1158	rBV4	22311	45270	2.07%	0.210%
14	10.124	1158	1163	1172	rVB	53693	107883	4.94%	0.501%
15	10.271	1180	1188	1195	rBV2	209905	385656	17.67%	1.790%
16	10.447	1212	1218	1222	rBV5	15468	29723	1.36%	0.138%
17	10.488	1222	1225	1233	rVV5	18109	39513	1.81%	0.183%
18	10.564	1233	1238	1245	rVB2	19084	33623	1.54%	0.156%
19	10.793	1271	1277	1279	rBV3	17777	32027	1.47%	0.149%
20	10.852	1279	1287	1290	rVV	73111	186667	8.55%	0.866%
21	10.887	1290	1293	1298	rVV2	142121	302218	13.85%	1.403%
22	10.935	1298	1301	1306	rVV3	87555	174965	8.02%	0.812%
23	10.987	1306	1310	1317	rVV	69419	121874	5.58%	0.566%
24	11.081	1317	1326	1332	rVB3	23550	48729	2.23%	0.226%
25	11.240	1347	1353	1358	rBV4	17867	26116	1.20%	0.121%
26	11.352	1366	1372	1378	rVB3	31149	56650	2.60%	0.263%
27	11.463	1383	1391	1395	rBV2	28120	55999	2.57%	0.260%
28	11.540	1400	1404	1411	rVB	40659	73873	3.38%	0.343%
29	11.792	1440	1447	1453	rBV	77576	138990	6.37%	0.645%
30	11.980	1470	1479	1485	rBV	71771	130813	5.99%	0.607%
31	12.068	1488	1494	1501	rVV2	86649	161502	7.40%	0.749%
32	12.192	1511	1515	1520	rVB2	23941	40856	1.87%	0.190%
33	12.256	1520	1526	1534	rBV3	51237	116774	5.35%	0.542%
34	12.350	1534	1542	1547	rVV5	20283	58121	2.66%	0.270%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
 Data File : BG038345.D
 Acq On : 5 Dec 2018 4:29
 Operator : JU/SJ
 Sample : J6003-23
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NON-UST-03R-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.421	1550	1554	1561	rVV2	62976	118725	5.44%	0.551%
36	12.492	1561	1566	1568	rVV2	19916	29844	1.37%	0.138%
37	12.539	1568	1574	1582	rVB	665210	1140387	52.24%	5.292%
38	12.762	1600	1612	1619	rBV	701826	1300595	59.58%	6.036%
39	12.826	1619	1623	1627	rVV3	19560	28664	1.31%	0.133%
40	12.962	1634	1646	1650	rBV8	13194	38621	1.77%	0.179%
41	13.044	1655	1660	1665	rVB5	19284	37152	1.70%	0.172%
42	13.326	1699	1708	1717	rVB	853697	1367449	62.65%	6.346%
43	13.631	1752	1760	1766	rBV3	39683	79987	3.66%	0.371%
44	13.696	1766	1771	1772	rBV4	23319	36904	1.69%	0.171%
45	13.737	1773	1778	1781	rBV	90522	152450	6.98%	0.707%
46	13.878	1790	1802	1810	rBV3	248467	714438	32.73%	3.316%
47	14.025	1820	1827	1832	rBV	479934	928047	42.52%	4.307%
48	14.078	1832	1836	1845	rVB	316418	534198	24.47%	2.479%
49	14.260	1860	1867	1871	rBV	218347	364840	16.71%	1.693%
50	14.295	1871	1873	1878	rVB	82991	97566	4.47%	0.453%
51	14.425	1890	1895	1904	rVB	133370	210212	9.63%	0.976%
52	14.671	1931	1937	1939	rBV3	69830	107412	4.92%	0.498%
53	14.707	1939	1943	1948	rVV2	223837	383947	17.59%	1.782%
54	14.777	1948	1955	1960	rVV3	86238	195079	8.94%	0.905%
55	14.824	1960	1963	1969	rVV	21314	33376	1.53%	0.155%
56	14.906	1970	1977	1986	rVV2	64747	171765	7.87%	0.797%
57	14.989	1986	1991	1998	rVV3	37117	86970	3.98%	0.404%
58	15.094	1998	2009	2016	rVV3	138642	301654	13.82%	1.400%
59	15.171	2016	2022	2029	rVV	102119	173317	7.94%	0.804%
60	15.312	2040	2046	2051	rBV	94834	168973	7.74%	0.784%
61	15.365	2051	2055	2062	rVB	75817	110877	5.08%	0.515%
62	15.482	2066	2075	2078	rVV4	65530	158697	7.27%	0.736%
63	15.517	2078	2081	2089	rVB2	49069	79839	3.66%	0.371%
64	15.658	2094	2105	2110	rBV5	35286	101236	4.64%	0.470%
65	15.752	2114	2121	2131	rVV4	87753	211490	9.69%	0.981%
66	15.882	2131	2143	2152	rVV2	177722	395094	18.10%	1.834%
67	15.958	2152	2156	2160	rVV5	22528	41251	1.89%	0.191%
68	16.011	2160	2165	2166	rVV3	21293	33827	1.55%	0.157%
69	16.034	2166	2169	2177	rVB4	26825	58705	2.69%	0.272%
70	16.199	2190	2197	2204	rBV2	697059	1088191	49.85%	5.050%
71	16.381	2221	2228	2230	rBV	12569	22430	1.03%	0.104%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
 Data File : BG038345.D
 Acq On : 5 Dec 2018 4:29
 Operator : JU/SJ
 Sample : J6003-23
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NON-UST-03R-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	16.410	2230	2233	2242	rVB2	18758	33215	1.52%	0.154%
73	16.551	2252	2257	2261	rBV4	15250	22991	1.05%	0.107%
74	16.734	2280	2288	2295	rBV6	31938	92445	4.24%	0.429%
75	16.804	2295	2300	2305	rBV2	74110	130063	5.96%	0.604%
76	16.898	2312	2316	2321	rVB4	21684	37018	1.70%	0.172%
77	17.004	2329	2334	2337	rBV6	14201	26008	1.19%	0.121%
78	17.274	2372	2380	2388	rVB	29106	54147	2.48%	0.251%
79	17.456	2404	2411	2415	rBV2	302381	480203	22.00%	2.228%
80	17.497	2415	2418	2423	rVB	102717	145110	6.65%	0.673%
81	17.644	2430	2443	2447	rBV6	15387	35495	1.63%	0.165%
82	17.856	2472	2479	2491	rVB8	8222	23696	1.09%	0.110%
83	18.326	2550	2559	2563	rBV	35186	70232	3.22%	0.326%
84	18.379	2563	2568	2577	rVB2	40881	78792	3.61%	0.366%
85	18.514	2585	2591	2595	rBV2	19390	31834	1.46%	0.148%
86	18.843	2639	2647	2656	rVB5	20936	37139	1.70%	0.172%
87	20.053	2847	2853	2863	rBV	1602841	2182828	100.00%	10.130%
88	21.734	3133	3139	3147	rBV	319323	537233	24.61%	2.493%
89	25.041	3684	3702	3716	rVB	174670	530286	24.29%	2.461%


Sum of corrected areas: 21548315

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
Data File : BG038345.D
Acq On : 5 Dec 2018 4:29
Operator : JU/SJ
Sample : J6003-23
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NON-UST-03R-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

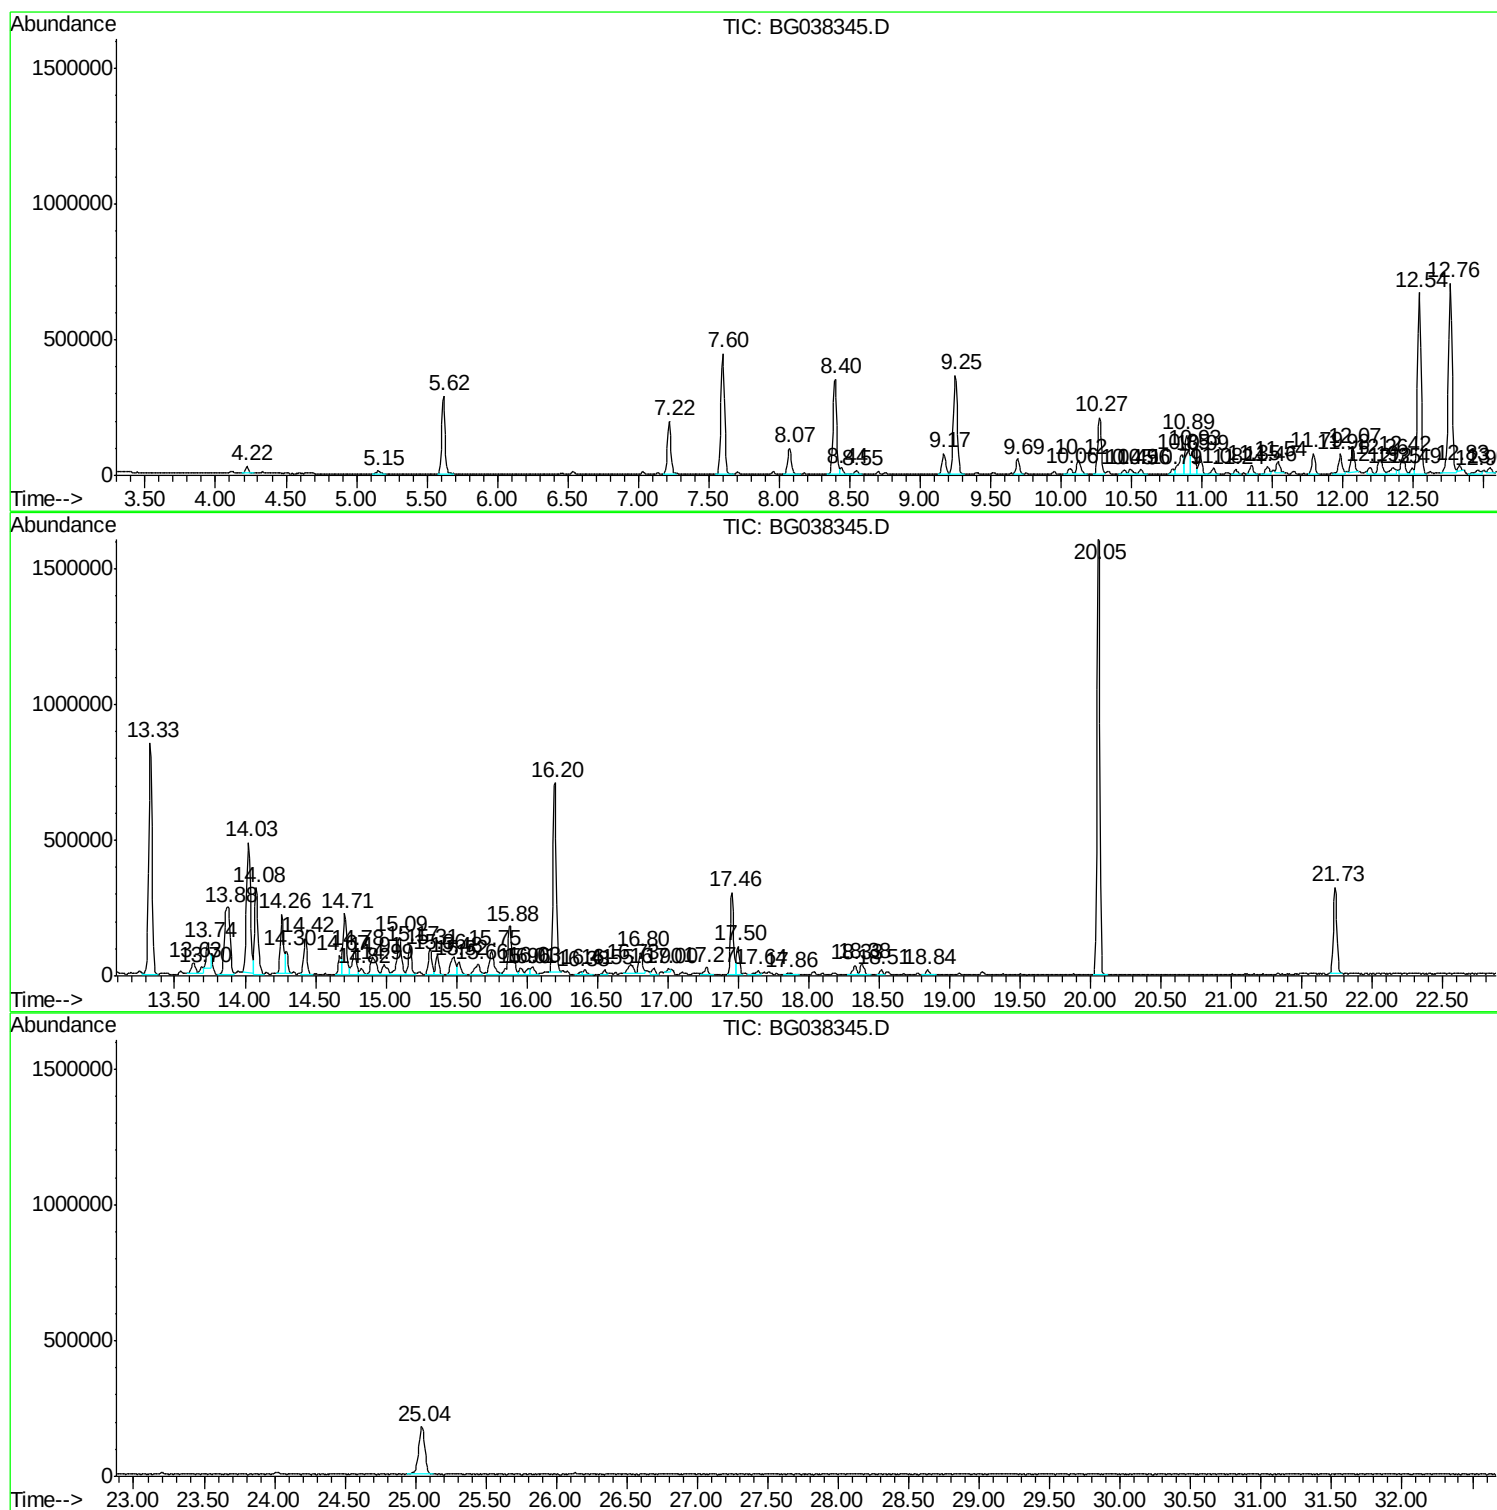

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120418\
Data_File : BG038345.D
Acq_On : 5_Dec_2018 4:299
Operator : JU/SJJ
Sample : J6003-233
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
NON-UST-03R-C

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
