


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
 Data File : BG038323.D
 Acq On : 4 Dec 2018 10:45
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

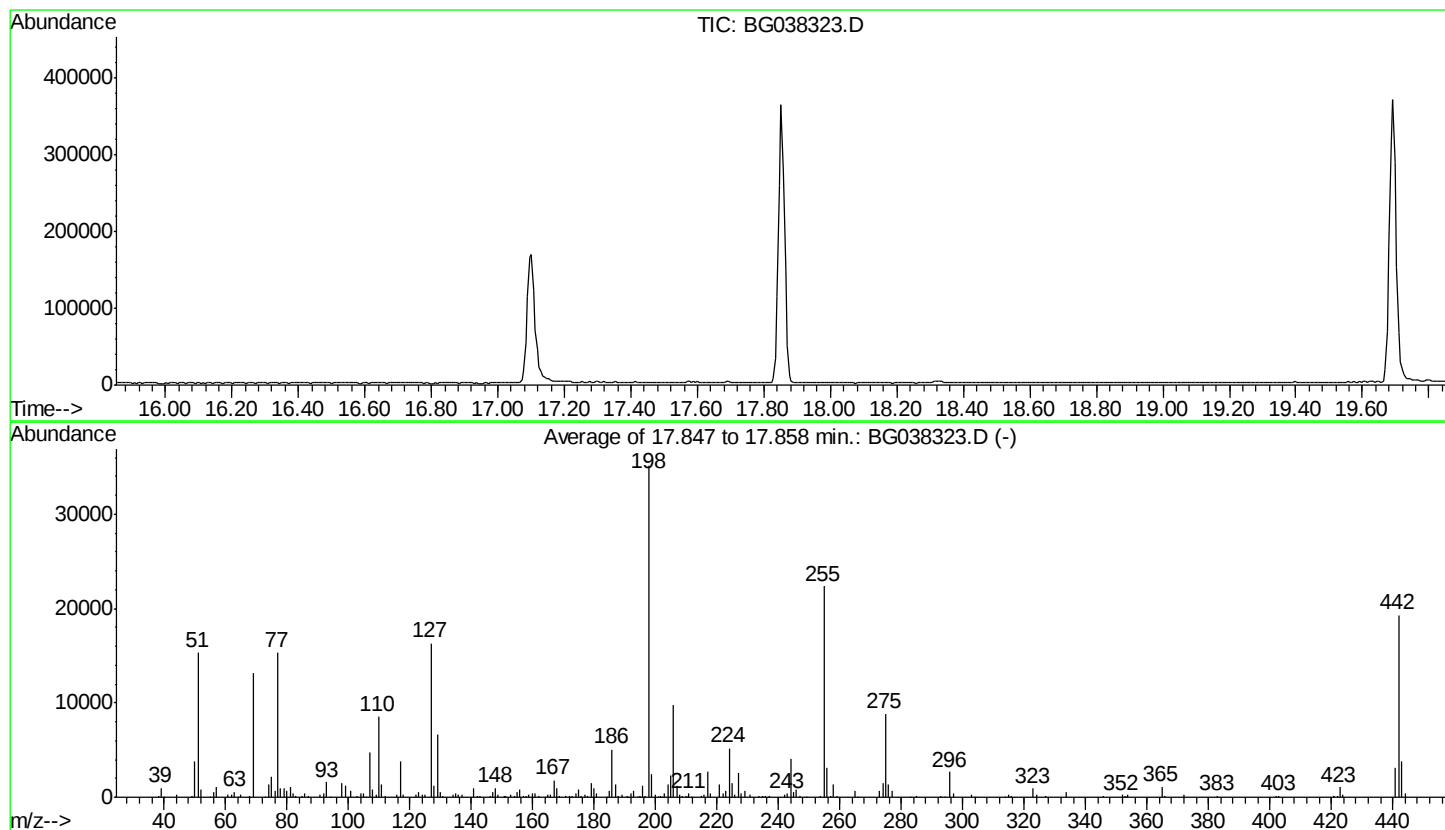

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	15279	PASS
68	69	0.00	2	1.4	189	PASS
69	198	0.00	100	37.6	13205	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	16328	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35141	PASS
199	198	5	9	6.8	2391	PASS
275	198	10	60	25.2	8847	PASS
365	198	1	100	3.2	1122	PASS
441	198	0.01	100	8.9	3137	PASS
442	198	50	100	55.0	19327	PASS
443	442	15	24	19.8	3829	PASS