


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120418\
Data File : BG038348.D
Acq On : 5 Dec 2018 7:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 04 17:15:40 2018

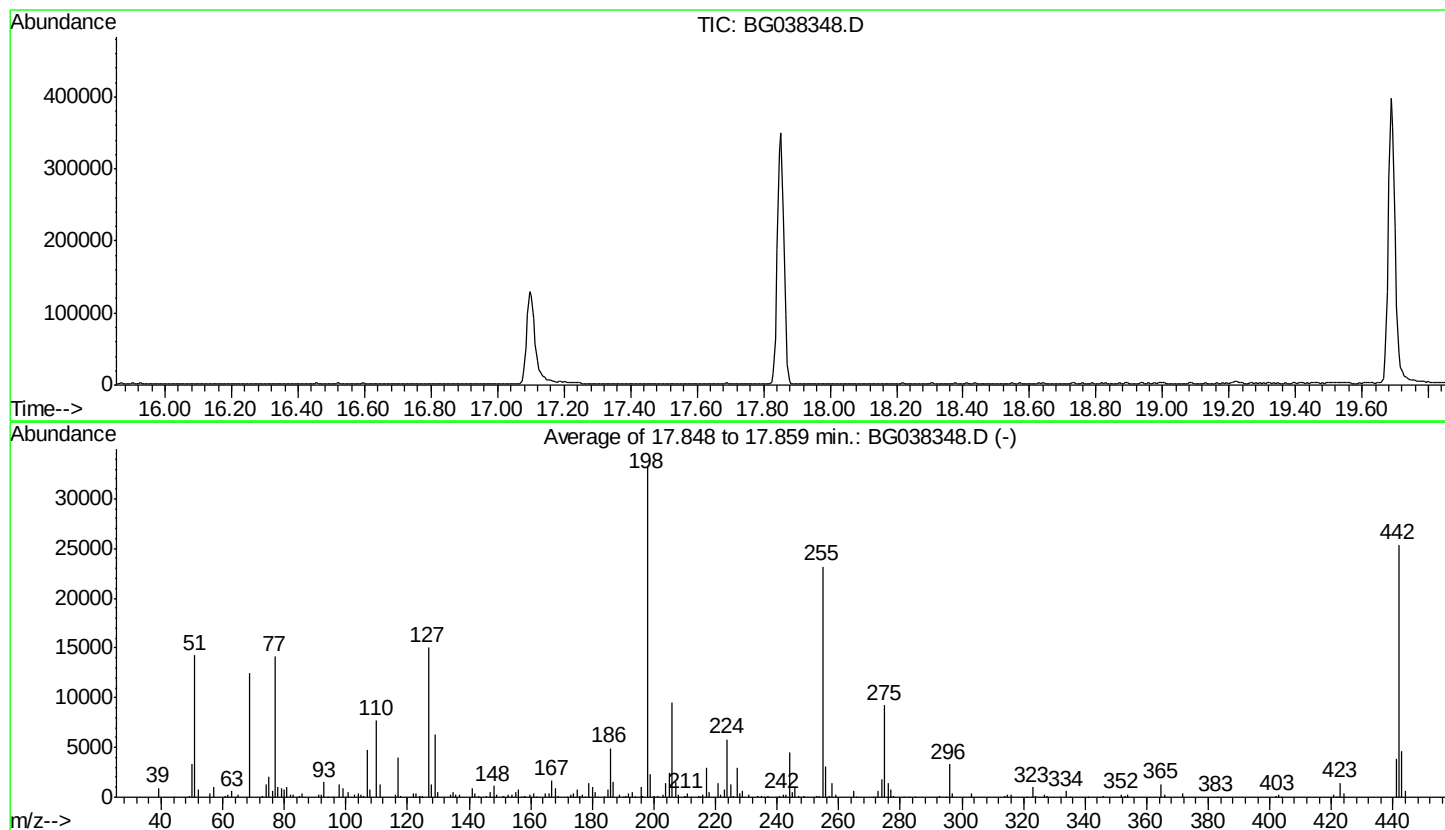

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	14230	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.4	12468	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.1	15024	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33325	PASS
199	198	5	9	7.1	2367	PASS
275	198	10	60	27.8	9251	PASS
365	198	1	100	4.1	1350	PASS
441	198	0.01	100	11.8	3925	PASS
442	198	50	100	76.2	25410	PASS
443	442	15	24	18.5	4697	PASS