

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120420\
 Data File : BG047604.D
 Acq On : 5 Dec 2020 13:52
 Operator : CG/JU
 Sample : L4864-13
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BH5

Quant Time: Dec 07 05:08:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 07 05:06:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.25	152	27986	20.00	ng/ul	-0.02
18) Naphthalene-d8	11.08	136	111881	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.86	164	91353	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.60	188	231705	20.00	ng/ul	-0.02
78) Chrysene-d12	21.88	240	220784	20.00	ng/ul	-0.02
86) Perylene-d12	25.26	264	231313	20.00	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.58	96	4090	5.31	ng/uL	-0.03
5) Phenol-d5	7.39	99	101333	36.11	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.56	67	54432	34.00	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.77	132	79618	42.30	ng/ul	-0.02
13) 4-Methylphenol-d8	8.94	113	82067	38.05	ng/ul	-0.02
19) Nitrobenzene-d5	9.42	128	40967	44.33	ng/ul	-0.02
22) 2-Nitrophenol-d4	10.15	143	50047	49.63	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.69	165	98825	42.81	ng/ul	-0.02
29) 4-Chloroaniline-d4	11.20	131	115566	49.50	ng/ul	-0.02
44) Dimethylphthalate-d6	14.26	166	352729	44.98	ng/ul	-0.02
47) Acenaphthylene-d8	14.56	160	399968	44.13	ng/ul	-0.02
52) 4-Nitrophenol-d4	15.03	143	53104	44.38	ng/ul	0.00
58) Fluorene-d10	15.85	176	327535	45.59	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.95	200	67296	51.03	ng/ul	-0.02
71) Anthracene-d10	17.70	188	536622	46.69	ng/ul	-0.02
79) Pyrene-d10	19.96	212	600128	46.71	ng/ul	-0.01
90) Benzo(a)pyrene-d12	25.04	264	617526	46.38	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	7.41	94	6988	2.599	ng/ul#	78
15) N-Nitroso-di-n-propylamine	8.94	70	3189	1.591	ng/ul#	1
21) Isophorone	10.15	82	9459	1.660	ng/ul#	73
45) Dimethylphthalate	14.30	163	92483	11.561	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120420\  
Data File : BG047604.D  
Acq On    : 5 Dec 2020 13:52  
Operator  : CG/JU  
Sample    : L4864-13  
Misc      :  
ALS Vial  : 37 Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
C0BH5

Quant Time: Dec 07 05:08:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 07 05:06:33 2020
Response via : Initial Calibration

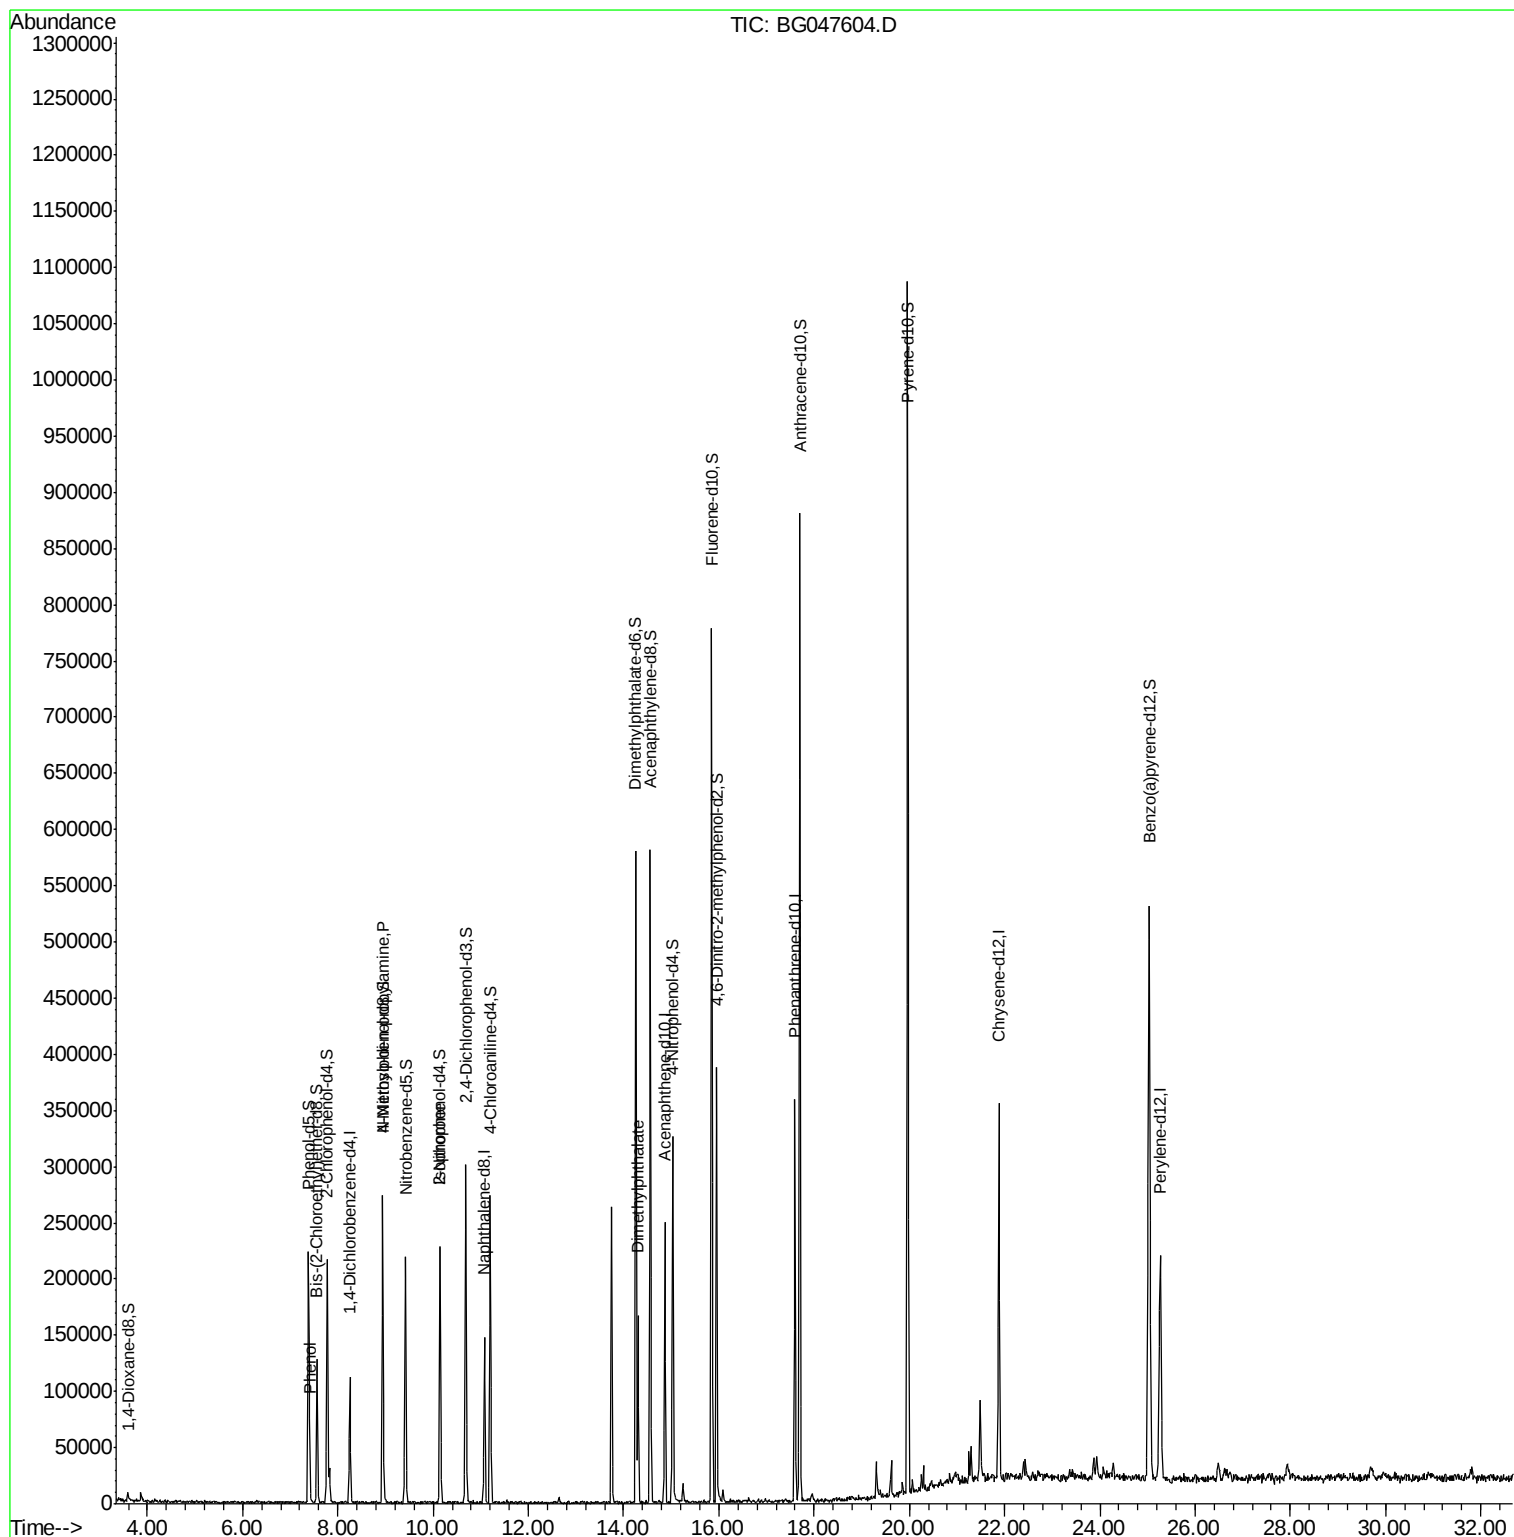

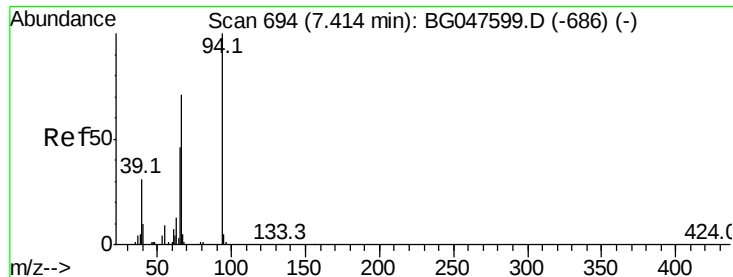

#6

Phenol

Concen: 2.599 ng/ul

RT: 7.41 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG047604.D

Acq: 5 Dec 2020 13:52

Instrument :

BNA_G

ClientSampleId :

C0BH5


Tot Ion: 94 Resp: 6988

Ion Ratio Lower Upper




94 100

65 68.3 31.2 46.8#

66 69.7 52.2 78.2

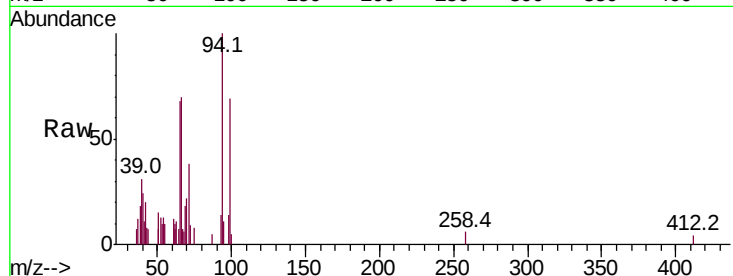

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

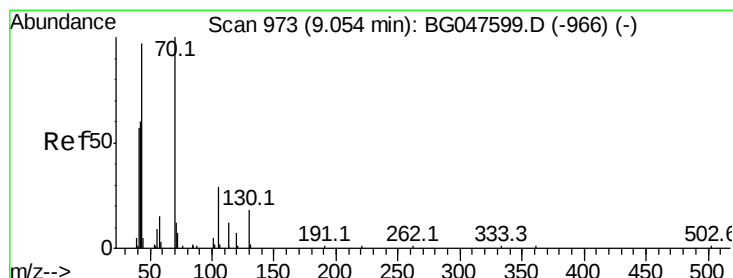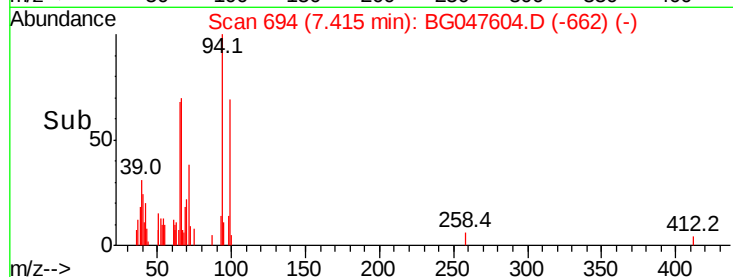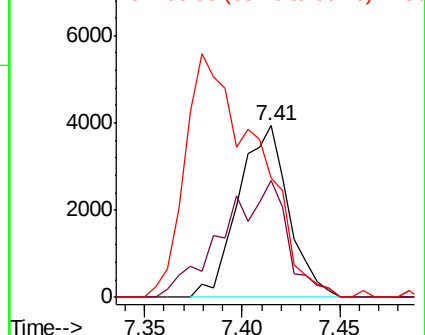

#15

N-Nitroso-di-n-propylamine

Concen: 1.591 ng/ul

RT: 8.94 min Scan# 953

Delta R.T. -0.14 min

Lab File: BG047604.D

Acq: 5 Dec 2020 13:52

Tgt Ion: 70 Resp: 3189


Ion Ratio Lower Upper

70 100



42 390.7 44.2 66.2#


101 0.0 9.0 13.6#

130 0.0 15.1 22.7#

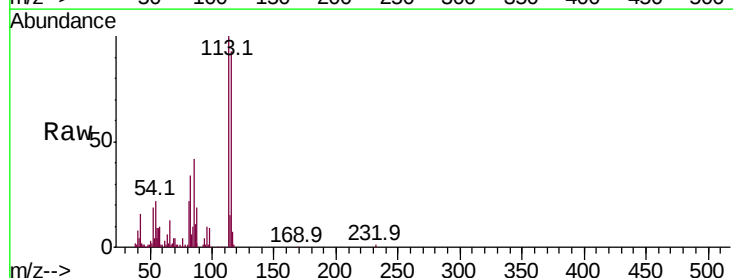

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

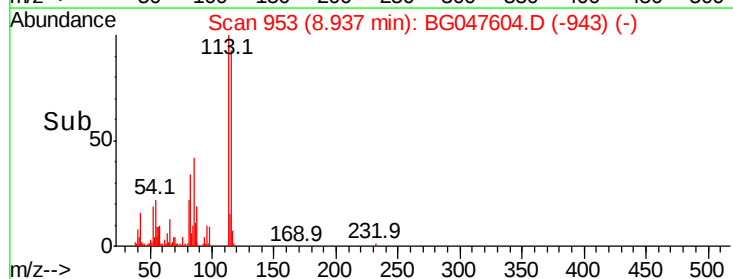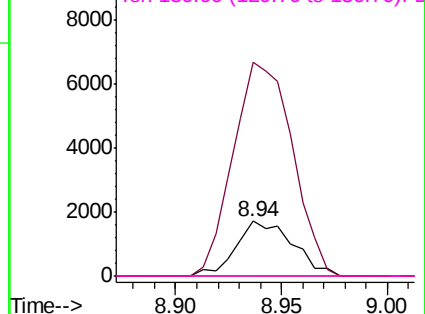

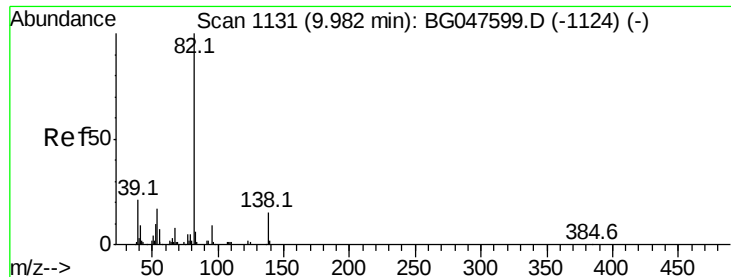

#21

Isophorone

Concen: 1.660 ng/ul

RT: 10.15 min Scan# 1159

Delta R.T. 0.14 min

Lab File: BG047604.D

Acq: 5 Dec 2020 13:52

Instrument :

BNA_G

ClientSampleId :

C0BH5


Tot Ion: 82 Resp: 9459

Ion Ratio Lower Upper




82 100

95 4.8 6.6 9.8#

138 0.0 12.1 18.1#

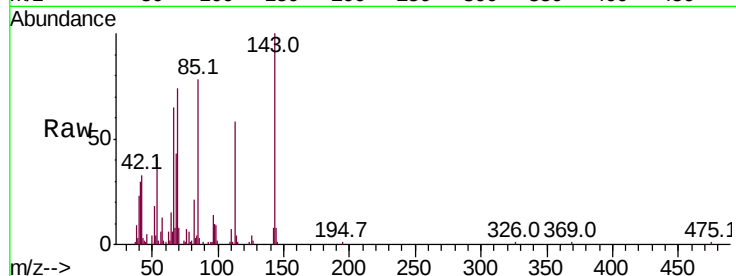

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 95.00 (94.70 to 95.70): BGC
Ion 138.00 (137.70 to 138.70): BGC

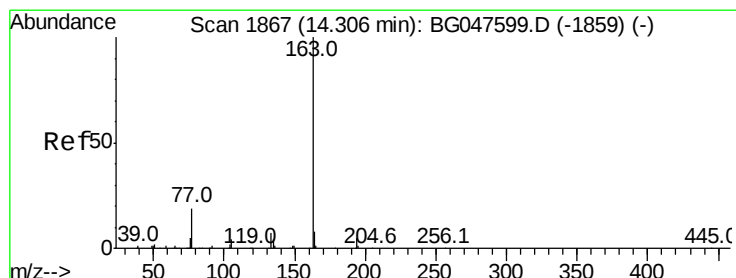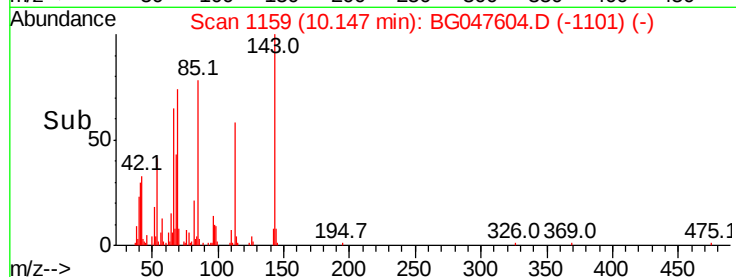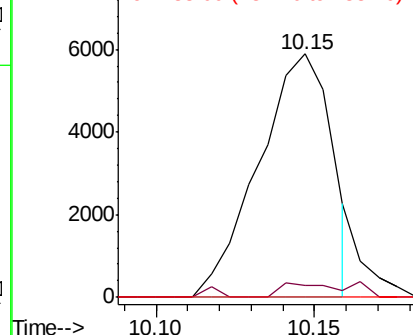

#45

Dimethylphthalate

Concen: 11.561 ng/ul

RT: 14.30 min Scan# 1866

Delta R.T. -0.02 min

Lab File: BG047604.D

Acq: 5 Dec 2020 13:52


Tgt Ion: 163 Resp: 92483

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 9.4 8.8 13.2

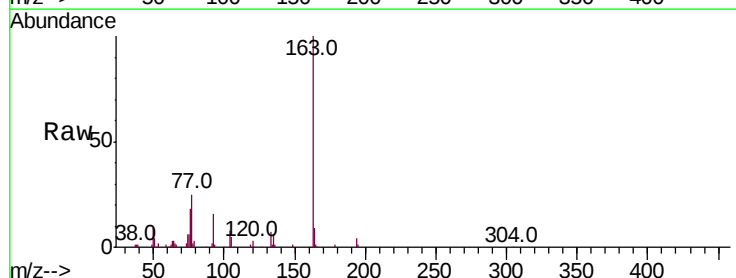

Abundance Ion 163.00 (162.70 to 163.70): BGC
Ion 194.00 (193.70 to 194.70): BGC
Ion 164.00 (163.70 to 164.70): BGC

