
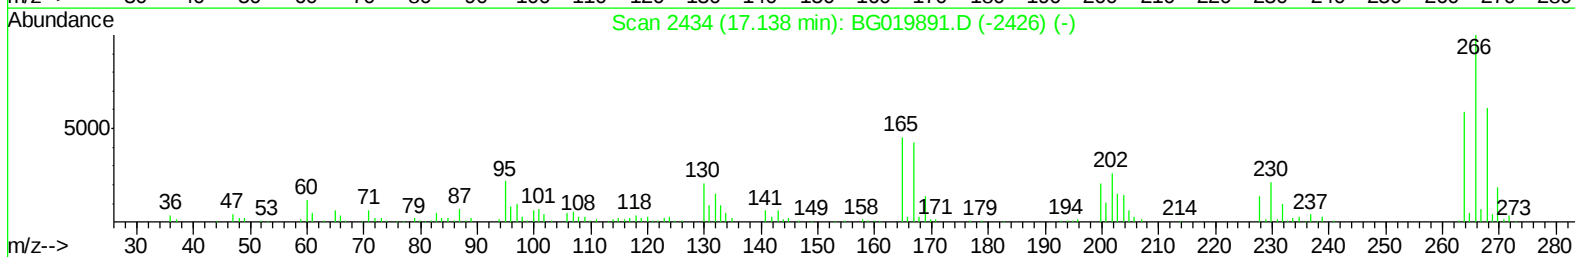
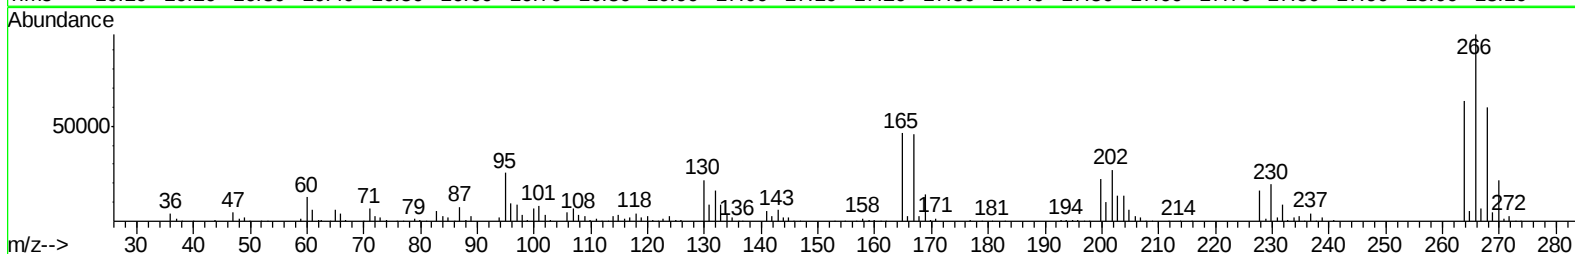


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120515\
Data File : BG019941.D
Acq On : 5 Dec 2015 14:26
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:53:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

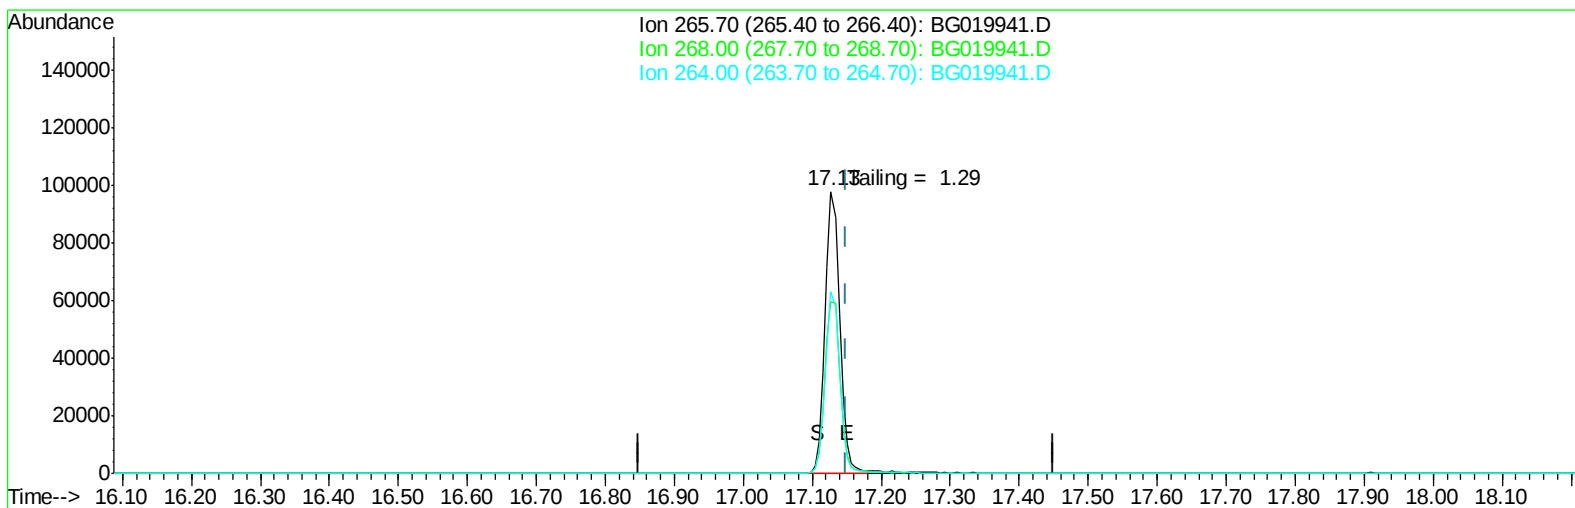

TIC: BG019941.D

(69) Pentachlorophenol (C)




17.127min (-0.023) 0.00ng

response 145647

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	61.00
264.00	60.10	64.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120515\
Data File : BG019941.D
Acq On : 5 Dec 2015 14:26
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:53:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

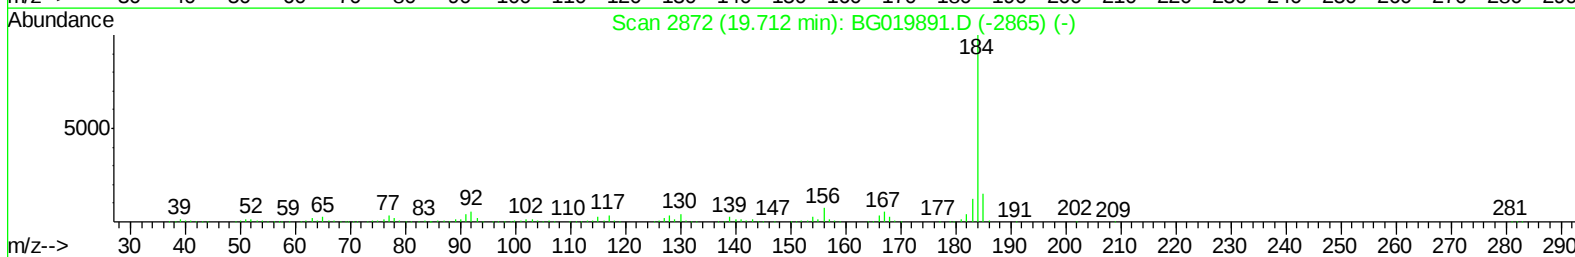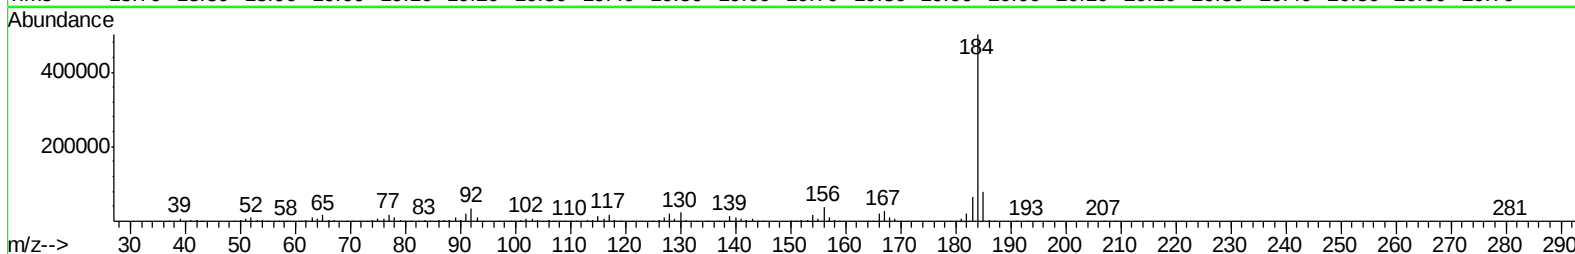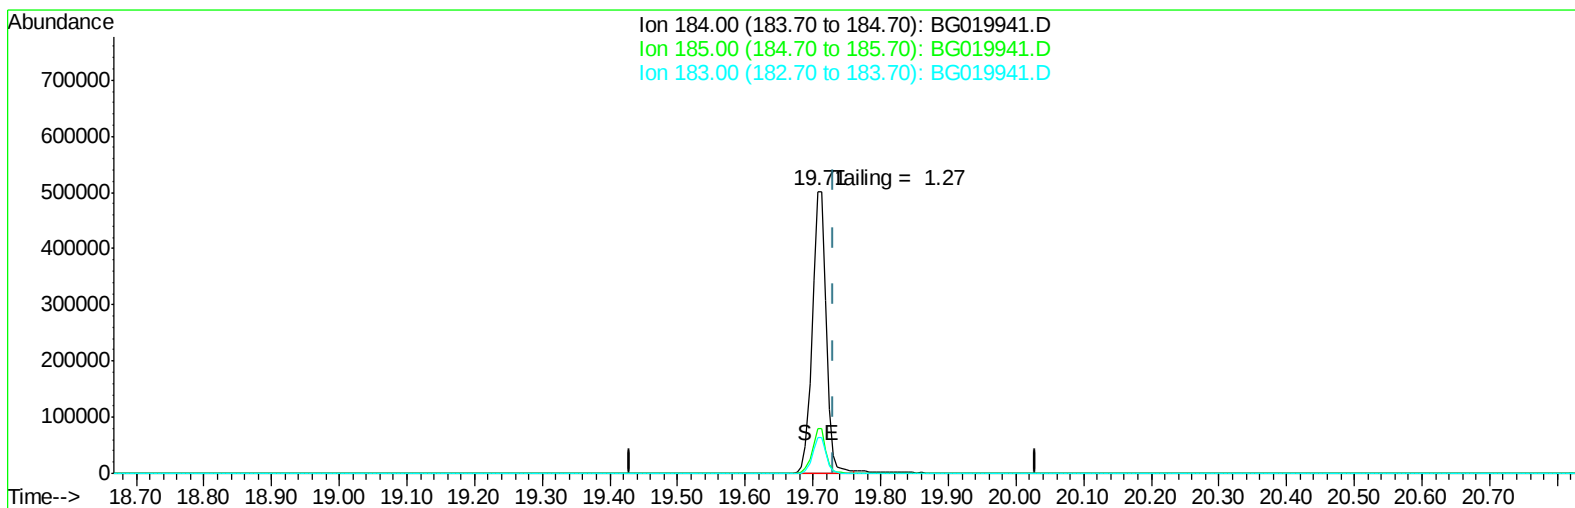

TIC: BG019941.D

(76) Benzidine

19.707min (-0.023) 0.00ng

response 735576

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	16.07
183.00	12.60	12.76
0.00	0.00	0.00