
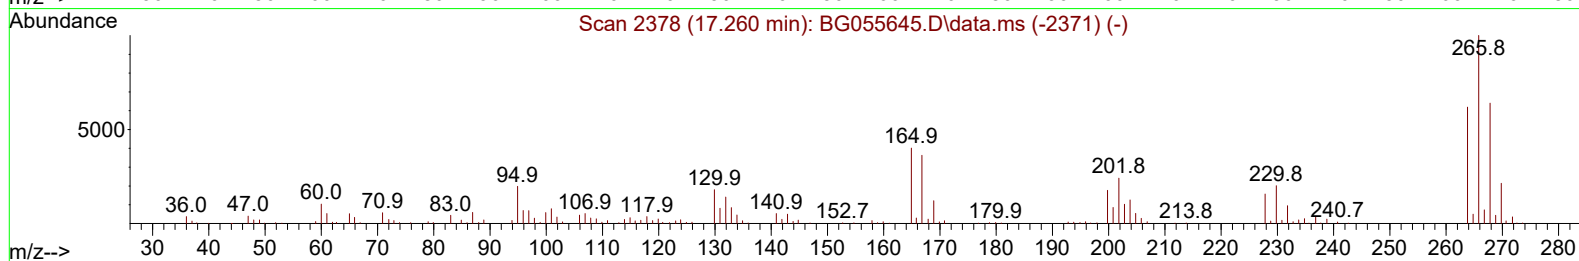
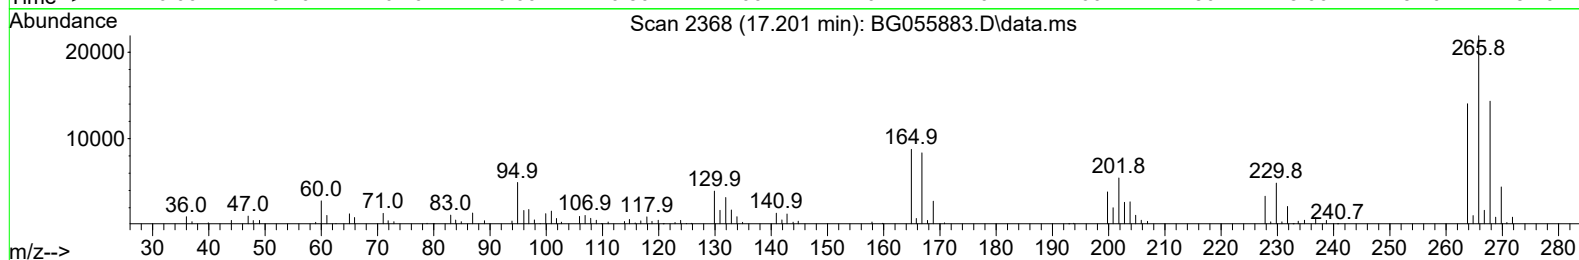


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120522\
Data File : BG055883.D
Acq On : 5 Dec 2022 12:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 06:07:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 04:41:17 2022
Response via : Initial Calibration

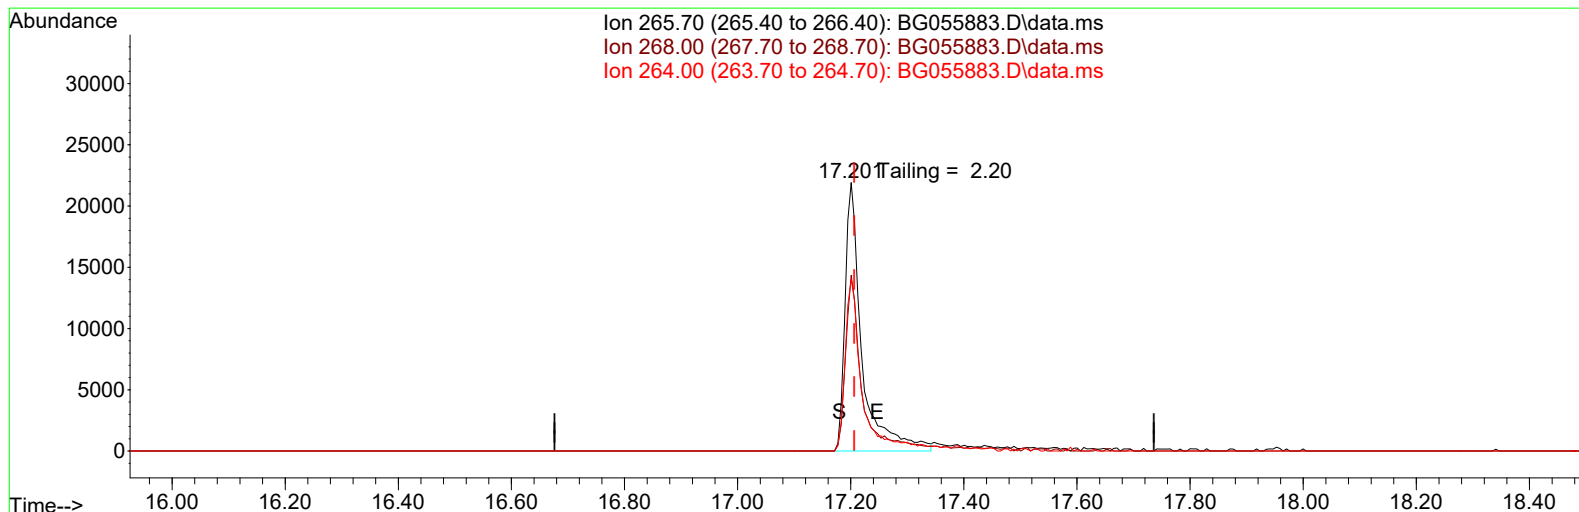

TIC: BG055883.D\data.ms

(70) Pentachlorophenol (C)




17.201min (-0.005) 17660.22 ng

response 44768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.46
264.00	61.90	64.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120522\
 Data File : BG055883.D
 Acq On : 5 Dec 2022 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 06:07:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 04:41:17 2022
 Response via : Initial Calibration

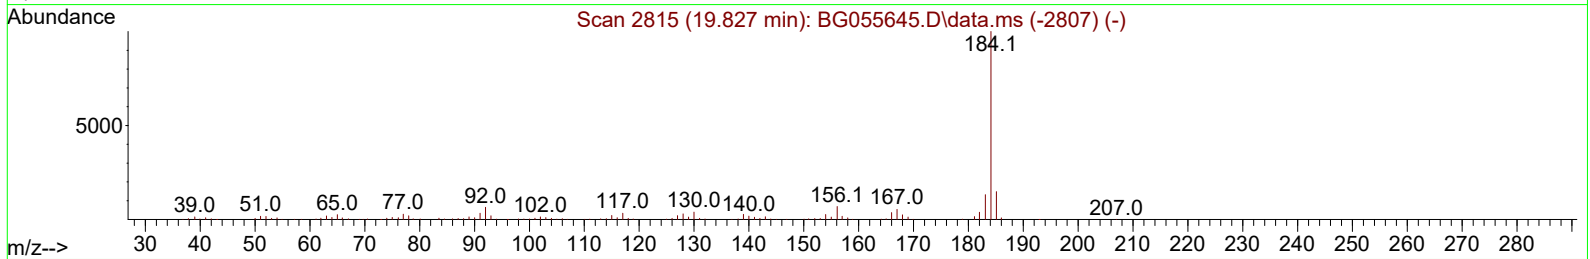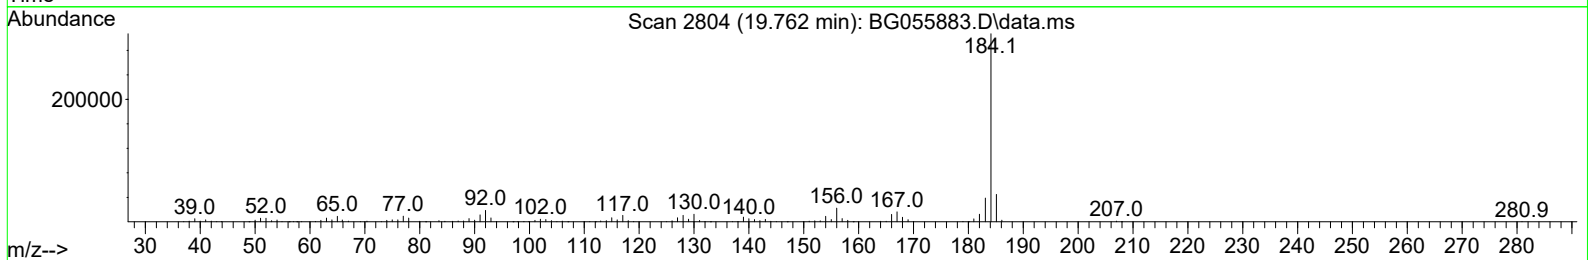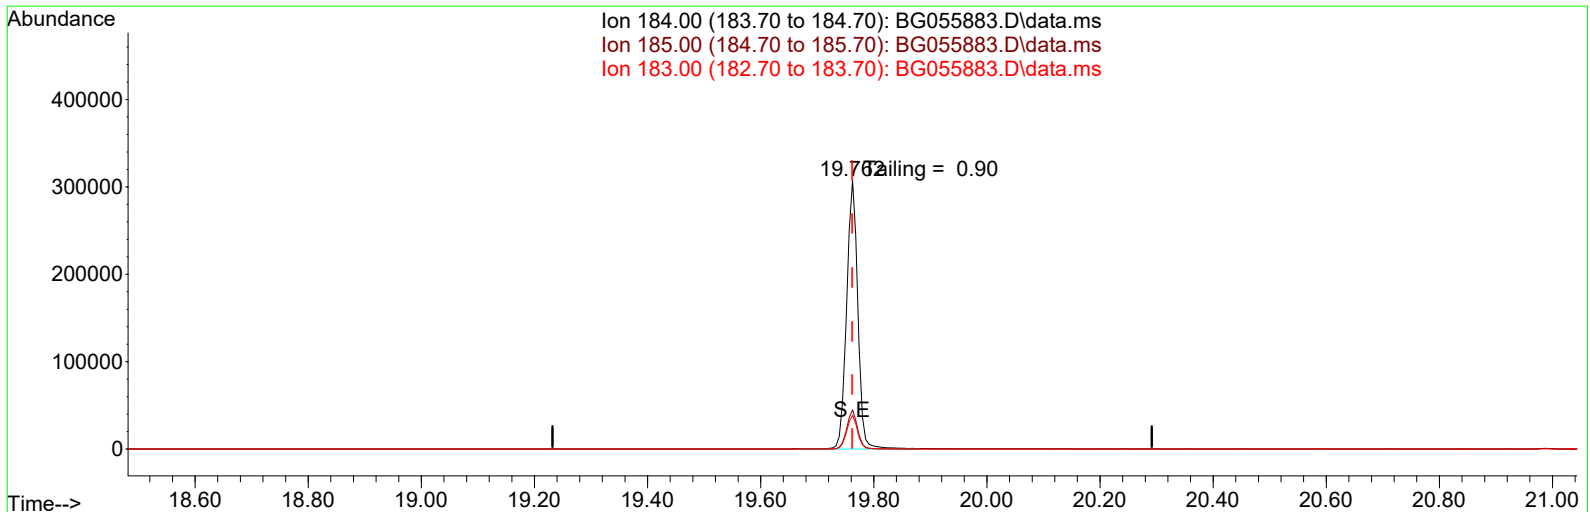

TIC: BG055883.D\data.ms

(77) Benzidine

19.762min (+ 0.000) 0.00 ng

response 425372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.61
183.00	13.20	12.61
0.00	0.00	0.00