

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120522\
 Data File : BG055893.D
 Acq On : 5 Dec 2022 20:33
 Operator : CG/JU
 Sample : N5870-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ML-1

Quant Time: Dec 06 04:48:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 04:41:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.173	152	29267	20.000	ng	0.00
21) Naphthalene-d8	10.999	136	126275	20.000	ng	0.00
39) Acenaphthene-d10	14.801	164	98268	20.000	ng	0.00
64) Phenanthrene-d10	17.545	188	251773	20.000	ng	0.00
76) Chrysene-d12	21.828	240	242479	20.000	ng	0.00
86) Perylene-d12	25.177	264	251491	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.706	112	177091	109.371	ng	0.00
7) Phenol-d6	7.327	99	252190	117.004	ng	0.00
23) Nitrobenzene-d5	9.342	82	147533	61.753	ng	0.00
42) 2,4,6-Tribromophenol	16.287	330	146839	106.117	ng	0.00
45) 2-Fluorobiphenyl	13.426	172	407634	62.145	ng	0.00
79) Terphenyl-d14	20.130	244	761755	62.835	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120522\
Data File : BG055893.D
Acq On : 5 Dec 2022 20:33
Operator : CG/JU
Sample : N5870-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ML-1

Quant Time: Dec 06 04:48:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 04:41:17 2022
Response via : Initial Calibration




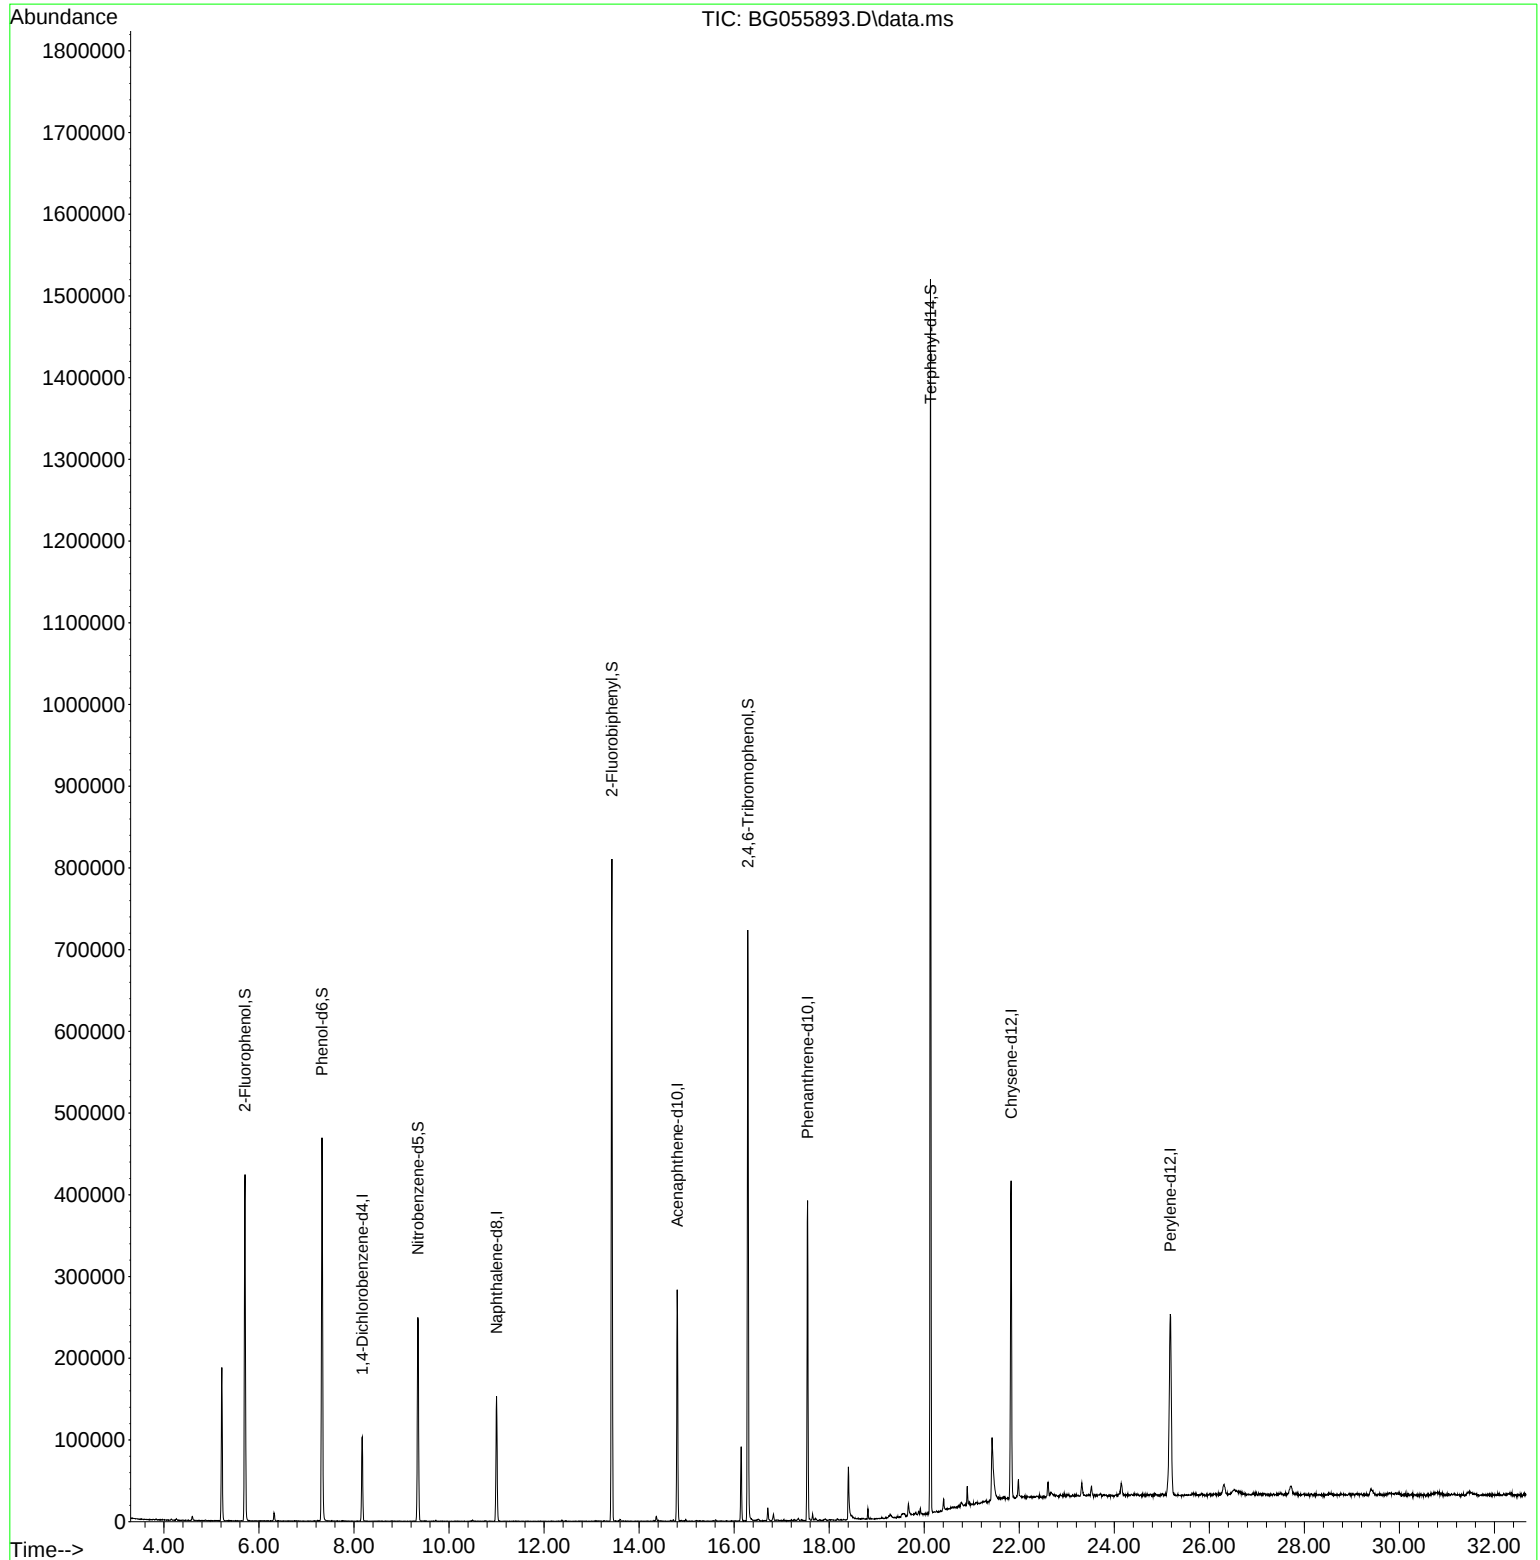


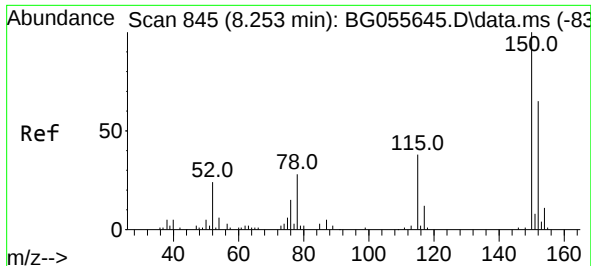

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.173 min Scan# 845
Delta R.T. -0.002 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33




Instrument :
BNA_G
ClientSampleId :
ML-1


Tgt Ion:152 Resp: 29267
Ion Ratio Lower Upper
152 100
150 150.6 123.0 184.6
115 56.8 47.0 70.4

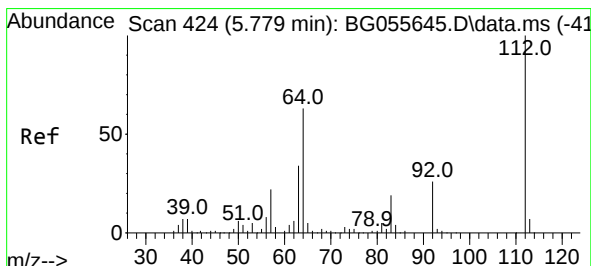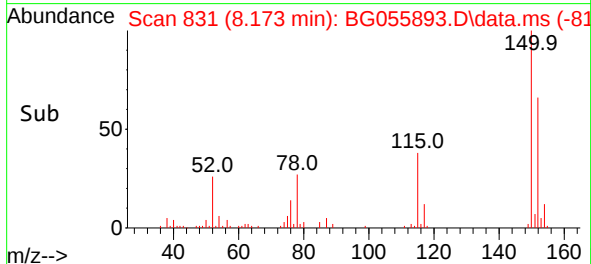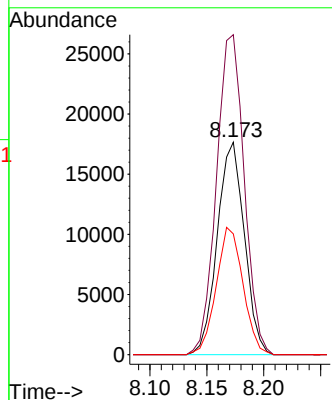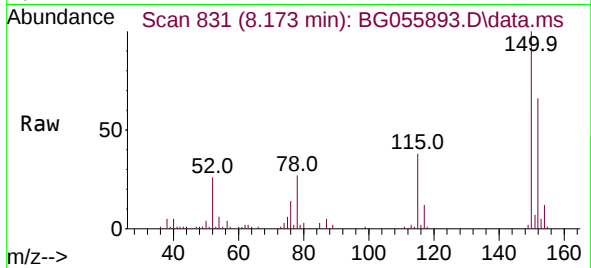

#5
2-Fluorophenol
Concen: 109.371 ng
RT: 5.706 min Scan# 411
Delta R.T. 0.004 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33

Tgt Ion:112 Resp: 177091
Ion Ratio Lower Upper
112 100
64 64.5 50.6 76.0
63 36.0 27.5 41.3


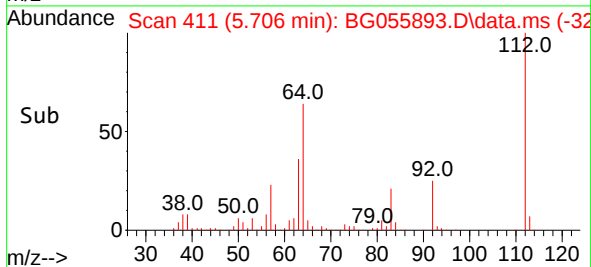
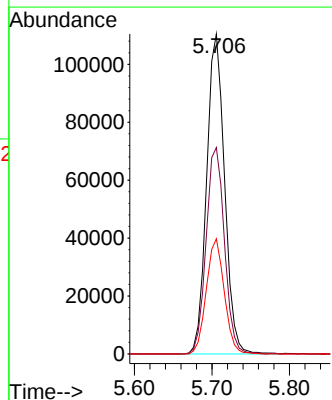
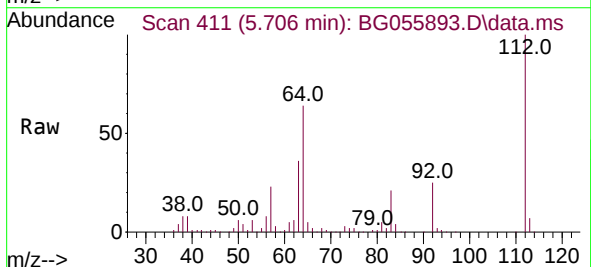


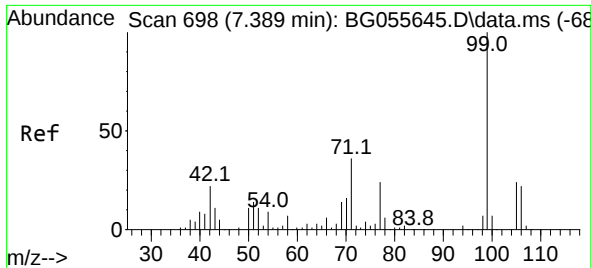

#7
Phenol-d6
Concen: 117.004 ng
RT: 7.327 min Scan# 68
Delta R.T. -0.002 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33




Instrument :
BNA_G
ClientSampleId :
ML-1


Tgt Ion: 99 Resp: 252190
Ion Ratio Lower Upper
99 100
42 24.0 18.0 27.0
71 36.8 29.0 43.6

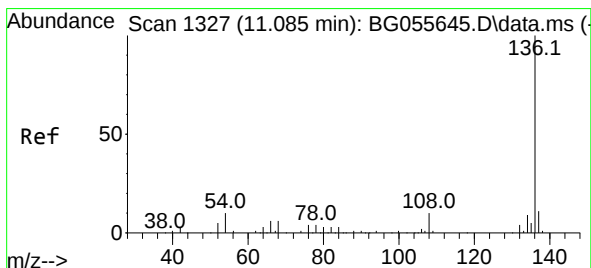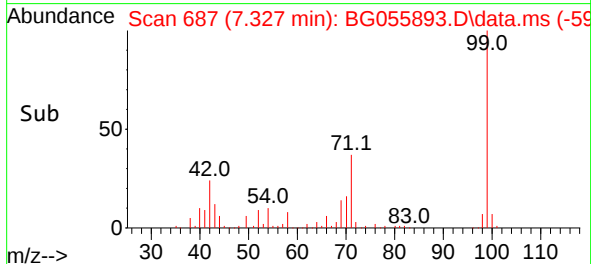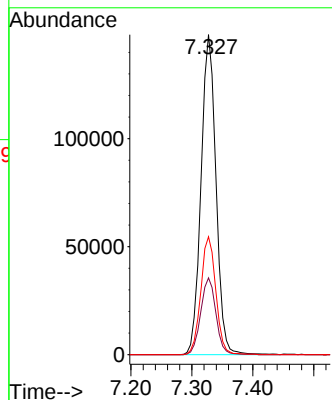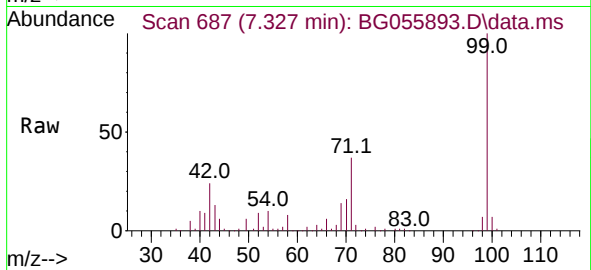

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.999 min Scan# 1312
Delta R.T. -0.002 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33

Tgt Ion:136 Resp: 126275
Ion Ratio Lower Upper
136 100
137 10.5 9.0 13.6
54 10.1 7.8 11.6
68 5.8 5.0 7.4

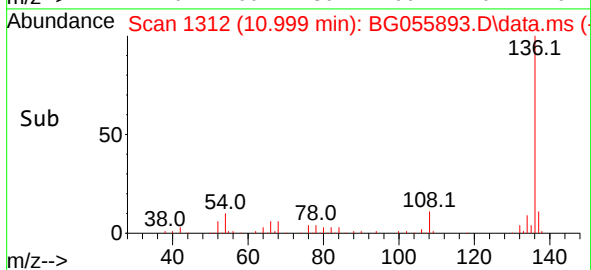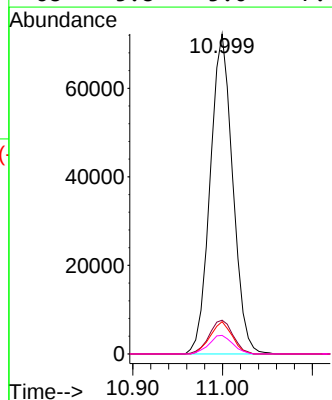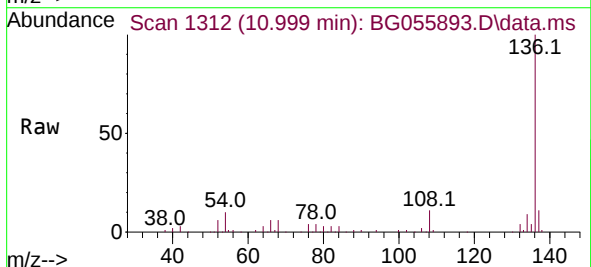

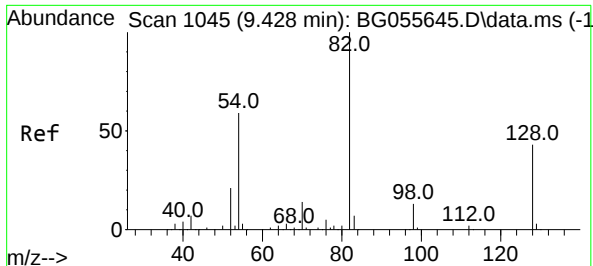

#23

Nitrobenzene-d5

Concen: 61.753 ng

RT: 9.342 min Scan# 1045

Delta R.T. -0.008 min

Lab File: BG055893.D

Acq: 5 Dec 2022 20:33

Instrument :

BNA_G

ClientSampleId :

ML-1





Tgt Ion: 82 Resp: 147533

Ion Ratio Lower Upper

82 100

128 40.6 34.1 51.1

54 59.9 47.3 70.9

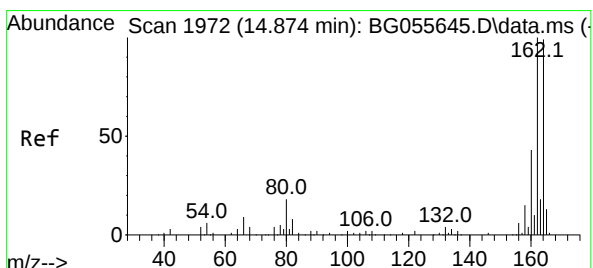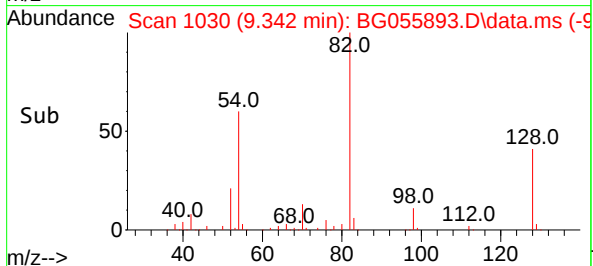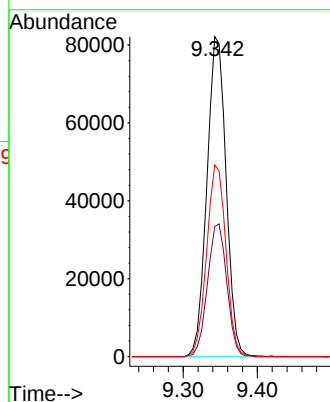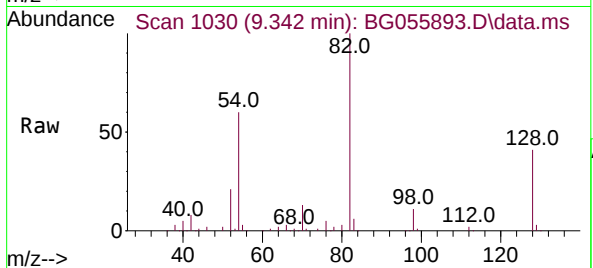

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.801 min Scan# 1959

Delta R.T. -0.008 min

Lab File: BG055893.D

Acq: 5 Dec 2022 20:33




Tgt Ion: 164 Resp: 98268


Ion Ratio Lower Upper

164 100

162 101.3 81.1 121.7

160 45.2 34.8 52.2


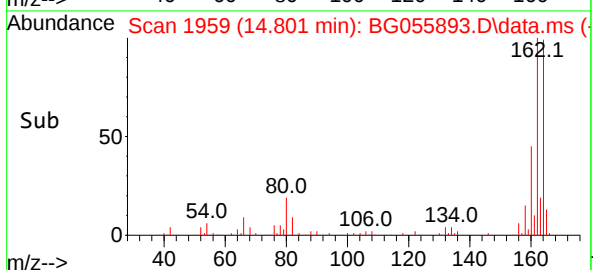
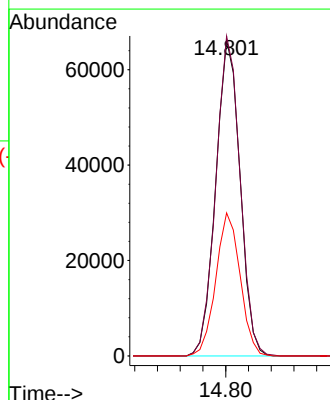
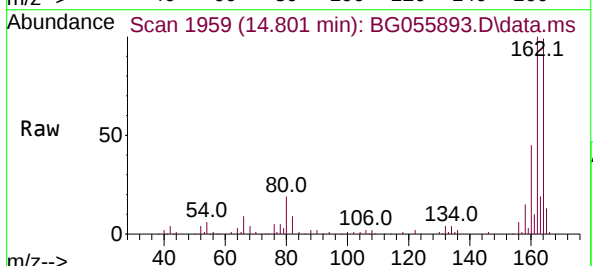


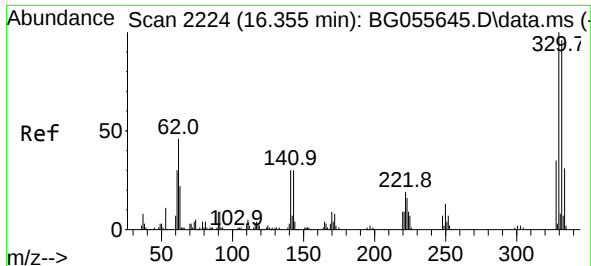

#42
2,4,6-Tribromophenol
Concen: 106.117 ng
RT: 16.287 min Scan# 21
Delta R.T. -0.008 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33




Instrument :
BNA_G
ClientSampleId :
ML-1


Tgt Ion:330 Resp: 146839
Ion Ratio Lower Upper
330 100
332 96.4 77.8 116.8
141 32.2 23.9 35.9

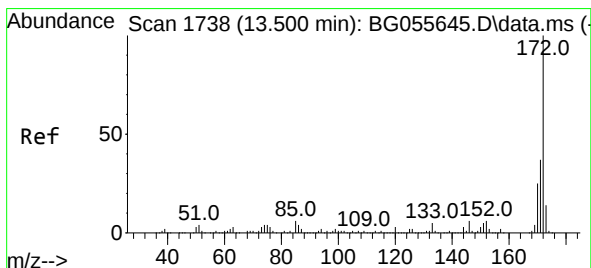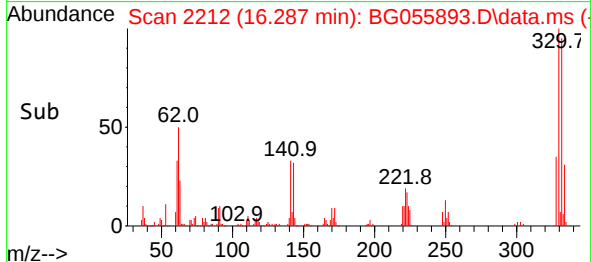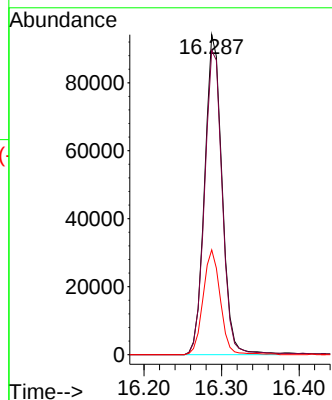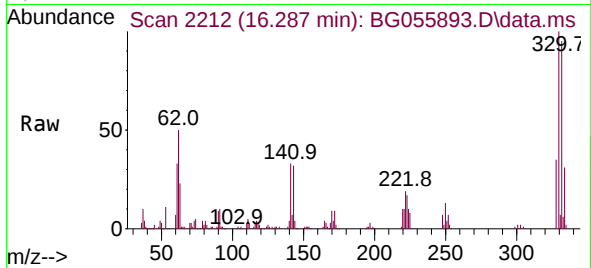

#45
2-Fluorobiphenyl
Concen: 62.145 ng
RT: 13.426 min Scan# 1725
Delta R.T. -0.002 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33

Tgt Ion:172 Resp: 407634
Ion Ratio Lower Upper
172 100
171 36.4 29.8 44.6
170 24.9 20.2 30.4


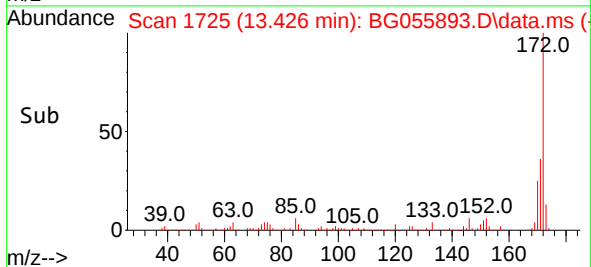
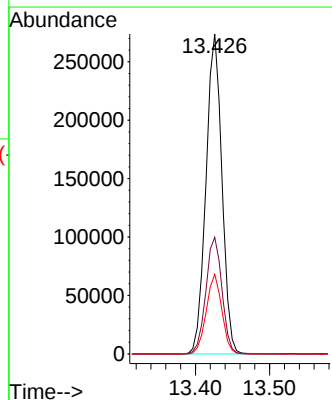
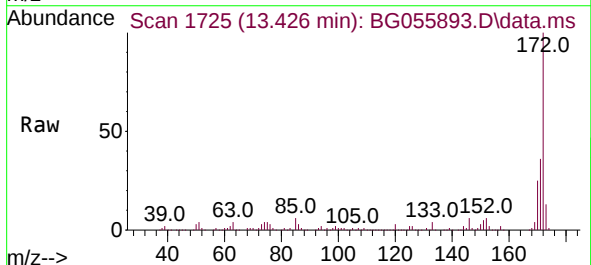


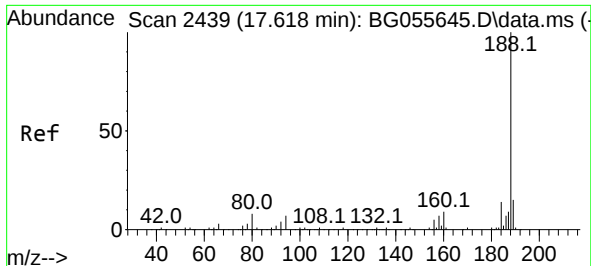

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.545 min Scan# 2439
Delta R.T. -0.002 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33




Instrument :
BNA_G
ClientSampleId :
ML-1


Tgt Ion:188 Resp: 251773
Ion Ratio Lower Upper
188 100
94 6.8 5.4 8.2
80 8.2 6.6 10.0

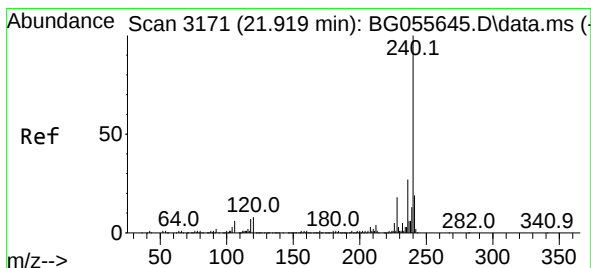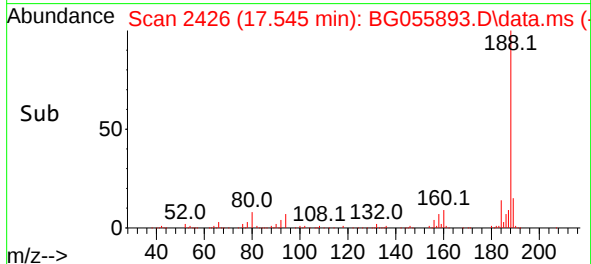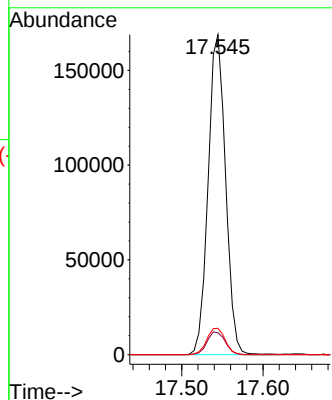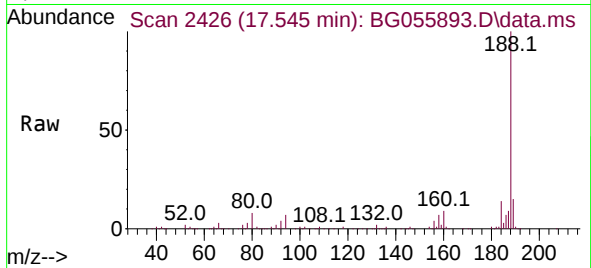

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.828 min Scan# 3155
Delta R.T. -0.008 min
Lab File: BG055893.D
Acq: 5 Dec 2022 20:33

Tgt Ion:240 Resp: 242479
Ion Ratio Lower Upper
240 100
120 8.0 6.3 9.5
236 26.5 21.9 32.9


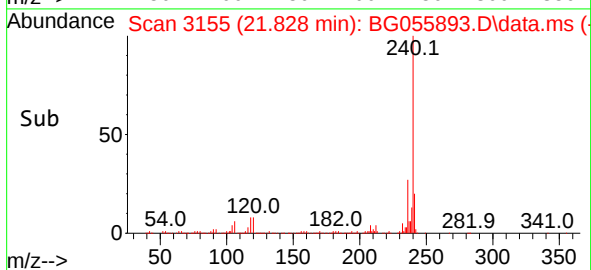
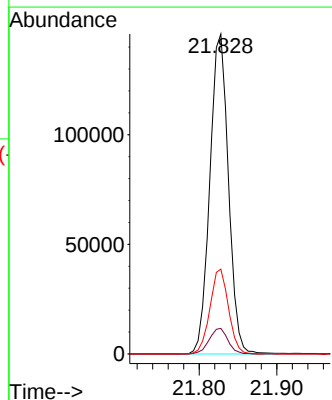
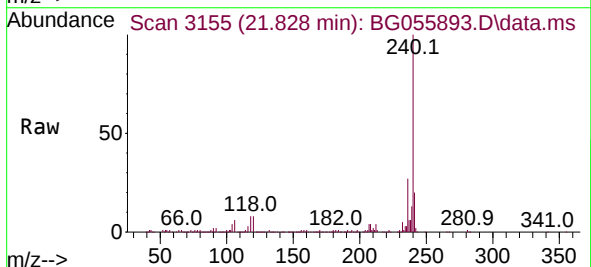


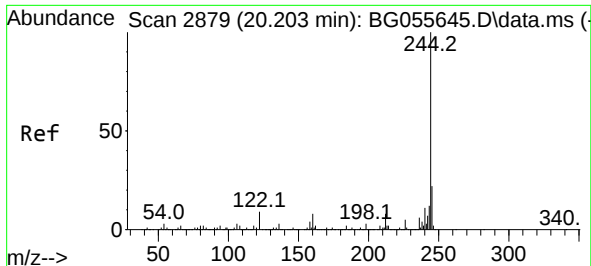

#79
 Terphenyl-d14
 Concen: 62.835 ng
 RT: 20.130 min Scan# 2879
 Delta R.T. -0.008 min
 Lab File: BG055893.D
 Acq: 5 Dec 2022 20:33

Instrument :
 BNA_G
 ClientSampleId :
 ML-1

Tgt Ion:244 Resp: 761755
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.3 9.5
 122 8.8 6.9 10.3

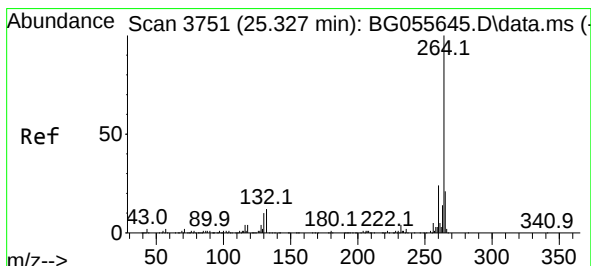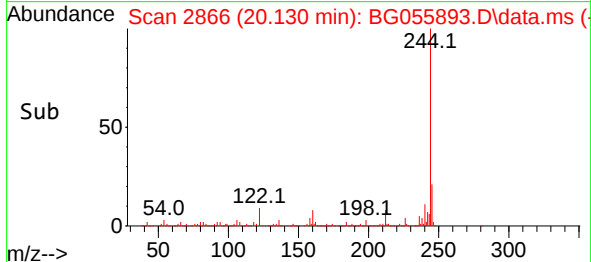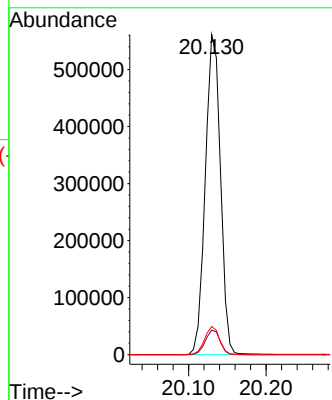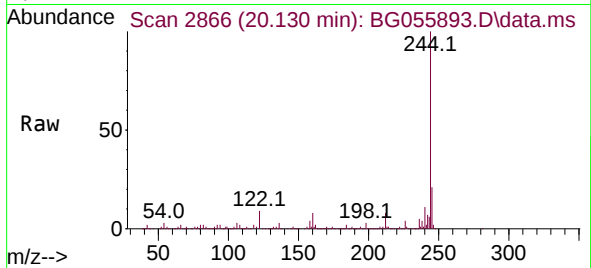

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.177 min Scan# 3725
 Delta R.T. -0.002 min
 Lab File: BG055893.D
 Acq: 5 Dec 2022 20:33

Tgt Ion:264 Resp: 251491
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.5 29.3
 265 22.7 17.1 25.7

