


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120522\
 Data File : BG055883.D
 Acq On : 5 Dec 2022 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 06 04:41:17 2022

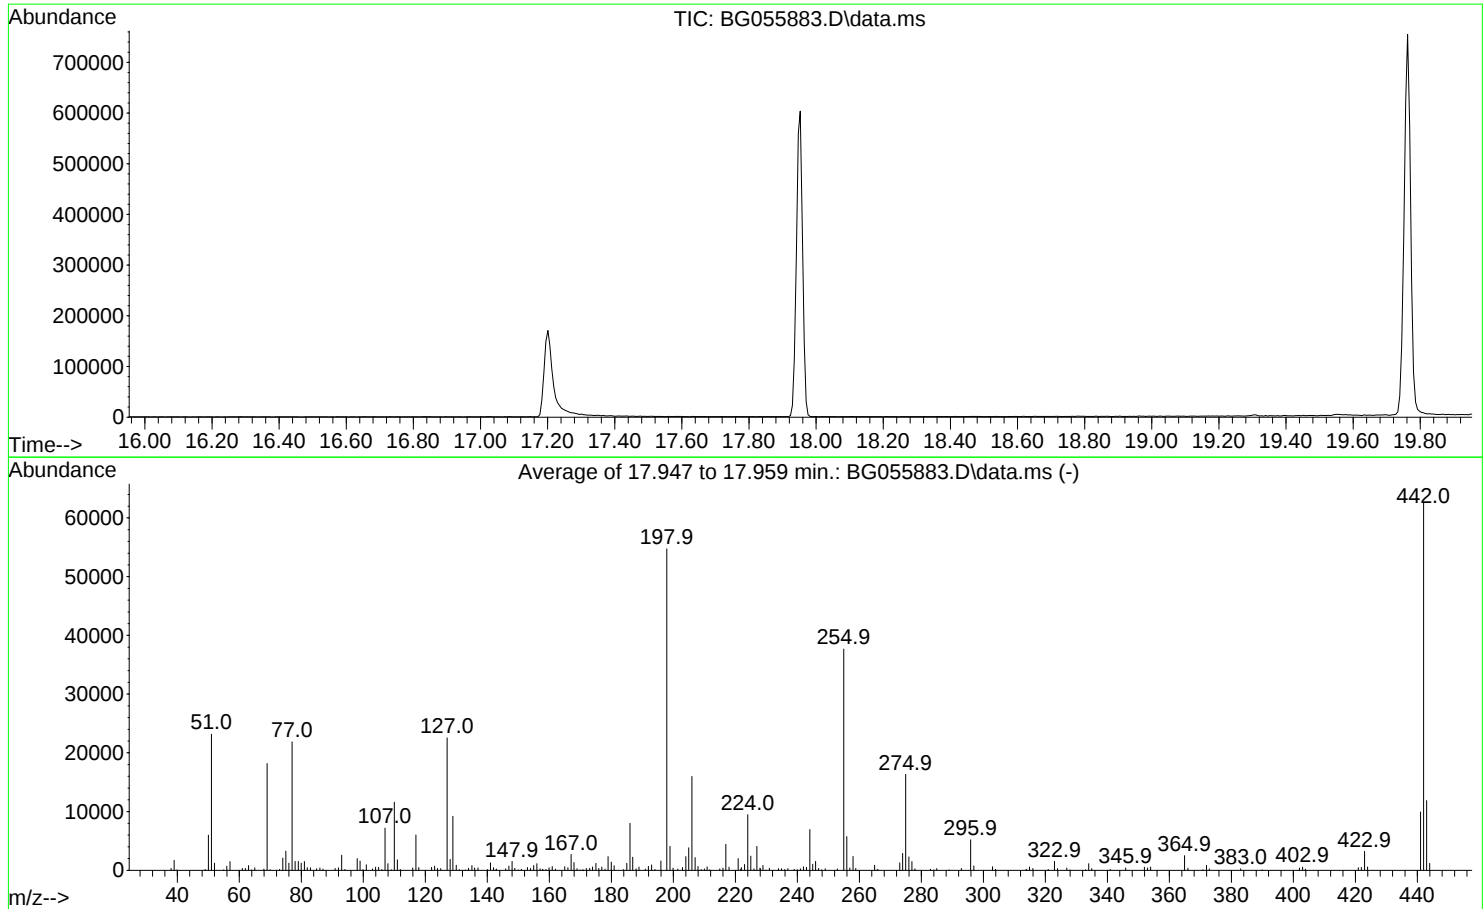




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	23176	PASS
68	69	0.00	2	1.2	217	PASS
69	198	0.00	100	33.2	18177	PASS
70	69	0.00	2	0.6	104	PASS
127	198	10	80	41.2	22541	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54720	PASS
199	198	5	9	7.4	4070	PASS
275	198	10	60	29.9	16334	PASS
365	198	1	100	4.6	2502	PASS
441	198	0.01	100	18.2	9944	PASS
442	442	50	100	100.0	62640	PASS
443	442	15	24	19.0	11877	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120522\
Data File : BG055883.D
Acq On : 5 Dec 2022 12:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 06 06:07:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 06 04:41:17 2022
Response via : Initial Calibration

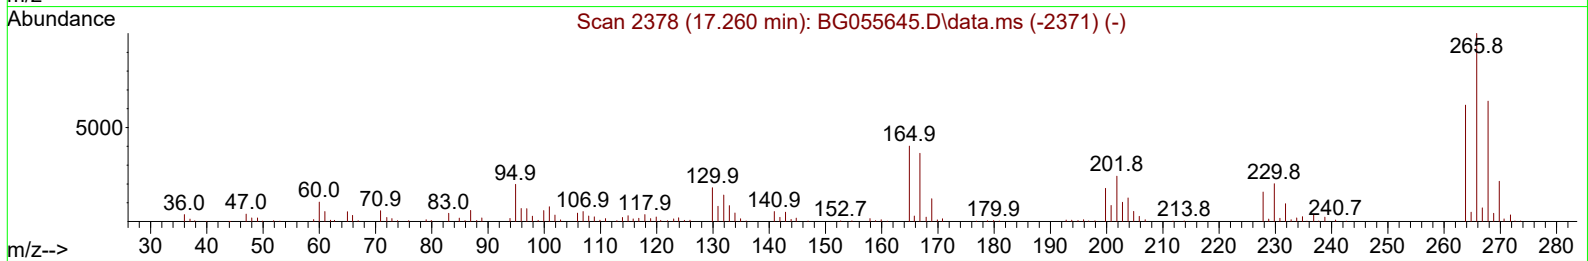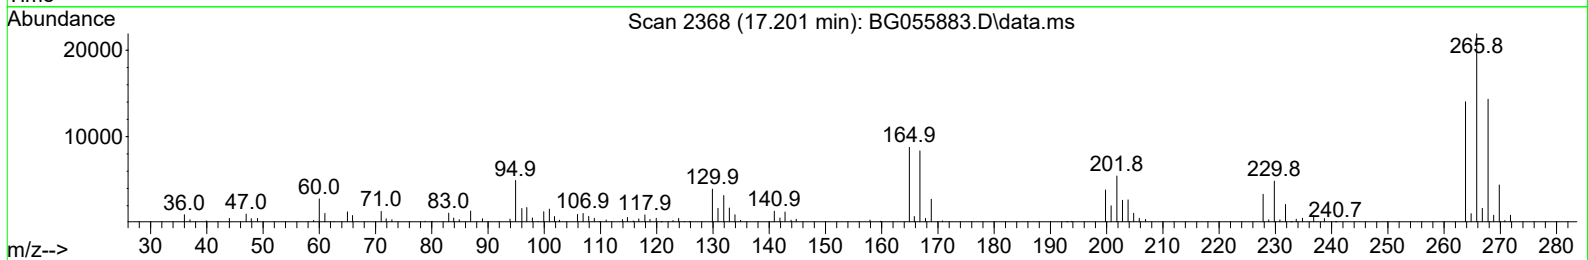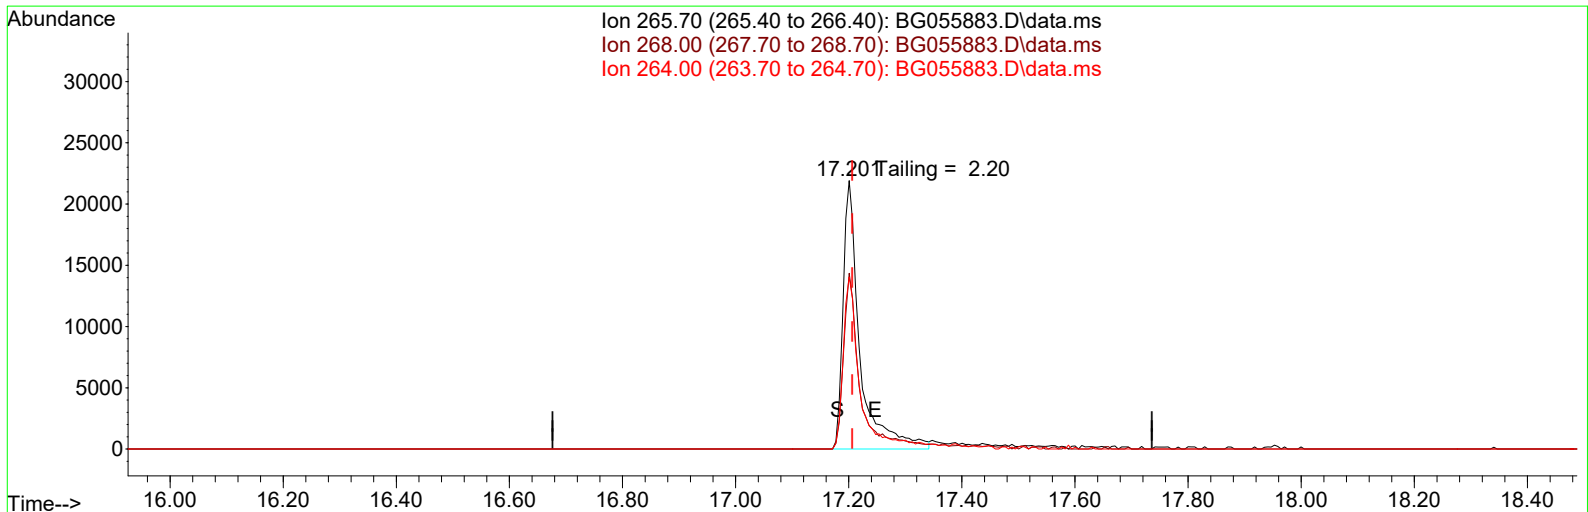

TIC: BG055883.D\data.ms

(70) Pentachlorophenol (C)

17.201min (-0.005) 17660.22 ng




response 44768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.46
264.00	61.90	64.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120522\
 Data File : BG055883.D
 Acq On : 5 Dec 2022 12:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 06 06:07:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 06 04:41:17 2022
 Response via : Initial Calibration

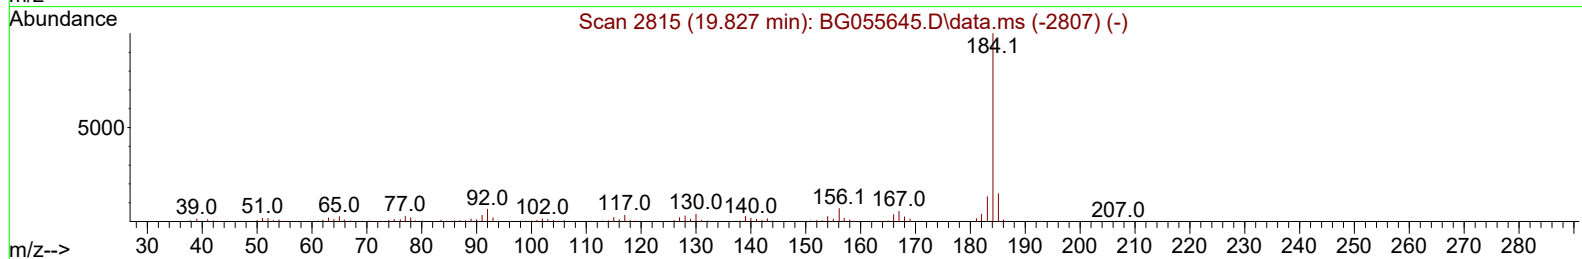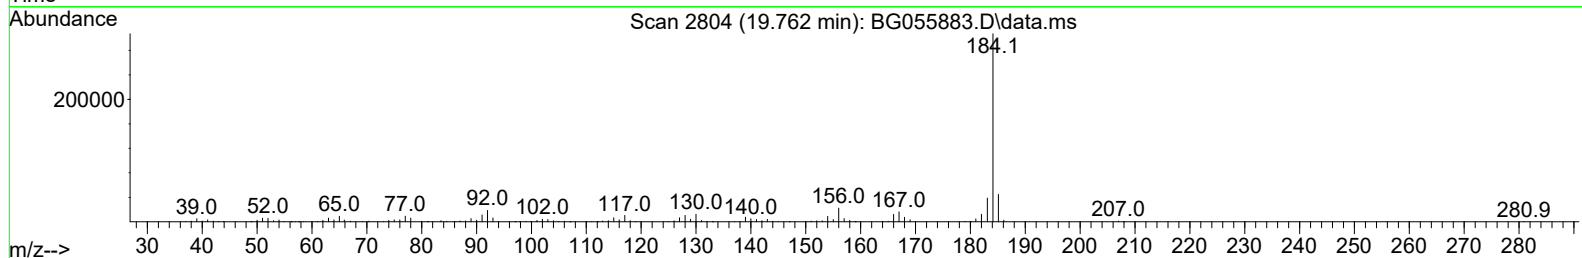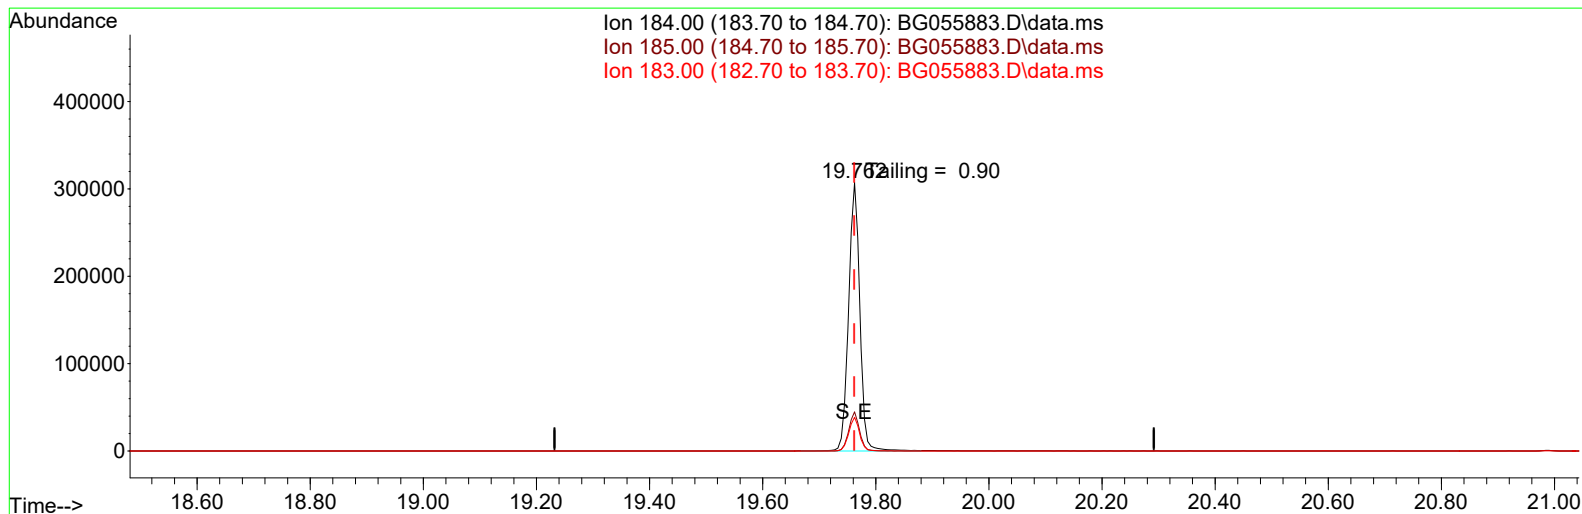

TIC: BG055883.D\data.ms

(77) Benzidine

19.762min (+ 0.000) 0.00 ng

response 425372

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.61
183.00	13.20	12.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/5/2022	BNA_G	<u>BG055883.D</u>
Compound Name	Response	Retention Time
DDT	186910	20.99
DDD	2563	20.591
DDE	281	20.05
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2844	189754	1.50

Instrument :
BNA_G
ClientSampleId :
DFTPP