
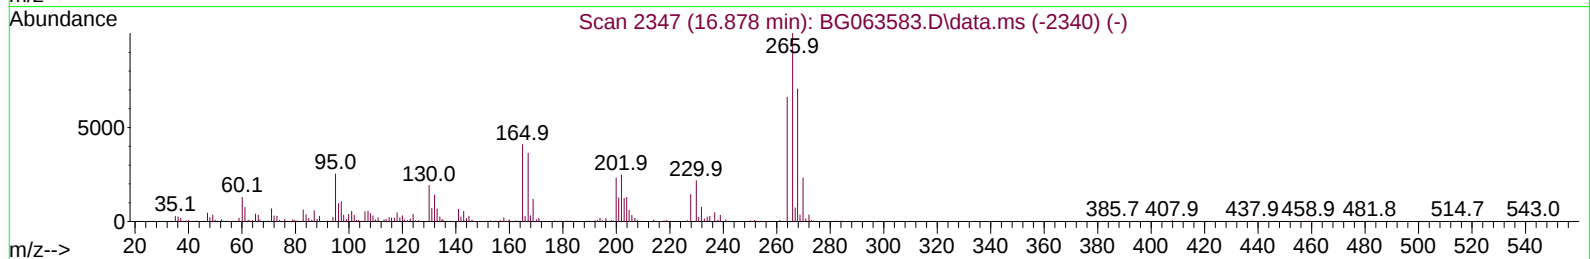
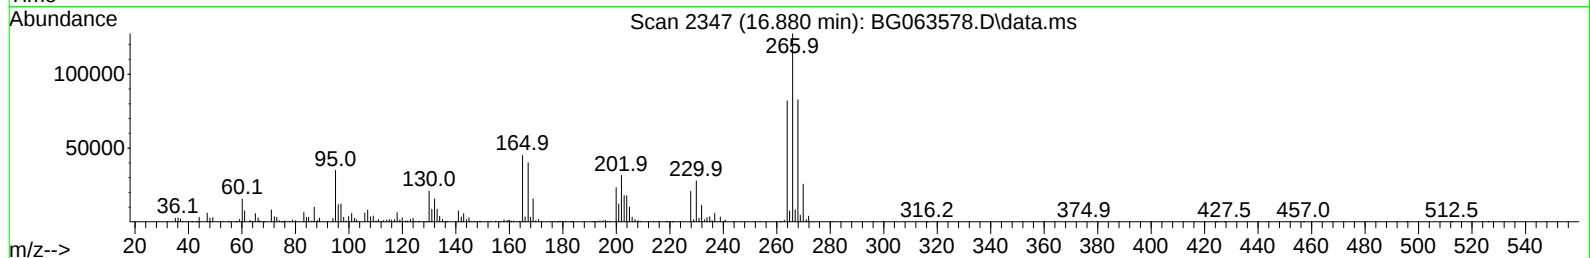


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120524\
Data File : BG063578.D
Acq On : 5 Dec 2024 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 01:09:20 2024
Response via : Initial Calibration

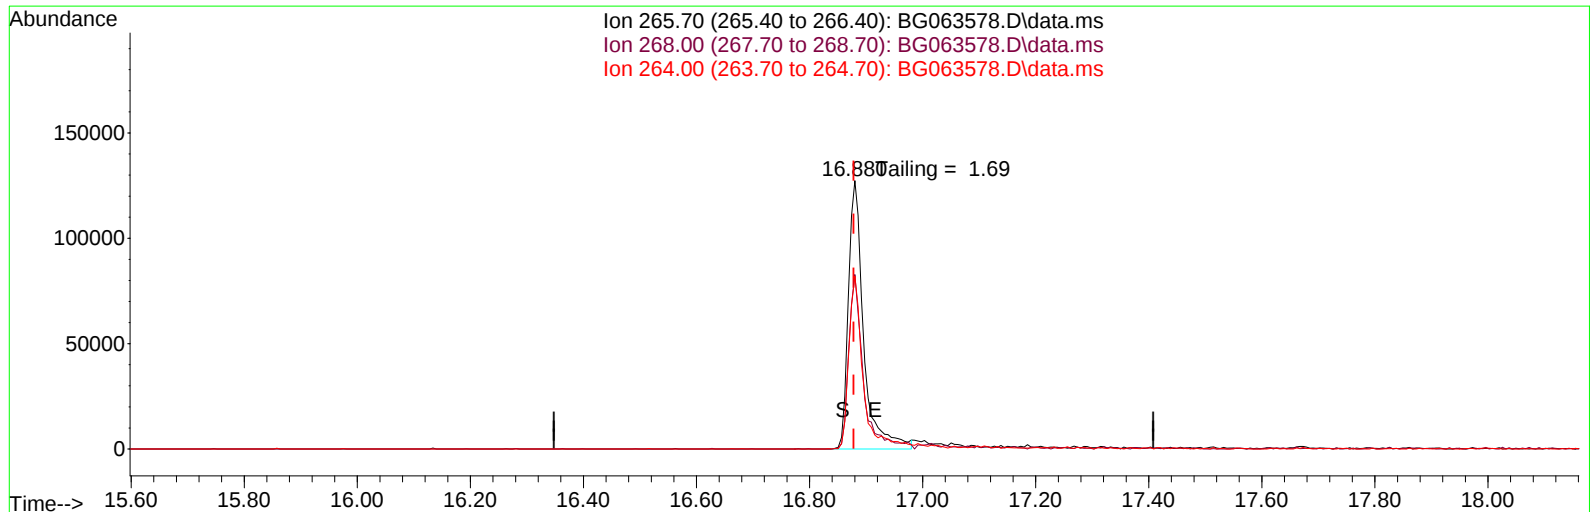

TIC: BG063578.D\data.ms

(70) Pentachlorophenol (C)




16.880min (+ 0.002) 431476.85 ng

response 238244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	74.00	65.00
264.00	66.10	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120524\
Data File : BG063578.D
Acq On : 5 Dec 2024 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 01:09:20 2024
Response via : Initial Calibration

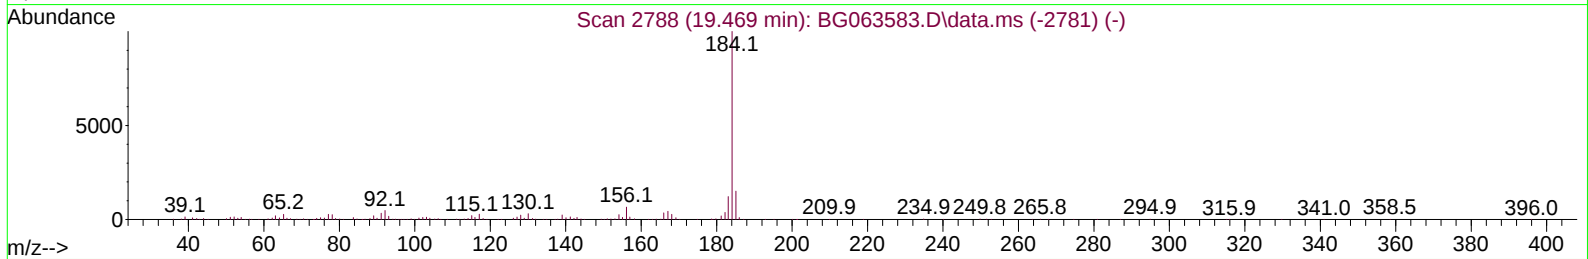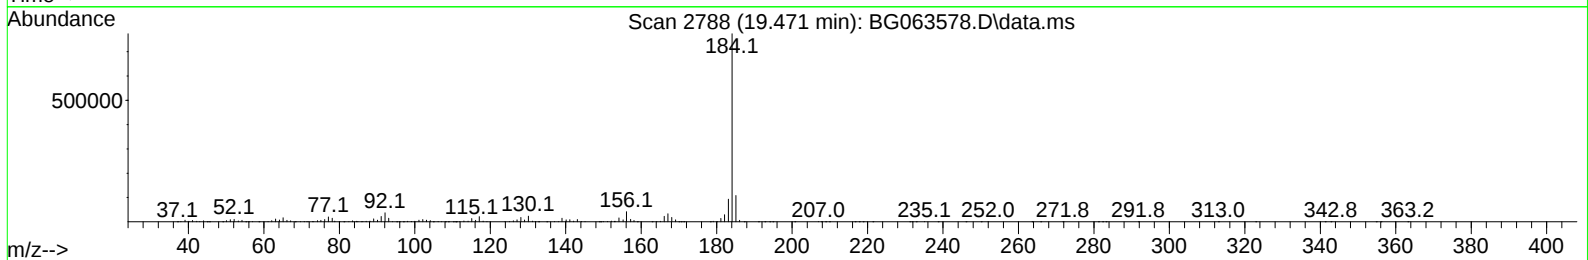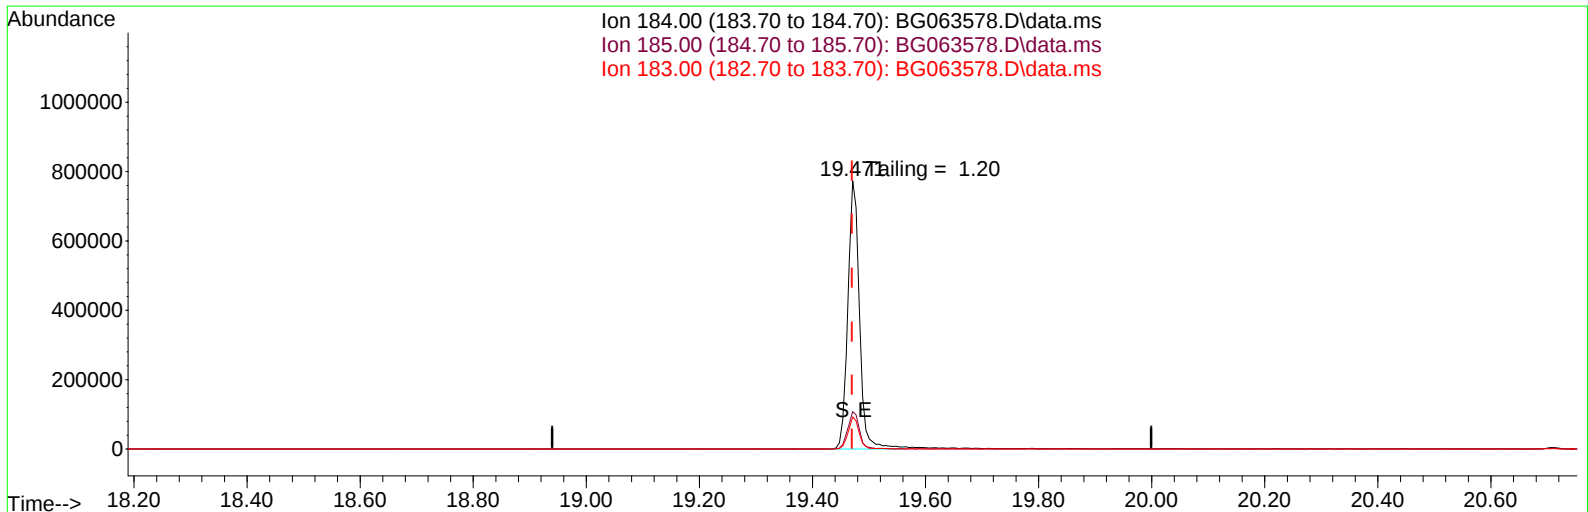

TIC: BG063578.D\data.ms

(77) Benzidine**19.471min (+ 0.002) 1677652.22 ng****response 1114025**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.99
183.00	12.40	11.99
0.00	0.00	0.00