


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120524\
Data File : BG063578.D
Acq On : 5 Dec 2024 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 06 01:09:20 2024

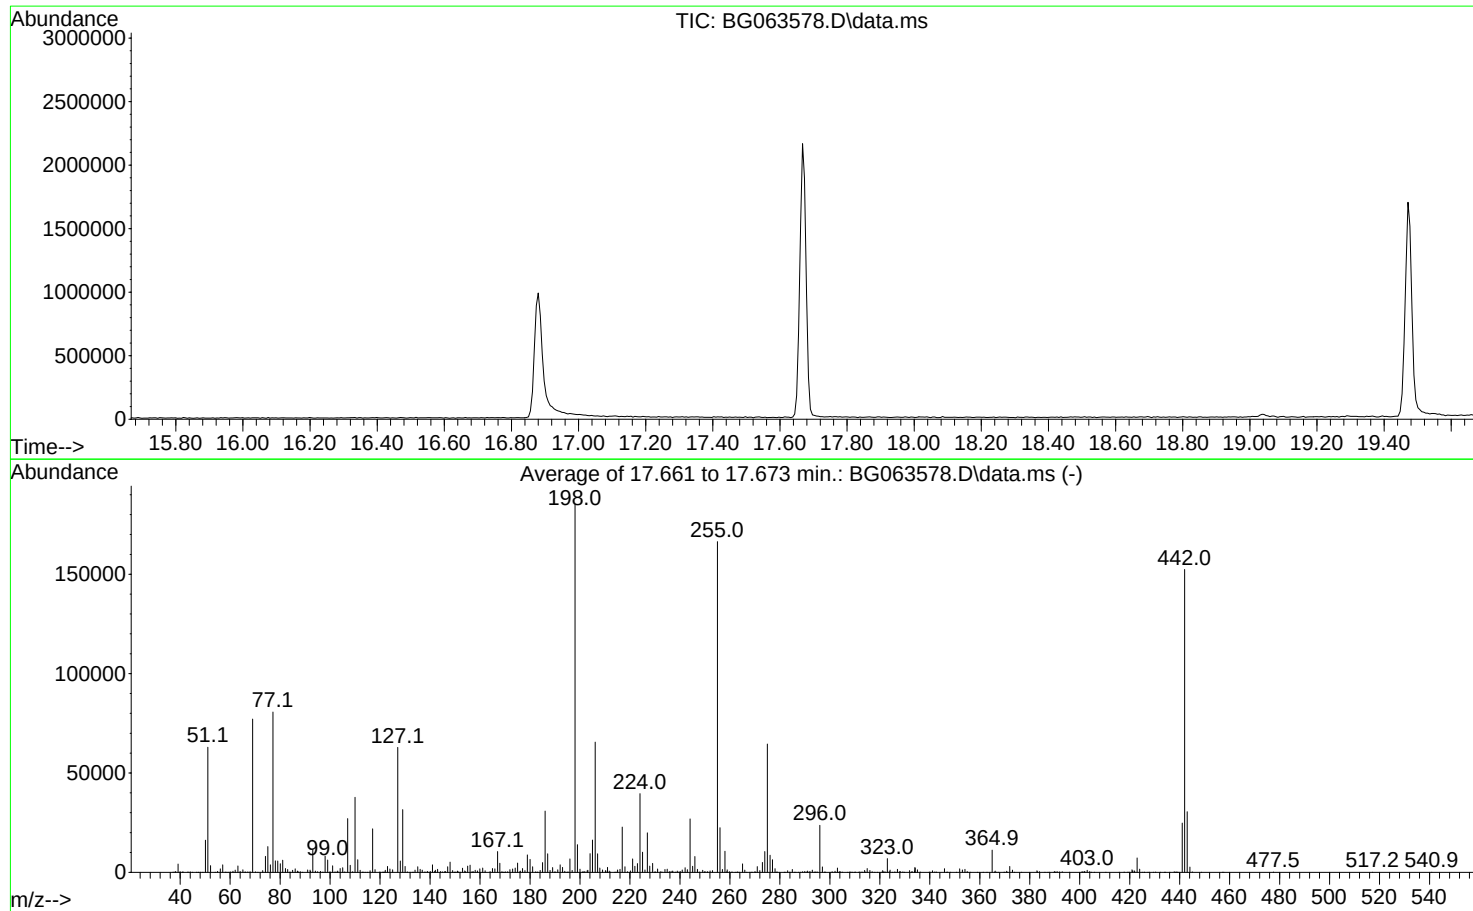




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	62923	PASS
68	69	0.00	2	0.5	351	PASS
69	198	0.00	100	41.7	77165	PASS
70	69	0.00	2	0.3	267	PASS
127	198	10	80	34.0	62856	PASS
197	198	0.00	2	0.5	993	PASS
198	198	100	100	100.0	185088	PASS
199	198	5	9	7.5	13958	PASS
275	198	10	60	34.9	64536	PASS
365	198	1	100	6.1	11205	PASS
441	198	0.01	100	13.4	24803	PASS
442	442	50	100	100.0	152403	PASS
443	442	15	24	20.0	30531	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120524\
Data File : BG063578.D
Acq On : 5 Dec 2024 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 06 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 01:09:20 2024
Response via : Initial Calibration

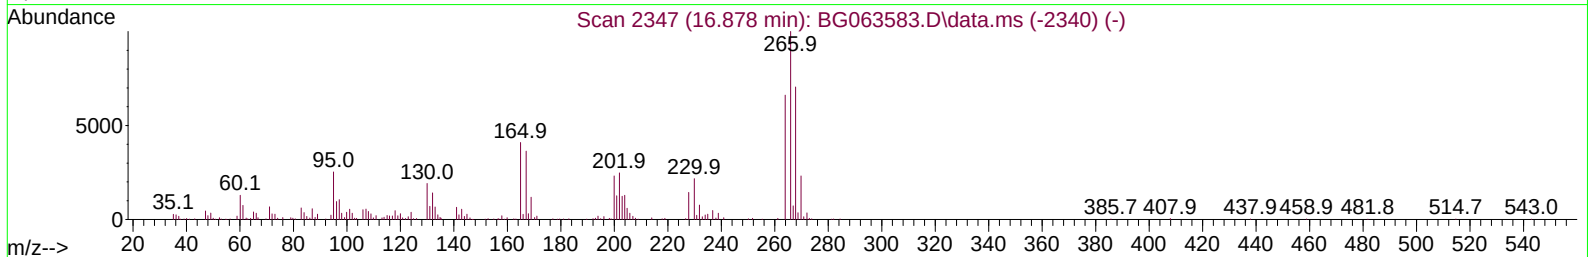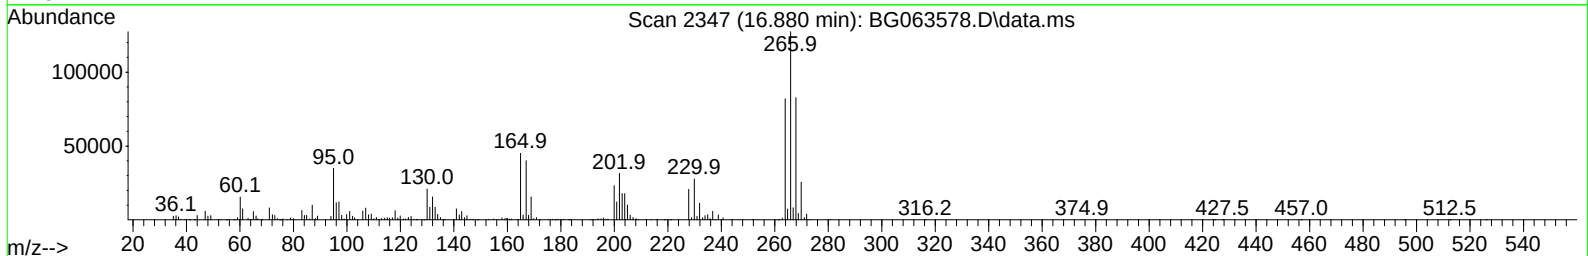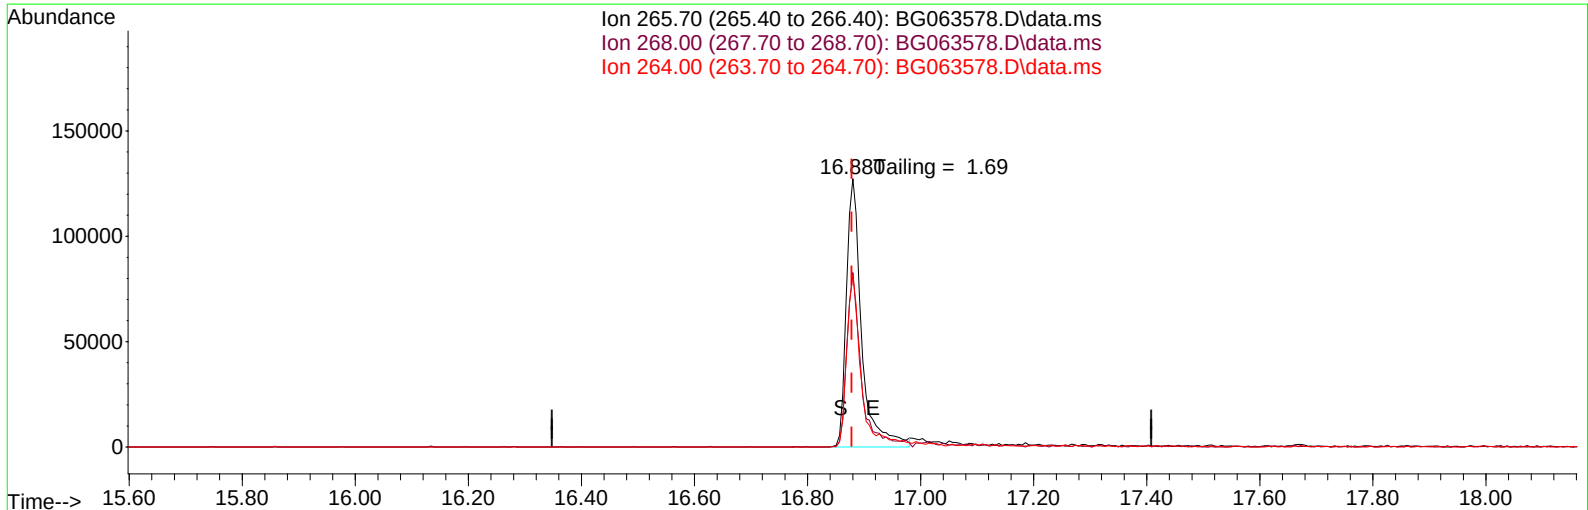

TIC: BG063578.D\data.ms

(70) Pentachlorophenol (C)

16.880min (+ 0.002) 431476.85 ng




response 238244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	74.00	65.00
264.00	66.10	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120524\
Data File : BG063578.D
Acq On : 5 Dec 2024 11:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 06 01:20:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG120524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 01:09:20 2024
Response via : Initial Calibration

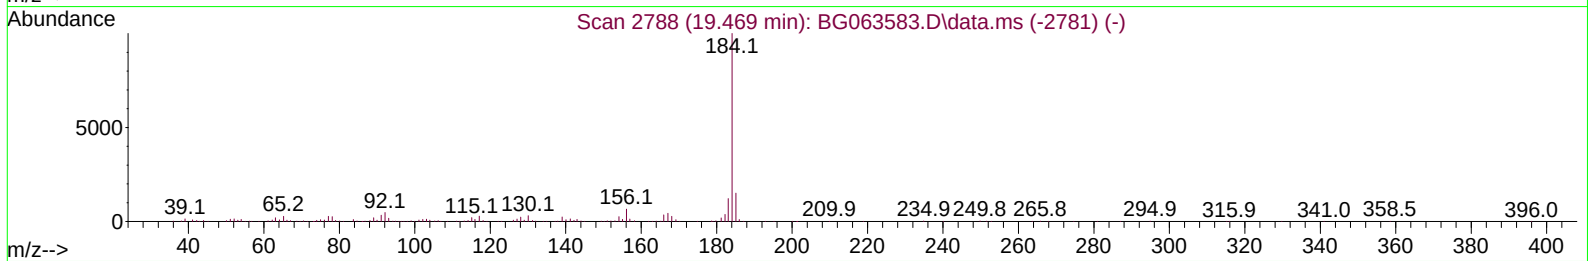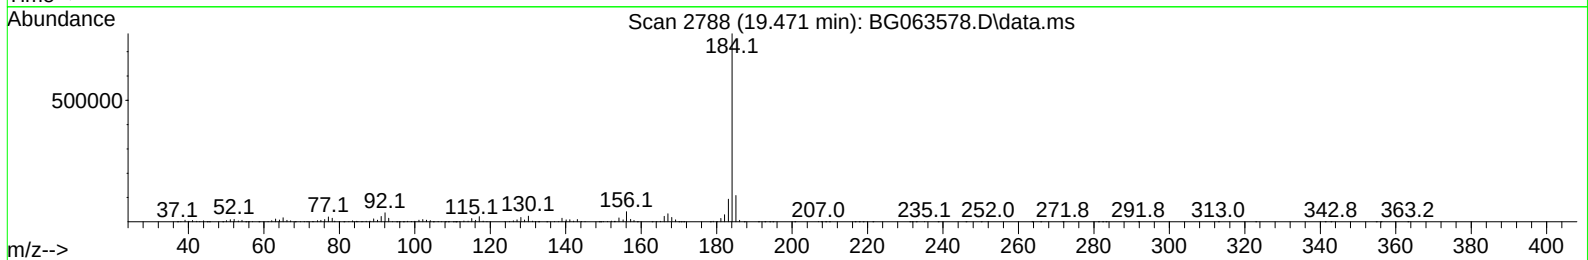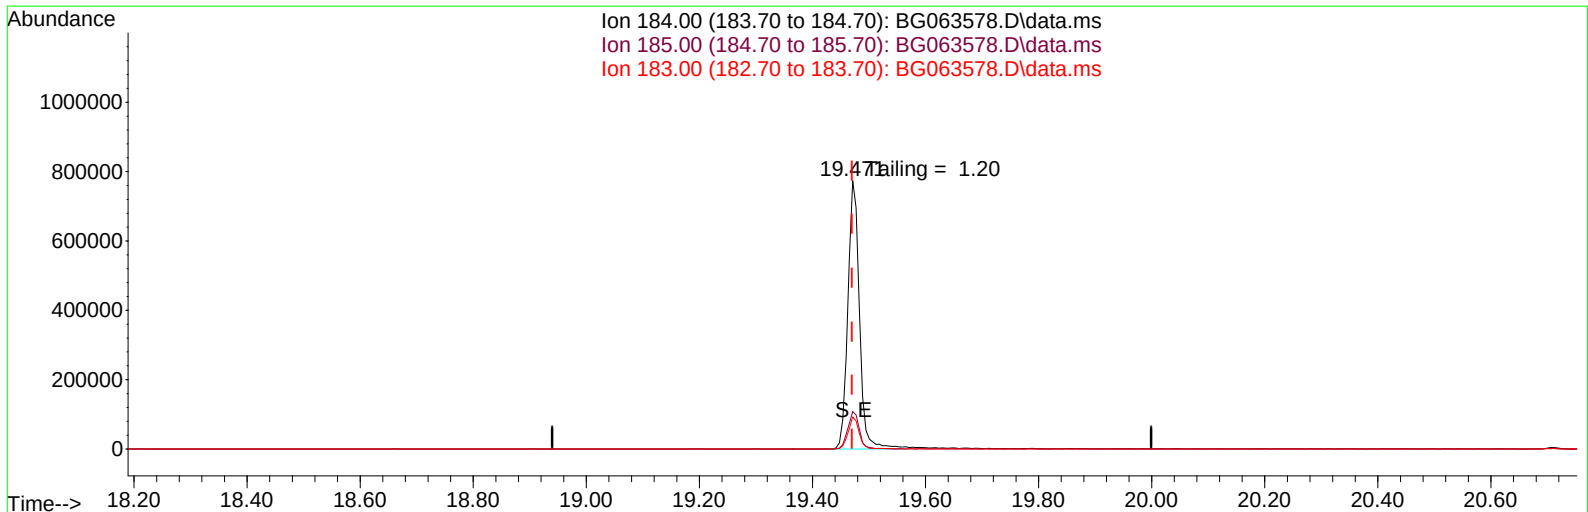

TIC: BG063578.D\data.ms

(77) Benzidine

19.471min (+ 0.002) 1677652.22 ng

response 1114025

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.99
183.00	12.40	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/5/2024	BNA_G	<u>BG063578.D</u>
Compound Name	Response	Retention Time
DDT	686320	20.711
DDD	14017	20.317
DDE	1265	19.765
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15282	701602	2.18

Instrument :
BNA_G
ClientSampleId :
DFTPP