

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120615\
 Data File : BG019971.D
 Acq On : 6 Dec 2015 17:41
 Operator : UM/NP
 Sample : G4633-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-1(11-15)

Quant Time: Dec 07 03:21:04 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	34639	20.00	ng	-0.02
21) Naphthalene-d8	10.93	136	152718	20.00	ng	-0.02
38) Acenaphthene-d10	14.74	164	105561	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	257753	20.00	ng	-0.02
75) Chrysene-d12	21.76	240	307545	20.00	ng	-0.04
86) Perylene-d12	25.03	264	295212	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	165007	86.10	ng	-0.01
7) Phenol-d6	7.26	99	370025	127.87	ng	-0.01
23) Nitrobenzene-d5	9.28	82	258328	86.33	ng	-0.02
41) 2,4,6-Tribromophenol	16.22	330	71122	44.03	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	521694	67.48	ng	-0.02
78) Terphenyl-d14	20.08	244	734202	58.23	ng	-0.03
Target Compounds						
10) Phenol	7.29	94	7298	2.40	ng	# 55
49) Dimethylphthalate	14.19	163	134516	14.17	ng	98
83) Bis(2-ethylhexyl)phthalate	21.64	149	36460	3.50	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120615\
Data File : BG019971.D
Acq On : 6 Dec 2015 17:41
Operator : UM/NP
Sample : G4633-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-1(11-15)

Quant Time: Dec 07 03:21:04 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

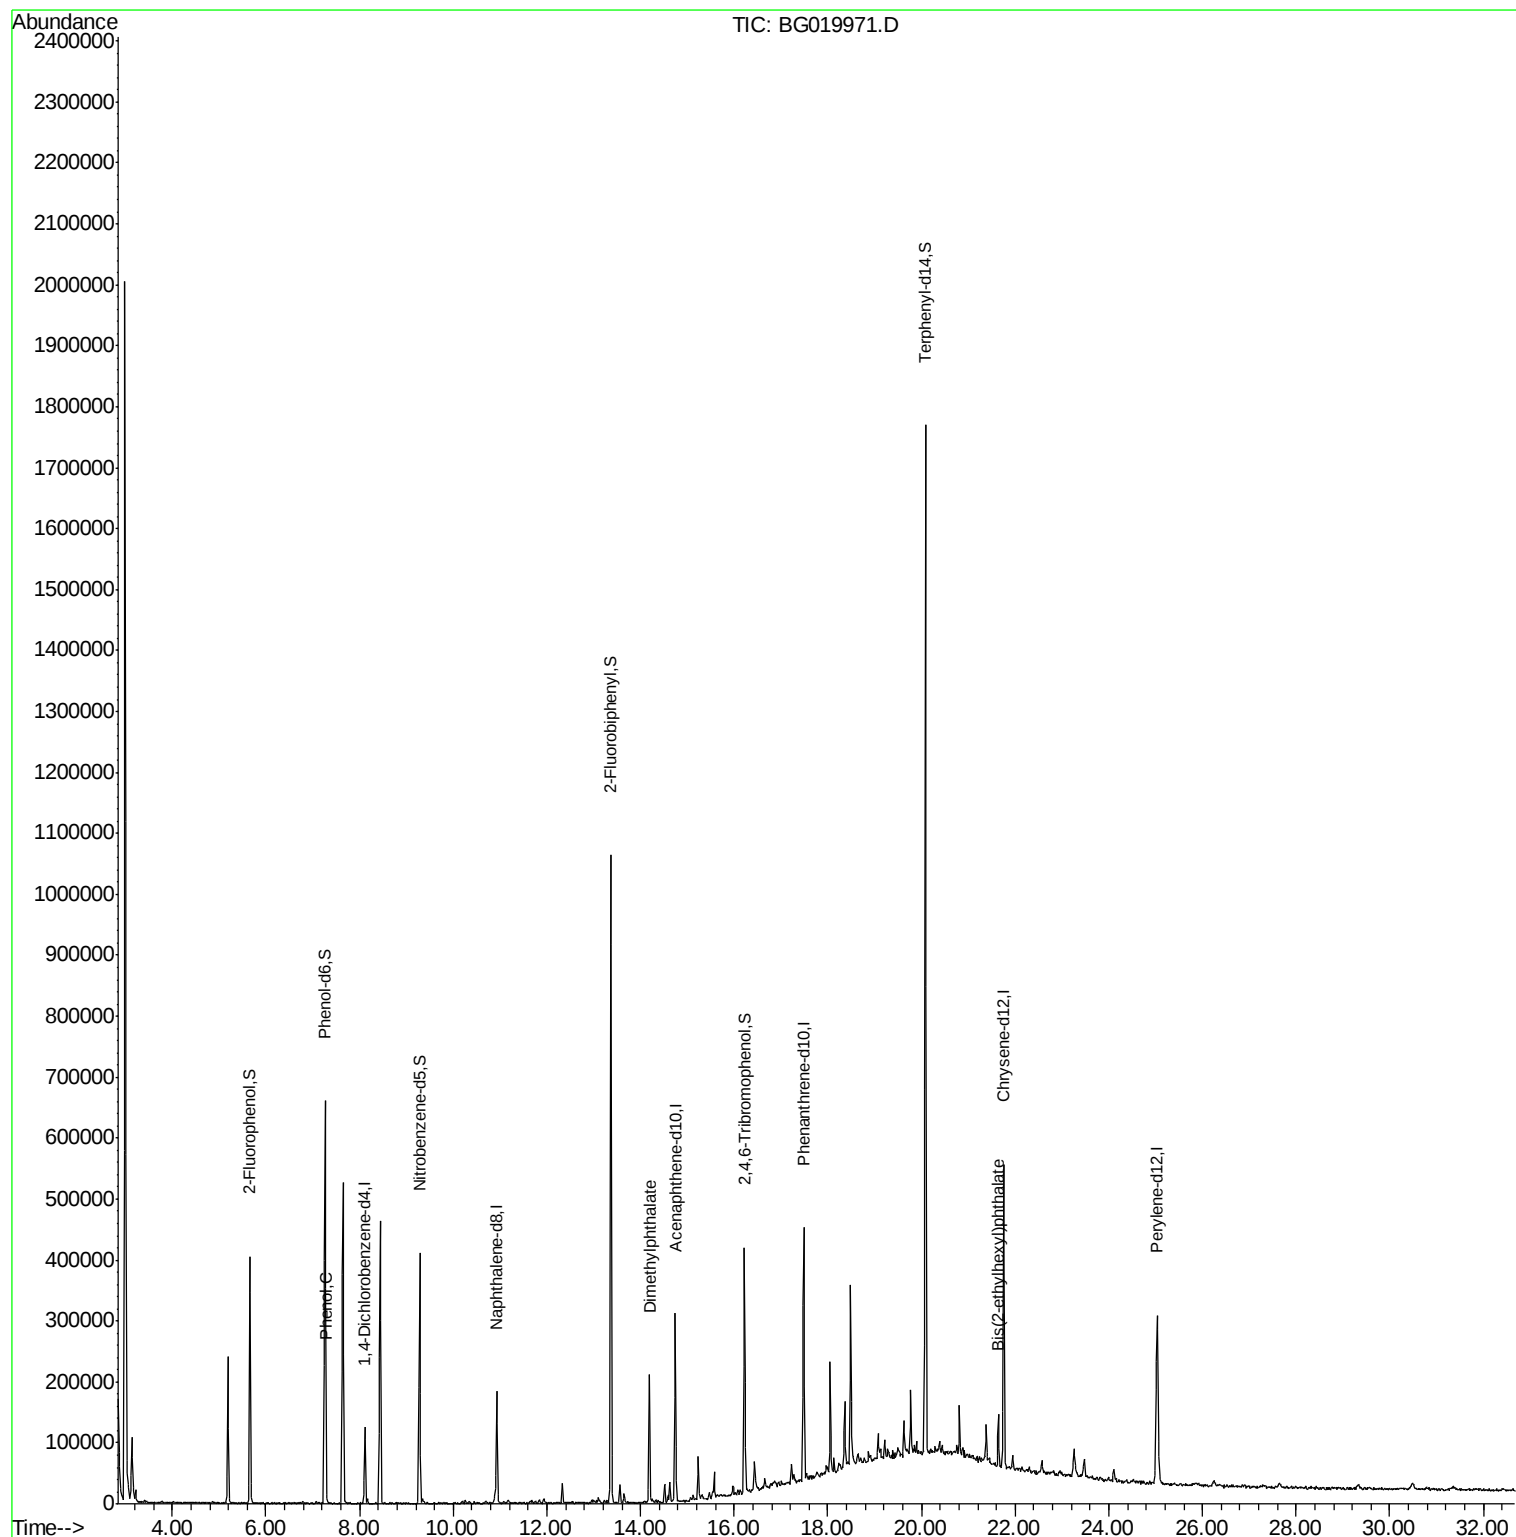

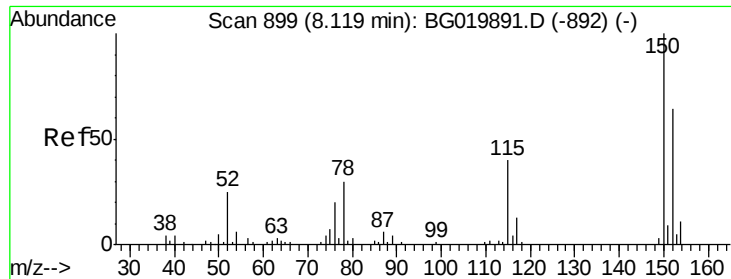

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.11 min Scan# 898

Delta R.T. -0.02 min

Lab File: BG019971.D

Acq: 6 Dec 2015 17:41

Instrument :

BNA_G

ClientSampleId :

SB-1(11-15)


Tgt Ion:152 Resp: 34639

Ion Ratio Lower Upper

152 100

150 162.2 115.0 172.4




115 59.0 43.9 65.9



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

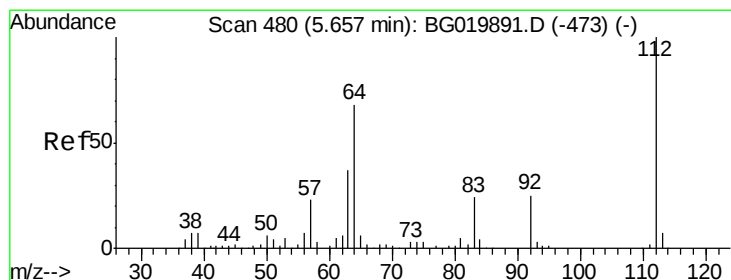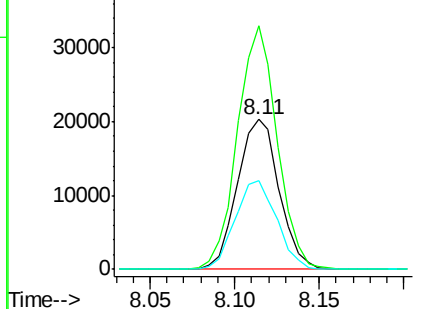

#5

2-Fluorophenol

Concen: 86.10 ng

RT: 5.66 min Scan# 480

Delta R.T. -0.01 min

Lab File: BG019971.D

Acq: 6 Dec 2015 17:41


Tgt Ion:112 Resp: 165007

Ion Ratio Lower Upper

112 100

64 67.3 43.7 65.5#



63 37.5 24.0 36.0#




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

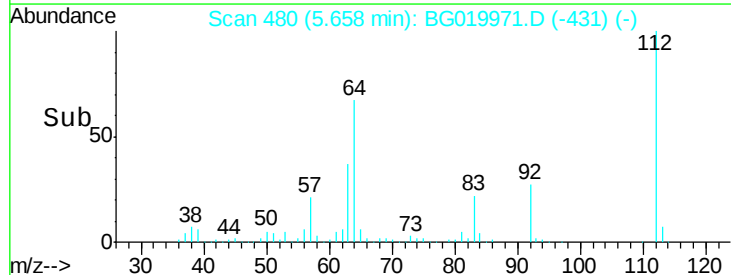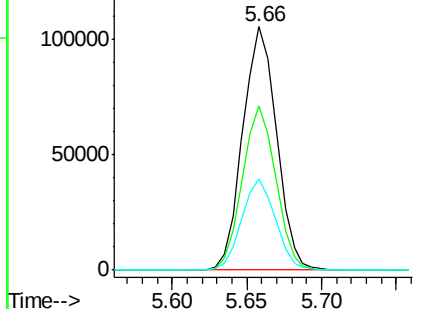

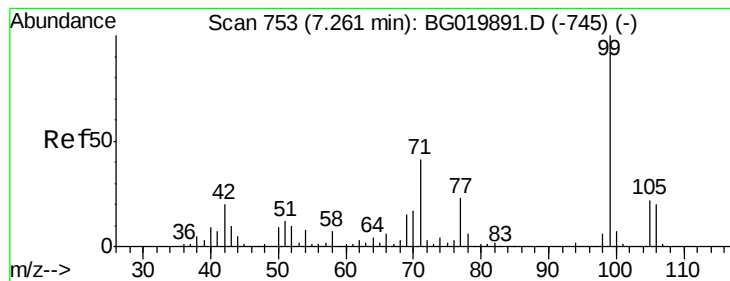

#7

Phenol-d6

Concen: 127.87 ng

RT: 7.26 min Scan# 753

Delta R.T. -0.01 min

Lab File: BG019971.D

Acq: 6 Dec 2015 17:41

Instrument :

BNA_G

ClientSampled :

SB-1(11-15)


Tgt Ion: 99 Resp: 370025

Ion Ratio Lower Upper




99 100

42 20.4 11.5 17.3#

71 40.6 22.6 34.0#

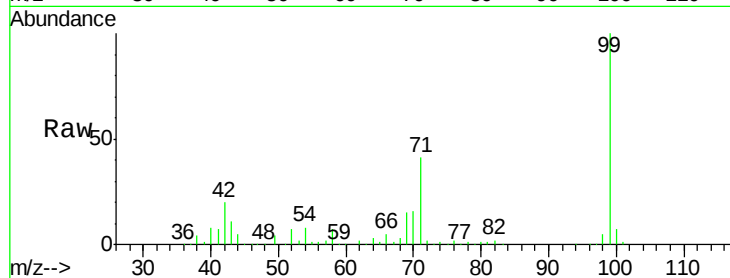

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

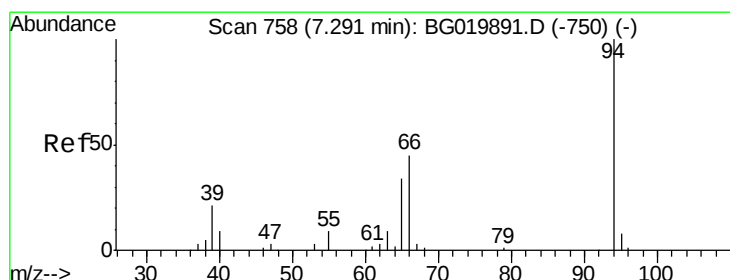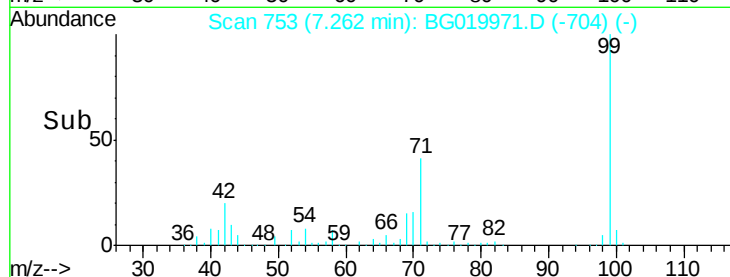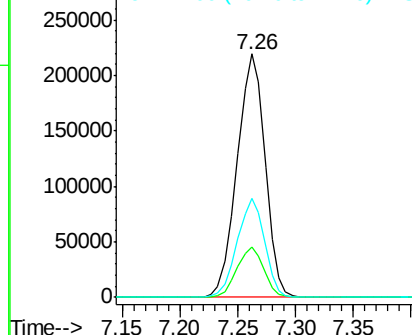

#10

Phenol

Concen: 2.40 ng

RT: 7.29 min Scan# 757

Delta R.T. -0.01 min

Lab File: BG019971.D

Acq: 6 Dec 2015 17:41


Tgt Ion: 94 Resp: 7298

Ion Ratio Lower Upper



94 100


65 34.6 5.4 45.4

66 68.4 11.8 51.8#

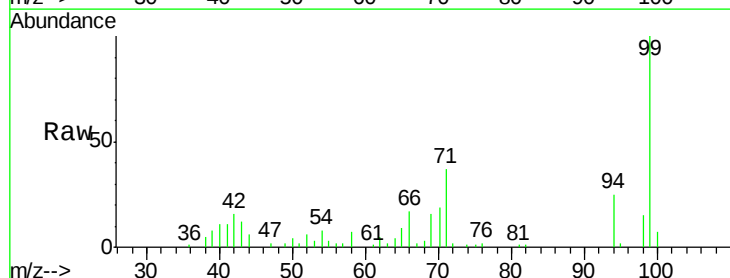

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

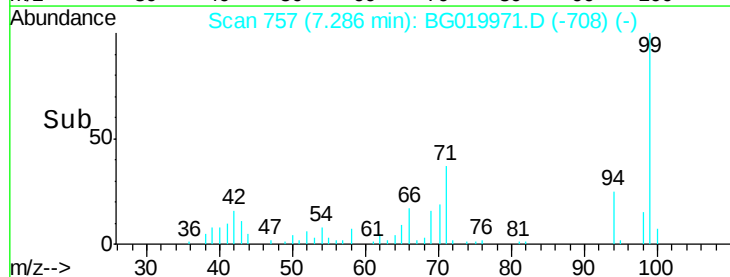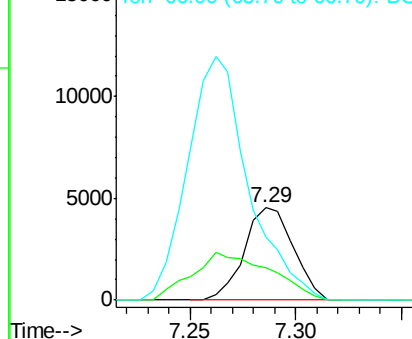


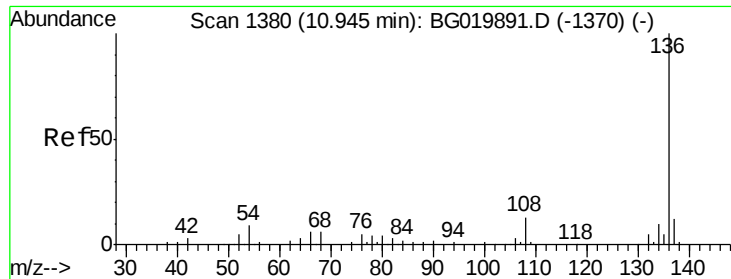




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.93 min Scan# 1377
Delta R.T. -0.02 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Instrument :
BNA_G
ClientSampleId :
SB-1(11-15)

Tgt Ion:	136	Resp:	152718
Ion	Ratio	Lower	Upper
136	100		
137	10.3	8.6	12.8
54	8.4	5.4	8.2#
68	5.7	5.3	7.9




Abundance Ion 136.00 (135.70 to 136.70): B
Ion 137.00 (136.70 to 137.70): B
Ion 54.00 (53.70 to 54.70): B
Ion 68.00 (67.70 to 68.70): B

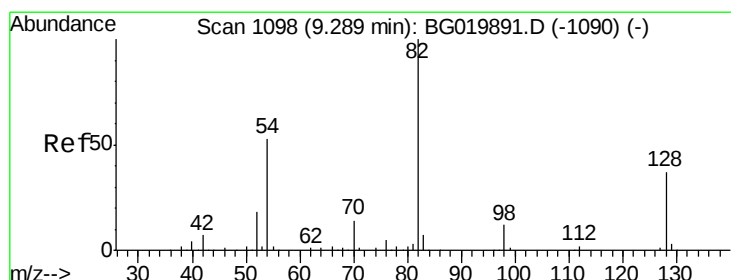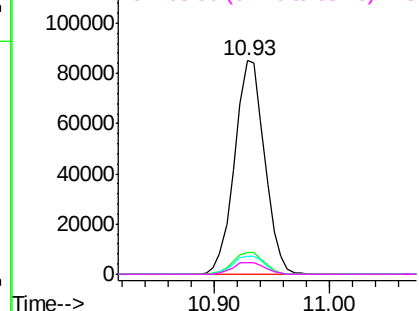




#23
Nitrobenzene-d5
Concen: 86.33 ng
RT: 9.28 min Scan# 1097
Delta R.T. -0.02 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Tgt Ion:	82	Resp:	258328
Ion	Ratio	Lower	Upper
82	100		
128	40.6	36.7	55.1
54	49.0	33.8	50.8



Abundance Ion 82.00 (81.70 to 82.70): B
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): B

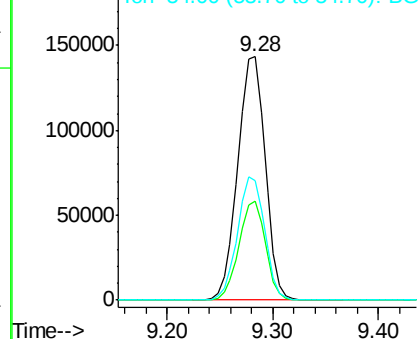


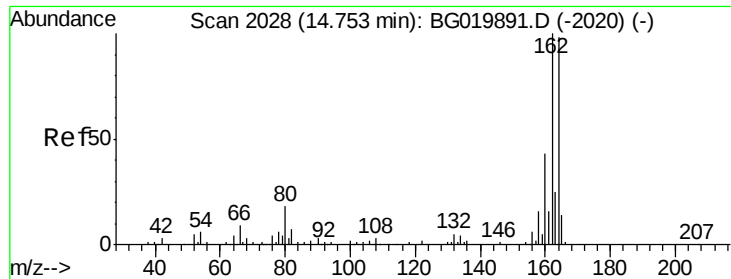




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.74 min Scan# 2026
Delta R.T. -0.02 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Instrument :
BNA_G
ClientSampleId :
SB-1(11-15)

Tgt Ion:164 Resp: 105561
Ion Ratio Lower Upper
164 100
162 110.2 78.8 118.2
160 46.5 36.4 54.6




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

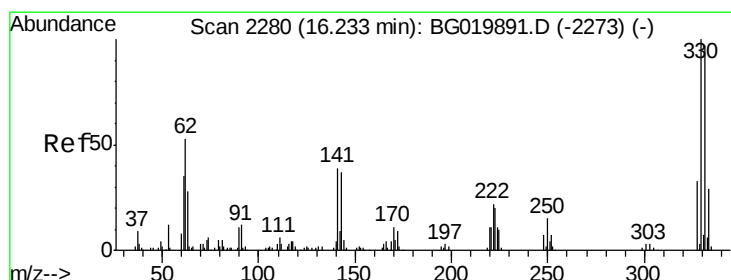
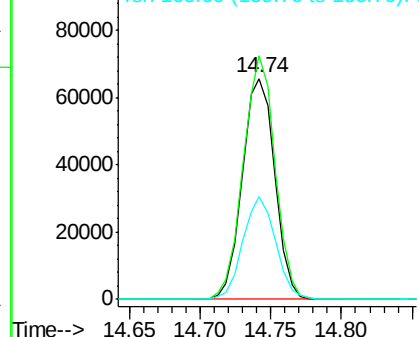



#41
2,4,6-Tribromophenol
Concen: 44.03 ng
RT: 16.22 min Scan# 2278
Delta R.T. -0.02 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Tgt Ion:330 Resp: 71122
Ion Ratio Lower Upper
330 100
332 95.4 78.1 117.1
141 38.1 28.2 42.2



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E




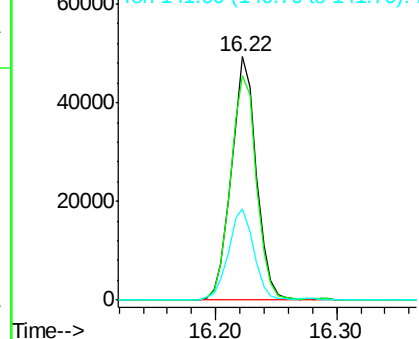


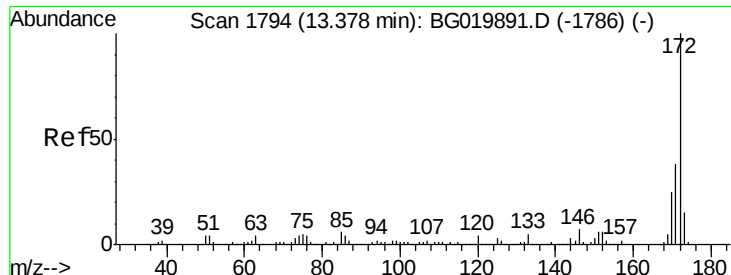

#44
2-Fluorobiphenyl
Concen: 67.48 ng
RT: 13.37 min Scan# 1792
Delta R.T. -0.02 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41




Instrument :
BNA_G
ClientSampleId :
SB-1(11-15)


Tgt Ion:172 Resp: 521694
Ion Ratio Lower Upper
172 100
171 38.3 29.0 43.6
170 24.4 19.9 29.9

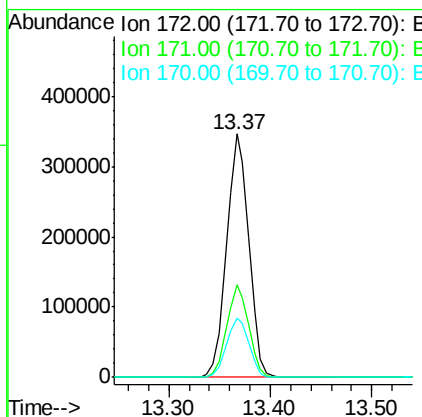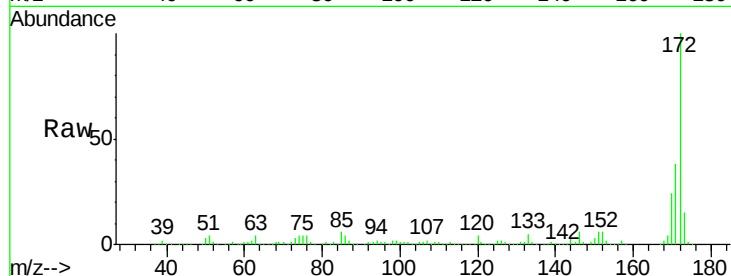

#49
Dimethylphthalate
Concen: 14.17 ng
RT: 14.19 min Scan# 1932
Delta R.T. -0.03 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Tgt Ion:163 Resp: 134516
Ion Ratio Lower Upper
163 100
194 4.4 3.1 4.7
164 10.0 8.8 13.2

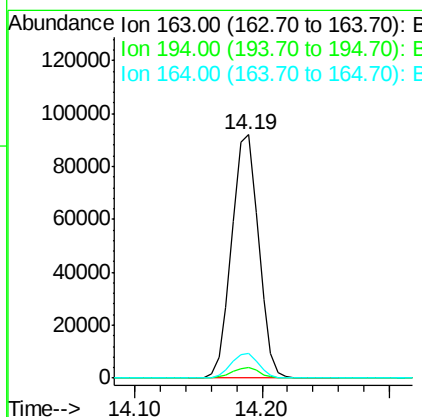







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.49 min Scan# 2493
Delta R.T. -0.02 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Instrument :
BNA_G
ClientSampleId :
SB-1(11-15)

Tgt Ion:188 Resp: 257753
Ion Ratio Lower Upper
188 100
94 6.8 7.7 11.5#
80 9.4 7.8 11.8




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

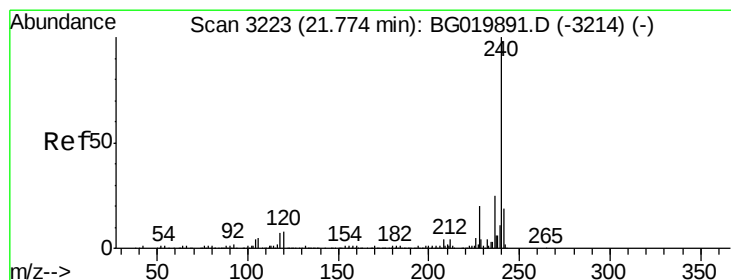
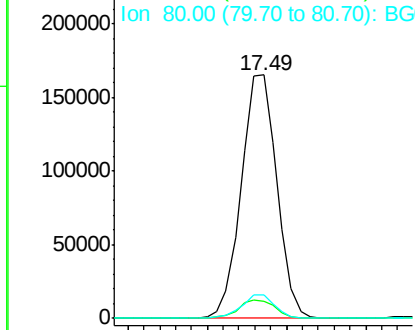



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.76 min Scan# 3220
Delta R.T. -0.04 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Tgt Ion:240 Resp: 307545
Ion Ratio Lower Upper
240 100
120 7.2 7.4 11.0#
236 25.7 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

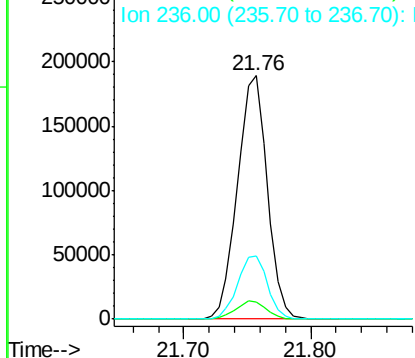

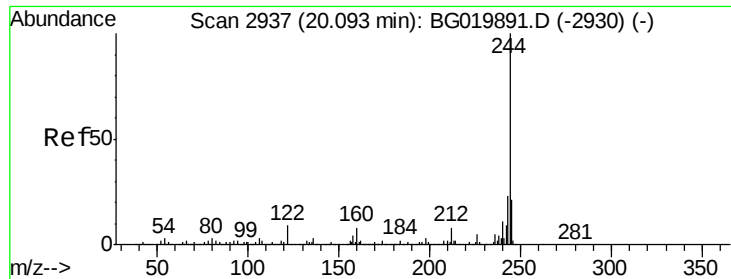

#78

Terphenyl-d14

Concen: 58.23 ng

RT: 20.08 min Scan# 2935

Delta R.T. -0.03 min

Lab File: BG019971.D

Acq: 6 Dec 2015 17:41

Instrument :

BNA_G

ClientSampleId :

SB-1(11-15)


Tgt Ion:244 Resp: 734202

Ion Ratio Lower Upper

244 100

212 8.5 6.9 10.3




122 8.2 10.2 15.2#

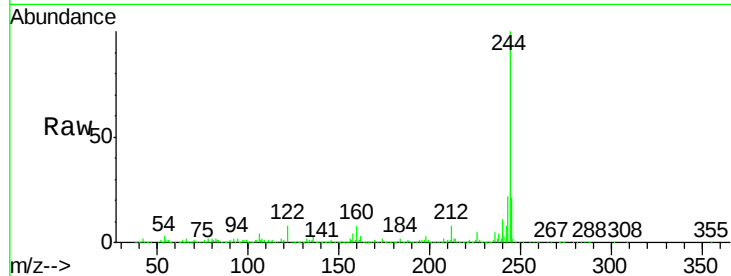

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

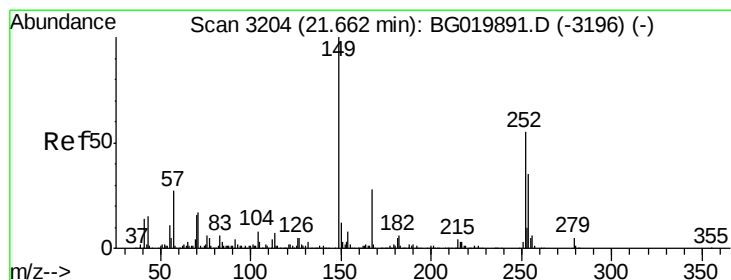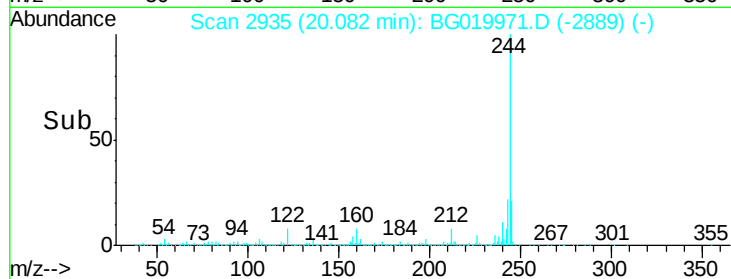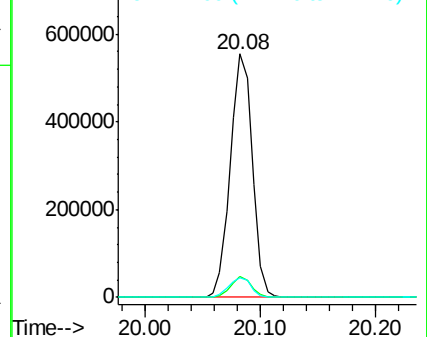

#83

Bis(2-ethylhexyl)phthalate

Concen: 3.50 ng

RT: 21.64 min Scan# 3200

Delta R.T. -0.05 min

Lab File: BG019971.D

Acq: 6 Dec 2015 17:41


Tgt Ion:149 Resp: 36460

Ion Ratio Lower Upper

149 100

167 24.6 23.8 35.8



279 5.8 3.4 5.2#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

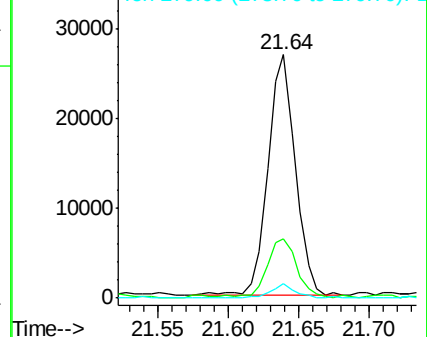


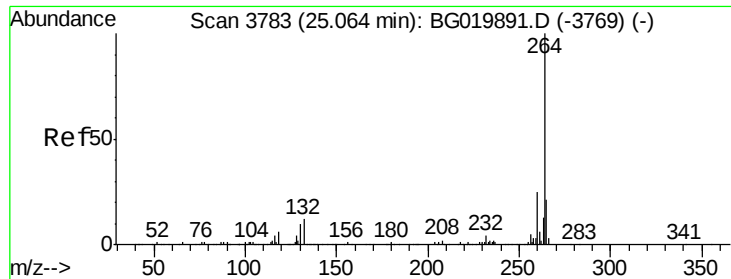

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.03 min Scan# 3777
Delta R.T. -0.06 min
Lab File: BG019971.D
Acq: 6 Dec 2015 17:41

Instrument :
BNA_G
ClientSampleId :
SB-1(11-15)

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.5	27.7
265	20.7	17.2	25.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

