
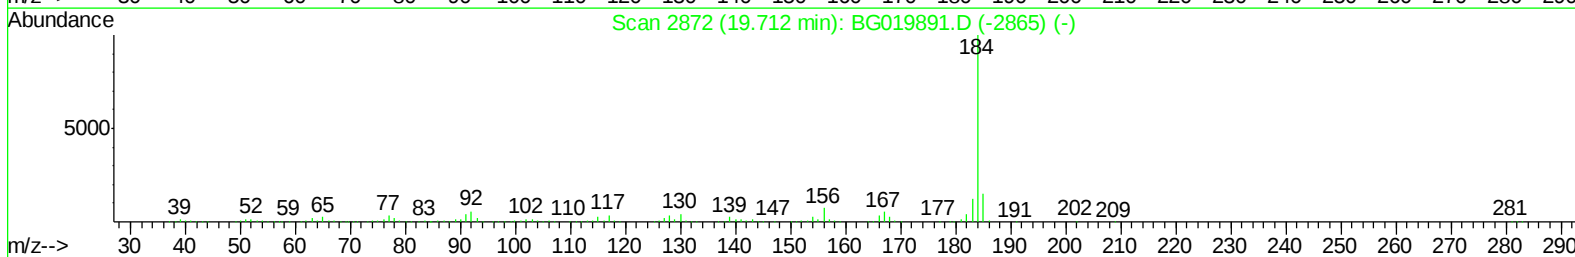
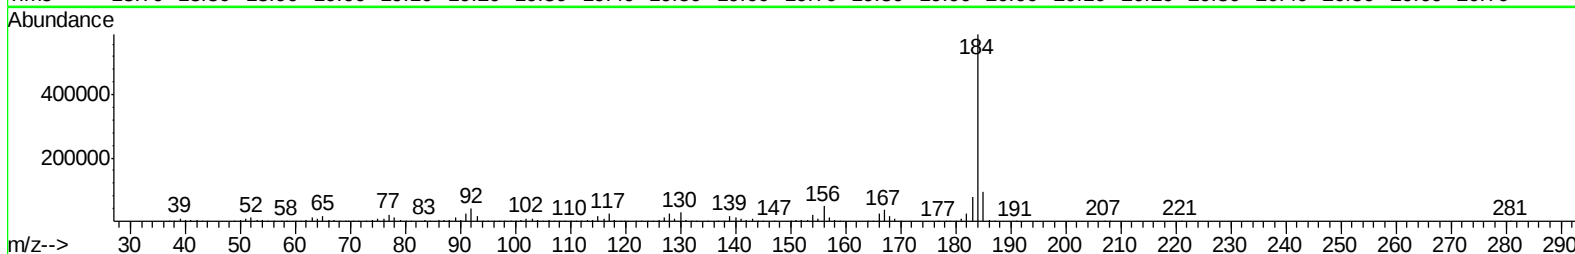


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120615\
Data File : BG019959.D
Acq On : 6 Dec 2015 9:51
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:59:14 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

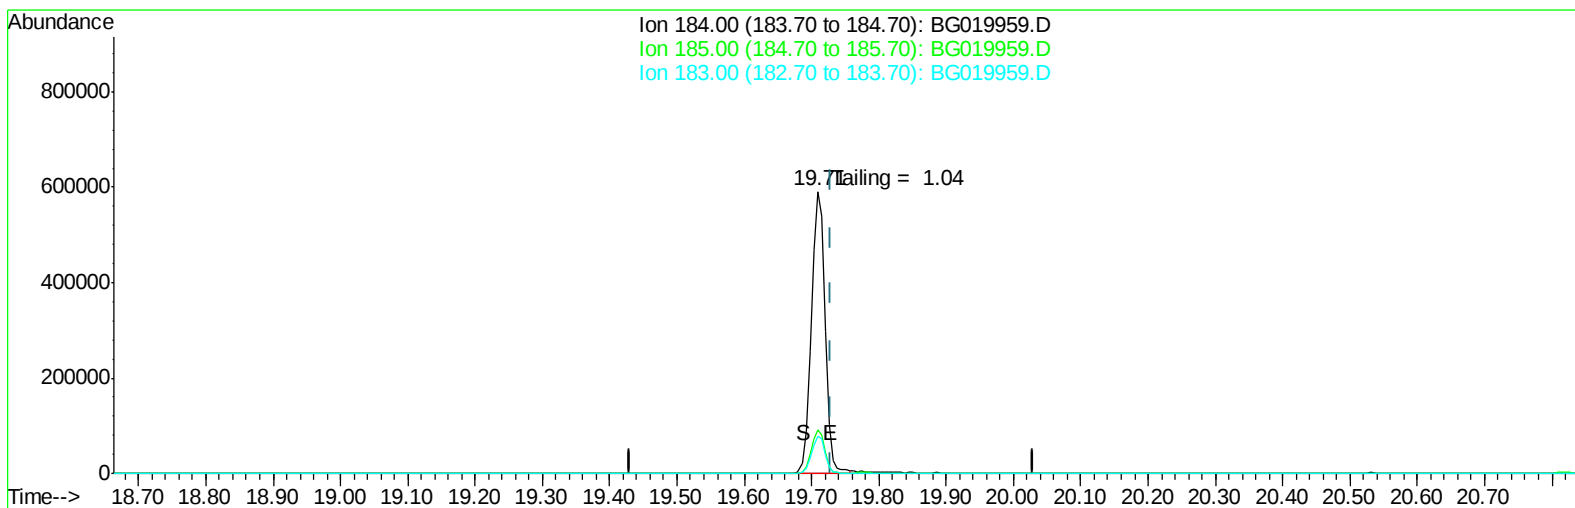

TIC: BG019959.D

(76) Benzidine

19.709min (-0.021) 72627.71ng

response 868378

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.62
183.00	12.60	13.14
0.00	0.00	0.00