


Data Path : Z:\HPCHEM1\BNA G\Data\BG120615\
 Data File : BG019959.D
 Acq On : 6 Dec 2015 9:51
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 18:50:01 2015

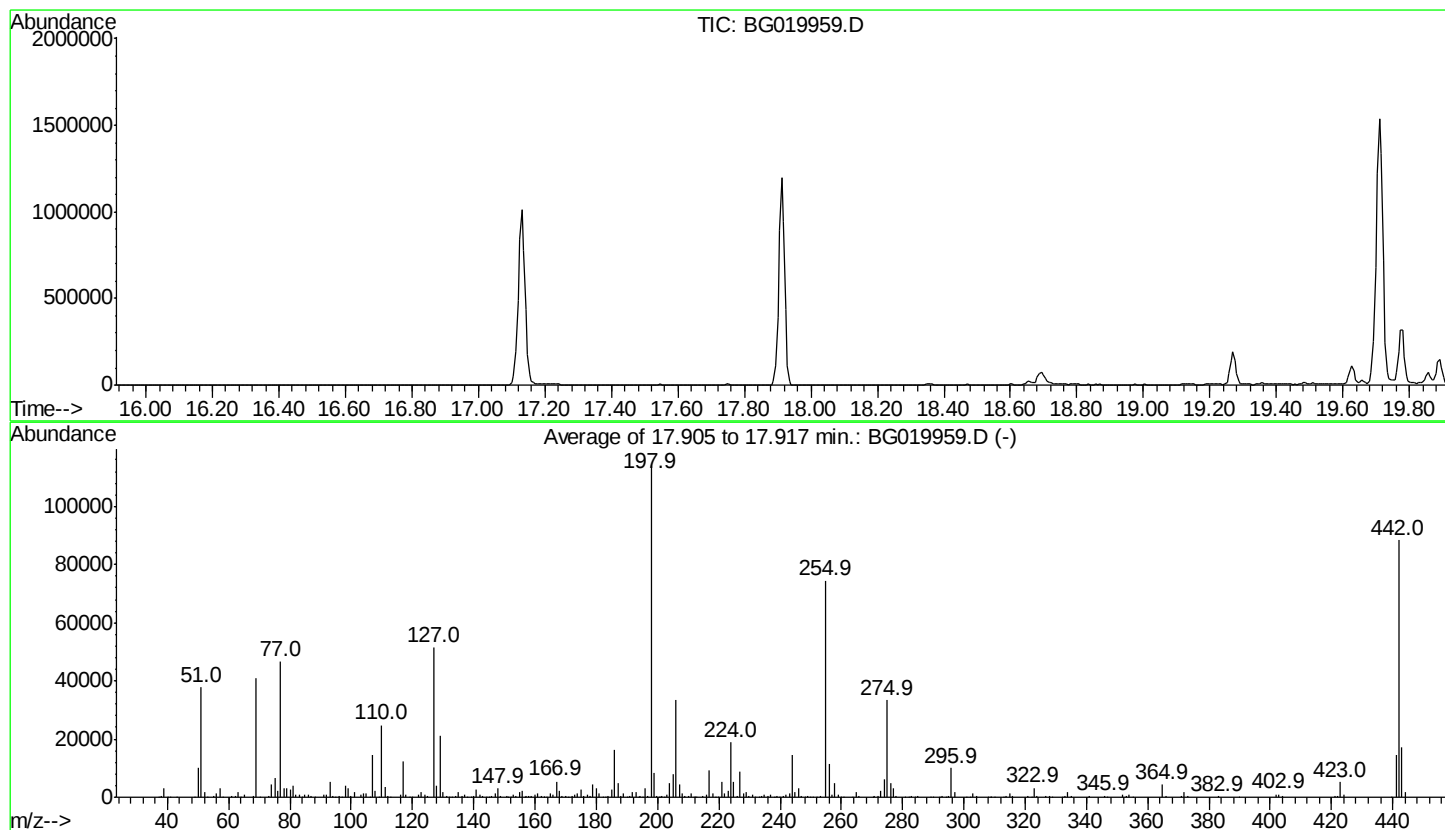

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	37829	PASS
68	69	0.00	2	1.5	634	PASS
69	198	0.00	100	35.9	40906	PASS
70	69	0.00	2	0.5	224	PASS
127	198	10	80	45.1	51437	PASS
197	198	0.00	2	0.3	386	PASS
198	198	100	100	100.0	114008	PASS
199	198	5	9	7.2	8185	PASS
275	198	10	60	29.3	33392	PASS
365	198	1	100	3.7	4202	PASS
441	442	0.01	24	16.6	14707	PASS
442	198	50	100	77.5	88341	PASS
443	442	15	24	19.7	17360	PASS