


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051344.D
 Acq On : 6 Dec 2021 10:28
 Operator : CG/JU
 Sample : DFTPP438
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION
 Last Update : Fri Dec 03 15:23:09 2021

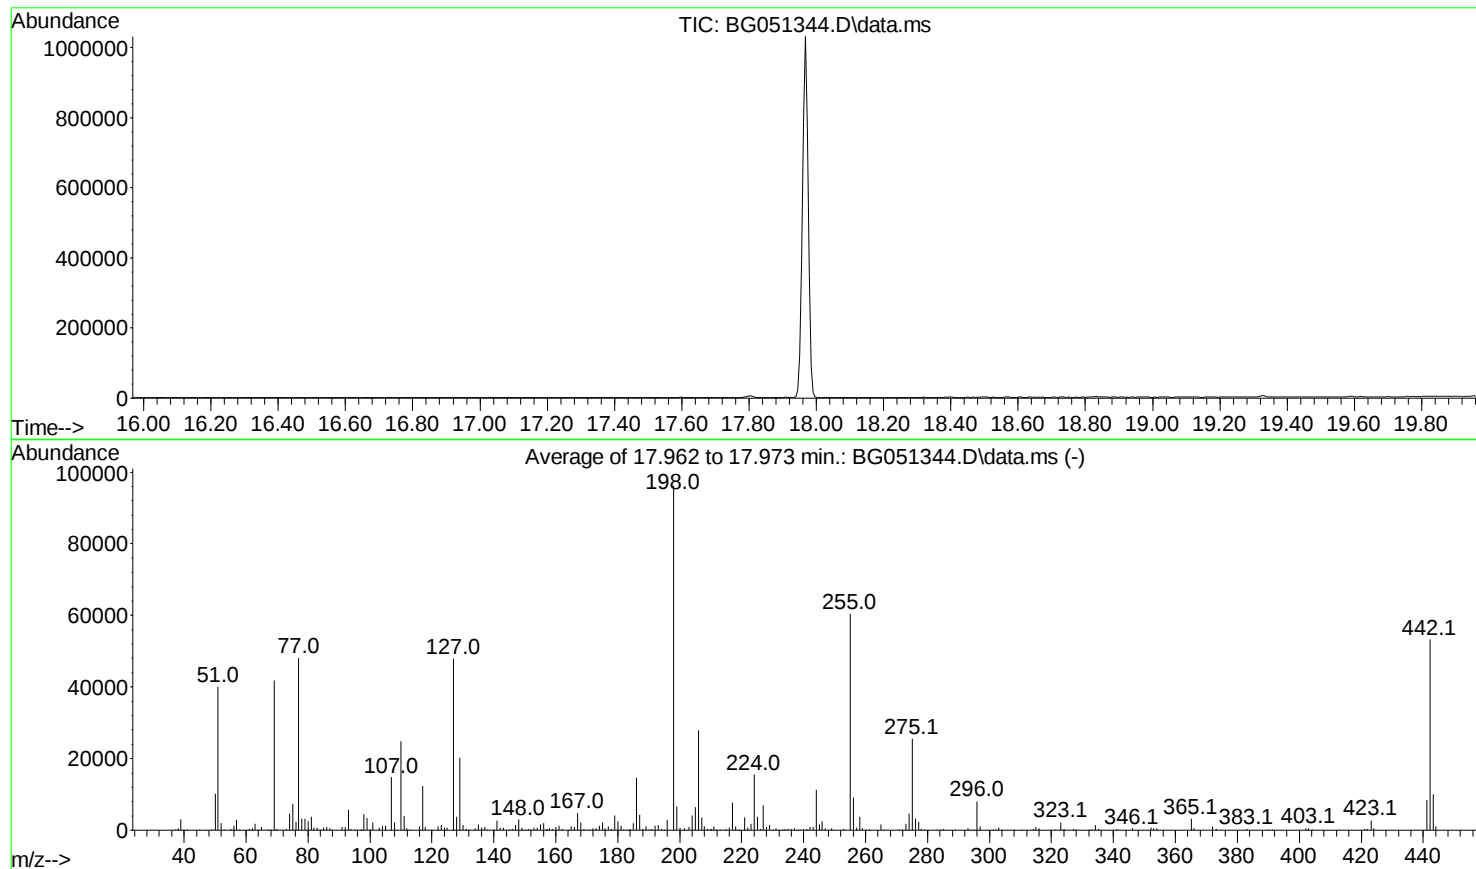

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	41.6	40032	PASS
68	69	0.00	2	0.6	239	PASS
69	198	0.00	100	43.5	41856	PASS
70	69	0.00	2	0.7	291	PASS
127	198	10	80	49.8	47928	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96176	PASS
199	198	5	9	6.9	6617	PASS
275	198	10	60	26.5	25491	PASS
365	198	1	100	3.3	3149	PASS
441	198	0.01	100	8.7	8338	PASS
442	198	50	100	55.4	53259	PASS
443	442	15	24	18.8	10002	PASS