

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051358.D
 Acq On : 6 Dec 2021 20:27
 Operator : CG/JU
 Sample : M4942-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR3

Quant Time: Dec 07 00:00:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 03 15:23:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.191	152	23315	20.000	ng/u1	-0.01
20) Naphthalene-d8	11.018	136	106689	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.825	164	70729	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.575	188	162060	20.000	ng/u1	0.00
79) Chrysene-d12	21.870	240	143406	20.000	ng/u1	-0.01
88) Perylene-d12	25.271	264	145252	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.526	96	2229	3.322	ng/uL	-0.02
4) Pyridine-d5	3.967	84	18718	9.508	ng/u1	-0.01
7) Phenol-d5	7.357	99	45172	19.603	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.504	67	31554	21.803	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.721	132	33572	20.232	ng/u1	-0.01
15) 4-Methylphenol-d8	8.908	113	38129	20.505	ng/u1	0.00
21) Nitrobenzene-d5	9.372	128	19138	21.250	ng/u1	0.00
24) 2-Nitrophenol-d4	10.095	143	22528	22.175	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.647	165	33987	19.717	ng/u1	0.00
31) 4-Chloroaniline-d4	11.159	131	46858	18.579	ng/u1	0.00
46) Dimethylphthalate-d6	14.214	166	130584	23.995	ng/u1	-0.01
49) Acenaphthylene-d8	14.519	160	146396	21.333	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.054	143	18483	20.982	ng/u1	0.00
60) Fluorene-d10	15.812	176	109335	22.310	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.953	200	13143	13.143	ng/u1	0.00
73) Anthracene-d10	17.674	188	177392	22.887	ng/u1	0.00
81) Pyrene-d10	19.954	212	201942	23.273	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.031	264	167178	21.551	ng/u1	-0.01
Target Compounds						
					Qvalue	
83) Butylbenzylphthalate	20.841	149	22321	5.150	ng/u1	94
86) Bis(2-ethylhexyl)phtha...	21.711	149	147515	23.653	ng/u1	99
89) Di-n-octyl phthalate	22.986	149	42697	4.057	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051358.D
Acq On : 6 Dec 2021 20:27
Operator : CG/JU
Sample : M4942-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR3

Quant Time: Dec 07 00:00:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 03 15:23:09 2021
Response via : Initial Calibration




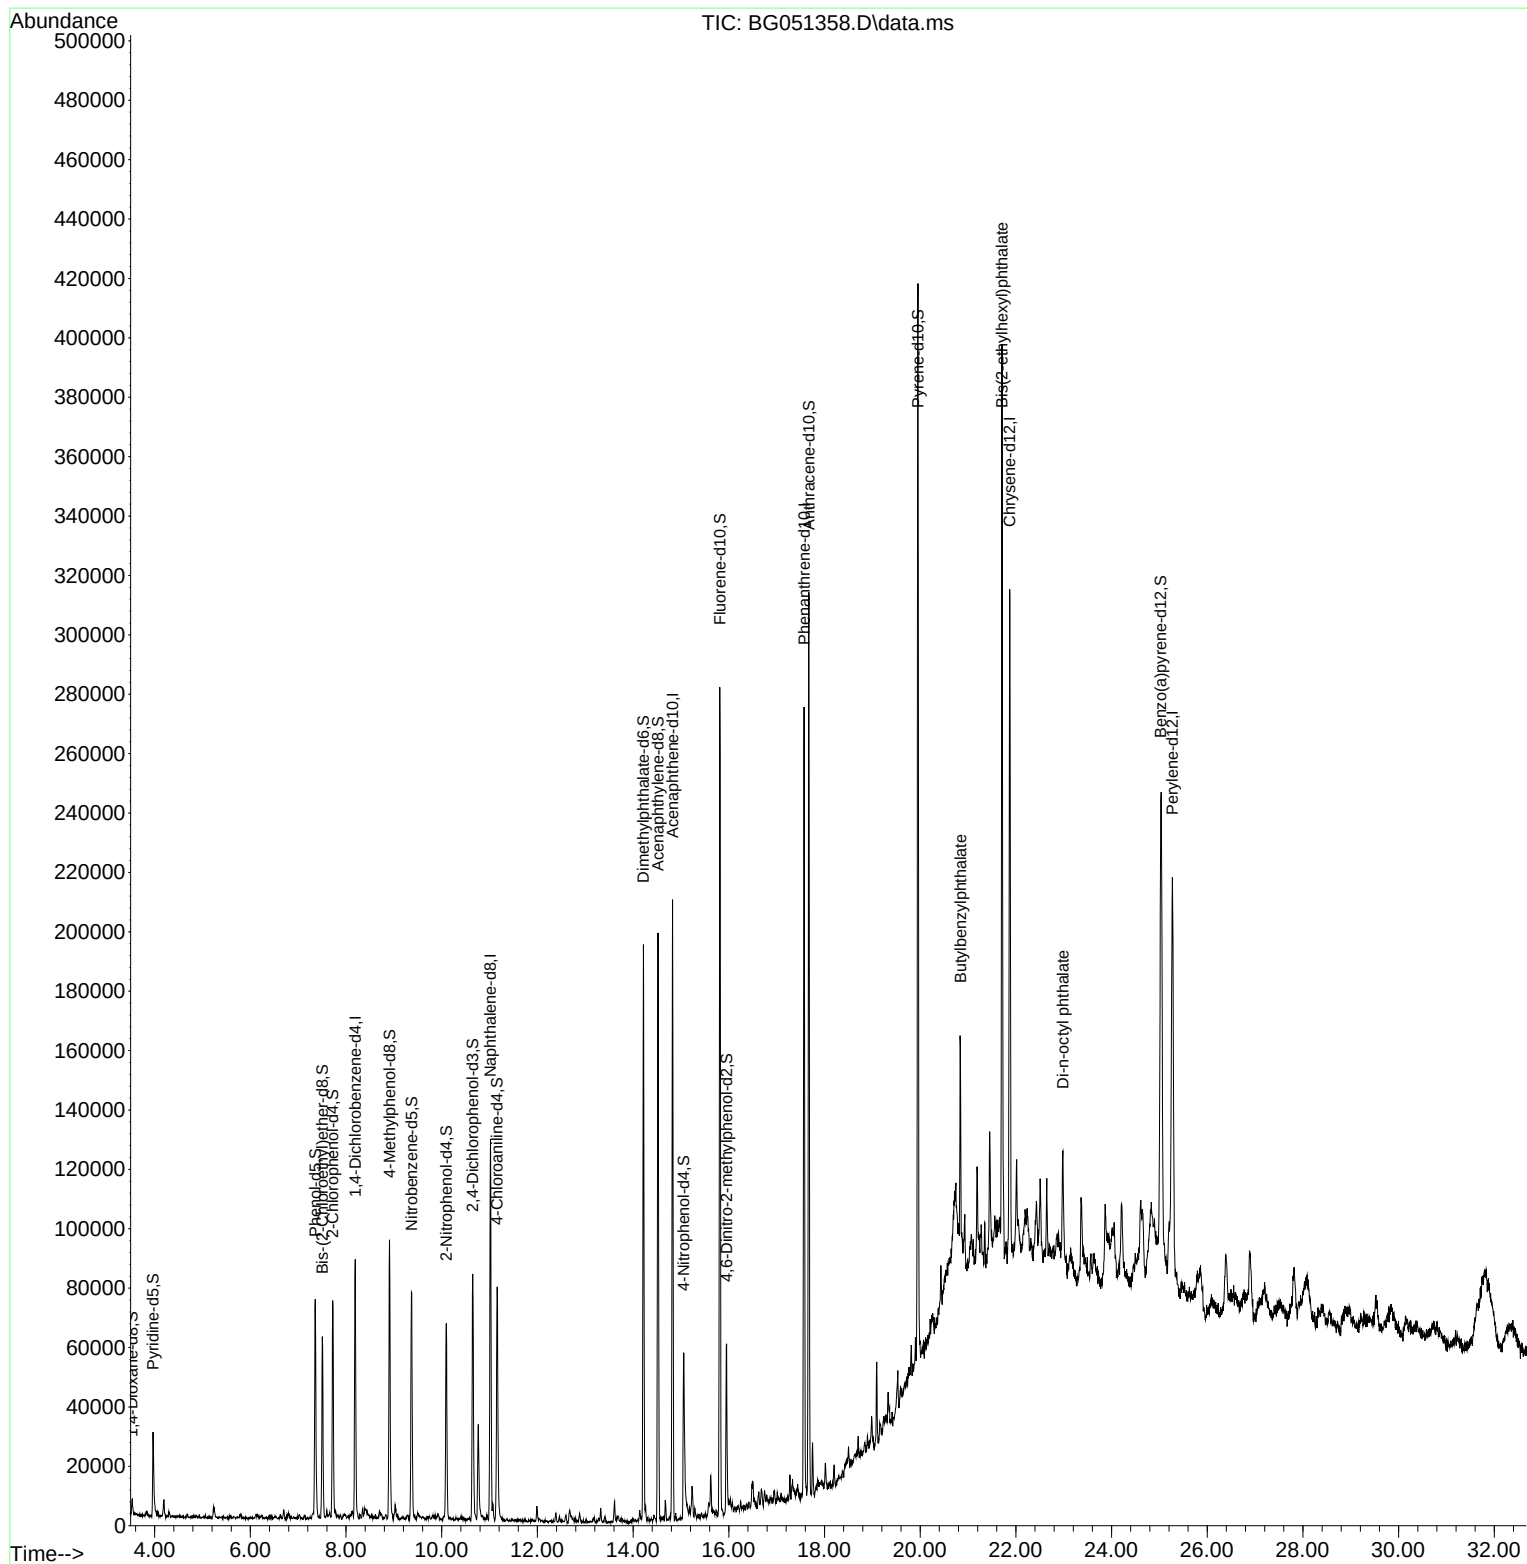


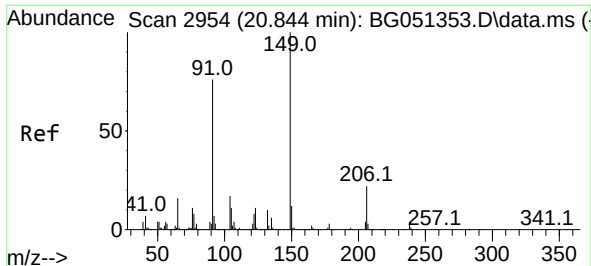

#83
 Butylbenzylphthalate
 Concen: 5.150 ng/ul
 RT: 20.841 min Scan# 2954
 Delta R.T. -0.006 min
 Lab File: BG051358.D
 Acq: 6 Dec 2021 20:27




Instrument :
 BNA_G
 ClientSampleId :
 BGKR3


Tgt Ion:149 Resp: 22321
 Ion Ratio Lower Upper
 149 100
 91 75.9 65.2 97.8
 206 22.3 16.2 24.2

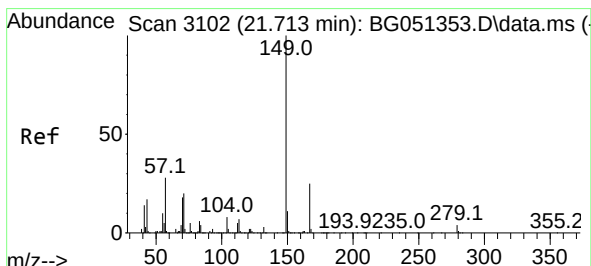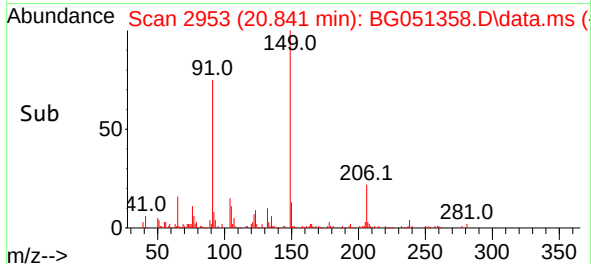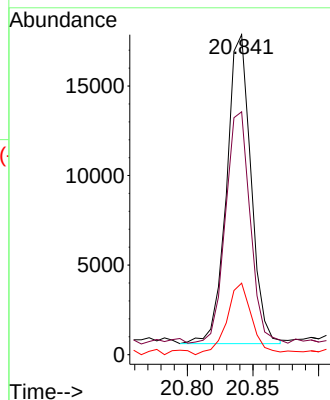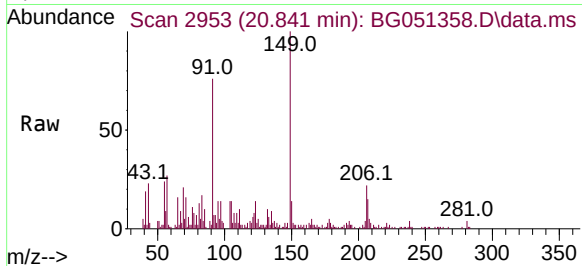

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 23.653 ng/ul
 RT: 21.711 min Scan# 3101
 Delta R.T. -0.012 min
 Lab File: BG051358.D
 Acq: 6 Dec 2021 20:27

Tgt Ion:149 Resp: 147515
 Ion Ratio Lower Upper
 149 100
 167 26.1 21.1 31.7
 279 3.6 2.7 4.1

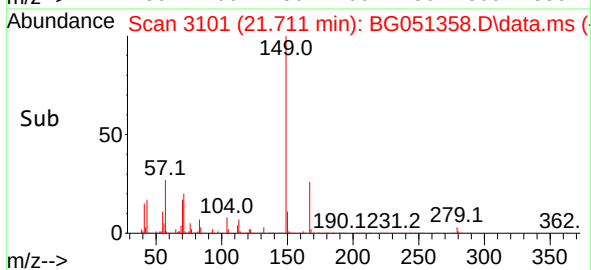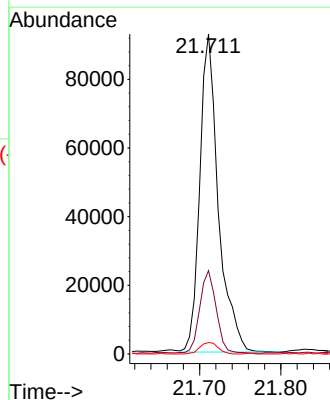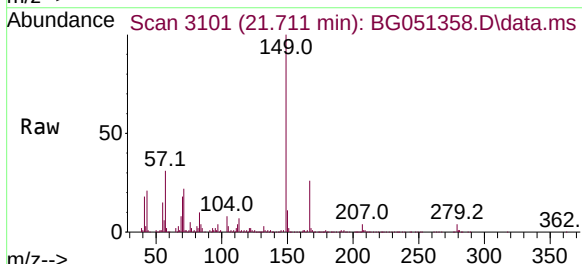

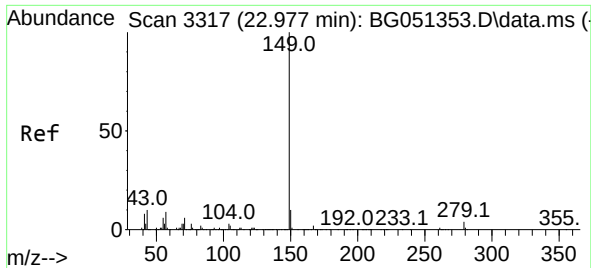

#89

Di-n-octyl phthalate

Concen: 4.057 ng/ul

RT: 22.986 min Scan# 31

Delta R.T. 0.000 min

Lab File: BG051358.D

Acq: 6 Dec 2021 20:27

Instrument :

BNA_G

ClientSampleId :

BGKR3

Tgt Ion:149 Resp: 42697

