

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051361.D
 Acq On : 6 Dec 2021 22:31
 Operator : CG/JU
 Sample : M4942-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.530	3	7	13	rVB3	3807	6485	1.34%	0.112%
2	3.964	78	81	91	rBV	16069	32221	6.67%	0.559%
3	4.188	115	119	124	rVB2	5699	8358	1.73%	0.145%
4	4.305	134	139	142	rBV4	1771	2969	0.61%	0.051%
5	5.234	293	297	303	rVB3	3867	6958	1.44%	0.121%
6	5.657	367	369	375	rVB3	975	758	0.16%	0.013%
7	6.479	507	509	511	rBV2	940	1184	0.25%	0.021%
8	7.355	652	658	667	rBV2	60531	113373	23.47%	1.965%
9	7.501	675	683	690	rBV	51668	90585	18.75%	1.570%
10	7.719	714	720	727	rBV	60438	108837	22.53%	1.887%
11	7.983	762	765	766	rBV2	798	903	0.19%	0.016%
12	8.189	794	800	813	rVB	98886	172186	35.64%	2.985%
13	8.906	916	922	934	rVB	72142	138360	28.64%	2.398%
14	9.023	940	942	945	rBV2	1180	805	0.17%	0.014%
15	9.370	994	1001	1009	rVB	61351	111997	23.18%	1.941%
16	9.769	1067	1069	1071	rBV	967	680	0.14%	0.012%
17	10.093	1117	1124	1134	rBV	53366	99252	20.54%	1.720%
18	10.651	1212	1219	1227	rBV	65047	128875	26.67%	2.234%
19	10.768	1233	1239	1250	rBV3	10524	22805	4.72%	0.395%
20	10.944	1266	1269	1271	rBV2	843	876	0.18%	0.015%
21	11.015	1274	1281	1296	rVB	138479	254963	52.77%	4.419%
22	11.156	1299	1305	1317	rBV	66180	134248	27.79%	2.327%
23	12.378	1512	1513	1518	rBV2	846	927	0.19%	0.016%
24	12.454	1524	1526	1527	rBV	1011	670	0.14%	0.012%
25	12.590	1546	1549	1550	rBV2	878	738	0.15%	0.013%
26	12.672	1560	1563	1568	rVB2	764	974	0.20%	0.017%
27	12.883	1593	1599	1602	rBV3	769	1295	0.27%	0.022%
28	13.160	1645	1646	1649	rBV2	970	1004	0.21%	0.017%
29	13.277	1661	1666	1670	rBV	569	823	0.17%	0.014%
30	13.324	1670	1674	1679	rVB2	874	1190	0.25%	0.021%
31	13.412	1686	1689	1692	rBV2	1162	1502	0.31%	0.026%
32	13.612	1718	1723	1727	rVB2	2716	3798	0.79%	0.066%
33	13.659	1729	1731	1733	rVV2	1123	853	0.18%	0.015%
34	13.688	1733	1736	1738	rVB2	934	974	0.20%	0.017%
35	14.211	1820	1825	1832	rBV	153459	234929	48.63%	4.072%
36	14.440	1860	1864	1869	rBV4	730	1606	0.33%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051361.D
 Acq On : 6 Dec 2021 22:31
 Operator : CG/JU
 Sample : M4942-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	14.523	1871	1878	1890	rVB	163607	269523	55.79%	4.672%
38	14.675	1899	1904	1907	rBV3	2797	3643	0.75%	0.063%
39	14.822	1922	1929	1937	rBV	233804	368920	76.36%	6.395%
40	14.981	1952	1956	1958	rBV2	614	788	0.16%	0.014%
41	15.063	1963	1970	1987	rVV3	25922	72612	15.03%	1.259%
42	15.192	1990	1992	1995	rVV2	1457	1726	0.36%	0.030%
43	15.239	1995	2000	2005	rVV2	11715	18121	3.75%	0.314%
44	15.281	2005	2007	2011	rVV4	789	1152	0.24%	0.020%
45	15.345	2014	2018	2020	rBV2	743	900	0.19%	0.016%
46	15.574	2052	2057	2061	rBV2	2290	3648	0.76%	0.063%
47	15.627	2061	2066	2070	rVV4	3176	4493	0.93%	0.078%
48	15.686	2074	2076	2080	rVB	643	766	0.16%	0.013%
49	15.815	2091	2098	2108	rVB	221809	350905	72.63%	6.082%
50	15.956	2117	2122	2131	rBV2	28639	51584	10.68%	0.894%
51	16.103	2146	2147	2149	rVB2	1339	666	0.14%	0.012%
52	16.121	2149	2150	2152	rBV	1115	726	0.15%	0.013%
53	16.180	2157	2160	2162	rVV3	999	1084	0.22%	0.019%
54	16.203	2162	2164	2166	rVB2	1155	908	0.19%	0.016%
55	16.244	2169	2171	2172	rBV2	1096	875	0.18%	0.015%
56	16.262	2172	2174	2175	rVB2	1300	696	0.14%	0.012%
57	16.368	2190	2192	2196	rVB	844	860	0.18%	0.015%
58	16.426	2196	2202	2207	rBV3	2014	4780	0.99%	0.083%
59	16.479	2207	2211	2213	rBV5	2700	3646	0.75%	0.063%
60	16.573	2225	2227	2231	rVB2	919	899	0.19%	0.016%
61	16.614	2231	2234	2239	rBV3	1601	2481	0.51%	0.043%
62	16.673	2242	2244	2245	rBV2	2080	1351	0.28%	0.023%
63	16.749	2253	2257	2262	rBV4	1340	2498	0.52%	0.043%
64	16.791	2262	2264	2268	rVV2	1001	1199	0.25%	0.021%
65	16.820	2268	2269	2273	rVB2	904	684	0.14%	0.012%
66	16.914	2283	2285	2288	rBV2	803	729	0.15%	0.013%
67	16.949	2288	2291	2295	rVB5	1577	2251	0.47%	0.039%
68	17.020	2297	2303	2305	rBV6	1828	3084	0.64%	0.053%
69	17.090	2313	2315	2320	rVB5	1290	1884	0.39%	0.033%
70	17.190	2330	2332	2333	rBV2	1030	682	0.14%	0.012%
71	17.278	2342	2347	2352	rBV4	2902	4406	0.91%	0.076%
72	17.325	2352	2355	2357	rBV3	1662	2002	0.41%	0.035%
73	17.572	2390	2397	2406	rBV	322262	483143	100.00%	8.375%
74	17.672	2408	2414	2422	rVV2	251147	399192	82.62%	6.919%
75	17.754	2424	2428	2432	rVB3	7643	10496	2.17%	0.182%
76	17.819	2436	2439	2443	rVB6	1295	2144	0.44%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051361.D
 Acq On : 6 Dec 2021 22:31
 Operator : CG/JU
 Sample : M4942-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

77	17.989	2465	2468	2469	rBV2	1144	957	0.20%	0.017%
78	18.019	2469	2473	2478	rVB5	2661	5422	1.12%	0.094%
79	18.060	2478	2480	2483	rBV3	1400	1478	0.31%	0.026%
80	18.195	2499	2503	2506	rBV4	4017	5174	1.07%	0.090%
81	18.248	2511	2512	2514	rBV2	968	687	0.14%	0.012%
82	18.500	2553	2555	2561	rVB4	2730	3086	0.64%	0.053%
83	19.088	2653	2655	2660	rVB3	8907	10742	2.22%	0.186%
84	19.329	2693	2696	2699	rBV5	4148	6693	1.39%	0.116%
85	19.952	2796	2802	2813	rBV	327399	481955	99.75%	8.354%
86	20.839	2950	2953	2957	rVB2	21759	25624	5.30%	0.444%
87	21.708	3097	3101	3109	rVB	109535	168580	34.89%	2.922%
88	21.873	3123	3129	3137	rVB	274247	470036	97.29%	8.147%
89	25.034	3660	3667	3678	rVB2	127865	368884	76.35%	6.394%
90	25.269	3700	3707	3719	rVB2	148938	448721	92.88%	7.778%




Sum of corrected areas: 5769147

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051361.D
Acq On : 6 Dec 2021 22:31
Operator : CG/JU
Sample : M4942-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

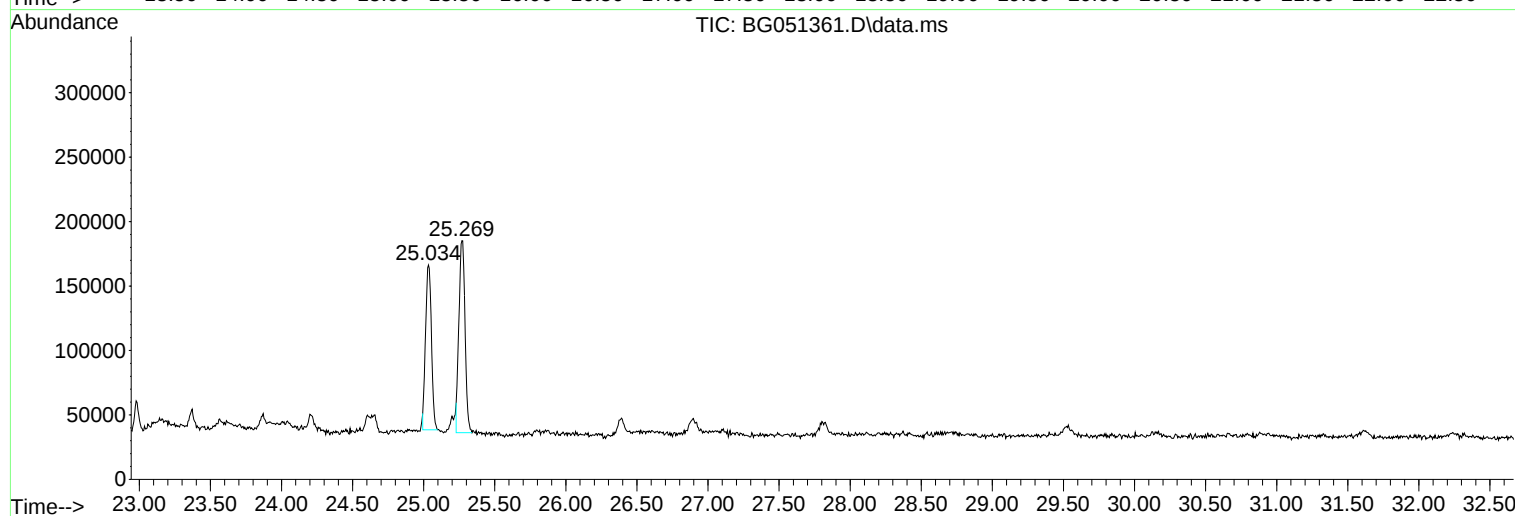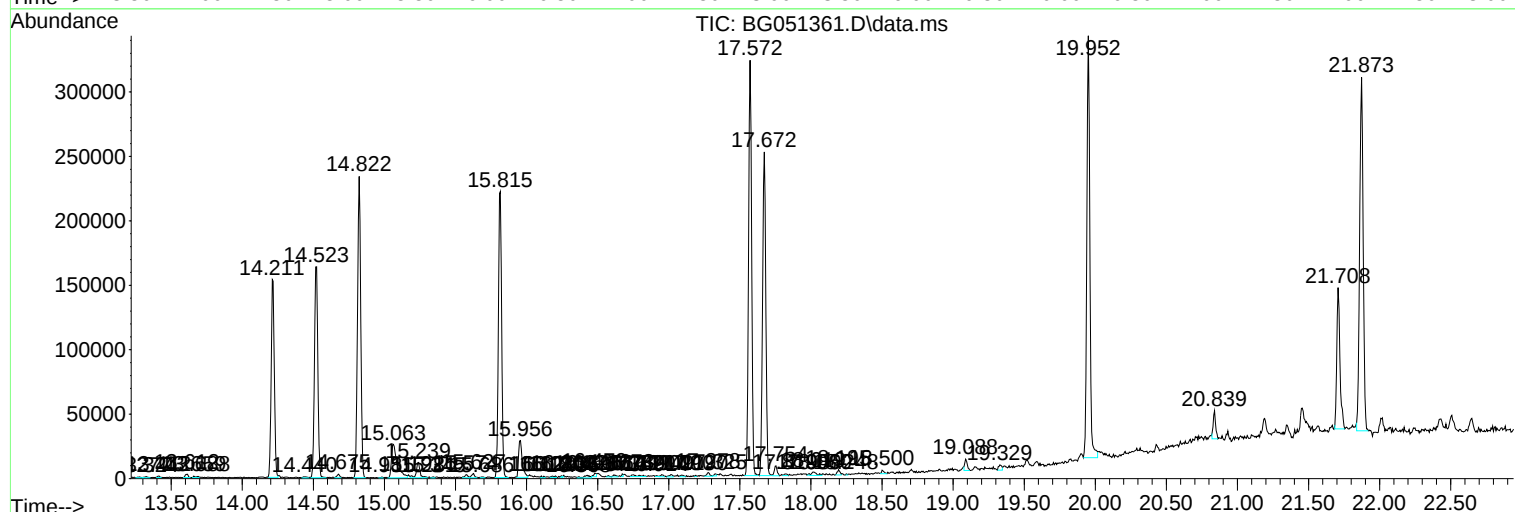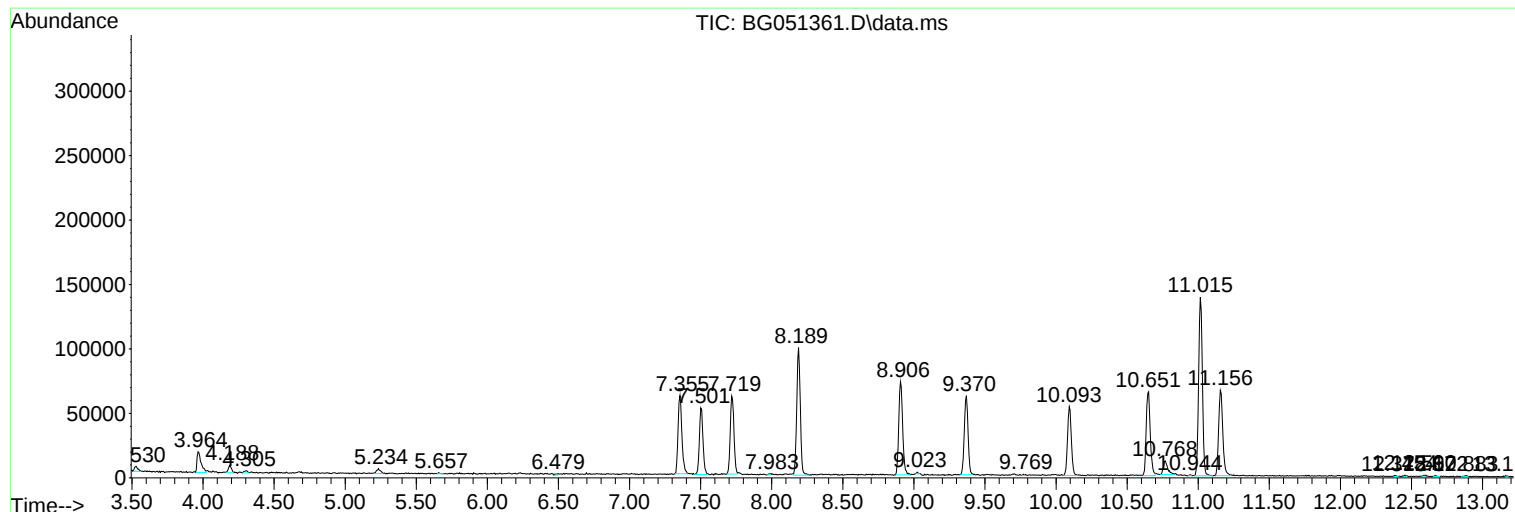

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051361.D
Acq On : 6 Dec 2021 22:31
Operator : CG/JU
Sample : M4942-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051361.D
Acq On : 6 Dec 2021 22:31
Operator : CG/JU
Sample : M4942-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------