

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051370.D
 Acq On : 7 Dec 2021 5:21
 Operator : CG/JU
 Sample : PB141154BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	3	7	13	rVB2	8884	11680	1.43%	0.129%
2	3.705	35	37	41	rVB2	944	889	0.11%	0.010%
3	3.957	76	80	94	rBV	103054	186036	22.79%	2.051%
4	4.298	133	138	143	rVB3	2889	4175	0.51%	0.046%
5	4.792	218	222	223	rBV2	660	833	0.10%	0.009%
6	4.968	247	252	253	rBV3	706	819	0.10%	0.009%
7	7.353	652	658	668	rBV	142528	257519	31.54%	2.839%
8	7.506	677	684	693	rVV	109751	186006	22.78%	2.050%
9	7.724	714	721	730	rBV	140601	245488	30.07%	2.706%
10	7.782	730	731	737	rVB3	1032	1538	0.19%	0.017%
11	8.194	793	801	810	rVB	109096	191293	23.43%	2.109%
12	8.910	916	923	935	rBV	166375	308964	37.84%	3.406%
13	9.239	975	979	984	rBV2	690	1120	0.14%	0.012%
14	9.369	994	1001	1016	rBV	137699	252940	30.98%	2.788%
15	10.097	1118	1125	1136	rBV	117976	218698	26.79%	2.411%
16	10.650	1212	1219	1231	rBV	160053	308830	37.83%	3.404%
17	11.020	1274	1282	1290	rBV	159151	292476	35.82%	3.224%
18	11.161	1299	1306	1319	rVB	160469	317379	38.87%	3.499%
19	12.600	1545	1551	1558	rBV3	2241	4173	0.51%	0.046%
20	14.216	1820	1826	1836	rBV	305672	467178	57.22%	5.150%
21	14.522	1869	1878	1887	rBV	361225	591042	72.39%	6.515%
22	14.827	1922	1930	1939	rBV	267739	422804	51.79%	4.661%
23	15.056	1964	1969	1988	rBV	82714	193482	23.70%	2.133%
24	15.274	2004	2006	2015	rVB3	773	1692	0.21%	0.019%
25	15.820	2092	2099	2110	rBV	448650	724701	88.76%	7.989%
26	15.961	2118	2123	2135	rBV2	60674	100740	12.34%	1.111%
27	16.055	2135	2139	2145	rVB2	1282	2002	0.25%	0.022%
28	17.242	2338	2341	2343	rBV2	996	892	0.11%	0.010%
29	17.289	2348	2349	2354	rBV2	521	826	0.10%	0.009%
30	17.359	2357	2361	2364	rBV3	899	1073	0.13%	0.012%
31	17.577	2391	2398	2405	rBV	322944	498488	61.06%	5.495%
32	17.677	2408	2415	2422	rBV2	509264	785467	96.21%	8.659%
33	17.894	2448	2452	2453	rBV3	869	905	0.11%	0.010%
34	17.970	2463	2465	2468	rVB3	1081	863	0.11%	0.010%
35	18.029	2472	2475	2480	rBV4	844	1482	0.18%	0.016%
36	18.217	2505	2507	2509	rBV3	964	900	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051370.D
 Acq On : 7 Dec 2021 5:21
 Operator : CG/JU
 Sample : PB141154BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK154

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	18.241	2509	2511	2514	rVB3	890	907	0.11%	0.010%
38	18.582	2566	2569	2571	rBV3	1402	1774	0.22%	0.020%
39	18.599	2571	2572	2575	rVV3	1078	1028	0.13%	0.011%
40	18.775	2599	2602	2604	rBV2	1753	2254	0.28%	0.025%
41	18.963	2631	2634	2636	rBV4	1316	1639	0.20%	0.018%
42	19.093	2654	2656	2657	rVB2	1358	847	0.10%	0.009%
43	19.245	2679	2682	2685	rBV4	1850	2985	0.37%	0.033%
44	19.269	2685	2686	2687	rBV	1759	1140	0.14%	0.013%
45	19.304	2690	2692	2693	rBV2	1862	1547	0.19%	0.017%
46	19.398	2705	2708	2709	rBV2	1714	1766	0.22%	0.019%
47	19.522	2725	2729	2734	rVB4	7279	10530	1.29%	0.116%
48	19.563	2734	2736	2737	rBV2	1896	1062	0.13%	0.012%
49	19.592	2737	2741	2747	rBV3	8286	11910	1.46%	0.131%
50	19.903	2792	2794	2795	rVB2	3209	1349	0.17%	0.015%
51	19.956	2797	2803	2810	rVV	545656	816439	100.00%	9.000%
52	21.878	3124	3130	3139	rVB2	245397	443753	54.35%	4.892%
53	25.050	3661	3670	3682	rVB2	244562	732345	89.70%	8.073%
54	25.291	3702	3711	3722	rVB2	147770	452786	55.46%	4.991%




Sum of corrected areas: 9071454

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051370.D
Acq On : 7 Dec 2021 5:21
Operator : CG/JU
Sample : PB141154BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

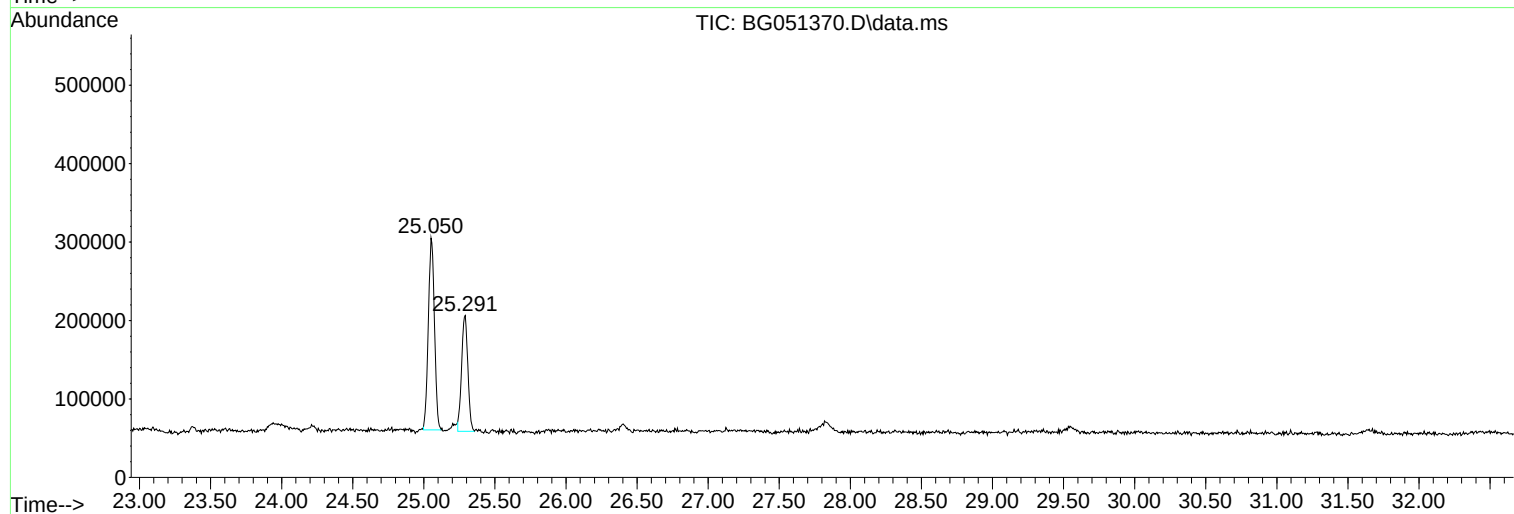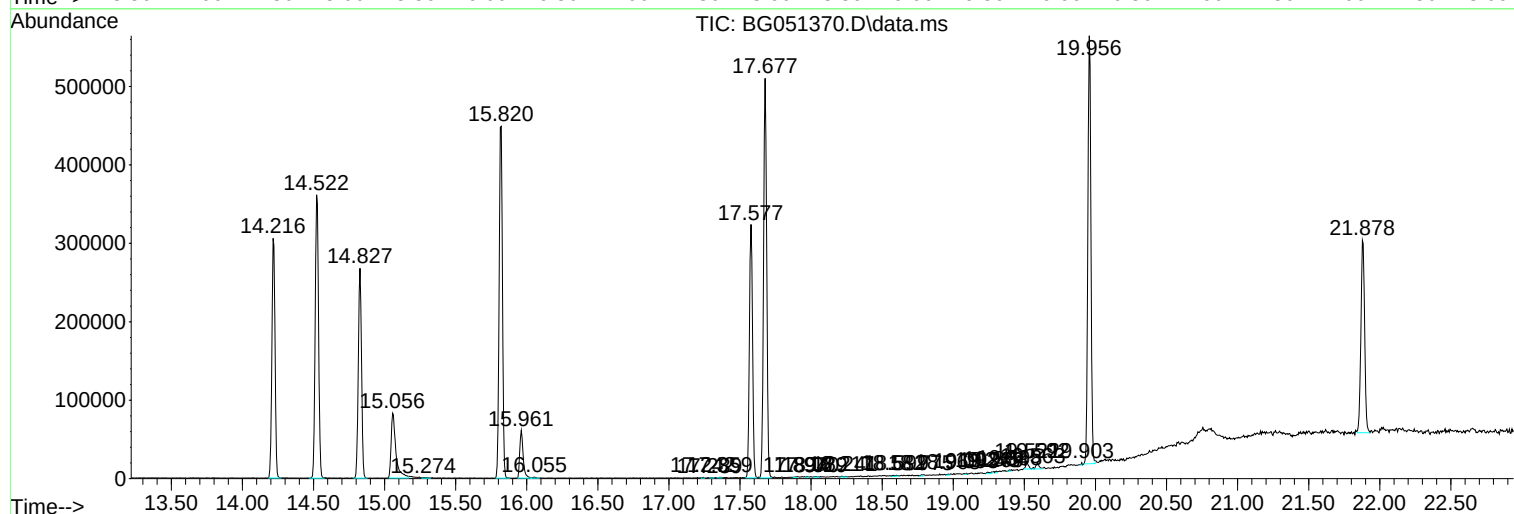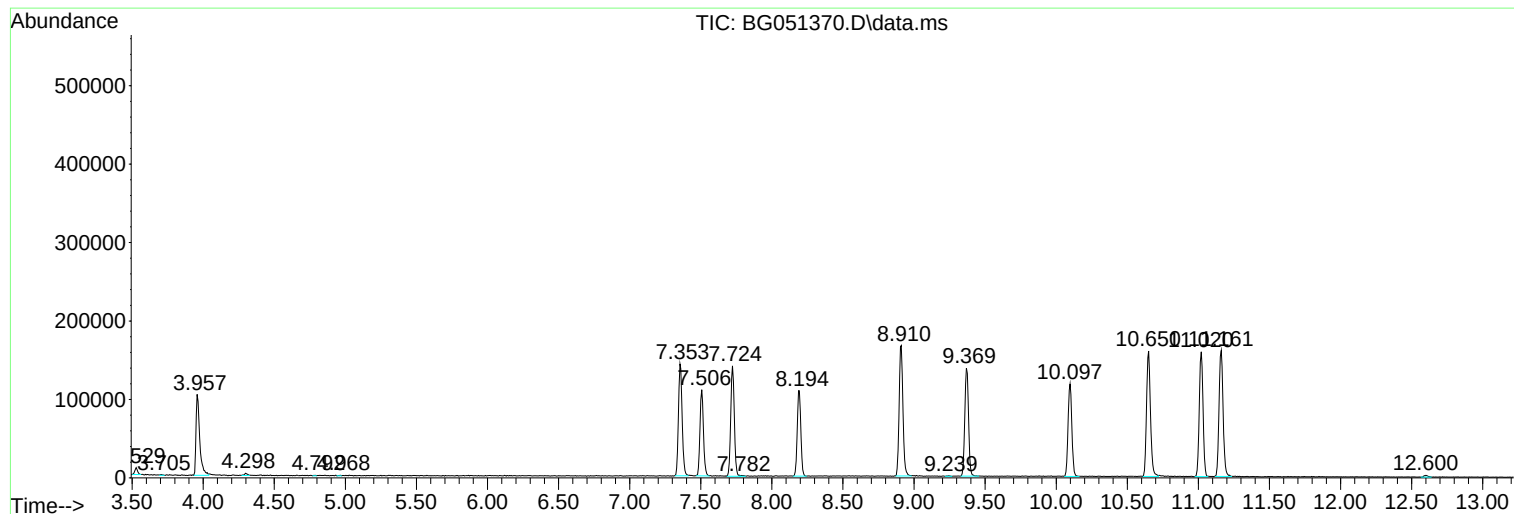

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051370.D
Acq On : 7 Dec 2021 5:21
Operator : CG/JU
Sample : PB141154BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051370.D
Acq On : 7 Dec 2021 5:21
Operator : CG/JU
Sample : PB141154BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK154

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc