

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051372.D
 Acq On : 7 Dec 2021 6:42
 Operator : CG/JU
 Sample : PB141156BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK156

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.526	3	6	12	rVB	7050	10179	1.38%	0.123%
2	3.955	75	79	96	rBV	86109	160746	21.84%	1.944%
3	4.302	136	138	142	rVB3	2410	2456	0.33%	0.030%
4	4.531	176	177	182	rBV3	759	859	0.12%	0.010%
5	4.695	201	205	207	rBV2	916	1141	0.16%	0.014%
6	5.007	255	258	260	rBV2	854	934	0.13%	0.011%
7	5.077	268	270	274	rVB3	649	843	0.11%	0.010%
8	5.283	301	305	310	rVB3	763	1727	0.23%	0.021%
9	6.082	437	441	445	rBV2	888	871	0.12%	0.011%
10	6.258	468	471	473	rBV	651	922	0.13%	0.011%
11	6.564	520	523	526	rBV	481	841	0.11%	0.010%
12	7.357	650	658	671	rBV	122592	225437	30.63%	2.727%
13	7.504	676	683	692	rVB	93200	160465	21.80%	1.941%
14	7.721	713	720	733	rVB	119380	211665	28.76%	2.560%
15	8.191	792	800	809	rVB	105224	182522	24.80%	2.208%
16	8.908	915	922	939	rBV	150805	274254	37.26%	3.317%
17	9.372	993	1001	1010	rBV	121102	223724	30.40%	2.706%
18	10.095	1118	1124	1132	rVV2	106022	191514	26.02%	2.316%
19	10.647	1211	1218	1235	rBV	140110	270028	36.69%	3.266%
20	11.017	1273	1281	1289	rBV	160607	284962	38.72%	3.447%
21	11.158	1296	1305	1320	rBV	136834	263198	35.76%	3.183%
22	12.598	1545	1550	1557	rVB3	1975	4150	0.56%	0.050%
23	14.219	1819	1826	1837	rVB	269057	417461	56.72%	5.049%
24	14.525	1870	1878	1888	rBV	330989	531410	72.20%	6.428%
25	14.824	1922	1929	1939	rVB	265957	412099	55.99%	4.984%
26	15.060	1963	1969	1986	rBV	71532	167441	22.75%	2.025%
27	15.242	1998	2000	2003	rVB3	865	944	0.13%	0.011%
28	15.817	2091	2098	2107	rBV	420980	648222	88.07%	7.840%
29	15.958	2118	2122	2131	rBV	54783	89274	12.13%	1.080%
30	16.052	2134	2138	2142	rVB2	1115	1523	0.21%	0.018%
31	17.363	2357	2361	2362	rBV2	977	1131	0.15%	0.014%
32	17.574	2391	2397	2405	rVB	316265	492021	66.85%	5.951%
33	17.674	2408	2414	2422	rBV2	438355	693733	94.25%	8.391%
34	17.897	2449	2452	2454	rBV2	750	942	0.13%	0.011%
35	17.927	2454	2457	2460	rVB3	685	873	0.12%	0.011%
36	18.209	2503	2505	2509	rVB2	1034	1027	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051372.D
 Acq On : 7 Dec 2021 6:42
 Operator : CG/JU
 Sample : PB141156BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK156

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	18.438	2541	2544	2545	rVV	773	774	0.11%	0.009%
38	18.461	2545	2548	2550	rVV2	860	1087	0.15%	0.013%
39	18.520	2552	2558	2560	rBV5	1257	2165	0.29%	0.026%
40	18.585	2566	2569	2572	rBV3	1074	1459	0.20%	0.018%
41	18.644	2575	2579	2580	rBV3	1172	1083	0.15%	0.013%
42	18.720	2590	2592	2595	rBV4	789	800	0.11%	0.010%
43	18.814	2605	2608	2609	rVB3	1167	856	0.12%	0.010%
44	18.855	2613	2615	2618	rBV4	1043	1031	0.14%	0.012%
45	18.920	2625	2626	2629	rBV2	1068	867	0.12%	0.010%
46	18.978	2634	2636	2637	rBV2	1190	1011	0.14%	0.012%
47	19.014	2641	2642	2644	rBV2	1307	878	0.12%	0.011%
48	19.072	2649	2652	2655	rBV3	1990	2658	0.36%	0.032%
49	19.219	2675	2677	2679	rBV3	1511	1172	0.16%	0.014%
50	19.302	2689	2691	2693	rVV2	1015	754	0.10%	0.009%
51	19.519	2724	2728	2734	rBV4	7758	12630	1.72%	0.153%
52	19.595	2736	2741	2744	rVB2	5942	8676	1.18%	0.105%
53	19.619	2744	2745	2747	rBV2	1665	1473	0.20%	0.018%
54	19.801	2774	2776	2778	rBV3	2839	2721	0.37%	0.033%
55	19.960	2796	2803	2809	rBV	490220	736033	100.00%	8.903%
56	20.065	2819	2821	2823	rVB3	1988	840	0.11%	0.010%
57	21.881	3123	3130	3137	rVB	250784	444202	60.35%	5.373%
58	25.048	3660	3669	3683	rVB2	216104	658621	89.48%	7.966%
59	25.289	3700	3710	3720	rVB2	146909	454333	61.73%	5.495%



Sum of corrected areas: 8267663

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051372.D
Acq On : 7 Dec 2021 6:42
Operator : CG/JU
Sample : PB141156BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

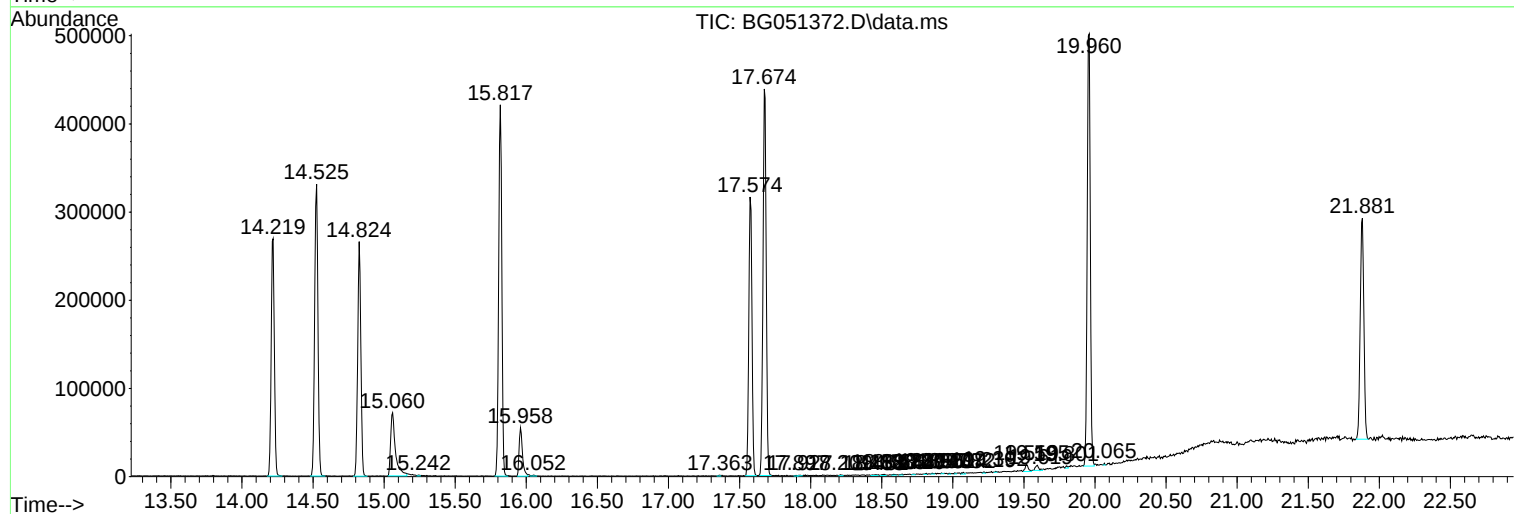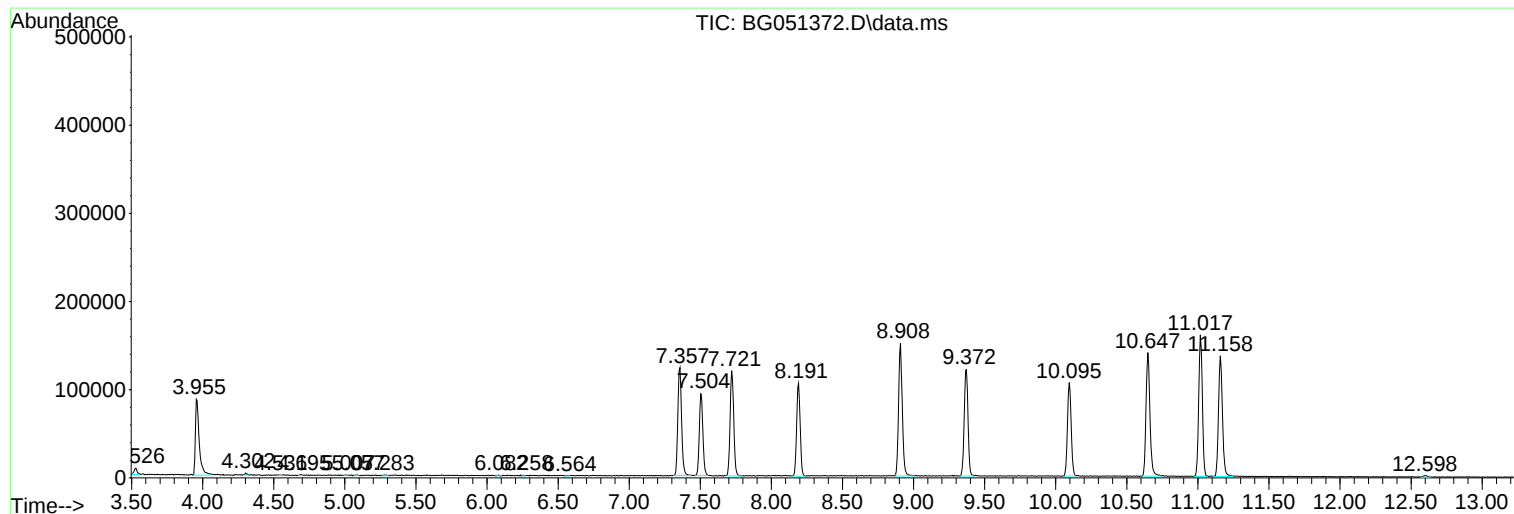

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051372.D
Acq On : 7 Dec 2021 6:42
Operator : CG/JU
Sample : PB141156BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051372.D
Acq On : 7 Dec 2021 6:42
Operator : CG/JU
Sample : PB141156BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK156

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc