

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051386.D
 Acq On : 7 Dec 2021 17:18
 Operator : CG/JU
 Sample : PB141220BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051386.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.525	3	6	14	rVB2	8738	13777	1.61%	0.159%
2	3.954	75	79	97	rBV	99078	185435	21.67%	2.145%
3	4.301	135	138	141	rVV4	1447	2066	0.24%	0.024%
4	4.630	191	194	198	rBV2	850	1183	0.14%	0.014%
5	5.447	330	333	336	rBV2	930	1036	0.12%	0.012%
6	6.040	432	434	439	rBV2	594	880	0.10%	0.010%
7	6.998	594	597	600	rBV2	866	1263	0.15%	0.015%
8	7.350	650	657	666	rBV	134262	244774	28.60%	2.832%
9	7.503	677	683	691	rBV	106755	181569	21.22%	2.101%
10	7.721	711	720	732	rBV	130401	235210	27.49%	2.721%
11	8.191	793	800	808	rBV	90151	153973	17.99%	1.781%
12	8.901	914	921	936	rBV	164117	301317	35.21%	3.486%
13	9.366	993	1000	1010	rBV	133983	244573	28.58%	2.830%
14	10.094	1117	1124	1135	rBV	118378	212730	24.86%	2.461%
15	10.647	1211	1218	1232	rBV	145871	294290	34.39%	3.405%
16	11.017	1273	1281	1291	rVB	130865	237463	27.75%	2.747%
17	11.158	1297	1305	1316	rBV	163557	324779	37.95%	3.757%
18	12.603	1543	1551	1556	rVB3	2119	4502	0.53%	0.052%
19	14.213	1819	1825	1836	rVB	304535	453526	53.00%	5.247%
20	14.518	1870	1877	1888	rBV	348475	563316	65.83%	6.517%
21	14.824	1922	1929	1938	rVB	209874	339589	39.68%	3.929%
22	15.053	1962	1968	1986	rBV2	76580	177732	20.77%	2.056%
23	15.229	1996	1998	2002	rVB3	787	875	0.10%	0.010%
24	15.811	2090	2097	2105	rBV	438828	687704	80.36%	7.956%
25	15.952	2116	2121	2135	rBV	82717	140964	16.47%	1.631%
26	16.052	2135	2138	2142	rVB3	1692	2138	0.25%	0.025%
27	17.356	2353	2360	2364	rVB2	724	1339	0.16%	0.015%
28	17.574	2390	2397	2404	rBV	274030	411367	48.07%	4.759%
29	17.674	2407	2414	2423	rVV	515326	768300	89.78%	8.889%
30	17.956	2457	2462	2464	rBV2	647	986	0.12%	0.011%
31	19.513	2723	2727	2733	rBV2	6526	9962	1.16%	0.115%
32	19.589	2736	2740	2746	rVB	5605	8600	1.00%	0.099%
33	19.677	2752	2755	2757	rVB3	1178	925	0.11%	0.011%
34	19.889	2787	2791	2793	rBV3	1506	1865	0.22%	0.022%
35	19.912	2793	2795	2796	rVV2	1146	943	0.11%	0.011%
36	19.953	2796	2802	2814	rVV	605731	855728	100.00%	9.900%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051386.D
 Acq On : 7 Dec 2021 17:18
 Operator : CG/JU
 Sample : PB141220BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK220

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	20.083	2820	2824	2826	rVB4	1079	1191	0.14%	0.014%
38	20.235	2847	2850	2853	rBV5	1294	1899	0.22%	0.022%
39	20.341	2864	2868	2869	rBV3	1013	1345	0.16%	0.016%
40	20.423	2880	2882	2883	rBV	1133	1033	0.12%	0.012%
41	20.441	2883	2885	2887	rVV3	1294	1228	0.14%	0.014%
42	20.459	2887	2888	2890	rVB2	1797	1067	0.12%	0.012%
43	20.476	2890	2891	2895	rBV3	1904	2322	0.27%	0.027%
44	20.523	2895	2899	2900	rBV3	1967	2293	0.27%	0.027%
45	20.835	2950	2952	2956	rVB4	1843	1817	0.21%	0.021%
46	21.046	2987	2988	2990	rBV2	2151	1603	0.19%	0.019%
47	21.640	3087	3089	3090	rBV2	2129	1321	0.15%	0.015%
48	21.875	3122	3129	3137	rVB	224427	388194	45.36%	4.491%
49	22.903	3302	3304	3308	rBV4	2270	1856	0.22%	0.021%
50	24.489	3572	3574	3575	rBV2	2319	1564	0.18%	0.018%
51	25.041	3656	3668	3680	rBV2	250466	747693	87.38%	8.650%
52	25.200	3689	3695	3697	rBV7	8527	15877	1.86%	0.184%
53	25.271	3697	3707	3717	rVB3	122281	372600	43.54%	4.311%
54	25.600	3761	3763	3764	rVB2	2711	1380	0.16%	0.016%
55	26.187	3860	3863	3864	rBV3	2688	3188	0.37%	0.037%
56	26.381	3891	3896	3902	rBV6	8890	20048	2.34%	0.232%
57	26.481	3912	3913	3915	rBV2	2628	2247	0.26%	0.026%
58	28.179	4200	4202	4204	rBV3	2724	1929	0.23%	0.022%
59	28.602	4273	4274	4276	rBV2	2996	1696	0.20%	0.020%
60	30.594	4611	4613	4616	rBV4	2334	1589	0.19%	0.018%




Sum of corrected areas: 8643659

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051386.D
Acq On : 7 Dec 2021 17:18
Operator : CG/JU
Sample : PB141220BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

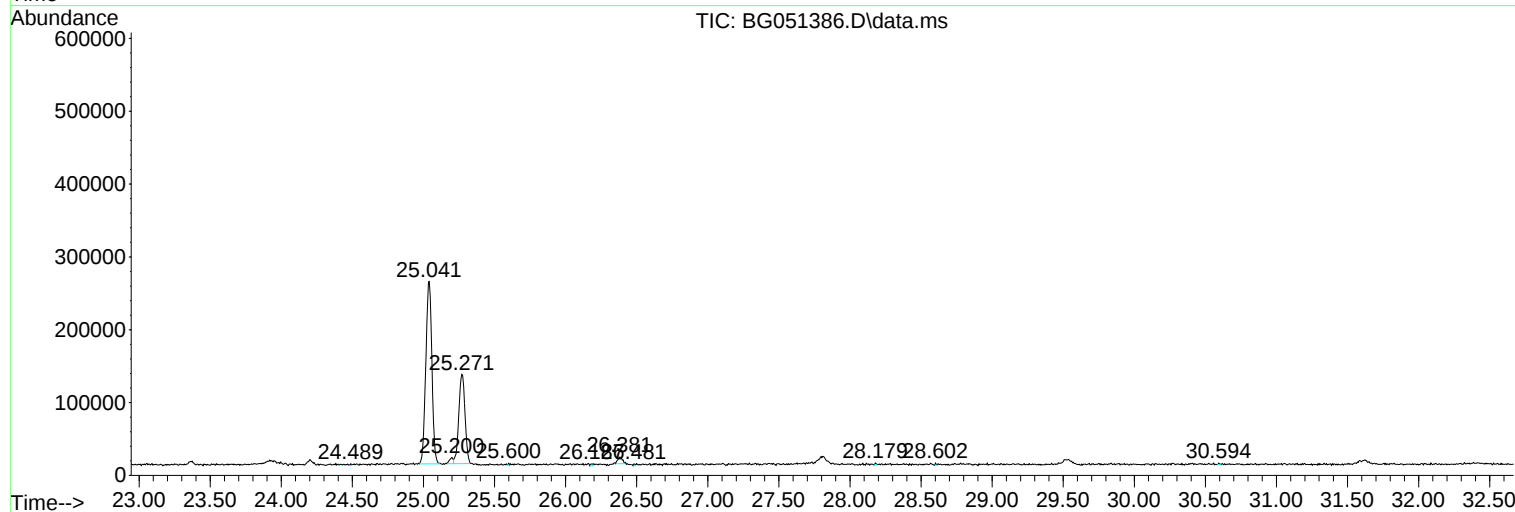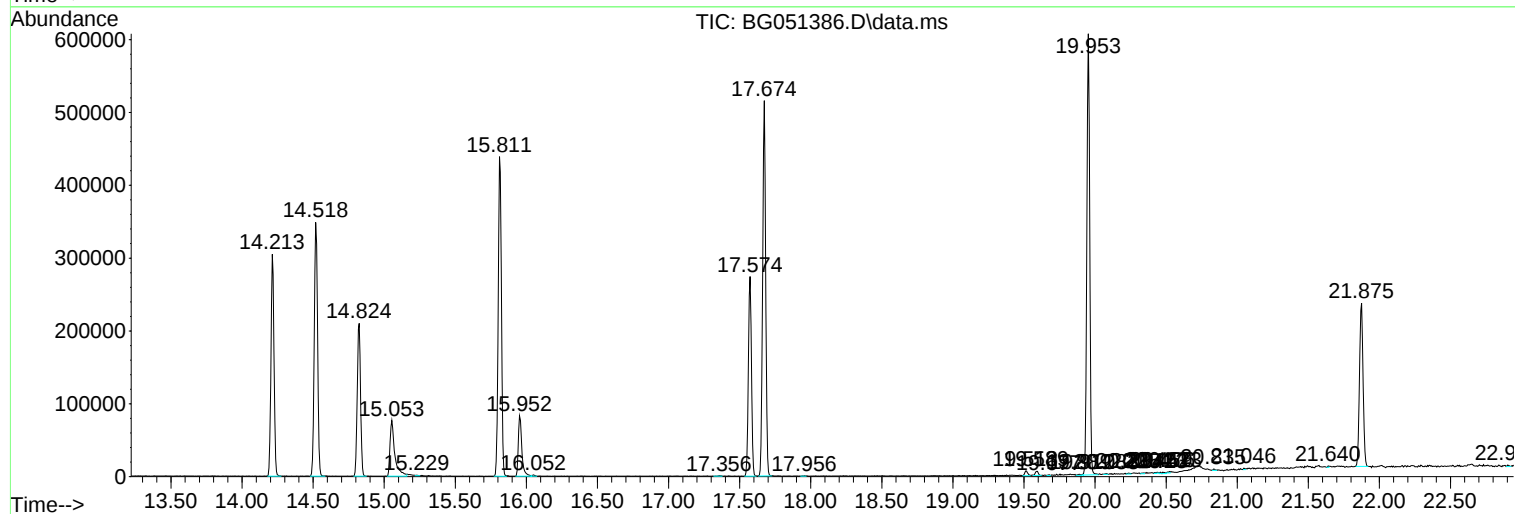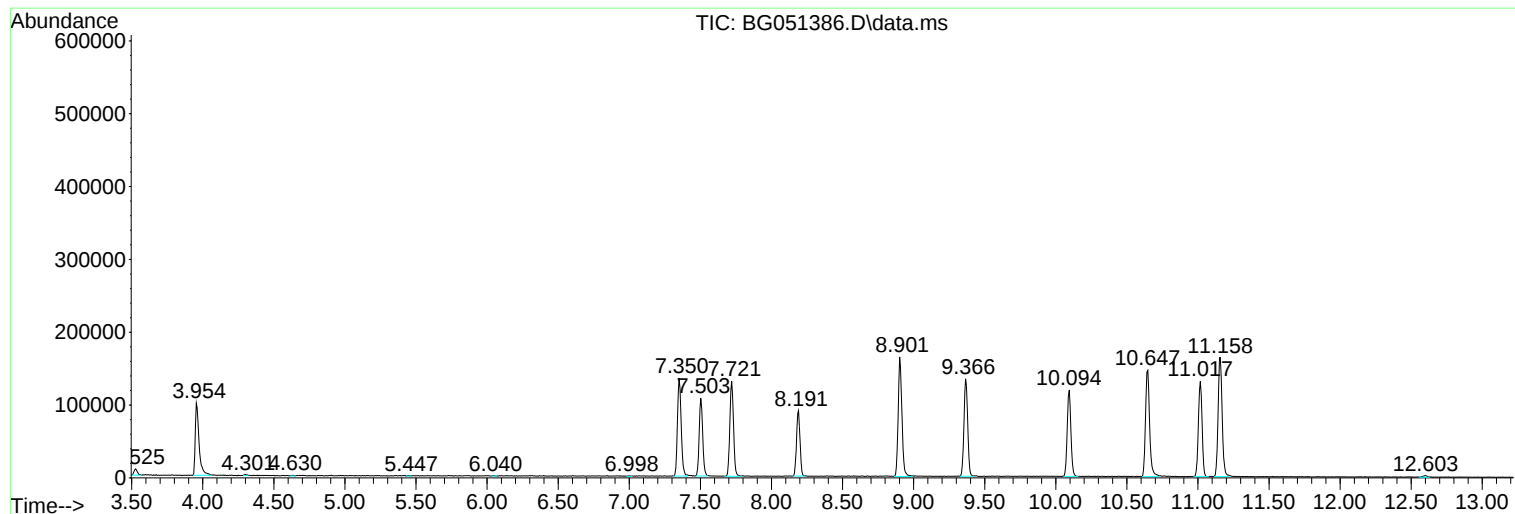

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051386.D
Acq On : 7 Dec 2021 17:18
Operator : CG/JU
Sample : PB141220BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051386.D
Acq On : 7 Dec 2021 17:18
Operator : CG/JU
Sample : PB141220BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc