

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051405.D
 Acq On : 8 Dec 2021 12:33
 Operator : CG/JU
 Sample : M4960-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.526	3	6	17	rVB3	3210	5460	1.30%	0.118%
2	3.967	78	81	88	rBV	11985	23051	5.49%	0.500%
3	4.067	95	98	103	rVB4	1645	2367	0.56%	0.051%
4	4.190	114	119	125	rVB3	3762	6617	1.58%	0.144%
5	4.537	176	178	182	rVV2	716	654	0.16%	0.014%
6	4.989	252	255	256	rBV	619	698	0.17%	0.015%
7	5.230	292	296	298	rBV4	1503	2266	0.54%	0.049%
8	5.430	328	330	333	rVB	597	666	0.16%	0.014%
9	5.494	339	341	344	rVB3	725	714	0.17%	0.015%
10	5.724	377	380	382	rBV2	553	650	0.15%	0.014%
11	6.546	519	520	523	rBV	808	634	0.15%	0.014%
12	7.022	599	601	604	rVB	674	666	0.16%	0.014%
13	7.357	651	658	670	rVB	47019	91645	21.83%	1.988%
14	7.504	677	683	689	rBV	35297	60321	14.37%	1.309%
15	7.721	714	720	727	rBV	45991	80787	19.24%	1.753%
16	7.768	727	728	732	rVB	963	858	0.20%	0.019%
17	7.986	761	765	768	rBV3	882	1445	0.34%	0.031%
18	8.033	771	773	779	rVB2	518	827	0.20%	0.018%
19	8.091	779	783	785	rBV2	620	702	0.17%	0.015%
20	8.185	793	799	810	rVB	82855	143911	34.28%	3.123%
21	8.632	872	875	877	rBV2	555	642	0.15%	0.014%
22	8.702	885	887	891	rBV2	454	658	0.16%	0.014%
23	8.908	916	922	930	rBV	54079	98756	23.52%	2.143%
24	9.026	938	942	948	rVB3	2868	4424	1.05%	0.096%
25	9.255	979	981	984	rBV2	678	806	0.19%	0.017%
26	9.366	994	1000	1009	rVV	46803	83491	19.89%	1.812%
27	9.513	1021	1025	1027	rVB	472	726	0.17%	0.016%
28	9.701	1053	1057	1061	rBV4	1359	2281	0.54%	0.049%
29	10.095	1118	1124	1132	rVV2	37663	70423	16.77%	1.528%
30	10.647	1212	1218	1228	rVV	47105	98212	23.39%	2.131%
31	10.776	1238	1240	1243	rBV2	750	755	0.18%	0.016%
32	11.017	1273	1281	1289	rBV	120320	215142	51.24%	4.668%
33	11.158	1298	1305	1317	rVB3	47443	113858	27.12%	2.470%
34	12.586	1546	1548	1549	rVV2	966	802	0.19%	0.017%
35	13.315	1670	1672	1677	rVB2	643	883	0.21%	0.019%
36	13.409	1682	1688	1692	rBV4	1481	2003	0.48%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051405.D
 Acq On : 8 Dec 2021 12:33
 Operator : CG/JU
 Sample : M4960-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

37	13.608	1718	1722	1726	rVB4	1362	1886	0.45%	0.041%
38	13.661	1728	1731	1733	rVV2	673	667	0.16%	0.014%
39	13.685	1733	1735	1739	rVB3	698	697	0.17%	0.015%
40	13.761	1746	1748	1752	rVB3	575	679	0.16%	0.015%
41	14.137	1807	1812	1816	rBV	634	1038	0.25%	0.023%
42	14.214	1819	1825	1831	rVV	116689	167588	39.91%	3.636%
43	14.437	1857	1863	1868	rVV5	2619	5167	1.23%	0.112%
44	14.519	1868	1877	1884	rVV	134548	212388	50.58%	4.608%
45	14.678	1900	1904	1909	rVB3	1555	2782	0.66%	0.060%
46	14.819	1922	1928	1940	rVB	195014	313902	74.76%	6.811%
47	14.936	1943	1948	1949	rBV3	419	727	0.17%	0.016%
48	14.972	1951	1954	1956	rVB	770	677	0.16%	0.015%
49	15.001	1956	1959	1960	rBV2	863	725	0.17%	0.016%
50	15.066	1964	1970	1981	rBV	26118	63822	15.20%	1.385%
51	15.142	1981	1983	1985	rVV2	3015	3174	0.76%	0.069%
52	15.183	1988	1990	1991	rVV2	1561	1296	0.31%	0.028%
53	15.207	1991	1994	1995	rVV3	1149	1147	0.27%	0.025%
54	15.242	1995	2000	2005	rVV5	4098	6411	1.53%	0.139%
55	15.283	2005	2007	2010	rVV3	792	670	0.16%	0.015%
56	15.312	2010	2012	2014	rVB2	1165	815	0.19%	0.018%
57	15.342	2014	2017	2020	rBV2	915	1108	0.26%	0.024%
58	15.442	2032	2034	2037	rBV2	1053	1030	0.25%	0.022%
59	15.577	2052	2057	2060	rBV4	2970	4832	1.15%	0.105%
60	15.624	2060	2065	2069	rVV5	2406	4110	0.98%	0.089%
61	15.765	2086	2089	2090	rVV3	1102	1019	0.24%	0.022%
62	15.812	2090	2097	2105	rVV	179072	272686	64.95%	5.917%
63	15.871	2105	2107	2110	rVB3	623	657	0.16%	0.014%
64	15.900	2110	2112	2115	rBV2	698	844	0.20%	0.018%
65	15.953	2115	2121	2129	rVV2	21492	35737	8.51%	0.775%
66	16.023	2131	2133	2135	rVV3	1522	1487	0.35%	0.032%
67	16.053	2137	2138	2140	rVV	1567	1037	0.25%	0.023%
68	16.106	2144	2147	2148	rVB3	881	872	0.21%	0.019%
69	16.129	2148	2151	2152	rBV3	1168	1079	0.26%	0.023%
70	16.153	2152	2155	2157	rVV3	1411	1430	0.34%	0.031%
71	16.188	2159	2161	2163	rVV	1333	1079	0.26%	0.023%
72	16.211	2163	2165	2166	rVB	1125	728	0.17%	0.016%
73	16.241	2166	2170	2175	rBV6	998	2306	0.55%	0.050%
74	16.317	2181	2183	2184	rBV	1089	634	0.15%	0.014%
75	16.376	2189	2193	2194	rBV2	1380	1443	0.34%	0.031%
76	16.423	2197	2201	2203	rBV4	1235	1938	0.46%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
 Data File : BG051405.D
 Acq On : 8 Dec 2021 12:33
 Operator : CG/JU
 Sample : M4960-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
 Title : SVOA CALIBRATION

77	16.458	2206	2207	2208	rBV	964	629	0.15%	0.014%
78	16.482	2209	2211	2212	rBV	1273	873	0.21%	0.019%
79	16.623	2232	2235	2236	rBV3	1438	1383	0.33%	0.030%
80	16.681	2242	2245	2248	rBV5	1772	2350	0.56%	0.051%
81	16.705	2248	2249	2253	rVB4	1400	957	0.23%	0.021%
82	16.893	2277	2281	2284	rVB5	1646	1560	0.37%	0.034%
83	17.022	2299	2303	2306	rVV6	1903	2197	0.52%	0.048%
84	17.110	2315	2318	2320	rBV4	1324	1556	0.37%	0.034%
85	17.151	2323	2325	2328	rBV4	1527	1742	0.41%	0.038%
86	17.275	2341	2346	2348	rBV5	4156	6155	1.47%	0.134%
87	17.439	2370	2374	2379	rVB6	5483	7620	1.81%	0.165%
88	17.504	2383	2385	2386	rBV2	1395	1077	0.26%	0.023%
89	17.574	2390	2397	2403	rVV	247456	395311	94.15%	8.577%
90	17.674	2407	2414	2420	rVV	211260	337293	80.33%	7.319%
91	17.751	2424	2427	2430	rVV5	4815	5431	1.29%	0.118%
92	17.927	2453	2457	2459	rBV5	3250	4439	1.06%	0.096%
93	18.321	2522	2524	2525	rBV2	2715	1668	0.40%	0.036%
94	18.808	2605	2607	2608	rBV2	4337	3507	0.84%	0.076%
95	19.008	2639	2641	2644	rBV4	4182	4214	1.00%	0.091%
96	19.954	2796	2802	2810	rBV	268955	419869	100.00%	9.110%
97	21.705	3097	3100	3111	rVB	45147	77505	18.46%	1.682%
98	21.875	3123	3129	3140	rVB	218757	400262	95.33%	8.685%
99	25.042	3660	3668	3677	rBV2	112555	314055	74.80%	6.814%
100	25.277	3700	3708	3718	rVB2	125406	375984	89.55%	8.158%




Sum of corrected areas: 4608752

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051405.D
Acq On : 8 Dec 2021 12:33
Operator : CG/JU
Sample : M4960-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

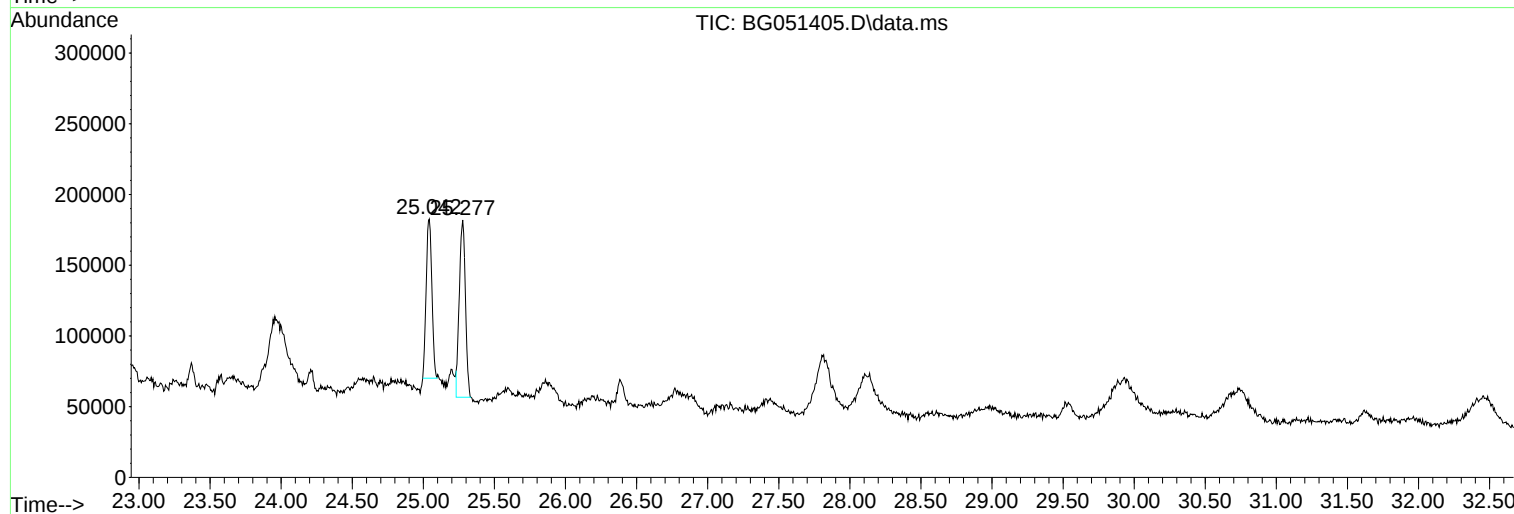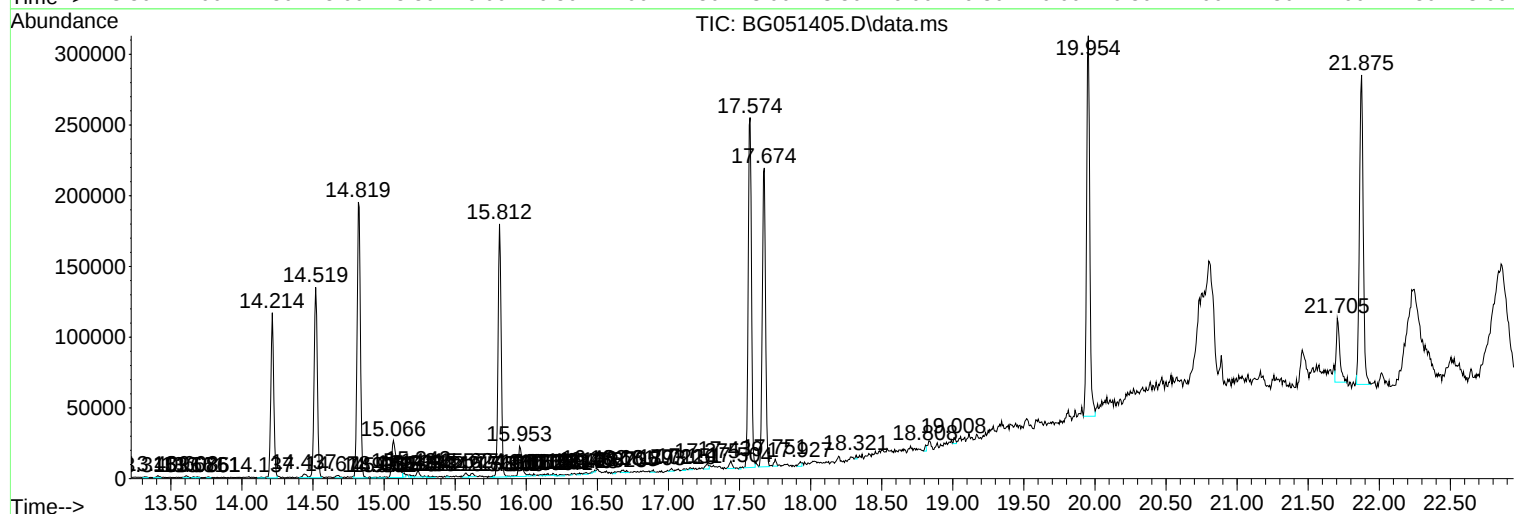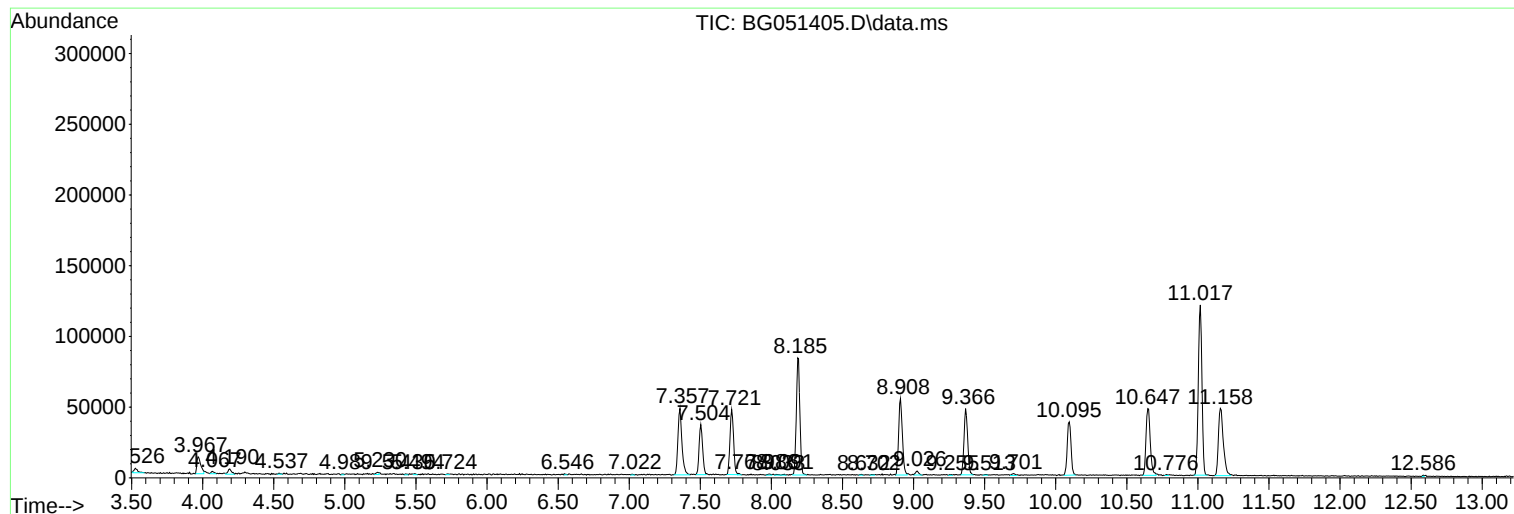

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051405.D
Acq On : 8 Dec 2021 12:33
Operator : CG/JU
Sample : M4960-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120621\
Data File : BG051405.D
Acq On : 8 Dec 2021 12:33
Operator : CG/JU
Sample : M4960-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc