
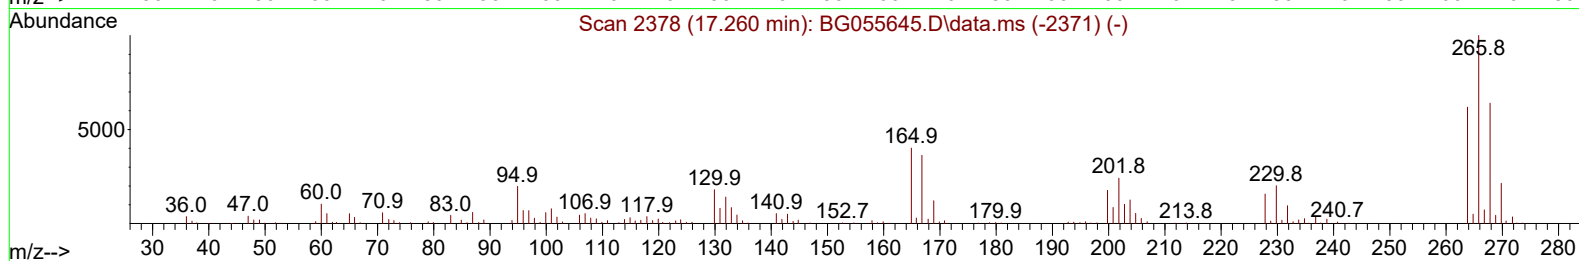
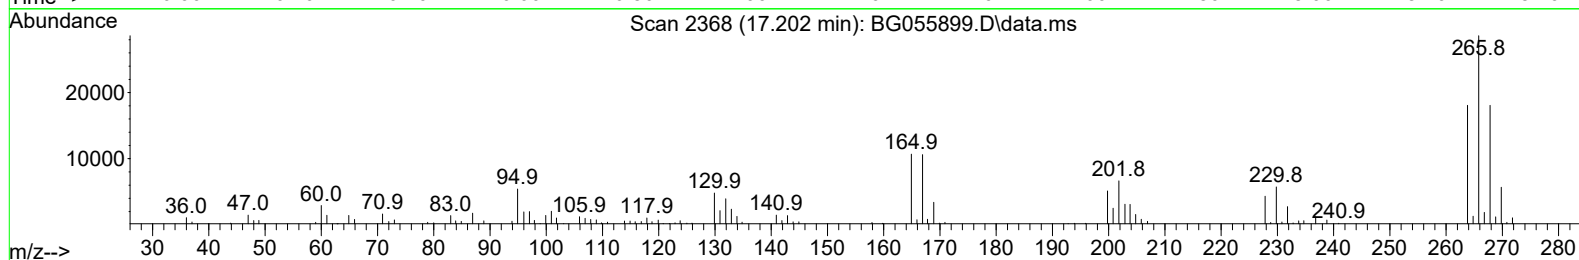


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120622\
Data File : BG055899.D
Acq On : 6 Dec 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:20:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

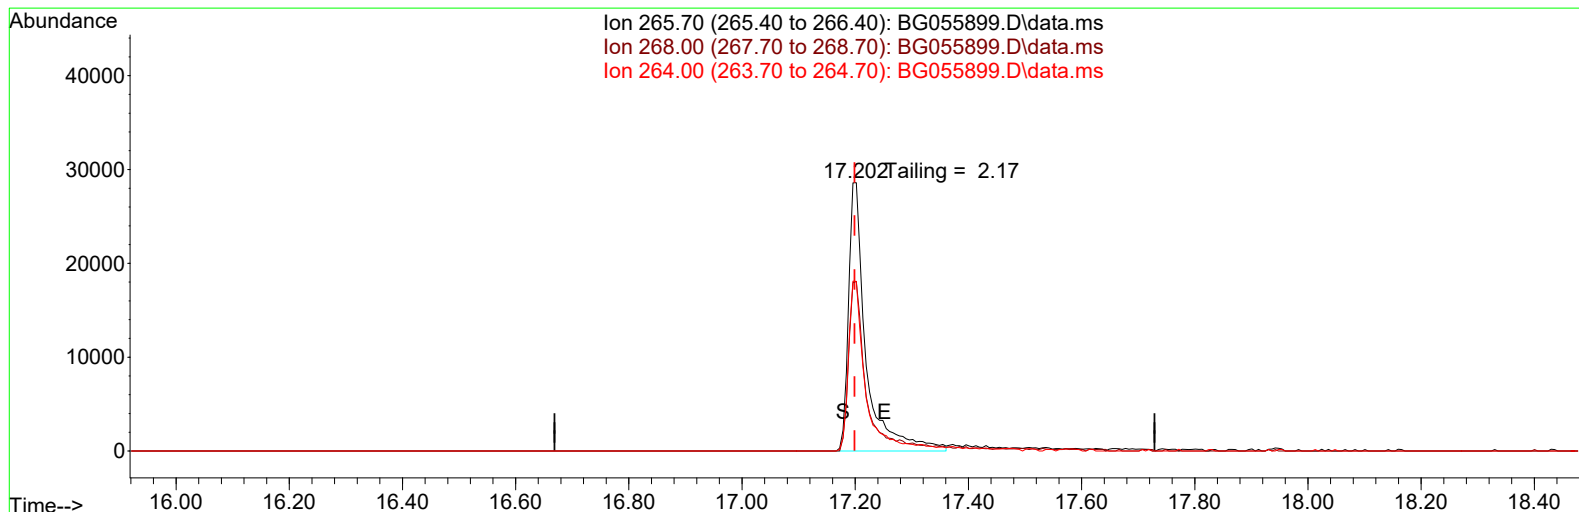

TIC: BG055899.D\data.ms

(70) Pentachlorophenol (C)




17.202min (+ 0.003) 19887.15 ng

response 62248

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.22
264.00	61.90	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120622\
Data File : BG055899.D
Acq On : 6 Dec 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 06:22:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

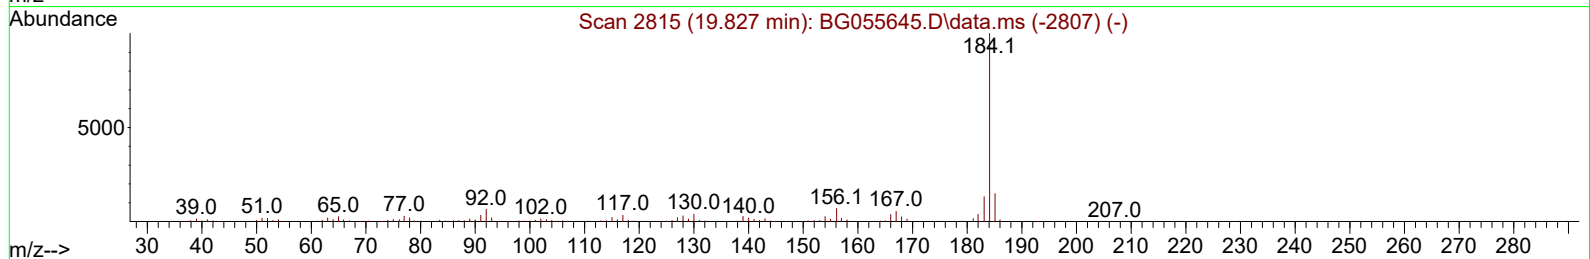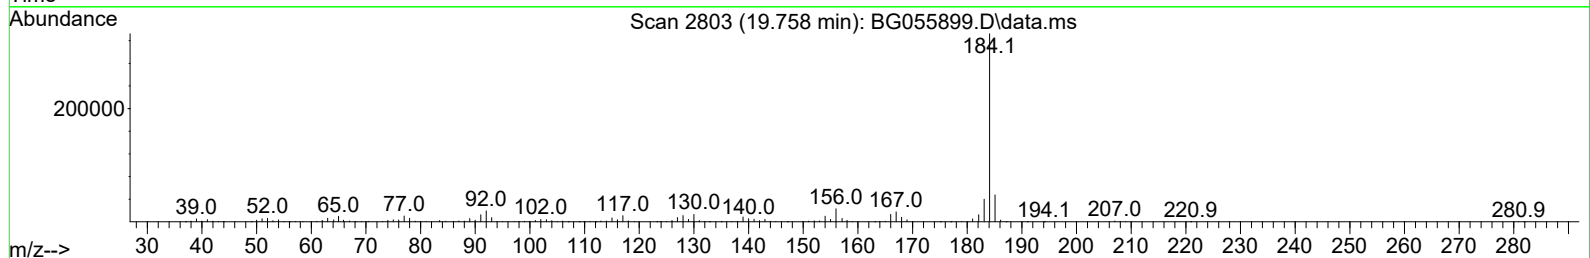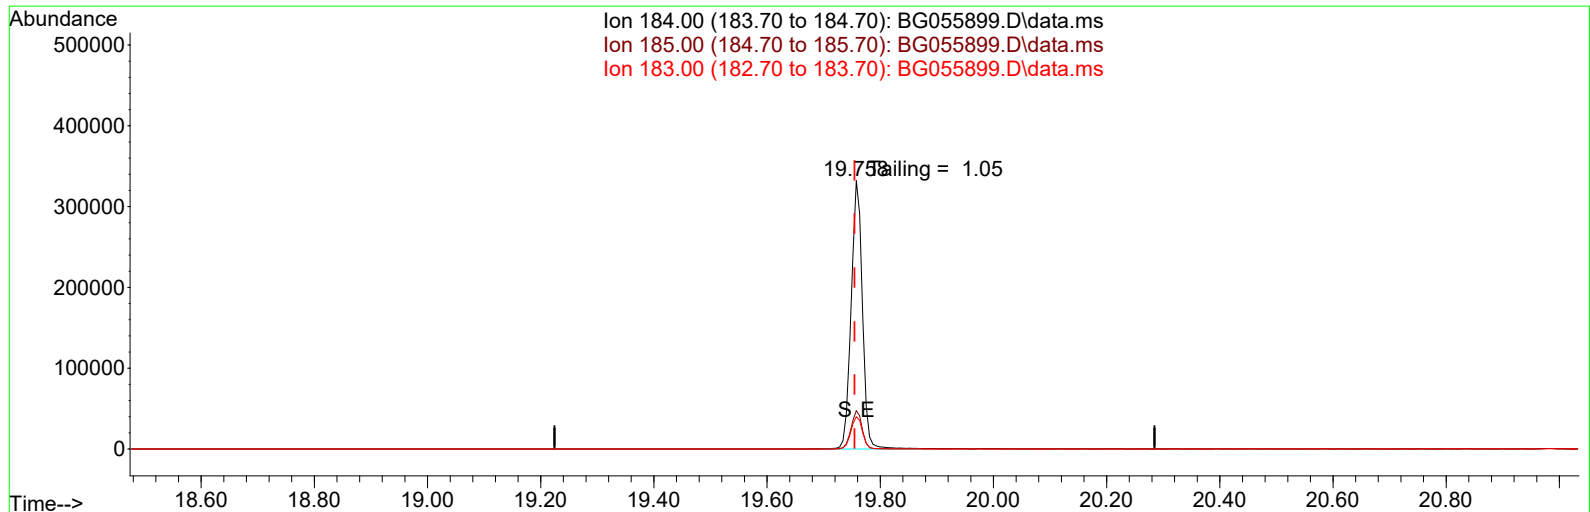

TIC: BG055899.D\data.ms

(77) Benzidine**19.758min (+ 0.003) 0.00 ng****response 461262**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.34
183.00	13.20	12.09
0.00	0.00	0.00