


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120622\
Data File : BG055899.D
Acq On : 6 Dec 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 07 05:04:10 2022

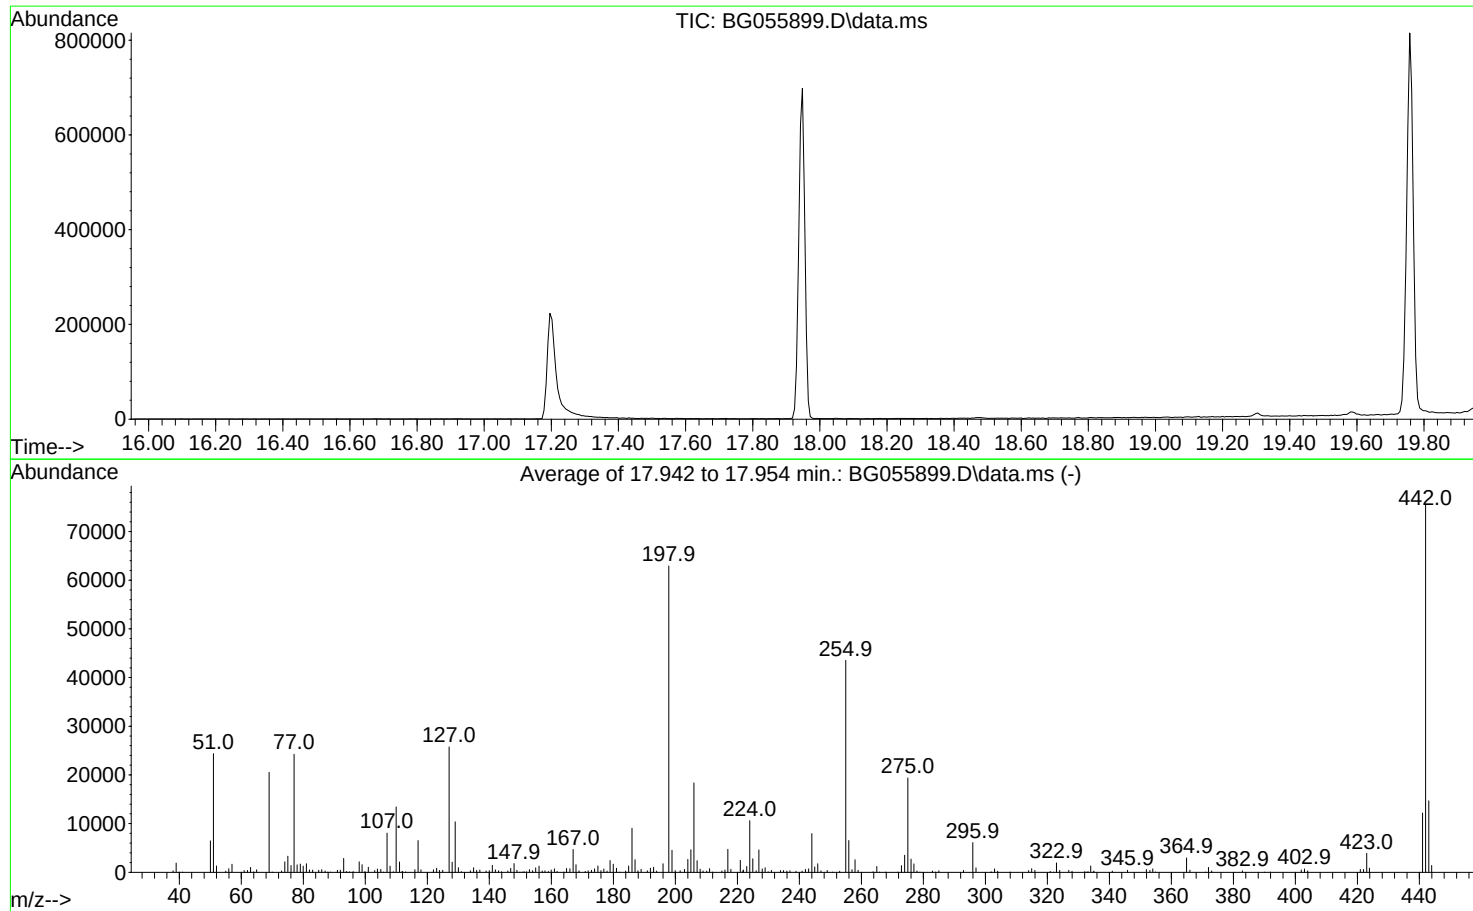




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	24377	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	20526	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	40.9	25749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62939	PASS
199	198	5	9	7.2	4509	PASS
275	198	10	60	30.8	19362	PASS
365	198	1	100	4.7	2959	PASS
441	198	0.01	100	19.4	12179	PASS
442	442	50	100	100.0	75563	PASS
443	442	15	24	19.4	14671	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120622\
Data File : BG055899.D
Acq On : 6 Dec 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 07 06:20:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

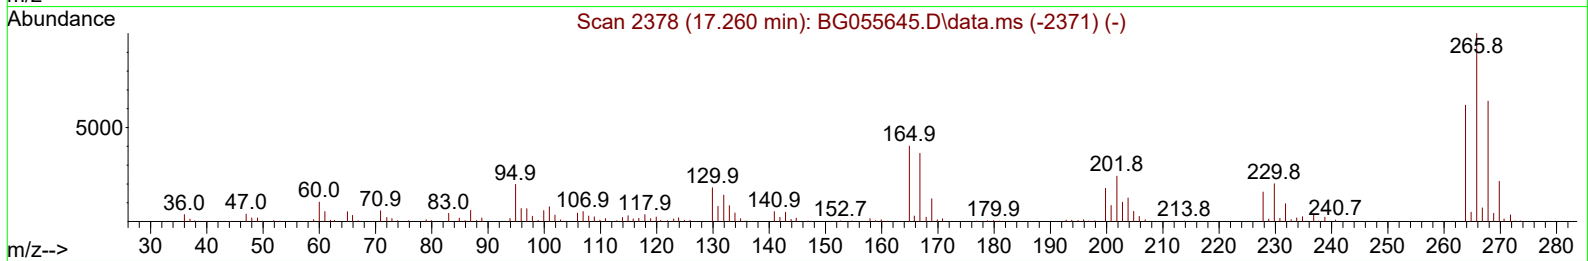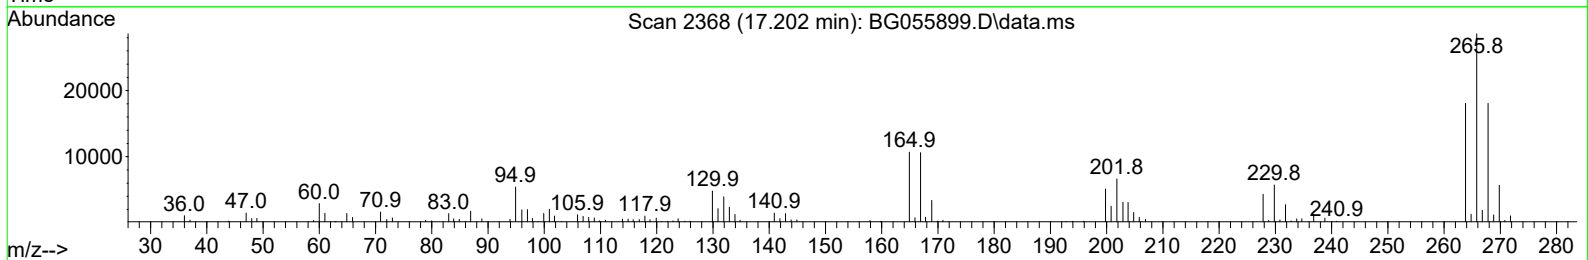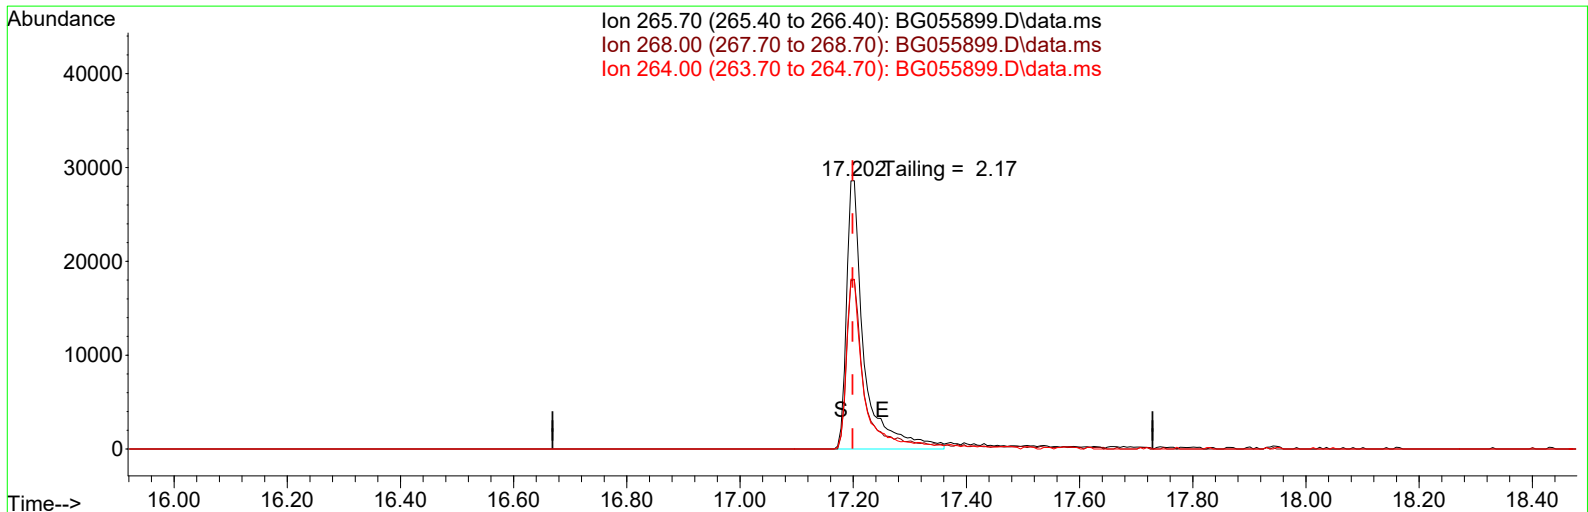

TIC: BG055899.D\data.ms

(70) Pentachlorophenol (C)

17.202min (+ 0.003) 19887.15 ng




response 62248

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.22
264.00	61.90	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120622\
Data File : BG055899.D
Acq On : 6 Dec 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 07 06:22:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

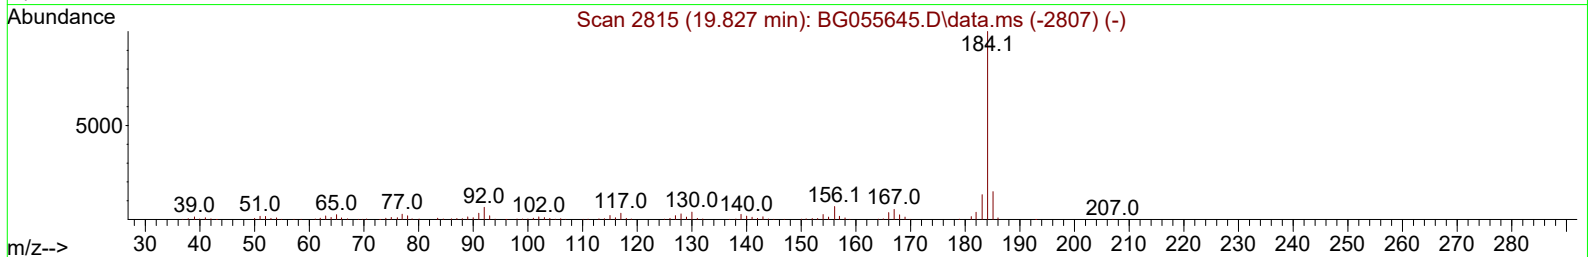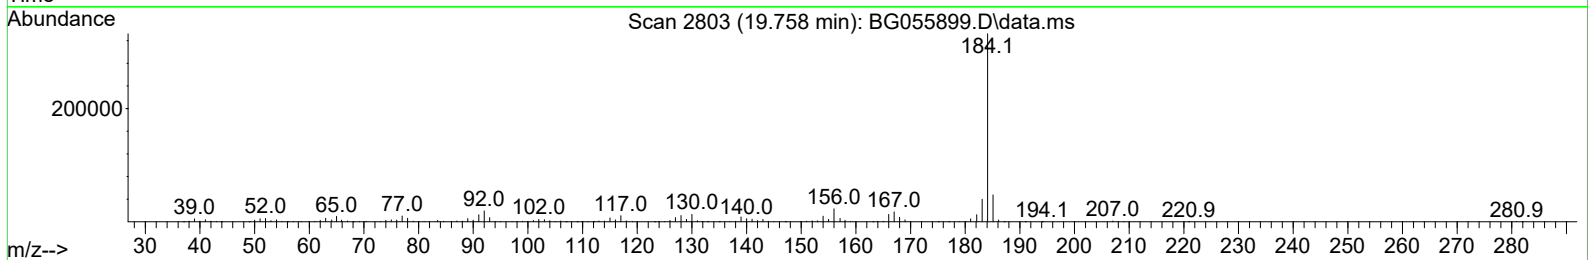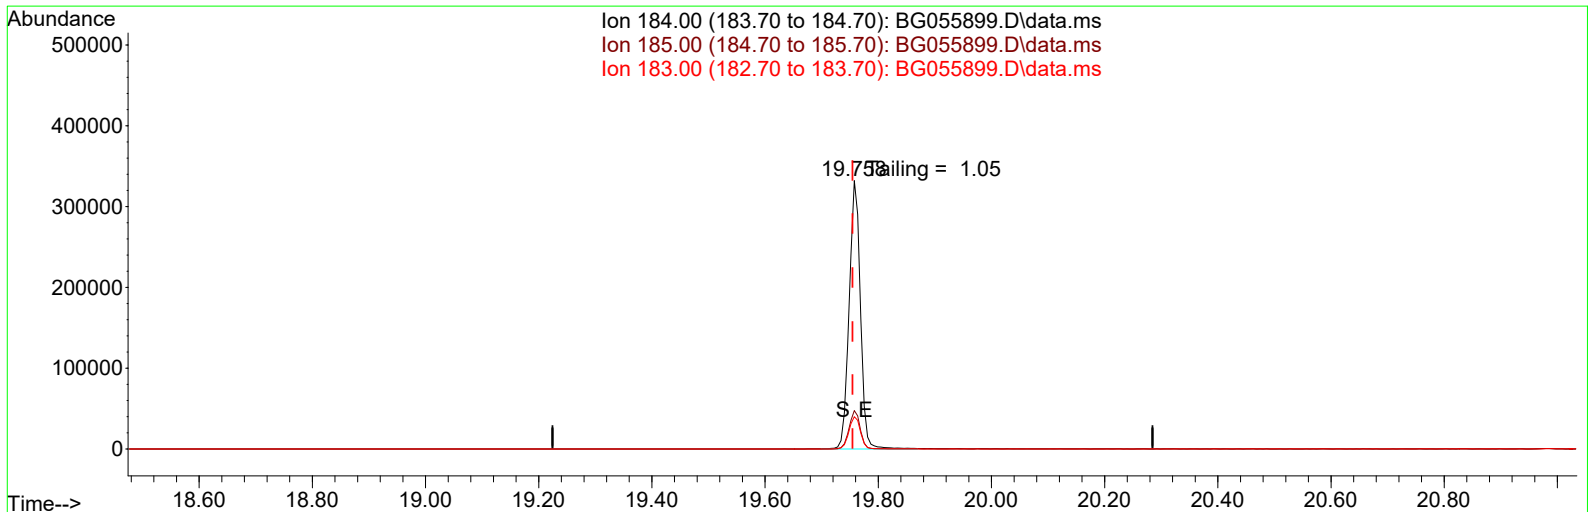

TIC: BG055899.D\data.ms

(77) Benzidine

19.758min (+ 0.003) 0.00 ng

response 461262

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.34
183.00	13.20	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2022	BNA_G	<u>BG055899.D</u>
Compound Name	Response	Retention Time
DDT	199700	20.986
DDD	3874	20.586
DDE	462	20.046
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4336	204036	2.13

Instrument :
BNA_G
ClientSampleId :
DFTPP