

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120715\
 Data File : BG019980.D
 Acq On : 7 Dec 2015 14:13
 Operator : UM/NP
 Sample : PB87054BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB87054BL

Quant Time: Dec 08 00:05:49 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	19444	20.00	ng	-0.02
21) Naphthalene-d8	10.93	136	85095	20.00	ng	-0.02
38) Acenaphthene-d10	14.74	164	62876	20.00	ng	-0.02
63) Phenanthrene-d10	17.49	188	161157	20.00	ng	-0.02
75) Chrysene-d12	21.76	240	194640	20.00	ng	-0.03
86) Perylene-d12	25.04	264	179766	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	132911	123.54	ng	-0.01
7) Phenol-d6	7.26	99	196936	121.24	ng	-0.01
23) Nitrobenzene-d5	9.28	82	127712	76.59	ng	-0.02
41) 2,4,6-Tribromophenol	16.23	330	99353	103.27	ng	-0.02
44) 2-Fluorobiphenyl	13.37	172	327444	71.11	ng	-0.02
78) Terphenyl-d14	20.09	244	584243	73.22	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120715\
Data File : BG019980.D
Acq On : 7 Dec 2015 14:13
Operator : UM/NP
Sample : PB87054BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB87054BL

Quant Time: Dec 08 00:05:49 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

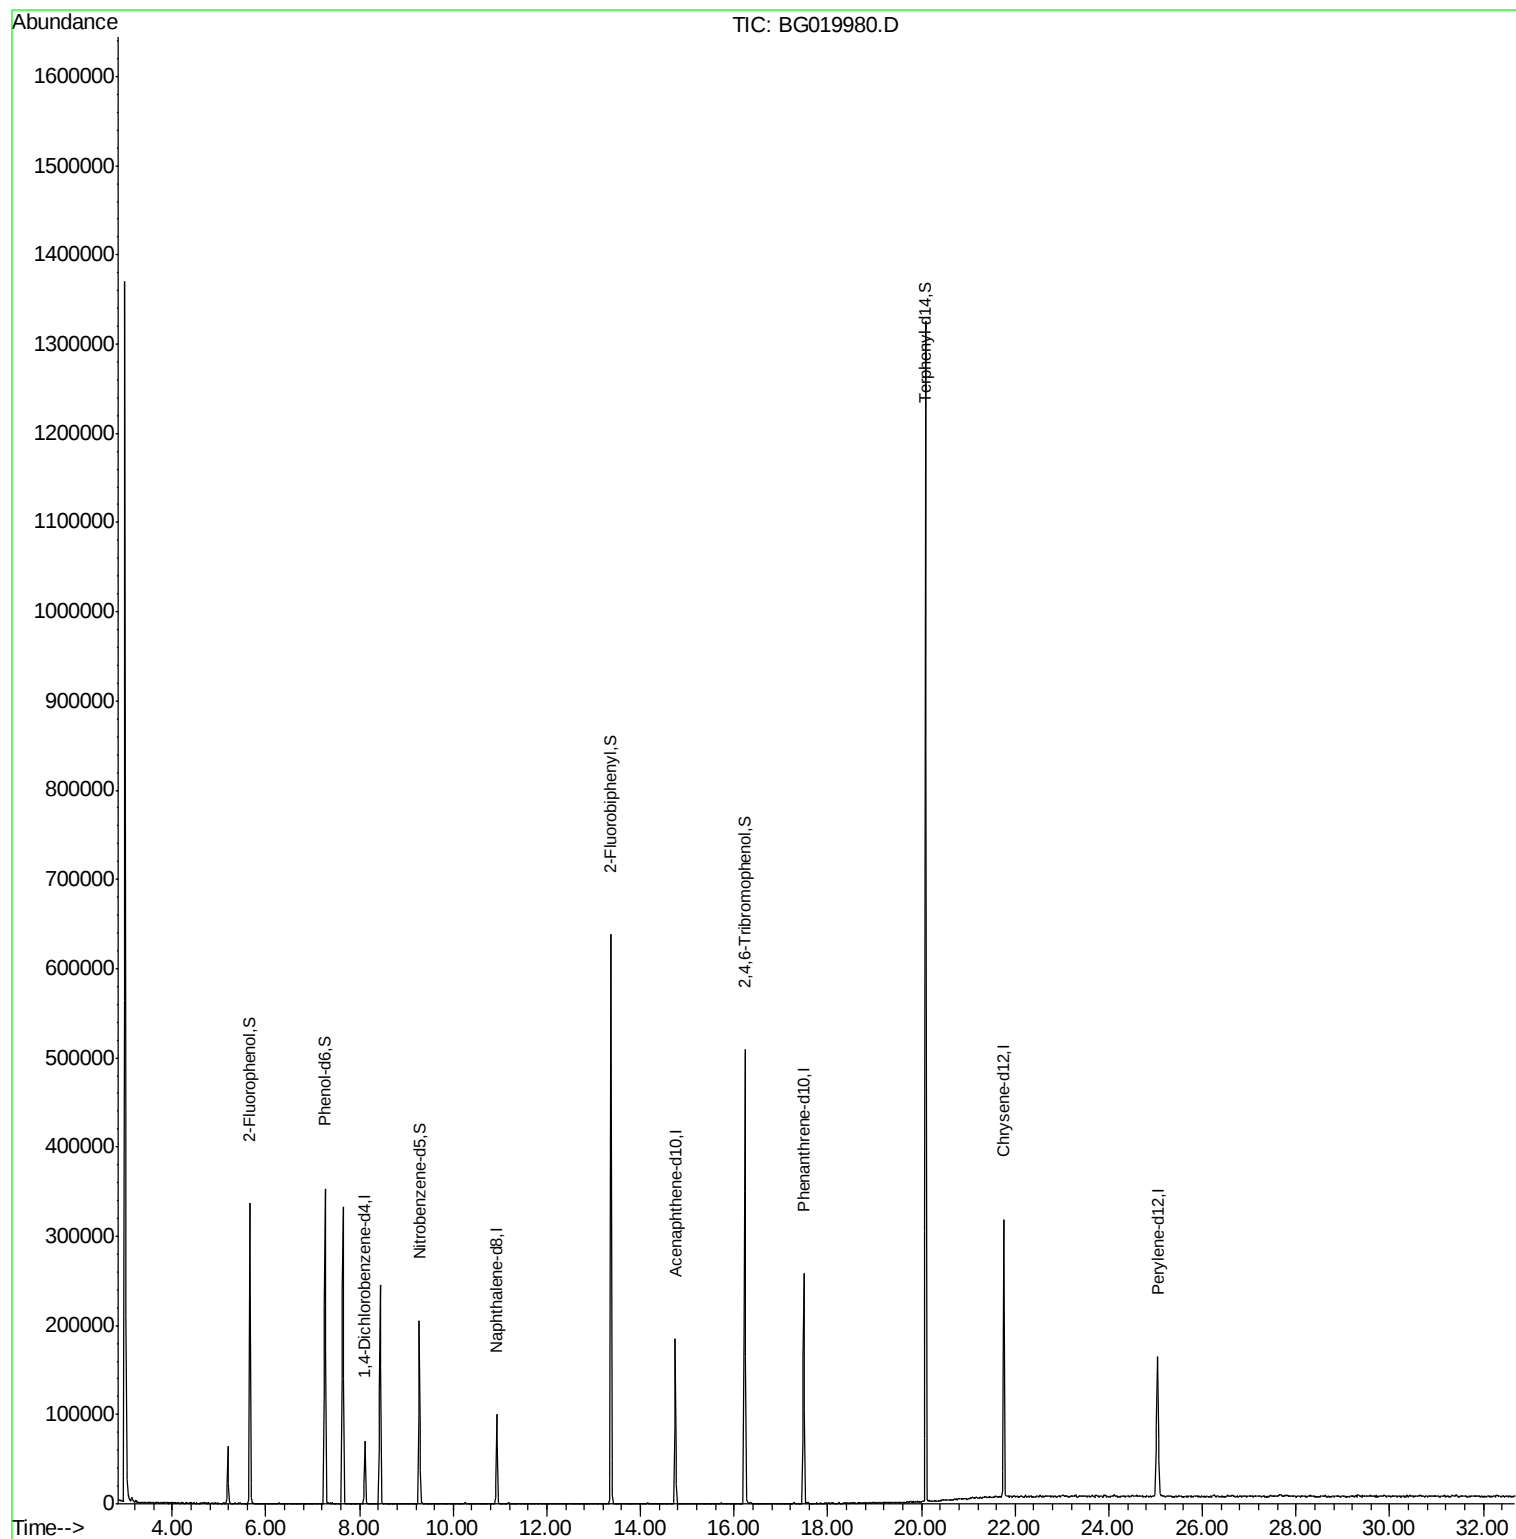

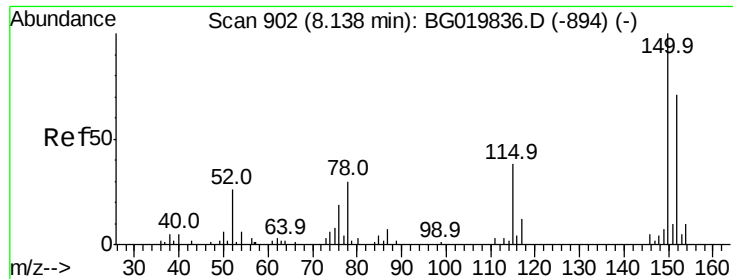

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.11 min Scan# 898

Delta R.T. -0.02 min

Lab File: BG019980.D

Acq: 7 Dec 2015 14:13

Instrument :

BNA_G

ClientSampleID :

PB87054BL


Tot Ion:152 Resp: 19444

Ion Ratio Lower Upper

152 100

150 154.3 115.0 172.4




115 60.5 43.9 65.9

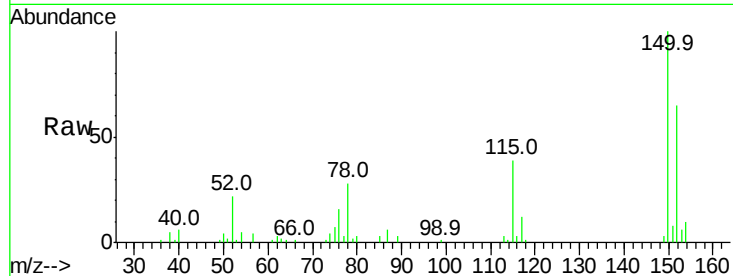

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

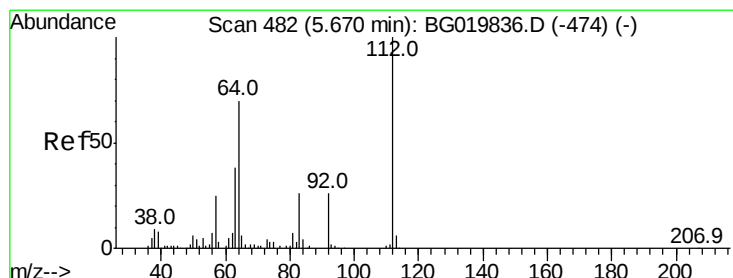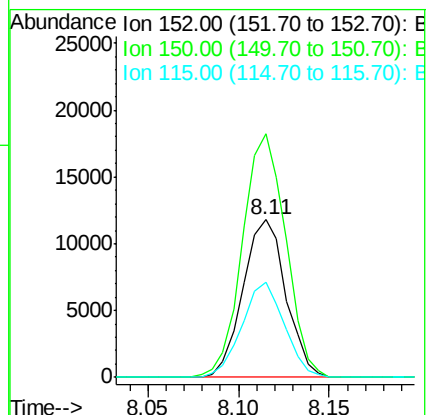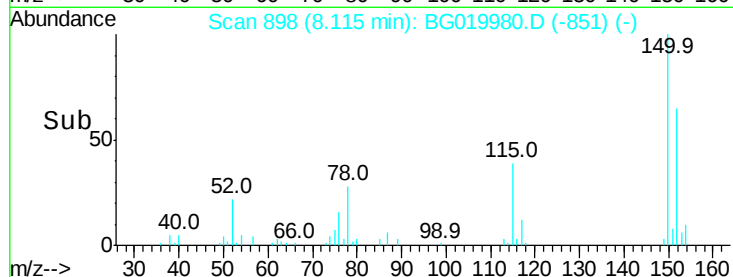

#5

2-Fluorophenol

Concen: 123.54 ng

RT: 5.66 min Scan# 480

Delta R.T. -0.01 min

Lab File: BG019980.D

Acq: 7 Dec 2015 14:13


Tgt Ion:112 Resp: 132911

Ion Ratio Lower Upper

112 100

64 67.8 43.7 65.5#



63 37.3 24.0 36.0#

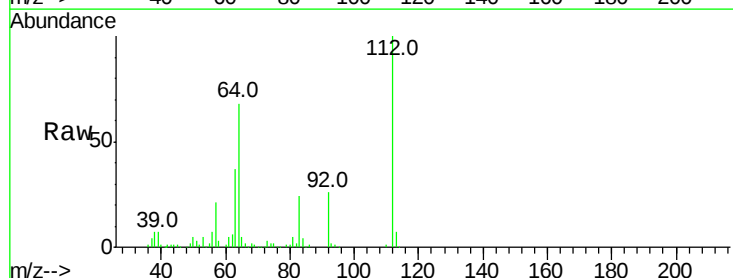


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

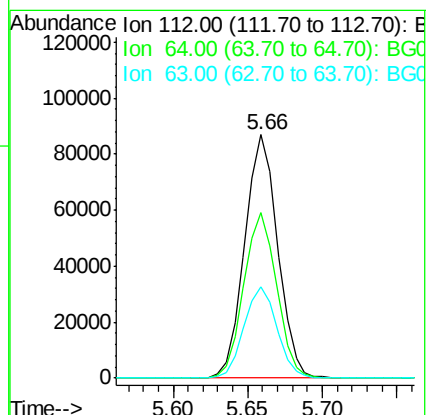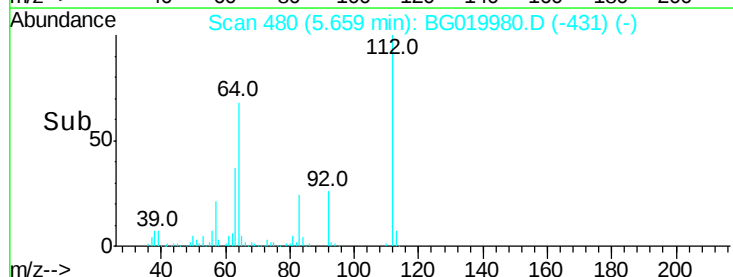

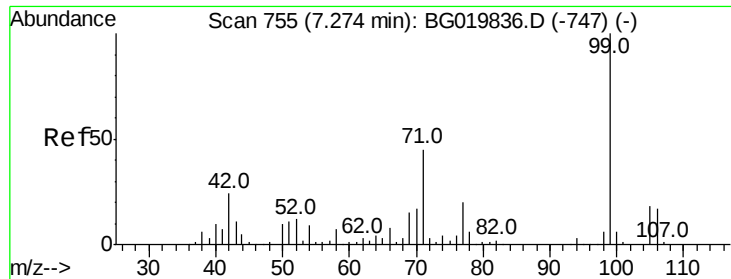

#7

Phenol-d6

Concen: 121.24 ng

RT: 7.26 min Scan# 753

Delta R.T. -0.01 min

Lab File: BG019980.D

Acq: 7 Dec 2015 14:13

Instrument :

BNA_G

ClientSampleId :

PB87054BL


Tot Ion: 99 Resp: 196936

Ion Ratio Lower Upper




99 100

42 19.5 11.5 17.3#

71 38.0 22.6 34.0#

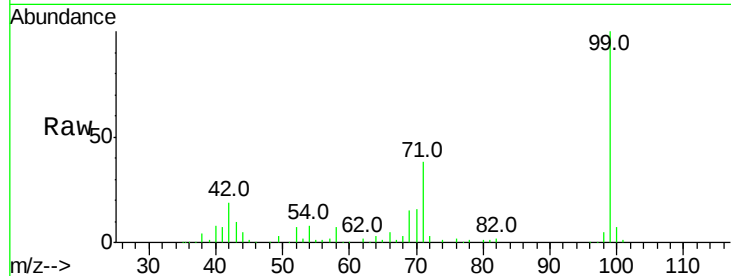

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

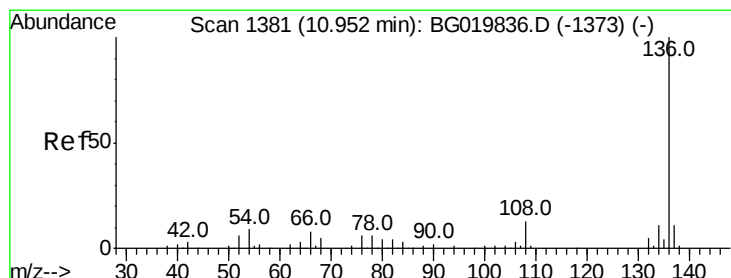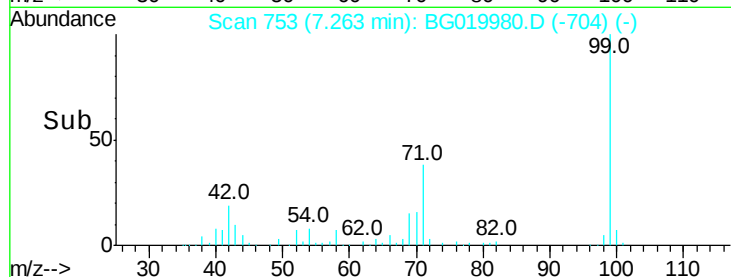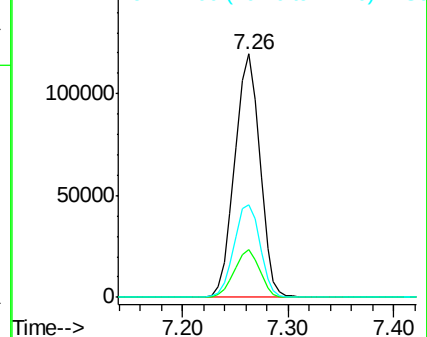

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1378

Delta R.T. -0.02 min

Lab File: BG019980.D

Acq: 7 Dec 2015 14:13

Tgt Ion: 136 Resp: 85095


Ion Ratio Lower Upper

136 100



137 11.4 8.6 12.8


54 9.1 5.4 8.2#

68 6.0 5.3 7.9

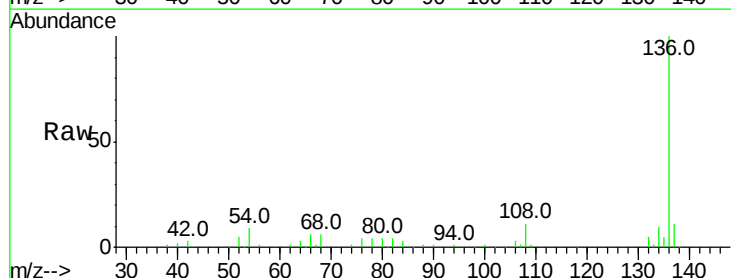

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



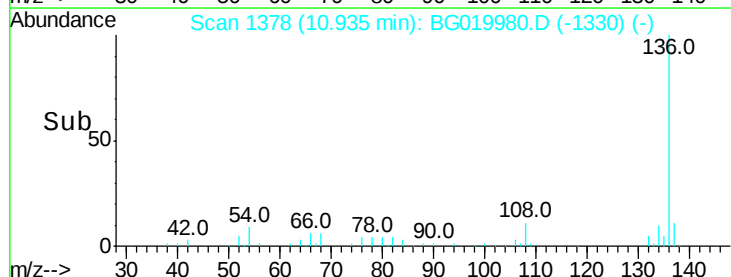
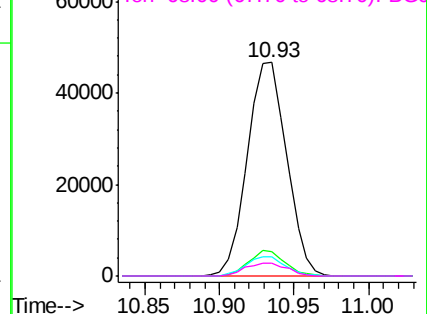


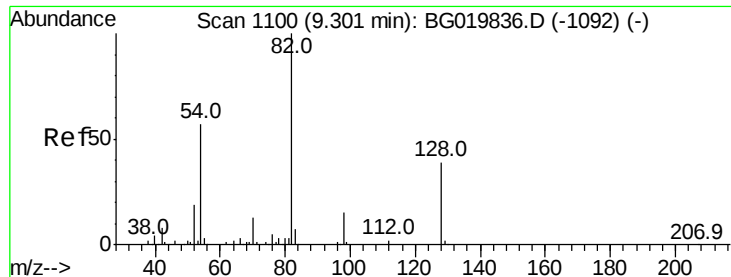

#23
Nitrobenzene-d5
Concen: 76.59 ng
RT: 9.28 min Scan# 1096
Delta R.T. -0.02 min
Lab File: BG019980.D
Acq: 7 Dec 2015 14:13




Instrument :
BNA_G
ClientSampleId :
PB87054BL


Tot Ion: 82 Resp: 127712
Ion Ratio Lower Upper
82 100
128 39.2 36.7 55.1
54 50.8 33.8 50.8#

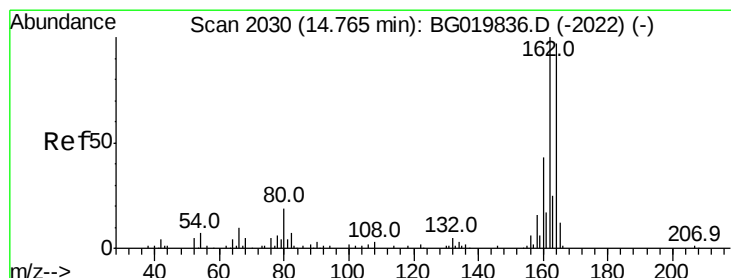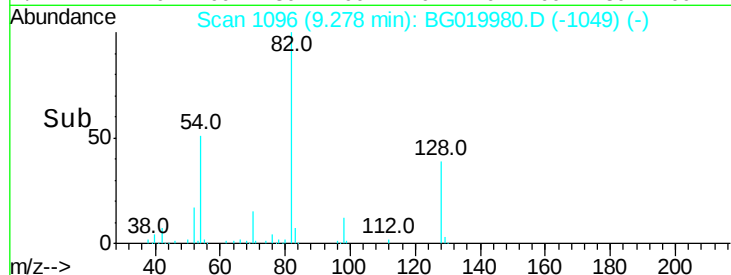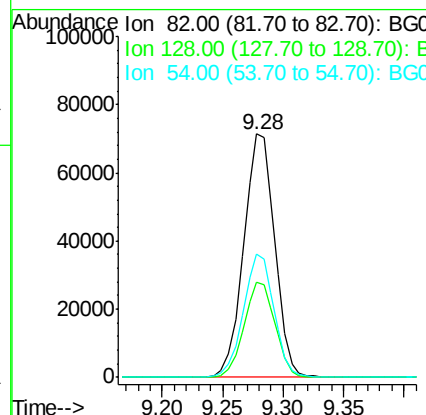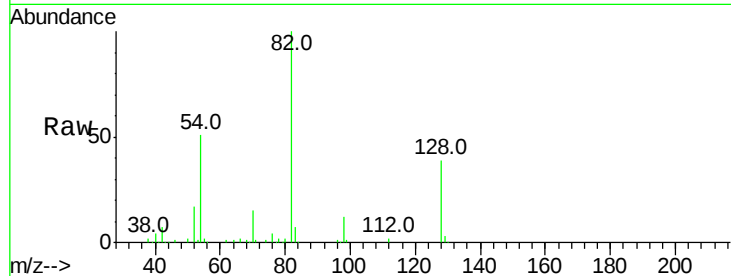

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.74 min Scan# 2026
Delta R.T. -0.02 min
Lab File: BG019980.D
Acq: 7 Dec 2015 14:13

Tgt Ion:164 Resp: 62876
Ion Ratio Lower Upper
164 100
162 106.4 78.8 118.2
160 47.5 36.4 54.6

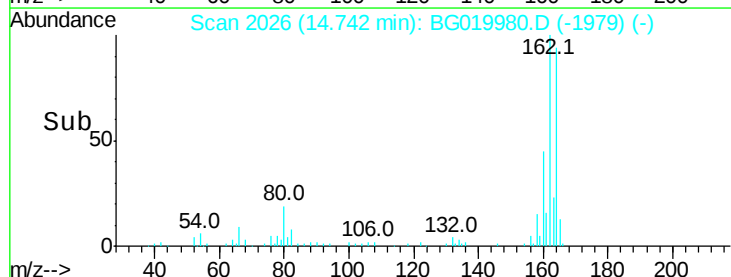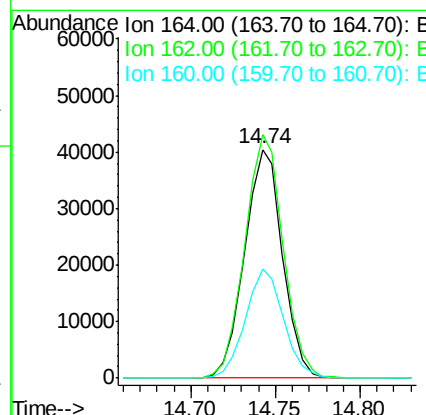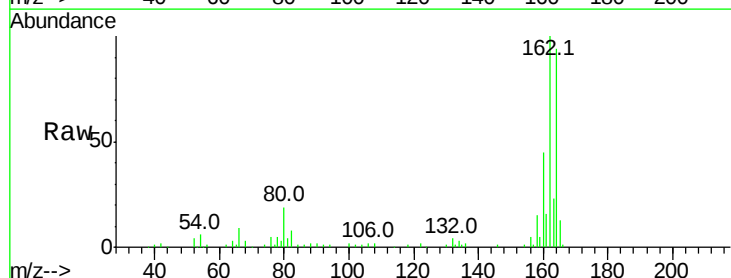


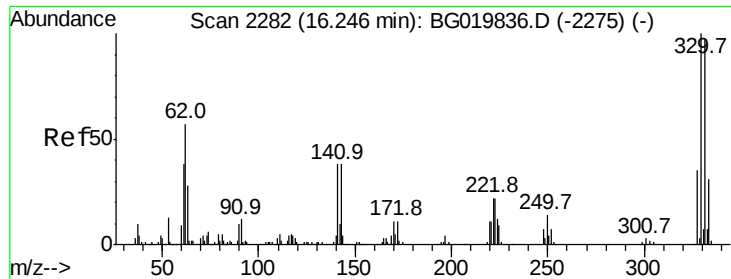




#41
 2,4,6-Tribromophenol
 Concen: 103.27 ng
 RT: 16.23 min Scan# 2279
 Delta R.T. -0.02 min
 Lab File: BG019980.D
 Acq: 7 Dec 2015 14:13

Instrument :
 BNA_G
 ClientSampleId :
 PB87054BL

Tot Ion:330 Resp: 99353
 Ion Ratio Lower Upper
 330 100
 332 95.1 78.1 117.1
 141 36.8 28.2 42.2

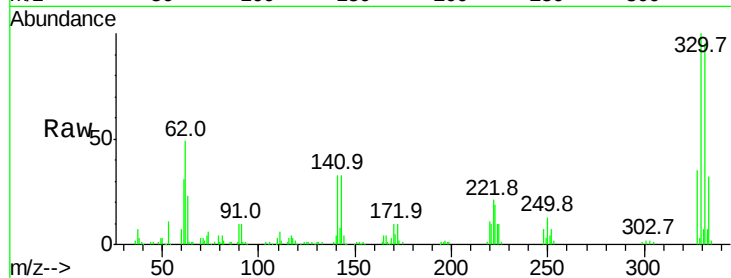


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

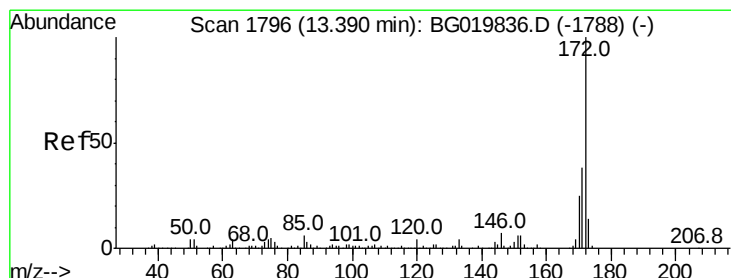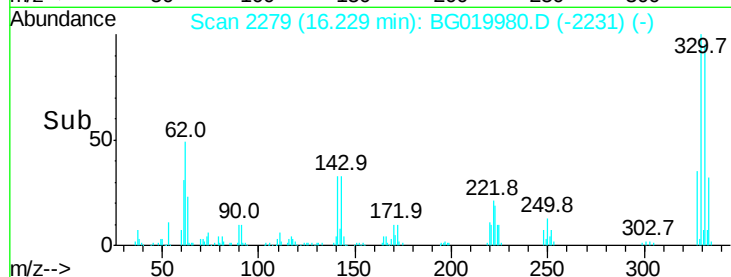
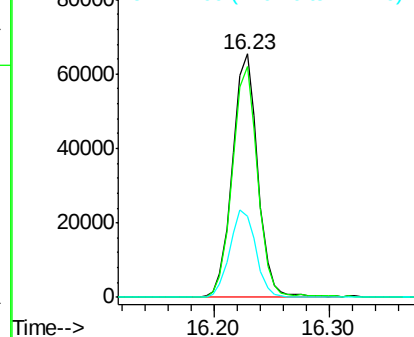



#44
 2-Fluorobiphenyl
 Concen: 71.11 ng
 RT: 13.37 min Scan# 1792
 Delta R.T. -0.02 min
 Lab File: BG019980.D
 Acq: 7 Dec 2015 14:13

Tgt Ion:172 Resp: 327444
 Ion Ratio Lower Upper
 172 100
 171 37.4 29.0 43.6
 170 23.9 19.9 29.9

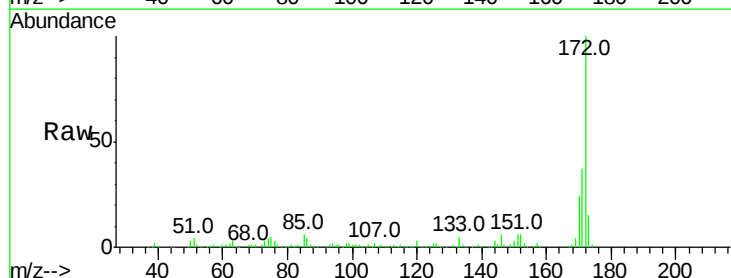

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



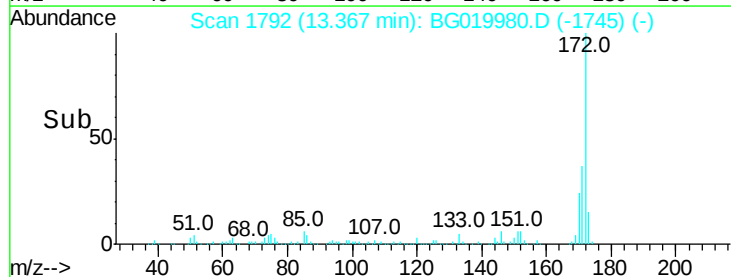
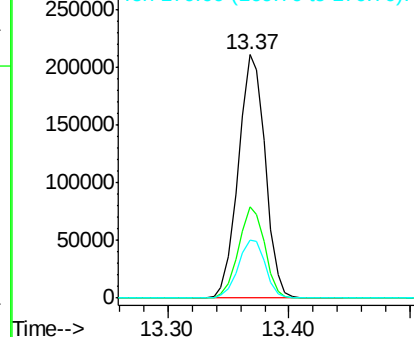


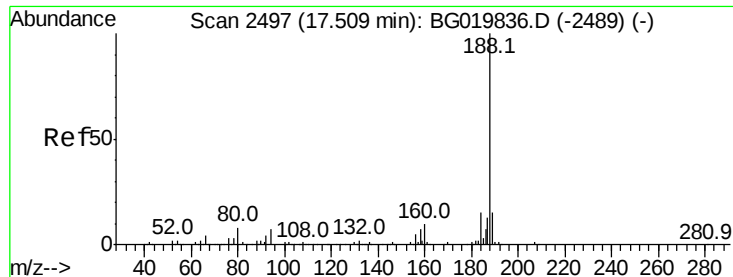

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.49 min Scan# 2493
Delta R.T. -0.02 min
Lab File: BG019980.D
Acq: 7 Dec 2015 14:13




Instrument :
BNA_G
ClientSampleId :
PB87054BL


Tot Ion	Ratio	Lower	Upper
188	100		
94	7.7	7.7	11.5
80	8.6	7.8	11.8

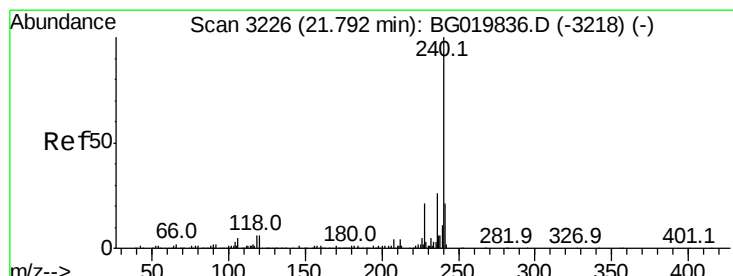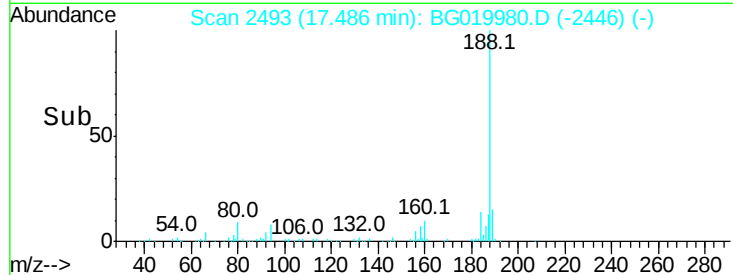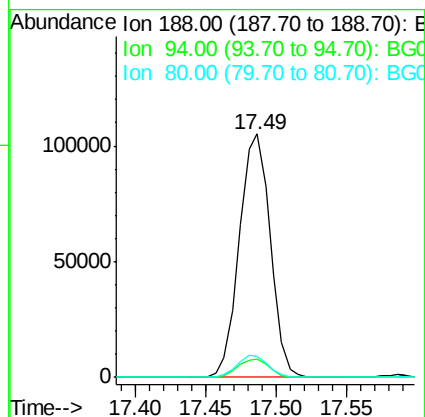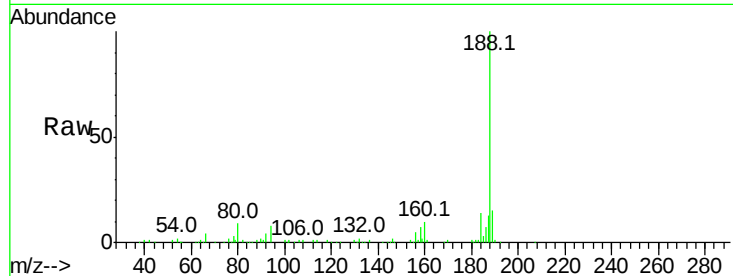

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.76 min Scan# 3220
Delta R.T. -0.03 min
Lab File: BG019980.D
Acq: 7 Dec 2015 14:13

Tgt Ion	Ratio	Lower	Upper
240	100		
120	7.7	7.4	11.0
236	26.1	20.7	31.1

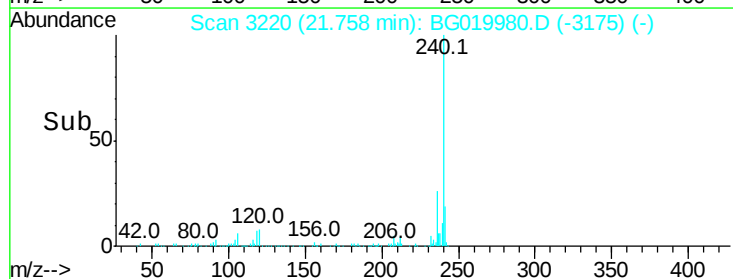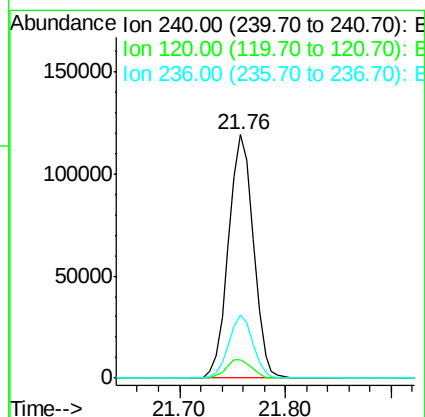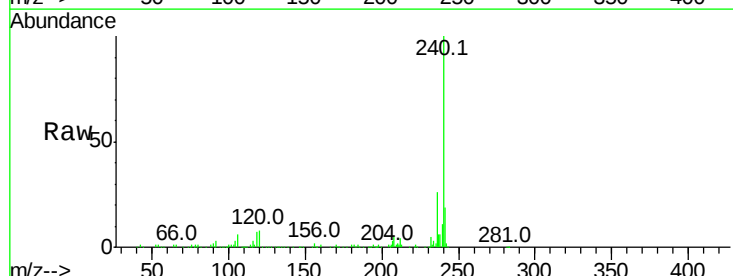

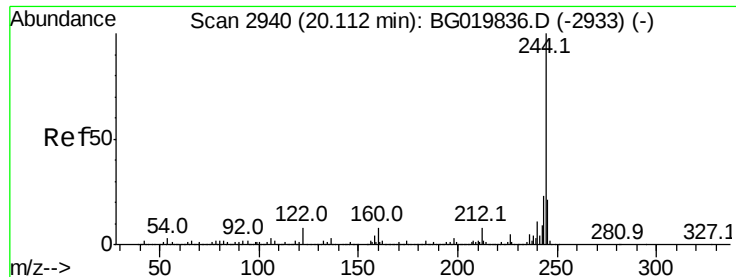

#78

Terphenyl-d14

Concen: 73.22 ng

RT: 20.09 min Scan# 2936

Delta R.T. -0.02 min

Lab File: BG019980.D

Acq: 7 Dec 2015 14:13

Instrument :

BNA_G

ClientSampleId :

PB87054BL





Tot Ion:244 Resp: 584243

Ion Ratio Lower Upper

244 100

212 8.1 6.9 10.3

122 8.3 10.2 15.2#

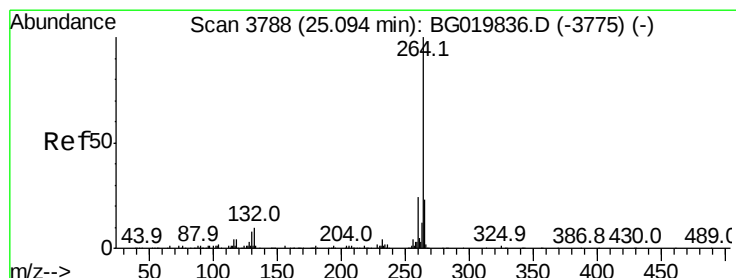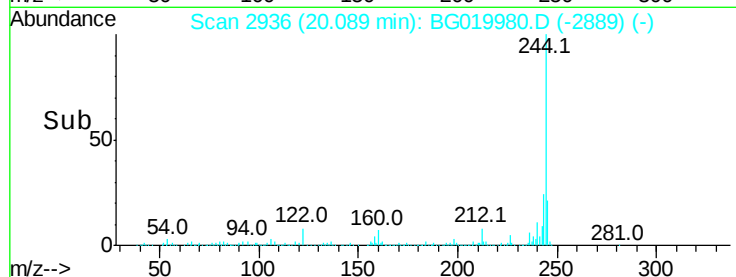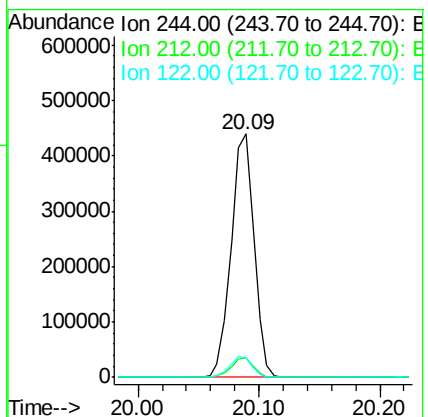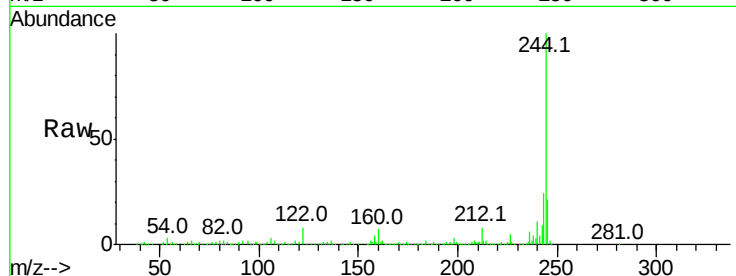

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.04 min Scan# 3779

Delta R.T. -0.05 min

Lab File: BG019980.D

Acq: 7 Dec 2015 14:13

Tgt Ion:264 Resp: 179766

Ion Ratio Lower Upper

264 100

260 23.4 18.5 27.7

265 21.3 17.2 25.8

