


Data Path : Z:\HPCHEM1\BNA G\Data\BG120715\
 Data File : BG019978.D
 Acq On : 7 Dec 2015 8:46
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 18:50:01 2015

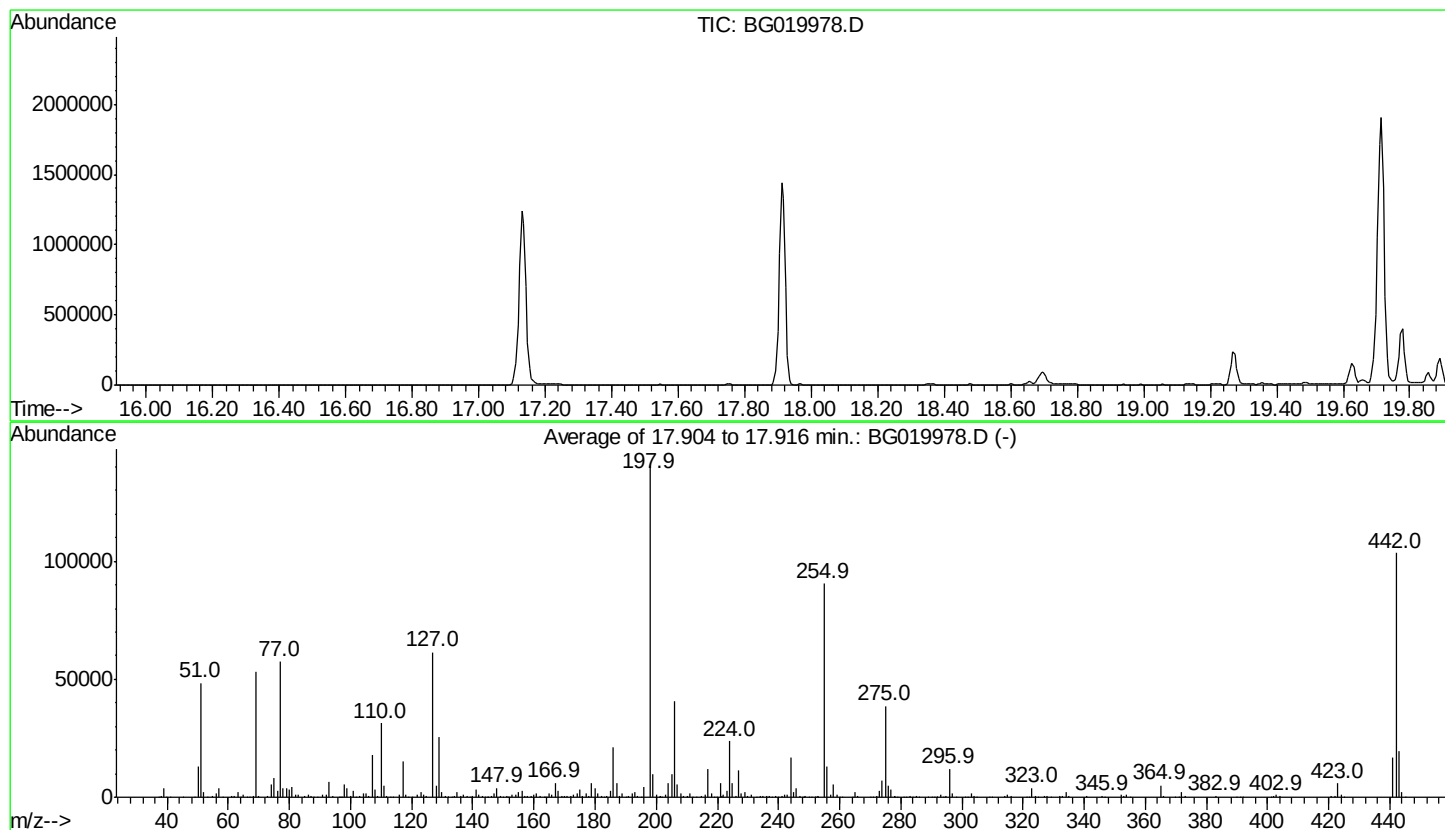

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	48360	PASS
68	69	0.00	2	1.0	556	PASS
69	198	0.00	100	37.7	52965	PASS
70	69	0.00	2	0.6	297	PASS
127	198	10	80	43.8	61576	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140554	PASS
199	198	5	9	6.9	9667	PASS
275	198	10	60	27.6	38786	PASS
365	198	1	100	3.6	5003	PASS
441	442	0.01	24	16.1	16618	PASS
442	198	50	100	73.6	103408	PASS
443	442	15	24	18.8	19434	PASS