


Data Path : Z:\HPCHEM1\BNA G\DATA\BG120715\
Data File : BG019989.D
Acq On : 7 Dec 2015 20:15
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 02 18:50:01 2015

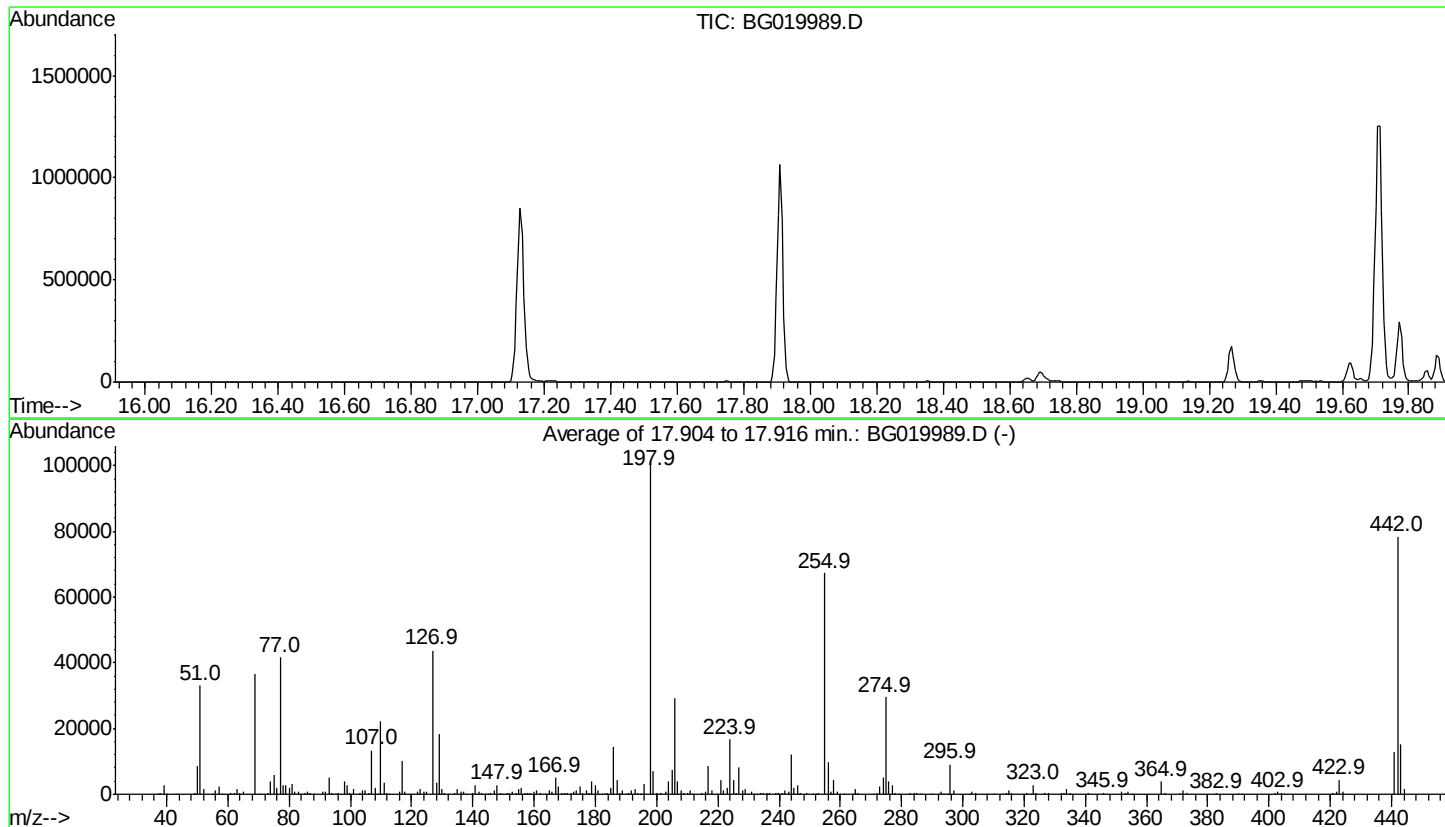

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	32978	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.5	36781	PASS
70	69	0.00	2	0.5	196	PASS
127	198	10	80	43.3	43645	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	100877	PASS
199	198	5	9	6.9	6985	PASS
275	198	10	60	29.3	29522	PASS
365	198	1	100	3.8	3826	PASS
441	442	0.01	24	16.3	12797	PASS
442	198	50	100	77.7	78426	PASS
443	442	15	24	19.4	15252	PASS