


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG120717\
 Data File : BG031397.D
 Acq On : 7 Dec 2017 14:09
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 06 17:58:37 2017

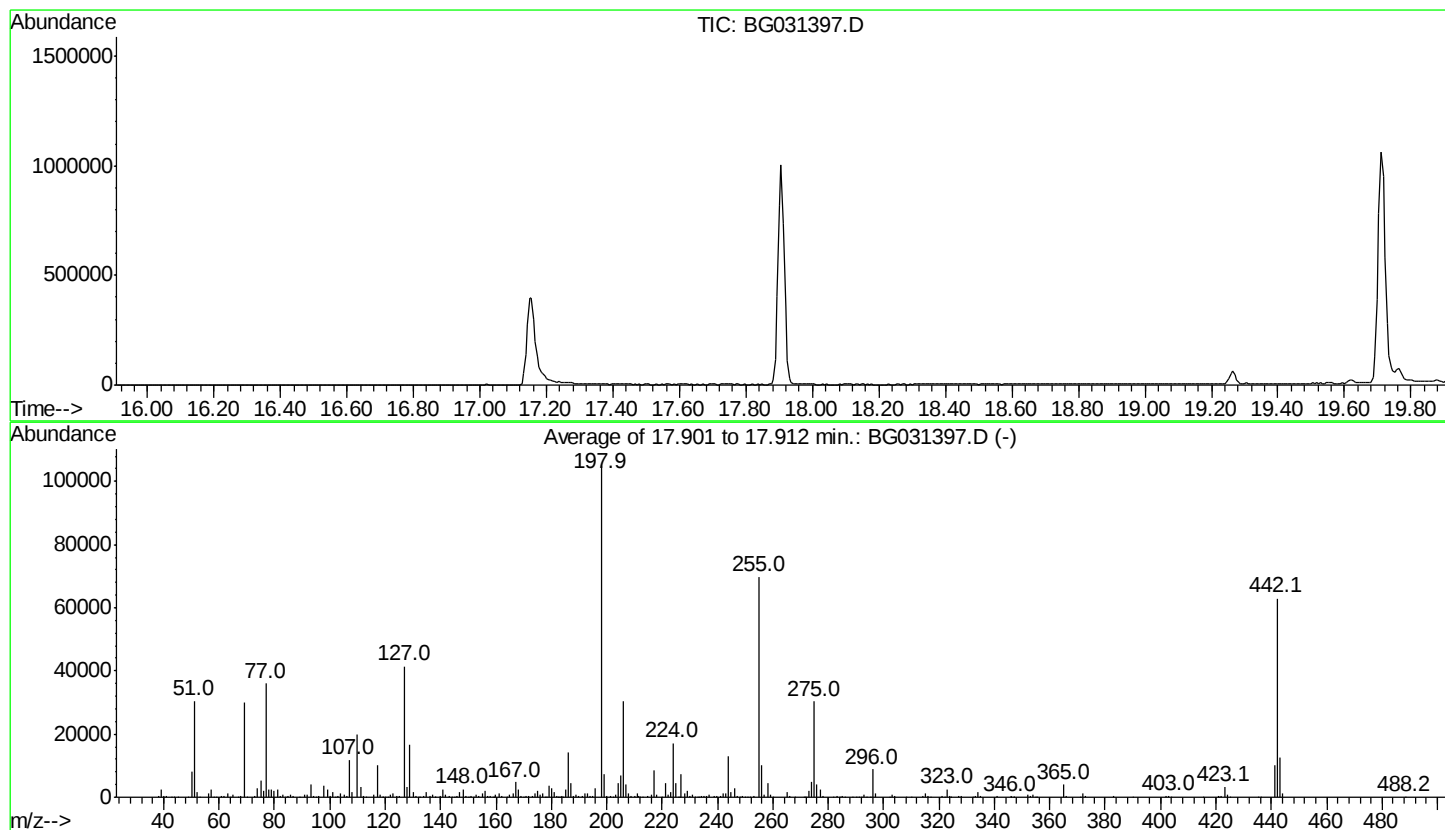

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	30469	PASS
68	69	0.00	2	1.7	520	PASS
69	198	0.00	100	28.7	30149	PASS
70	69	0.00	2	0.7	201	PASS
127	198	10	80	39.6	41544	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105013	PASS
199	198	5	9	7.0	7345	PASS
275	198	10	60	28.9	30317	PASS
365	198	1	100	3.8	3998	PASS
441	442	0.01	24	15.9	9987	PASS
442	198	50	100	59.9	62893	PASS
443	442	15	24	19.9	12519	PASS