
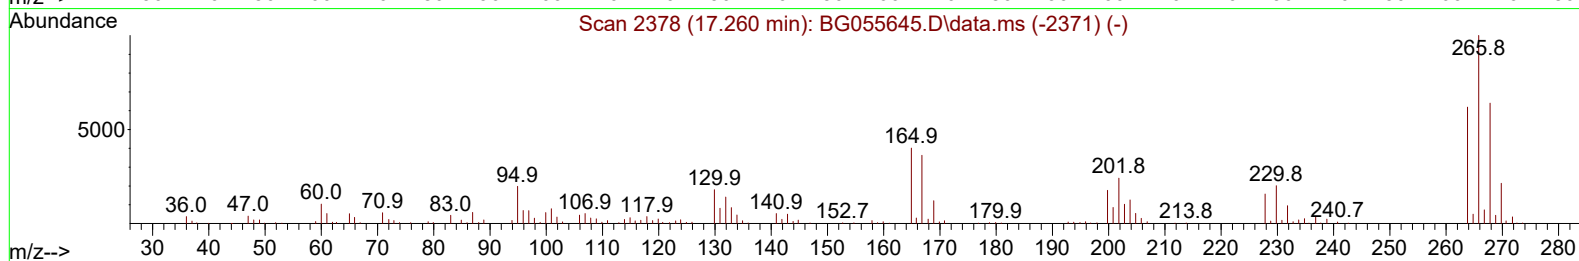
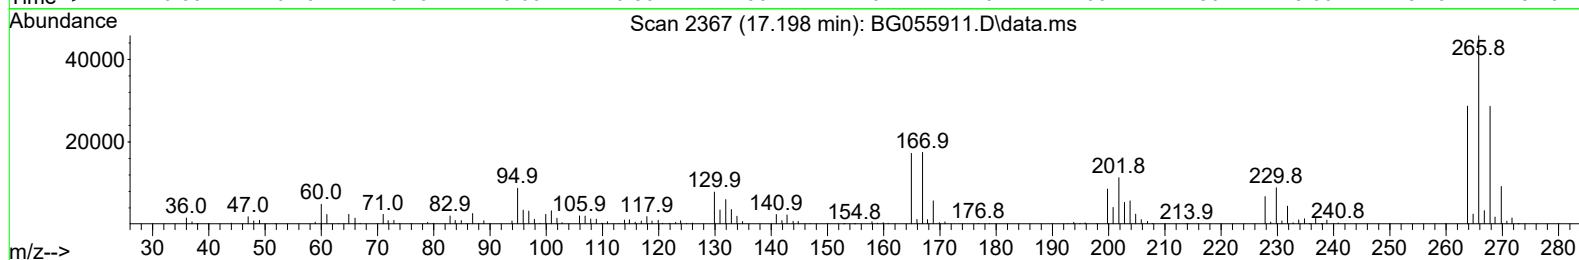


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120722\  
Data File : BG055911.D  
Acq On    : 7 Dec 2022 11:21  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Dec 08 06:36:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

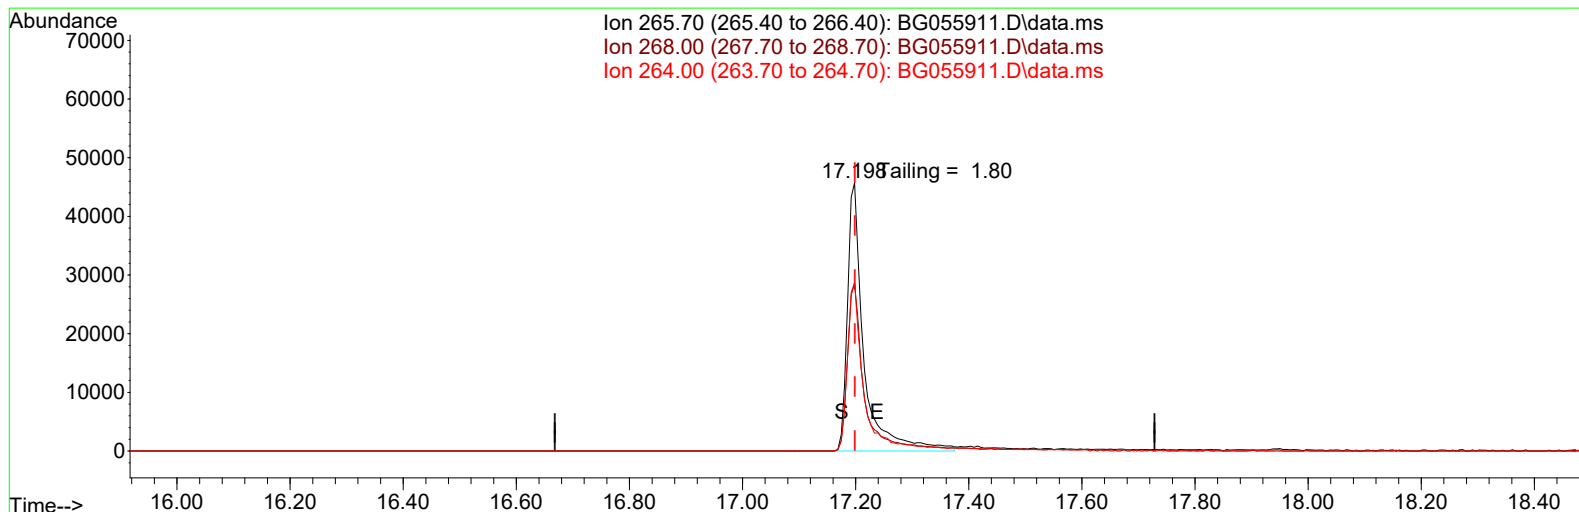

TIC: BG055911.D\data.ms

(70) Pentachlorophenol (C)




17.198min (-0.001) 94999.07 ng

response 93244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	66.50
264.00	61.90	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120722\
Data File : BG055911.D
Acq On : 7 Dec 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 06:36:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

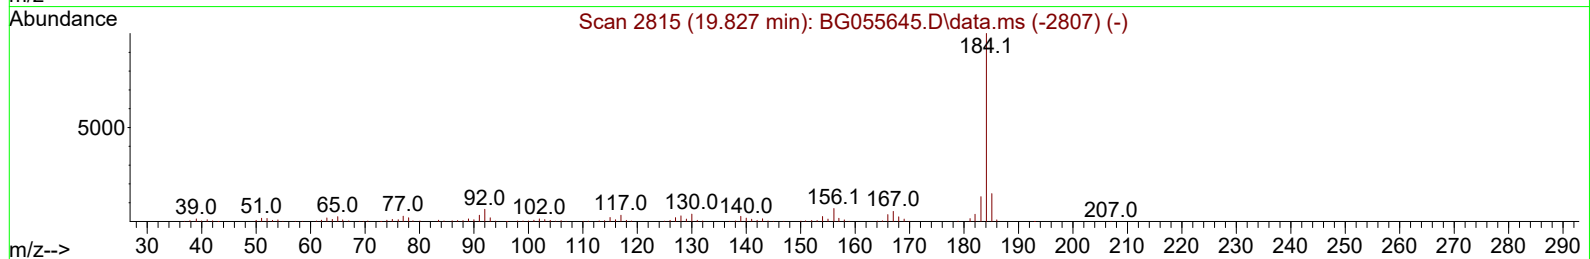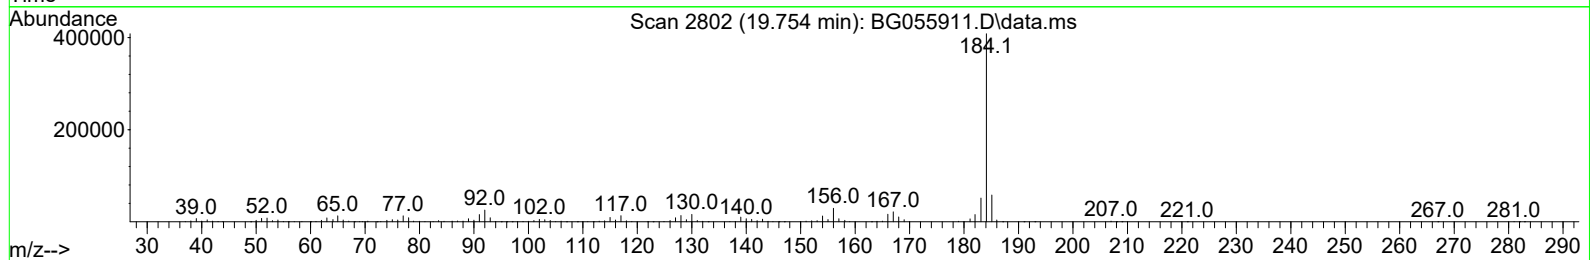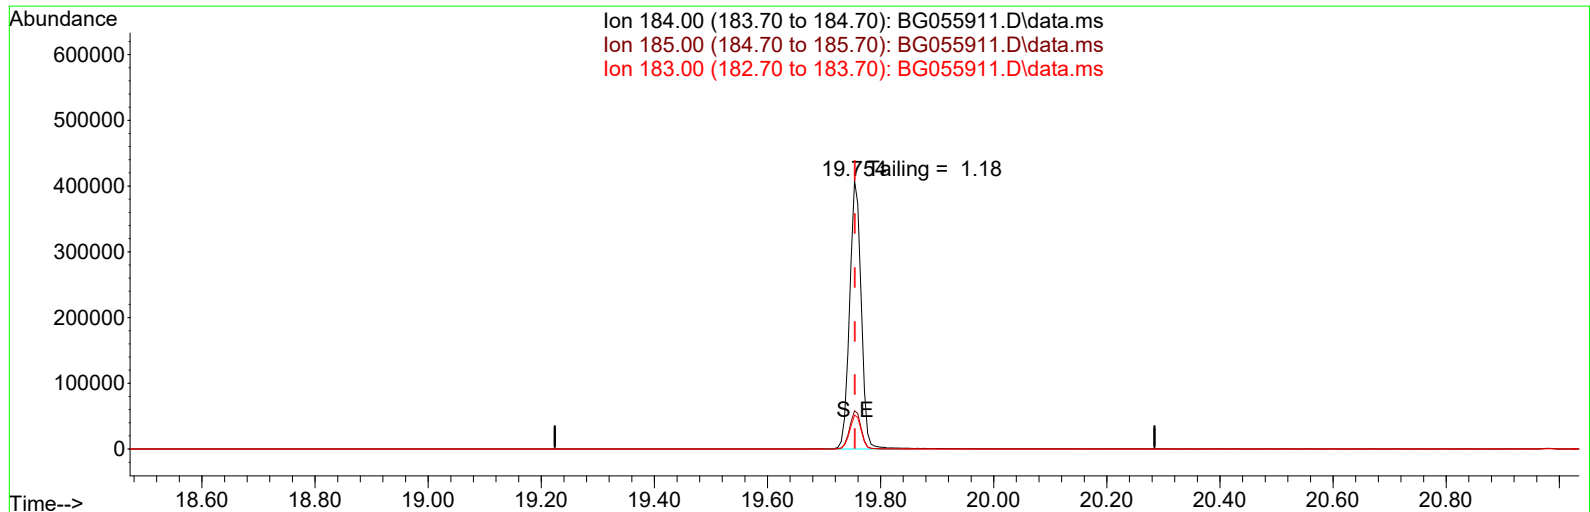

TIC: BG055911.D\data.ms

(77) Benzidine

19.754min (-0.001) 9618.76 ng

response 585018

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.28
183.00	13.20	12.65
0.00	0.00	0.00