


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120722\
 Data File : BG055911.D
 Acq On : 7 Dec 2022 11:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 07 05:04:10 2022

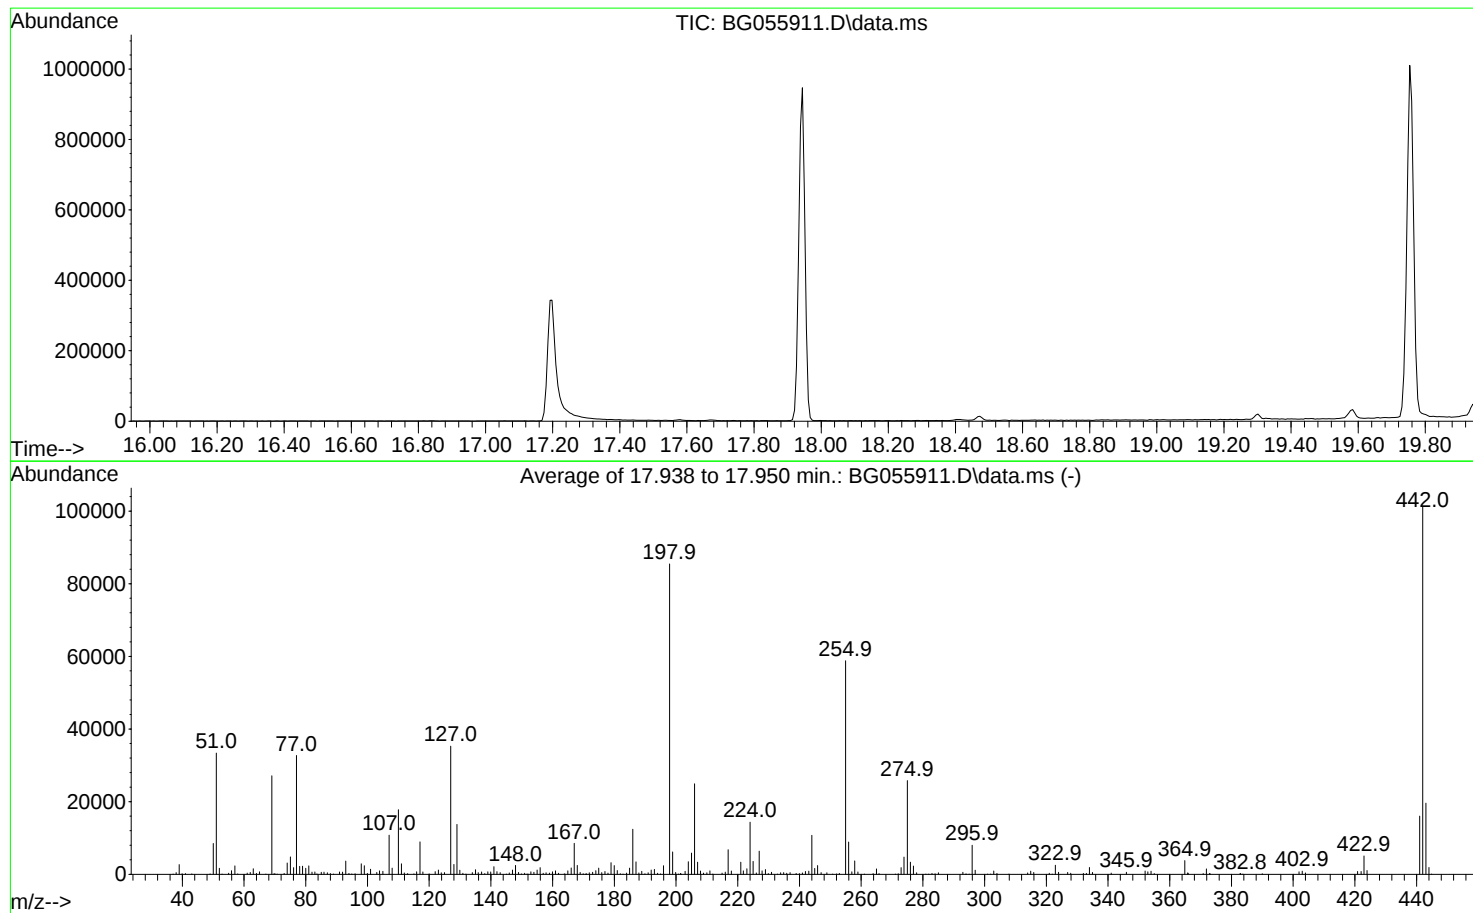




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	33384	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.7	27117	PASS
70	69	0.00	2	0.7	194	PASS
127	198	10	80	41.3	35275	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85443	PASS
199	198	5	9	7.2	6169	PASS
275	198	10	60	30.2	25779	PASS
365	198	1	100	4.4	3782	PASS
441	198	0.01	100	18.8	16039	PASS
442	442	50	100	100.0	101283	PASS
443	442	15	24	19.4	19605	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120722\
Data File : BG055911.D
Acq On : 7 Dec 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 08 06:36:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

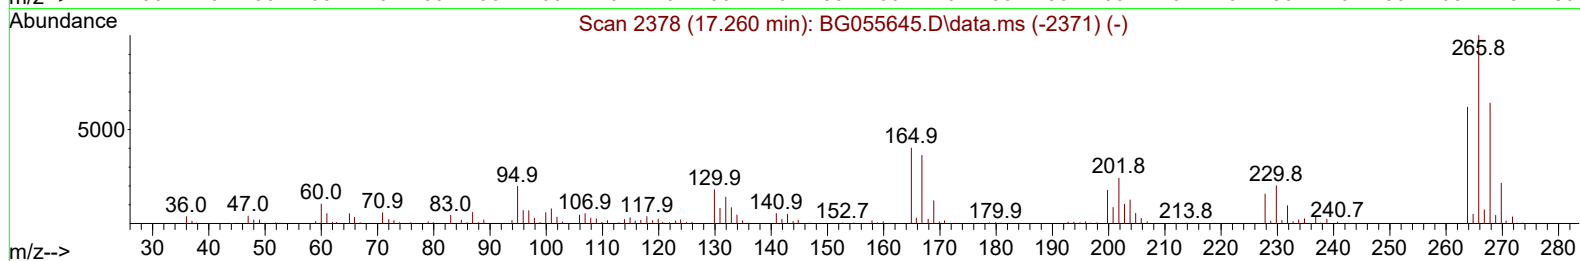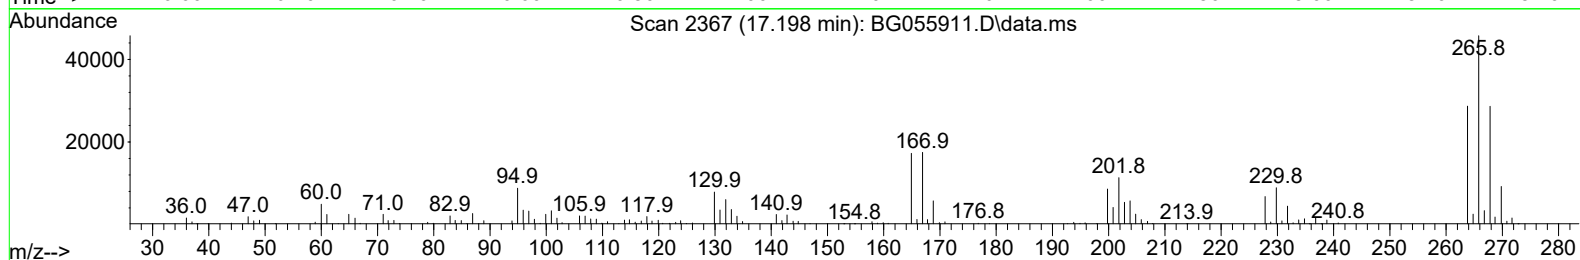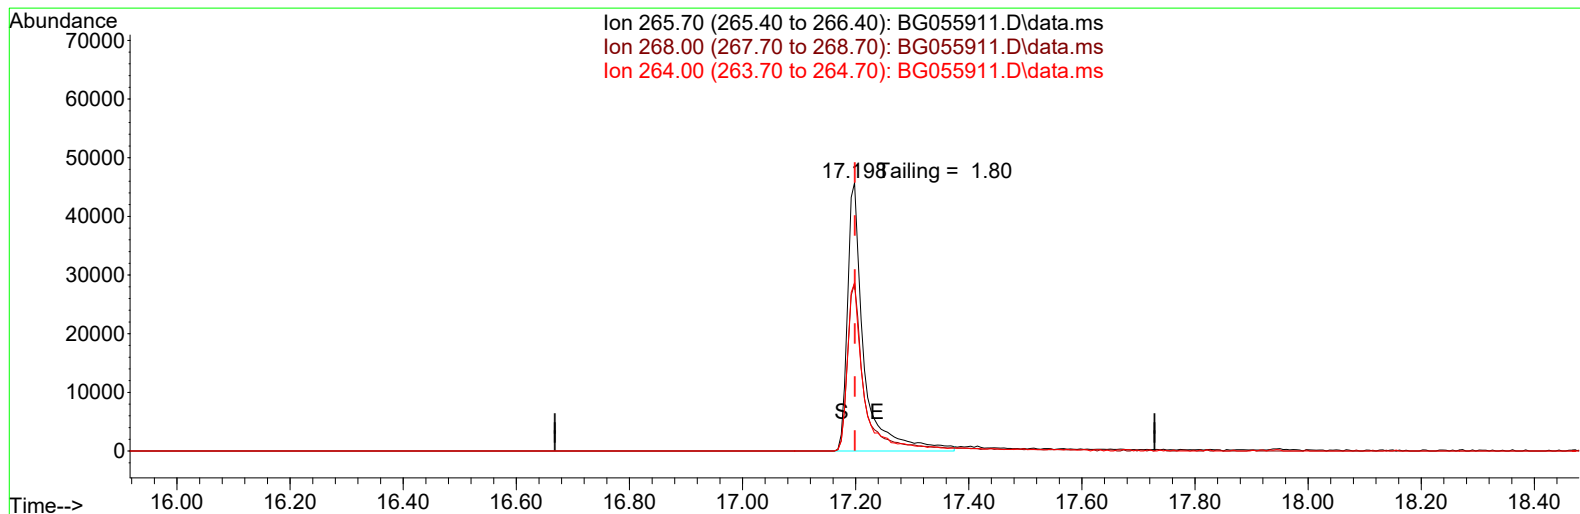

TIC: BG055911.D\data.ms

(70) Pentachlorophenol (C)

17.198min (-0.001) 94999.07 ng


response 93244

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	66.50
264.00	61.90	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120722\
Data File : BG055911.D
Acq On : 7 Dec 2022 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 08 06:36:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 07 05:04:10 2022
Response via : Initial Calibration

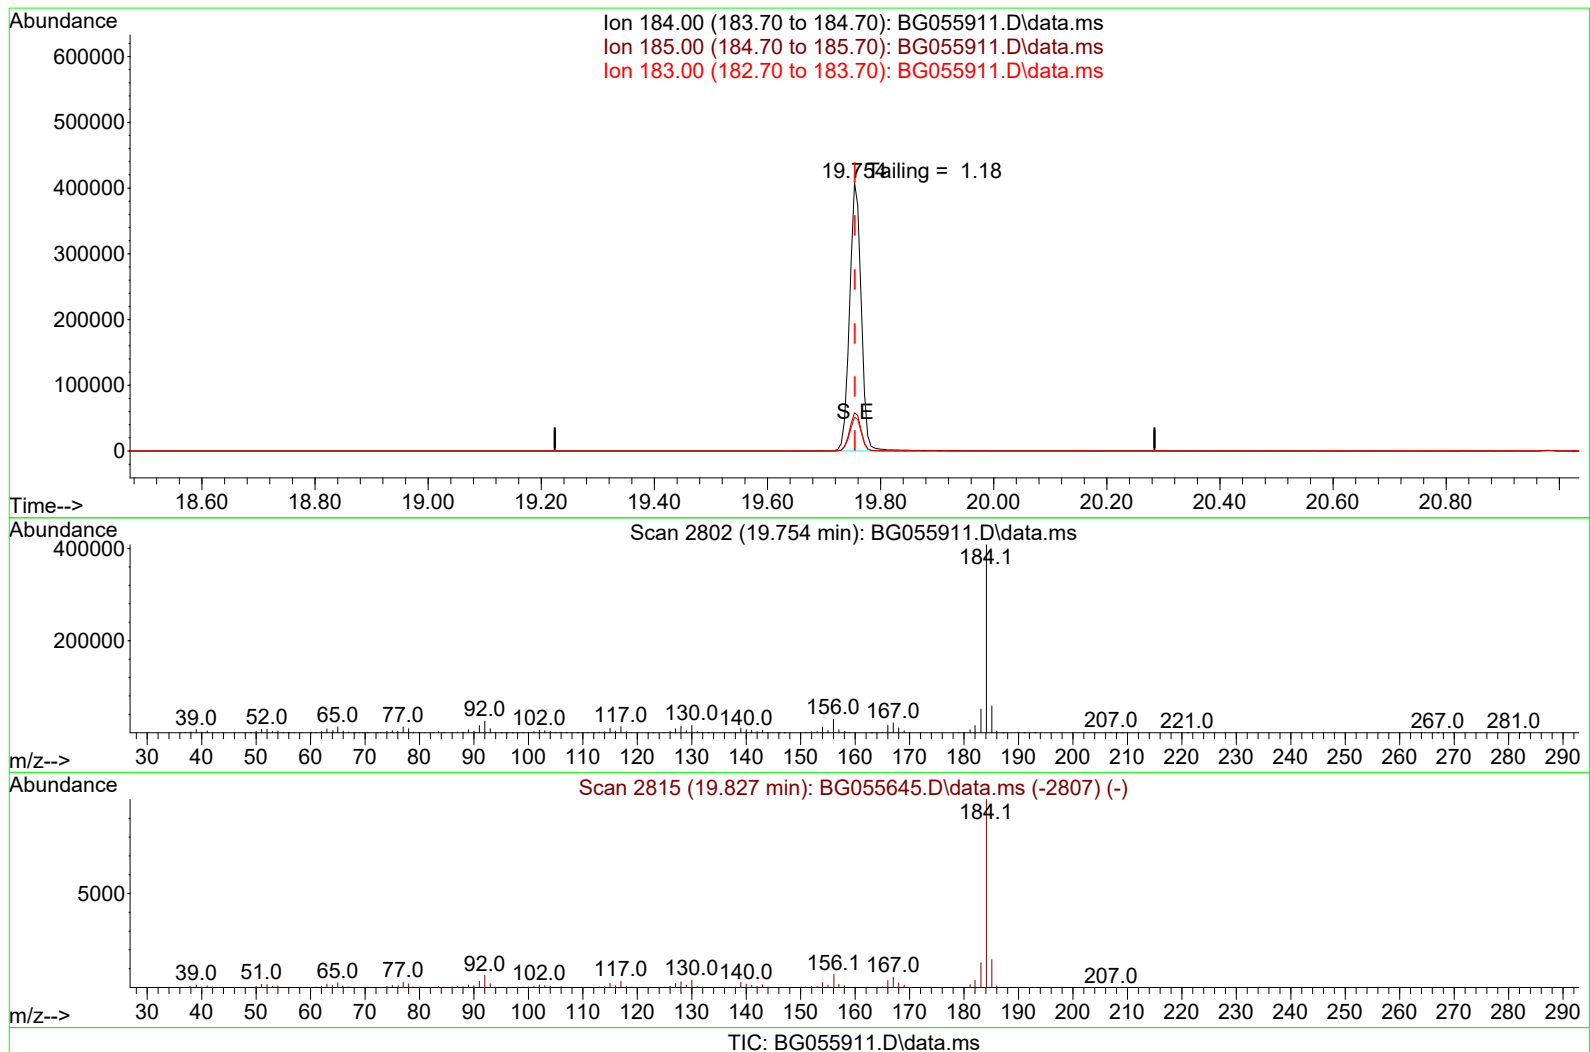

TIC: BG055911.D\data.ms

(77) Benzidine**19.754min (-0.001) 9618.76 ng****response 585018**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.28
183.00	13.20	12.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2022	BNA_G	<u>BG055911.D</u>
Compound Name	Response	Retention Time
DDT	274175	20.982
DDD	5711	20.588
DDE	194	20.042
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5905	280080	2.11

Instrument :
BNA_G
ClientSampleId :
DFTPP