
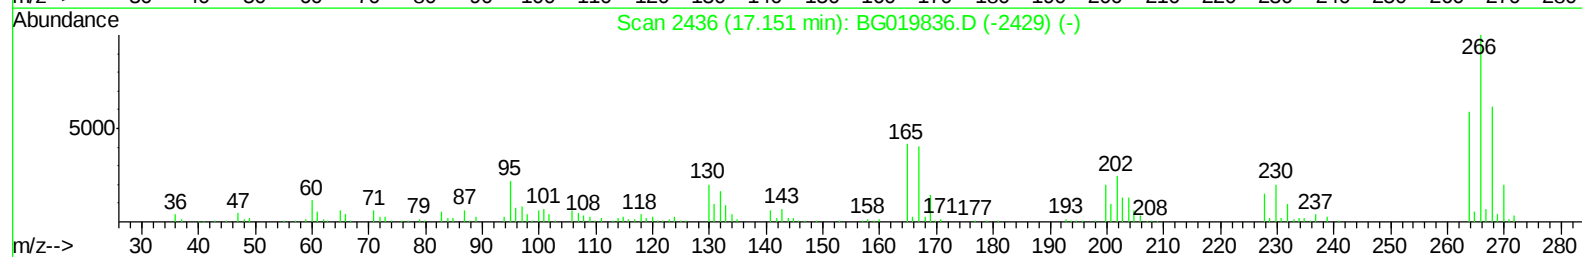
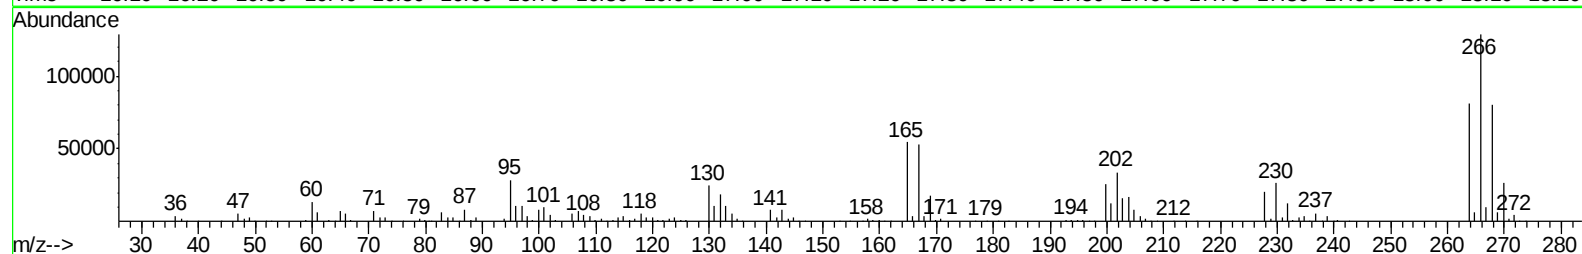


Data Path : Z:\HPCHEM1\BNA_G\Data\BG120815\
Data File : BG020007.D
Acq On : 8 Dec 2015 7:51
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 08:06:30 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 18:50:01 2015
Response via : Initial Calibration

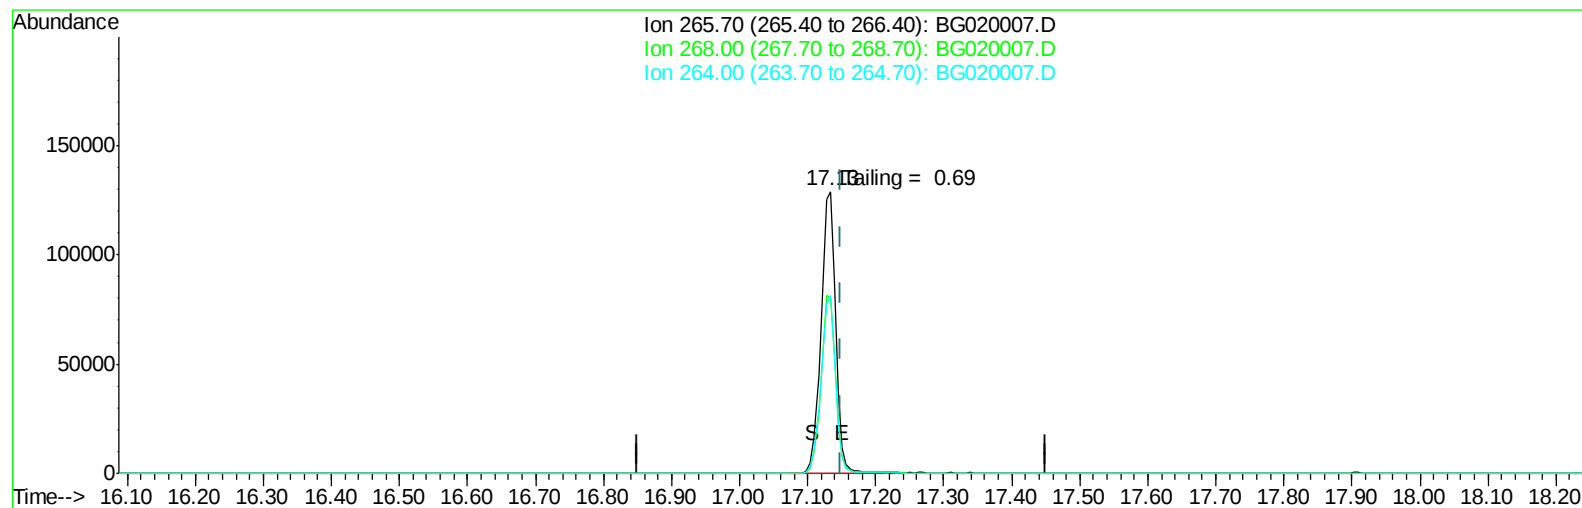

TIC: BG020007.D

(69) Pentachlorophenol (C)




17.133min (-0.017) 0.00ng

response 196894

Ion	Exp%	Act%
265.70	100	100
268.00	59.50	62.17
264.00	60.10	63.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG120815\
 Data File : BG020007.D
 Acq On : 8 Dec 2015 7:51
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 08:06:30 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 18:50:01 2015
 Response via : Initial Calibration

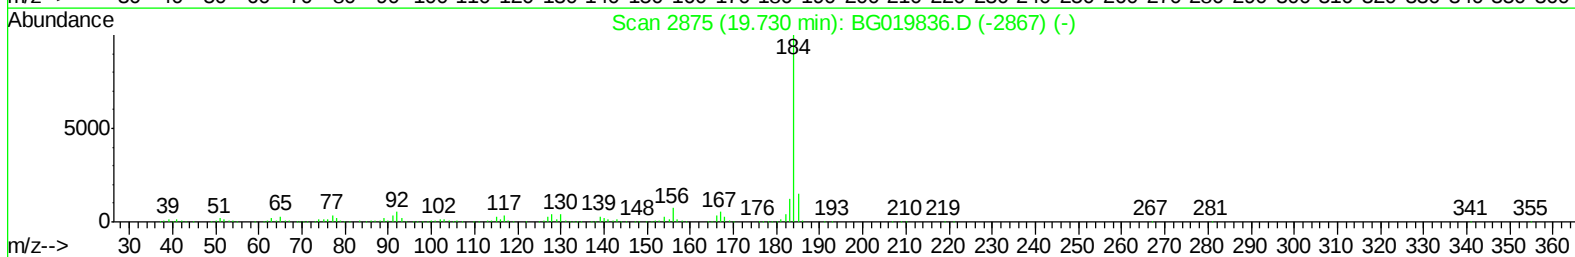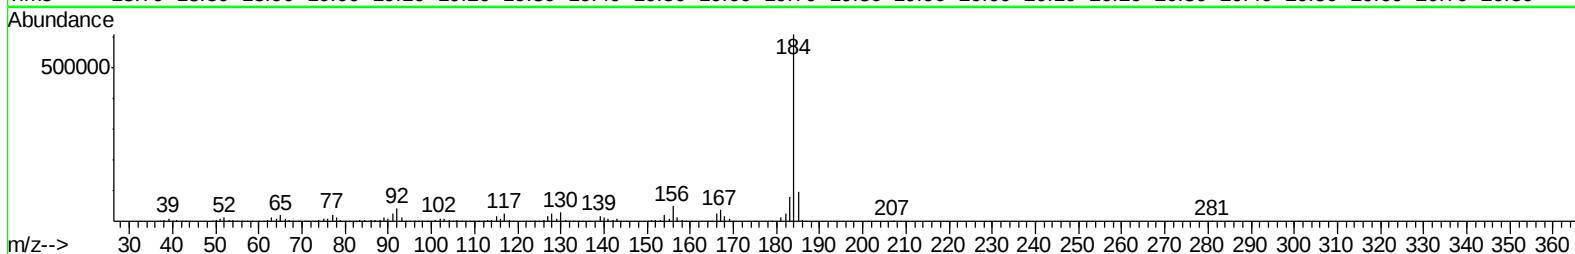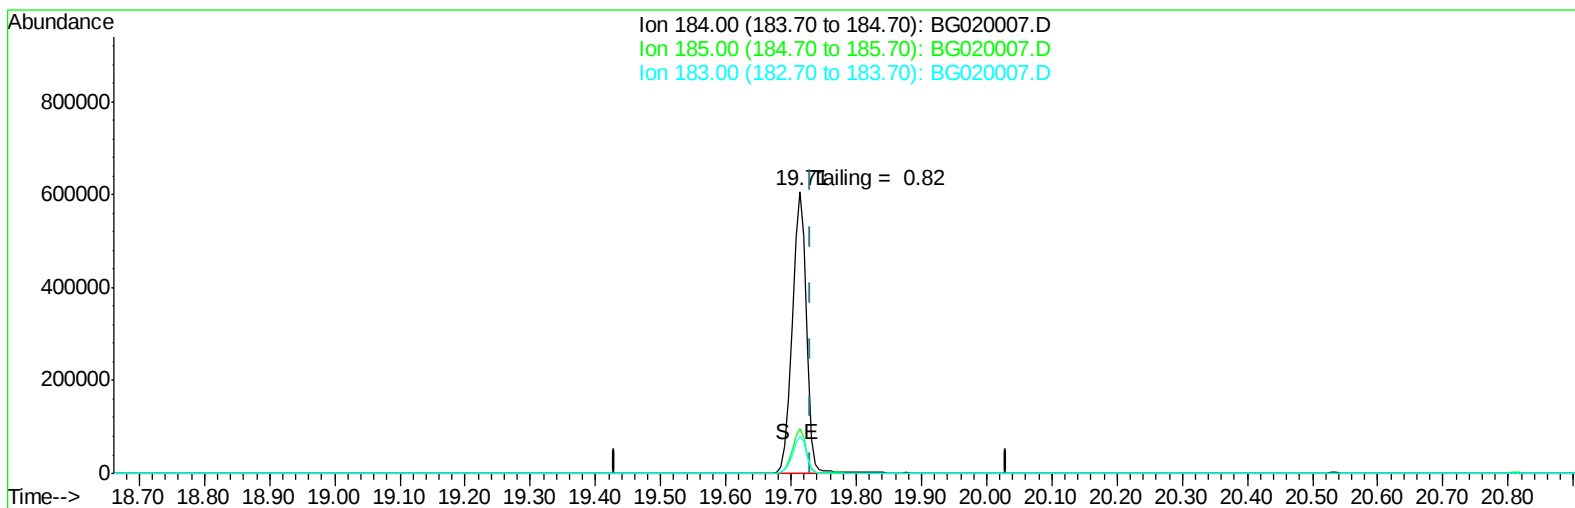

TIC: BG020007.D

(76) Benzidine

19.713min (-0.017) 98582.14ng

response 919648

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.80
183.00	12.60	13.30
0.00	0.00	0.00