


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120816\
Data File : BG025028.D
Acq On : 9 Dec 2016 5:09
Operator : UM/SJ
Sample : H5863-20 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
DA800

Manual Integrations
APPROVED

sohil
12/9/2016 3:42:01 PM

Quant Time: Dec 09 06:57:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 01:31:52 2016
Response via : Initial Calibration

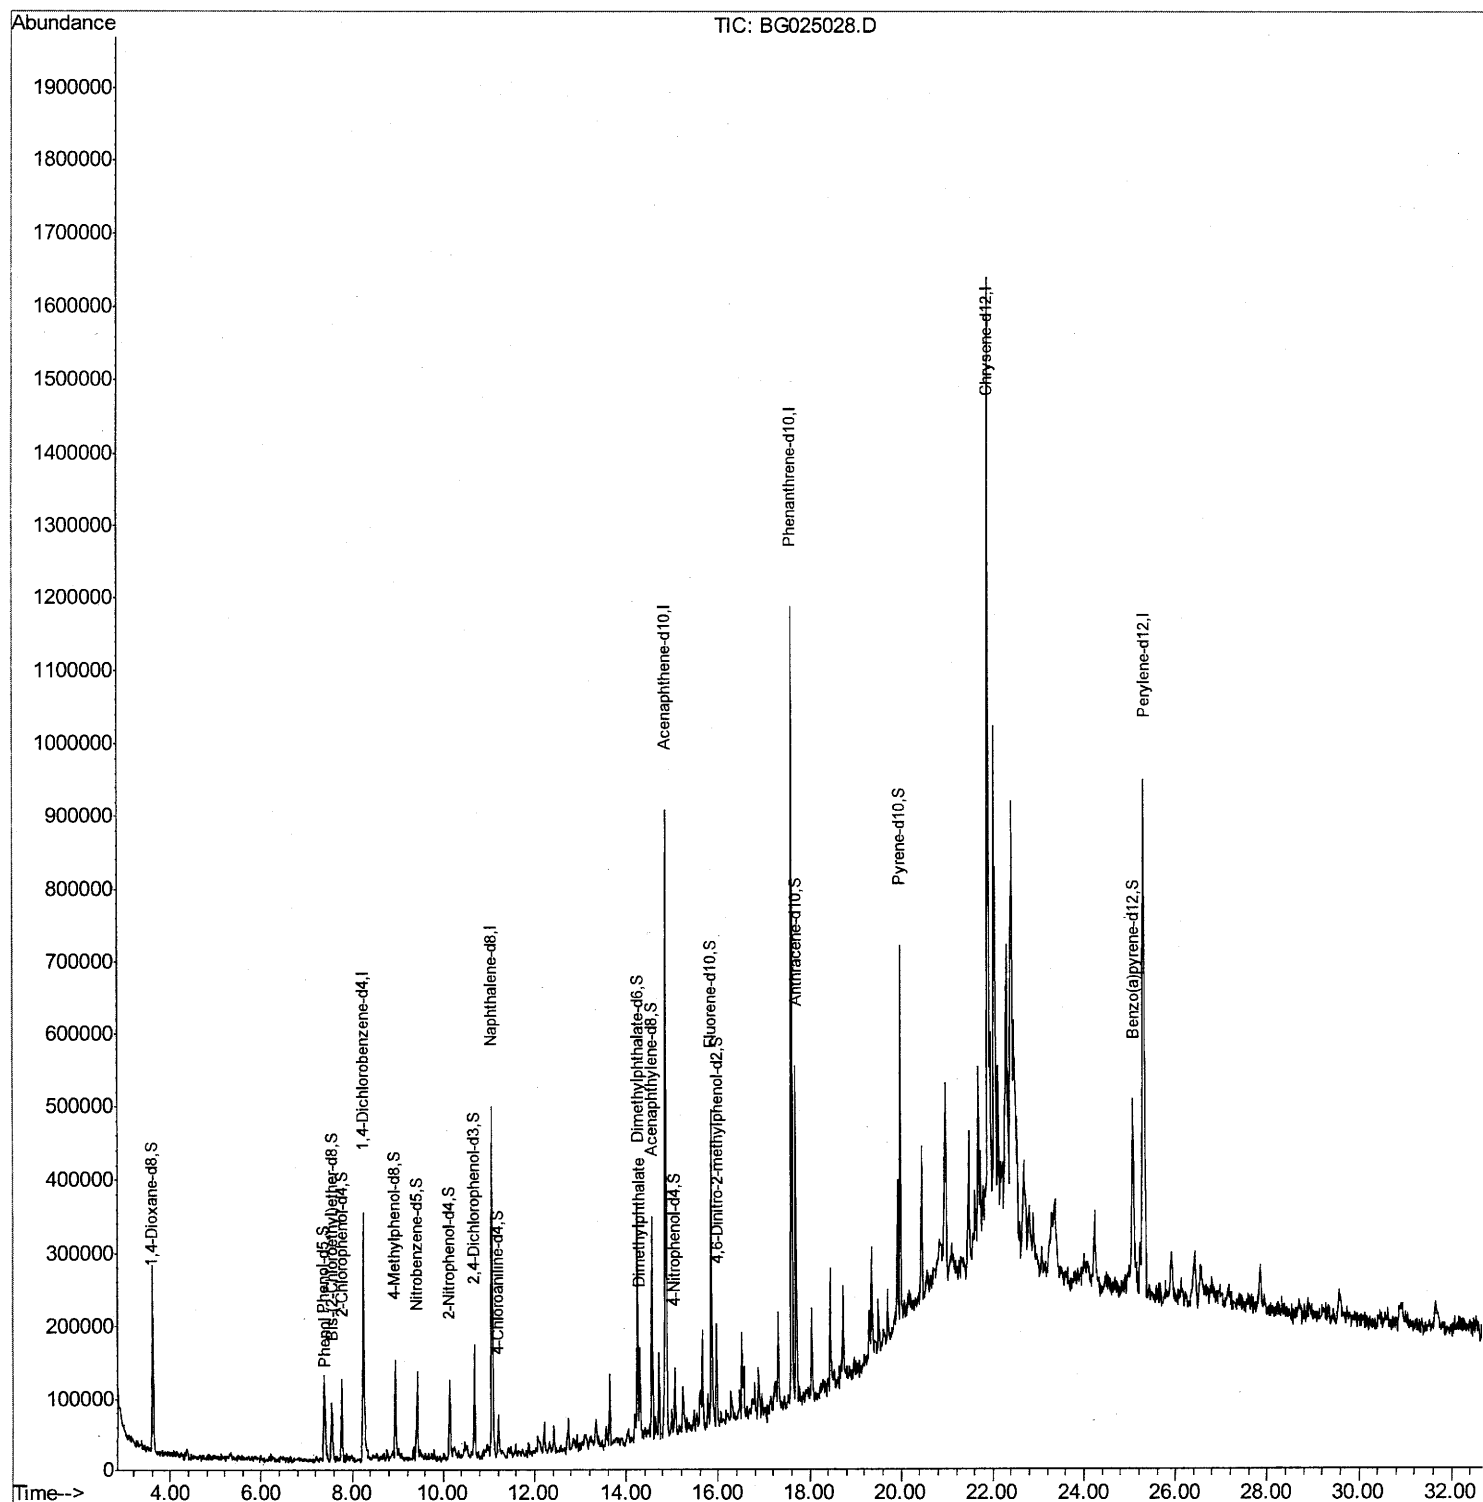




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120816\
Data File : BG025028.D
Acq On : 9 Dec 2016 5:09
Operator : UM/SJ
Sample : H5863-20 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DA800

Manual Integrations
APPROVED

sohil
12/9/2016 3:42:01 PM

Quant Time: Dec 09 06:35:39 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 01:31:52 2016
Response via : Initial Calibration

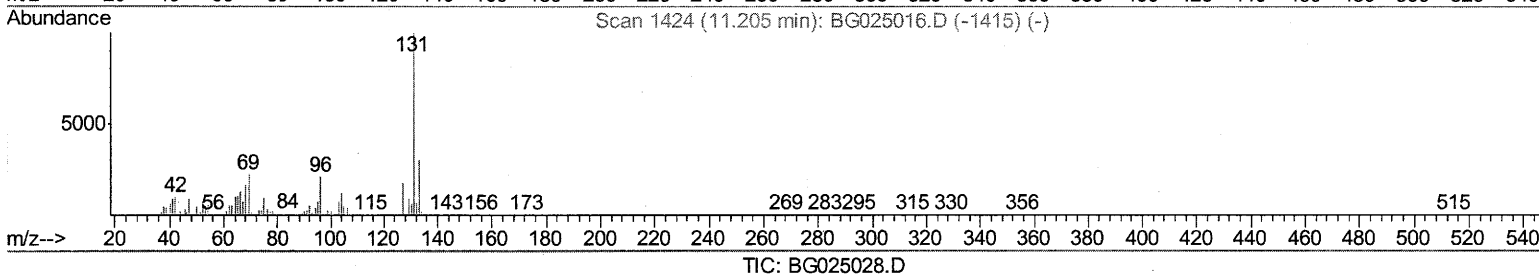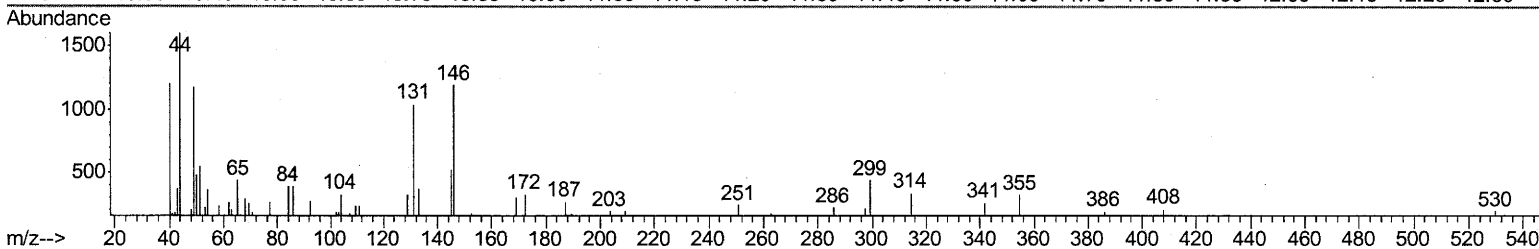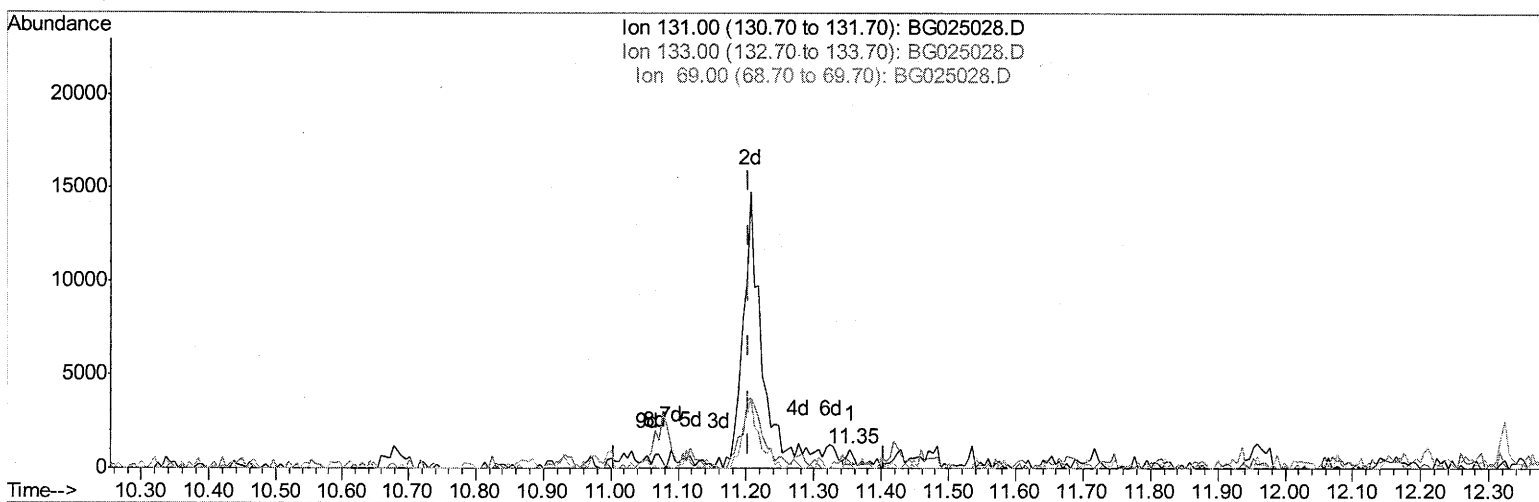

(29) 4-Chloroaniline-d4 (S)

11.353min (+0.149) 0.10ng/ul

response 611

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	35.77
69.00	23.80	24.42
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120816\
Data File : BG025028.D
Acq On : 9 Dec 2016 5:09
Operator : UM/SJ
Sample : H5863-20 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
DA800

Manual Integrations
APPROVED

sohil
12/9/2016 3:42:01 PM

Quant Time: Dec 09 06:35:39 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 01:31:52 2016
Response via : Initial Calibration

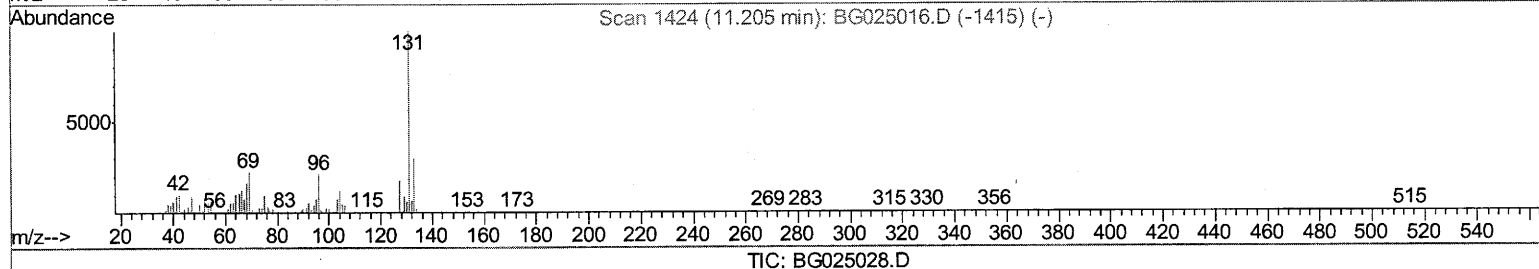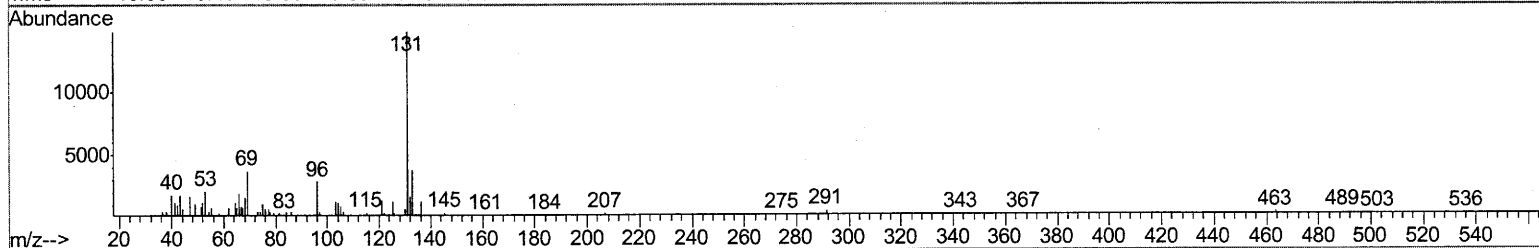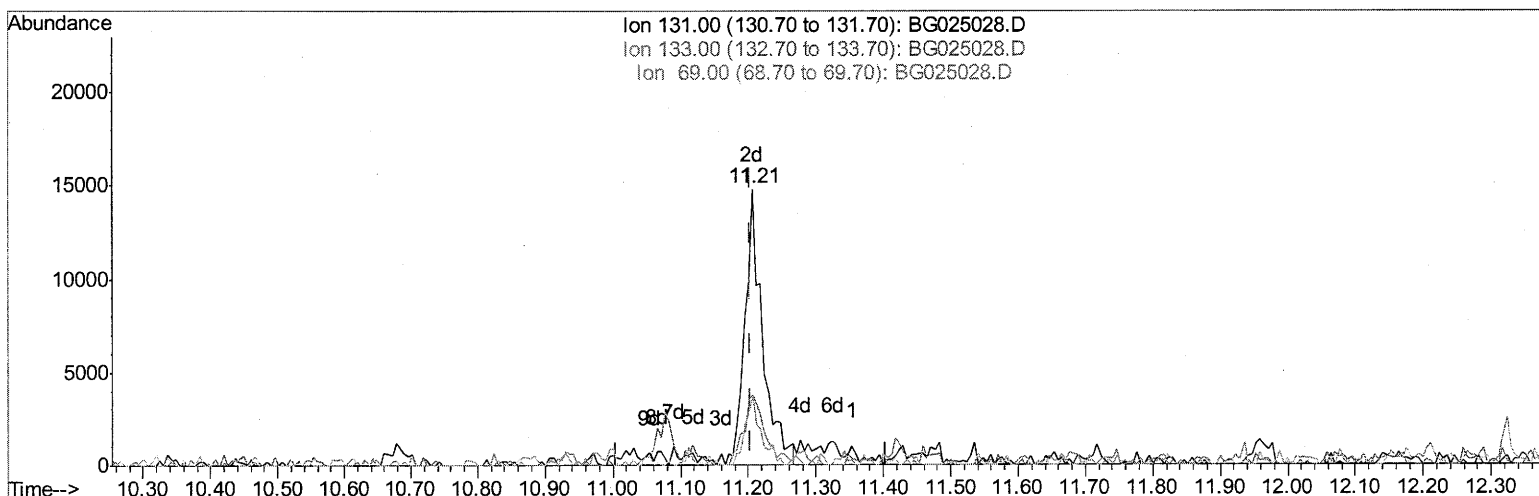

(29) 4-Chloroaniline-d4 (S)

11.207min (+0.002) 4.29ng/ul m

response 27396

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	25.68#
69.00	23.80	24.87
0.00	0.00	0.00

UM

12/09/16

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120816\
 Data File : BG025028.D
 Acq On : 9 Dec 2016 5:09
 Operator : UM/SJ
 Sample : H5863-20 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DA800

Manual Integrations
 APPROVED

sohil
 12/9/2016 3:42:01 PM

Quant Time: Dec 09 06:57:37 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 01:31:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.25	152	90760	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	382810	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.86	164	316256	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.60	188	695735	20.00	ng/ul	0.00
75) Chrysene-d12	21.89	240	855282	20.00	ng/ul	0.00
83) Perylene-d12	25.31	264	914079	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.60	96	2756	1.57	ng/uL	0.00
5) Phenol-d5	7.39	99	65015	8.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.56	67	40236	8.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.77	132	46407	8.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.94	113	55297	8.45	ng/ul	0.00
19) Nitrobenzene-d5	9.42	128	26181	9.66	ng/ul	0.00
22) 2-Nitrophenol-d4	10.15	143	28826	8.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.68	165	54861	8.44	ng/ul	0.00
29) 4-Chloroaniline-d4	11.21	131	27396m	4.29	ng/ul	0.00
43) Dimethylphthalate-d6	14.26	166	212098	9.75	ng/ul	0.00
46) Acenaphthylene-d8	14.56	160	218182	9.16	ng/ul	0.00
51) 4-Nitrophenol-d4	15.05	143	21678	5.80	ng/ul	0.00
57) Fluorene-d10	15.85	176	183107	8.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.96	200	33558	7.80	ng/ul	0.00
70) Anthracene-d10	17.70	188	271827	9.26	ng/ul	0.00
76) Pyrene-d10	19.97	212	309738	8.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.07	264	314050	8.48	ng/ul	0.00

um
 12/09/16

Target Compounds

					Qvalue
6) Phenol	7.41	94	13740	1.71 ng/ul#	79
44) Dimethylphthalate	14.30	163	75039	3.51 ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed