

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
 Data File : BG051418.D
 Acq On : 8 Dec 2021 22:29
 Operator : CG/JU
 Sample : PB141247BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.531	3	7	14	rVB3	8213	12915	1.80%	0.179%
2	3.684	31	33	37	rVB3	1240	947	0.13%	0.013%
3	3.831	56	58	59	rBV	1032	756	0.11%	0.010%
4	3.966	77	81	94	rBV	77956	152288	21.24%	2.111%
5	4.301	135	138	143	rBV3	1893	2562	0.36%	0.036%
6	4.383	150	152	156	rVB3	953	1122	0.16%	0.016%
7	4.412	156	157	160	rBV3	814	824	0.11%	0.011%
8	4.747	212	214	216	rBV2	878	754	0.11%	0.010%
9	4.912	239	242	244	rVB3	928	821	0.11%	0.011%
10	5.094	271	273	277	rVB3	933	1170	0.16%	0.016%
11	5.135	277	280	281	rBV2	903	811	0.11%	0.011%
12	5.911	409	412	415	rBV2	521	791	0.11%	0.011%
13	6.310	477	480	482	rBV2	959	1290	0.18%	0.018%
14	6.516	510	515	516	rBV2	568	724	0.10%	0.010%
15	6.951	585	589	593	rBV3	693	1397	0.19%	0.019%
16	7.033	601	603	605	rBV	881	722	0.10%	0.010%
17	7.356	652	658	668	rBV	94523	184414	25.72%	2.557%
18	7.438	671	672	676	rBV2	769	743	0.10%	0.010%
19	7.503	676	683	694	rBV	81195	143718	20.04%	1.992%
20	7.720	713	720	729	rBV	100421	184460	25.72%	2.557%
21	7.861	743	744	749	rVB3	888	774	0.11%	0.011%
22	7.938	754	757	761	rBV4	891	1550	0.22%	0.021%
23	8.184	793	799	807	rVV	78947	141730	19.76%	1.965%
24	8.666	878	881	884	rVV2	765	1273	0.18%	0.018%
25	8.907	916	922	937	rBV	114629	227192	31.68%	3.150%
26	9.025	940	942	944	rVV2	1110	941	0.13%	0.013%
27	9.060	946	948	950	rVB2	943	838	0.12%	0.012%
28	9.189	967	970	975	rVB	859	1277	0.18%	0.018%
29	9.365	993	1000	1012	rBV	102774	189939	26.49%	2.633%
30	10.094	1117	1124	1137	rVV	86022	164990	23.01%	2.287%
31	10.200	1141	1142	1148	rVB2	891	1270	0.18%	0.018%
32	10.247	1148	1150	1153	rBV2	783	1138	0.16%	0.016%
33	10.652	1212	1219	1237	rVV	96339	210507	29.36%	2.918%
34	10.823	1246	1248	1253	rVV2	736	872	0.12%	0.012%
35	11.016	1273	1281	1289	rBV	115057	210302	29.33%	2.916%
36	11.157	1298	1305	1324	rBV	103311	228174	31.82%	3.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
 Data File : BG051418.D
 Acq On : 8 Dec 2021 22:29
 Operator : CG/JU
 Sample : PB141247BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK247

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

37	12.609	1548	1552	1556	rBV3	1801	2643	0.37%	0.037%
38	13.801	1752	1755	1759	rVB2	434	721	0.10%	0.010%
39	13.890	1767	1770	1776	rVB	557	942	0.13%	0.013%
40	14.213	1819	1825	1836	rBV	236210	373604	52.10%	5.180%
41	14.518	1870	1877	1890	rVB	275281	446848	62.31%	6.195%
42	14.824	1922	1929	1937	rBV	191385	311718	43.47%	4.322%
43	15.076	1966	1972	1990	rBV2	42502	127093	17.72%	1.762%
44	15.247	1999	2001	2004	rVB3	1310	1202	0.17%	0.017%
45	15.811	2090	2097	2106	rBV	337327	545235	76.03%	7.559%
46	15.952	2116	2121	2135	rBV	71514	138368	19.30%	1.918%
47	16.046	2135	2137	2143	rVB4	1971	3302	0.46%	0.046%
48	16.199	2161	2163	2167	rBV2	1255	1644	0.23%	0.023%
49	16.498	2210	2214	2218	rBV3	488	722	0.10%	0.010%
50	16.627	2234	2236	2242	rVB2	540	973	0.14%	0.013%
51	16.957	2288	2292	2294	rBV	606	826	0.12%	0.011%
52	17.039	2302	2306	2307	rBV2	582	740	0.10%	0.010%
53	17.056	2307	2309	2313	rVV2	614	720	0.10%	0.010%
54	17.573	2390	2397	2404	rBV	252970	384616	53.63%	5.332%
55	17.673	2407	2414	2426	rVB	399807	615054	85.77%	8.527%
56	18.537	2559	2561	2564	rVB3	887	738	0.10%	0.010%
57	18.566	2564	2566	2567	rBV2	1031	734	0.10%	0.010%
58	18.702	2587	2589	2590	rBV	1264	920	0.13%	0.013%
59	18.796	2601	2605	2607	rBV3	666	736	0.10%	0.010%
60	18.837	2608	2612	2613	rBV2	789	814	0.11%	0.011%
61	18.931	2626	2628	2630	rVB2	1129	725	0.10%	0.010%
62	19.048	2644	2648	2652	rVB4	1533	1939	0.27%	0.027%
63	19.101	2654	2657	2662	rBV5	1062	1843	0.26%	0.026%
64	19.224	2676	2678	2681	rBV2	800	860	0.12%	0.012%
65	19.313	2691	2693	2694	rBV	1661	1249	0.17%	0.017%
66	19.401	2704	2708	2709	rBV4	864	922	0.13%	0.013%
67	19.465	2718	2719	2720	rBV	1426	798	0.11%	0.011%
68	19.518	2723	2728	2732	rVV5	6423	8620	1.20%	0.120%
69	19.595	2736	2741	2748	rVV3	4620	8614	1.20%	0.119%
70	19.689	2753	2757	2759	rBV3	1336	1673	0.23%	0.023%
71	19.783	2772	2773	2775	rBV2	1120	934	0.13%	0.013%
72	19.953	2796	2802	2811	rVB	480665	717103	100.00%	9.942%
73	20.229	2847	2849	2850	rBV2	1173	1036	0.14%	0.014%
74	21.874	3123	3129	3140	rVB2	218021	402373	56.11%	5.578%
75	23.355	3379	3381	3387	rVB7	5899	9392	1.31%	0.130%
76	25.041	3658	3668	3680	rVB2	213578	632550	88.21%	8.770%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
Data File : BG051418.D
Acq On : 8 Dec 2021 22:29
Operator : CG/JU
Sample : PB141247BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK247

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Title : SVOA CALIBRATION

77	25.270	3699	3707	3722	rVB2	122776	385418	53.75%	5.343%
----	--------	------	------	------	------	--------	--------	--------	--------




Sum of corrected areas: 7212958

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
Data File : BG051418.D
Acq On : 8 Dec 2021 22:29
Operator : CG/JU
Sample : PB141247BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK247

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

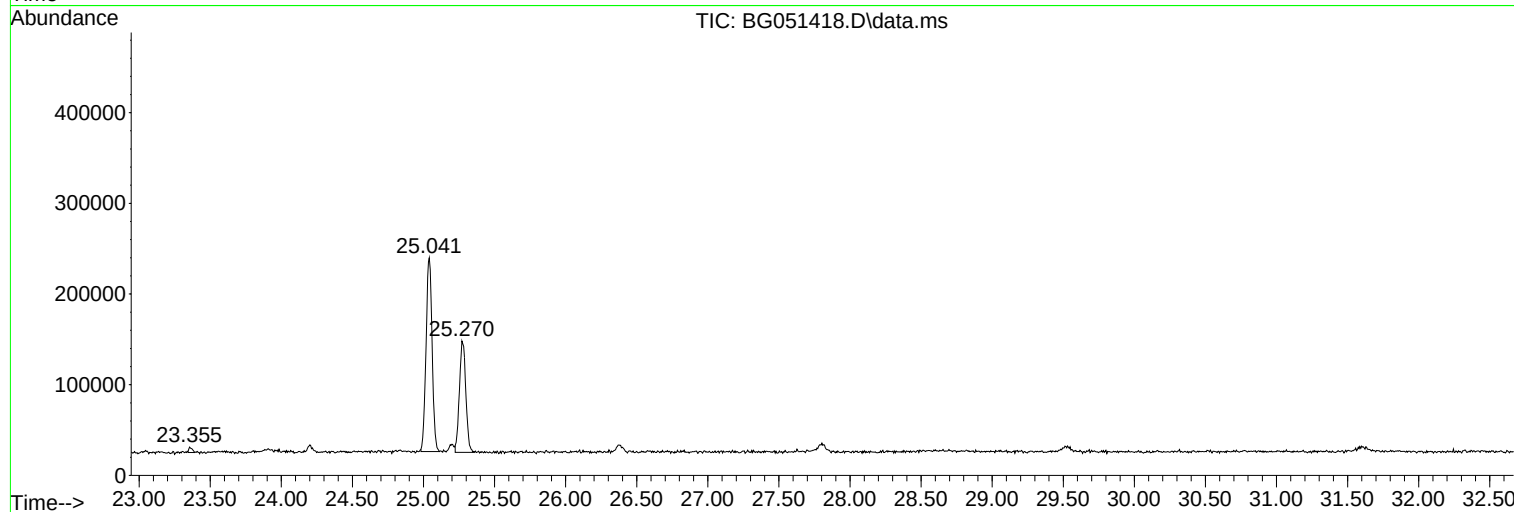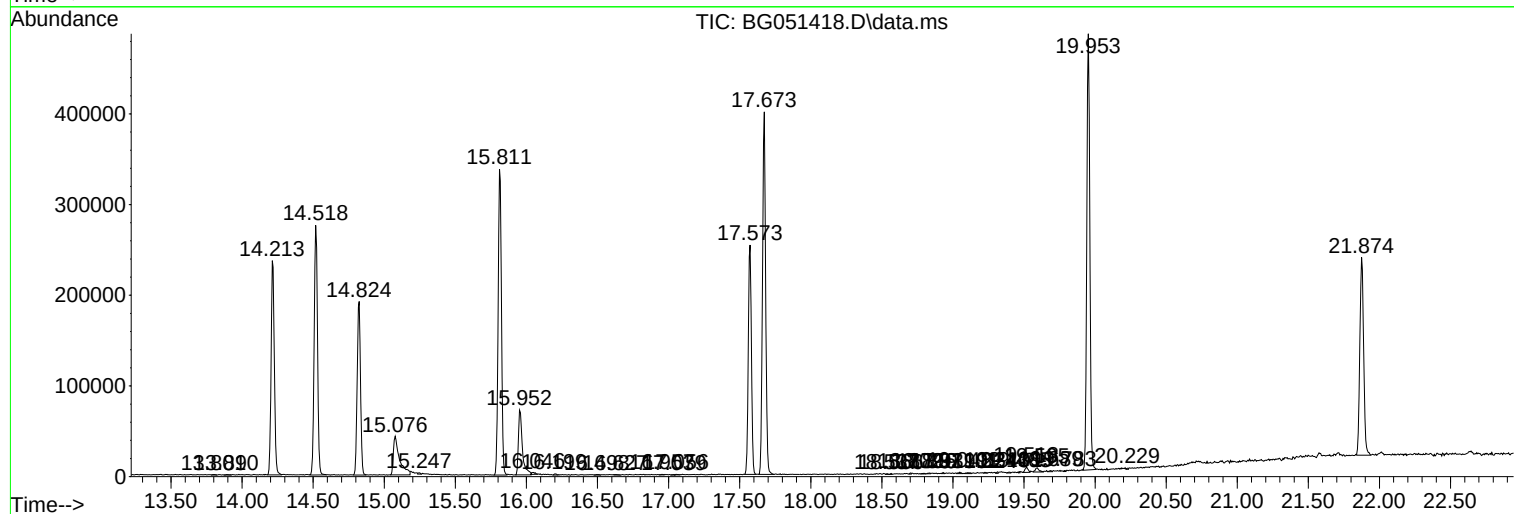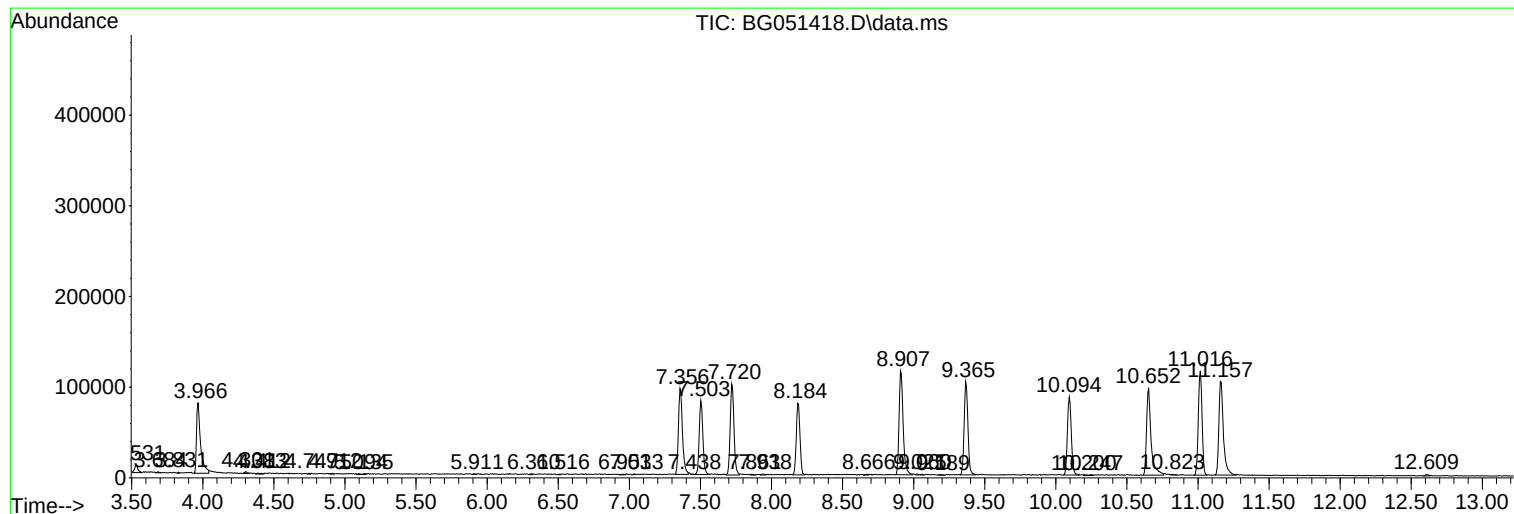

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
Data File : BG051418.D
Acq On : 8 Dec 2021 22:29
Operator : CG/JU
Sample : PB141247BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK247

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
Data File : BG051418.D
Acq On : 8 Dec 2021 22:29
Operator : CG/JU
Sample : PB141247BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK247

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc