

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
 Data File : BG051422.D
 Acq On : 9 Dec 2021 1:12
 Operator : CG/JU
 Sample : M4960-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.529	3	7	16	rVB2	5707	9175	1.03%	0.131%
2	3.729	40	41	43	rBV	1167	910	0.10%	0.013%
3	3.882	64	67	69	rBV2	899	1009	0.11%	0.014%
4	3.976	79	83	90	rBV	20946	41125	4.62%	0.588%
5	4.193	115	120	124	rVB4	3361	4926	0.55%	0.070%
6	4.299	133	138	145	rVB5	2122	4777	0.54%	0.068%
7	4.399	153	155	157	rBV	753	890	0.10%	0.013%
8	4.675	198	202	206	rBV3	2601	4146	0.47%	0.059%
9	6.655	536	539	541	rBV2	774	994	0.11%	0.014%
10	6.866	571	575	577	rVB2	849	1165	0.13%	0.017%
11	6.896	577	580	584	rBV3	810	1530	0.17%	0.022%
12	7.125	614	619	620	rBV	828	949	0.11%	0.014%
13	7.336	650	655	656	rBV2	3356	5160	0.58%	0.074%
14	7.372	656	661	670	rVB	15205	32804	3.69%	0.469%
15	7.501	677	683	695	rBV	87721	157064	17.65%	2.247%
16	7.724	715	721	732	rBV	62643	114135	12.83%	1.633%
17	8.188	793	800	805	rBV	76942	138862	15.60%	1.987%
18	8.229	805	807	815	rVB2	9330	14422	1.62%	0.206%
19	8.917	917	924	934	rVV	49097	101874	11.45%	1.458%
20	9.029	937	943	950	rVB4	3863	7849	0.88%	0.112%
21	9.299	984	989	994	rBV2	4450	7895	0.89%	0.113%
22	9.369	994	1001	1016	rVB	112905	208195	23.40%	2.979%
23	9.810	1072	1076	1078	rVB2	639	905	0.10%	0.013%
24	10.092	1119	1124	1130	rVB2	4302	6832	0.77%	0.098%
25	10.304	1157	1160	1165	rVB2	703	1236	0.14%	0.018%
26	10.656	1215	1220	1233	rBV2	27963	65855	7.40%	0.942%
27	10.738	1233	1234	1237	rVV3	2466	1827	0.21%	0.026%
28	10.785	1237	1242	1254	rVV5	5972	15560	1.75%	0.223%
29	11.014	1274	1281	1292	rVB	115896	212128	23.84%	3.035%
30	11.161	1298	1306	1327	rVB	112387	242492	27.25%	3.470%
31	11.825	1415	1419	1422	rVB2	723	1009	0.11%	0.014%
32	12.401	1514	1517	1520	rVB2	1047	1266	0.14%	0.018%
33	12.430	1520	1522	1528	rBV2	842	1046	0.12%	0.015%
34	12.601	1546	1551	1555	rVB3	1941	3216	0.36%	0.046%
35	13.165	1643	1647	1650	rBV2	1532	2064	0.23%	0.030%
36	13.406	1681	1688	1693	rVB4	2950	4797	0.54%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
 Data File : BG051422.D
 Acq On : 9 Dec 2021 1:12
 Operator : CG/JU
 Sample : M4960-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

37	13.682	1726	1735	1741	rBV5	9299	17825	2.00%	0.255%
38	14.146	1809	1814	1815	rBV2	604	930	0.10%	0.013%
39	14.217	1818	1826	1838	rBV	269403	409333	46.00%	5.857%
40	14.516	1870	1877	1887	rBV	299432	485492	54.56%	6.947%
41	14.822	1918	1929	1936	rBV	184108	300325	33.75%	4.297%
42	14.886	1936	1940	1944	rVB2	2188	3110	0.35%	0.044%
43	15.580	2054	2058	2061	rBV	1764	2297	0.26%	0.033%
44	15.621	2061	2065	2070	rVB3	1817	2651	0.30%	0.038%
45	15.809	2091	2097	2108	rBV	384842	621190	69.80%	8.888%
46	16.050	2135	2138	2143	rBV3	1197	1861	0.21%	0.027%
47	16.097	2143	2146	2149	rVB3	1416	1149	0.13%	0.016%
48	16.179	2152	2160	2167	rVB3	4789	8770	0.99%	0.125%
49	16.408	2194	2199	2201	rBV3	764	1131	0.13%	0.016%
50	16.960	2289	2293	2295	rBV2	667	993	0.11%	0.014%
51	17.143	2321	2324	2328	rBV3	1094	1943	0.22%	0.028%
52	17.272	2342	2346	2350	rVB3	694	1086	0.12%	0.016%
53	17.489	2381	2383	2390	rBV3	1344	2005	0.23%	0.029%
54	17.571	2390	2397	2405	rVV	234304	360426	40.50%	5.157%
55	17.671	2407	2414	2430	rVB2	477151	769559	86.48%	11.011%
56	17.818	2435	2439	2446	rVB	5362	7288	0.82%	0.104%
57	18.065	2478	2481	2488	rBV3	1353	2110	0.24%	0.030%
58	18.200	2499	2504	2511	rVB5	11718	20134	2.26%	0.288%
59	18.259	2511	2514	2520	rBV4	883	1590	0.18%	0.023%
60	18.418	2538	2541	2544	rVB	789	963	0.11%	0.014%
61	18.441	2544	2545	2548	rBV3	1066	976	0.11%	0.014%
62	18.500	2551	2555	2560	rVV	12521	15640	1.76%	0.224%
63	18.553	2560	2564	2565	rVB3	946	1122	0.13%	0.016%
64	18.606	2571	2573	2578	rVB3	1213	1592	0.18%	0.023%
65	18.641	2578	2579	2581	rBV2	1228	1046	0.12%	0.015%
66	18.705	2586	2590	2593	rBV3	831	1646	0.18%	0.024%
67	18.940	2626	2630	2631	rBV3	950	1186	0.13%	0.017%
68	18.952	2631	2632	2635	rVV2	1597	1510	0.17%	0.022%
69	19.011	2639	2642	2643	rBV2	1810	1183	0.13%	0.017%
70	19.070	2650	2652	2653	rVB	1596	969	0.11%	0.014%
71	19.081	2653	2654	2655	rBV	1675	917	0.10%	0.013%
72	19.240	2680	2681	2684	rBV2	1347	1005	0.11%	0.014%
73	19.281	2685	2688	2692	rVV5	1359	1990	0.22%	0.028%
74	19.316	2692	2694	2697	rVV3	1477	1462	0.16%	0.021%
75	19.358	2697	2701	2705	rVB3	6869	8268	0.93%	0.118%
76	19.516	2723	2728	2732	rVB5	5742	7829	0.88%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
 Data File : BG051422.D
 Acq On : 9 Dec 2021 1:12
 Operator : CG/JU
 Sample : M4960-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGKR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
 Title : SVOA CALIBRATION

77	19.593	2736	2741	2746	rBV3	6797	9681	1.09%	0.139%
78	19.787	2771	2774	2775	rBV3	997	934	0.10%	0.013%
79	19.822	2778	2780	2783	rVB3	1443	1658	0.19%	0.024%
80	19.951	2796	2802	2812	rVB	599673	889894	100.00%	12.733%
81	20.145	2833	2835	2836	rBV	1975	1139	0.13%	0.016%
82	20.268	2854	2856	2859	rBV3	1738	2253	0.25%	0.032%
83	20.926	2966	2968	2971	rBV4	3735	4469	0.50%	0.064%
84	21.872	3123	3129	3139	rVB	214919	382758	43.01%	5.477%
85	23.365	3379	3383	3388	rVB7	7067	12024	1.35%	0.172%
86	25.039	3657	3668	3681	rVB2	273229	822153	92.39%	11.764%
87	25.274	3699	3708	3721	rVB2	119989	369308	41.50%	5.284%




Sum of corrected areas: 6988862

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
Data File : BG051422.D
Acq On : 9 Dec 2021 1:12
Operator : CG/JU
Sample : M4960-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

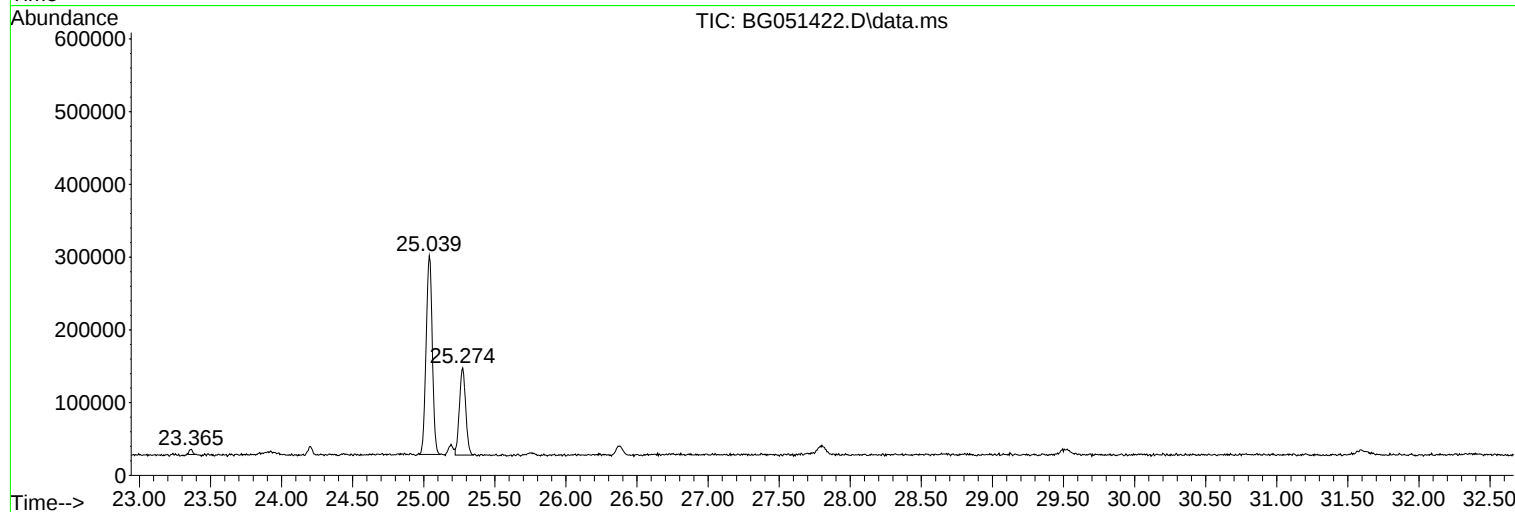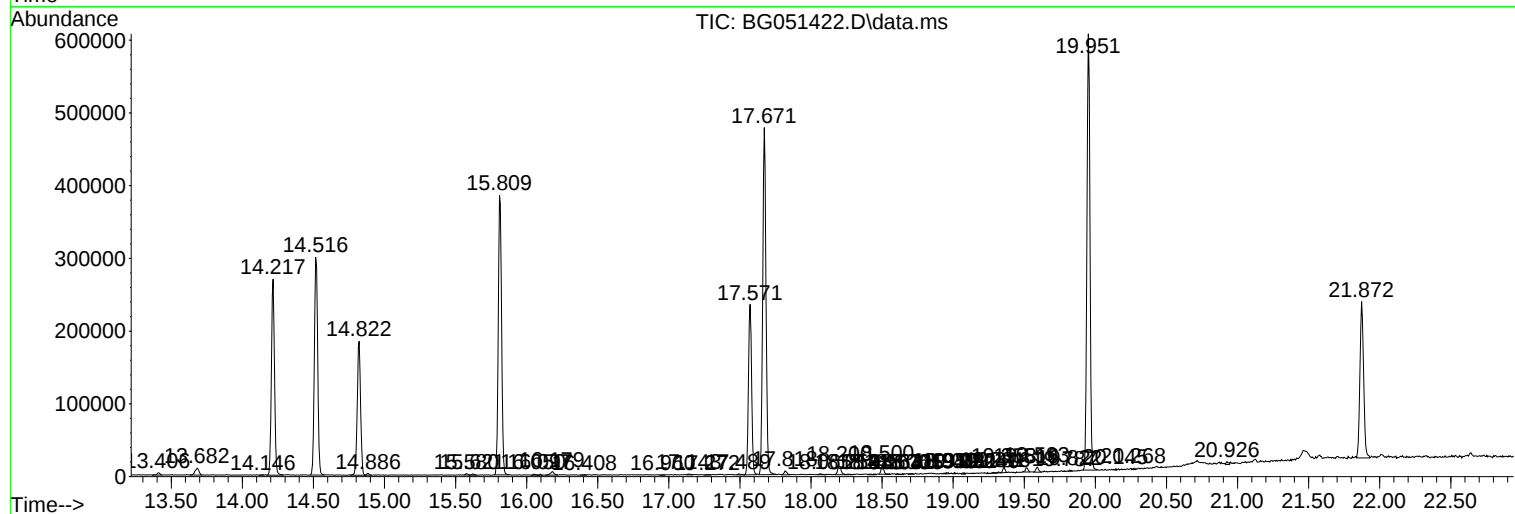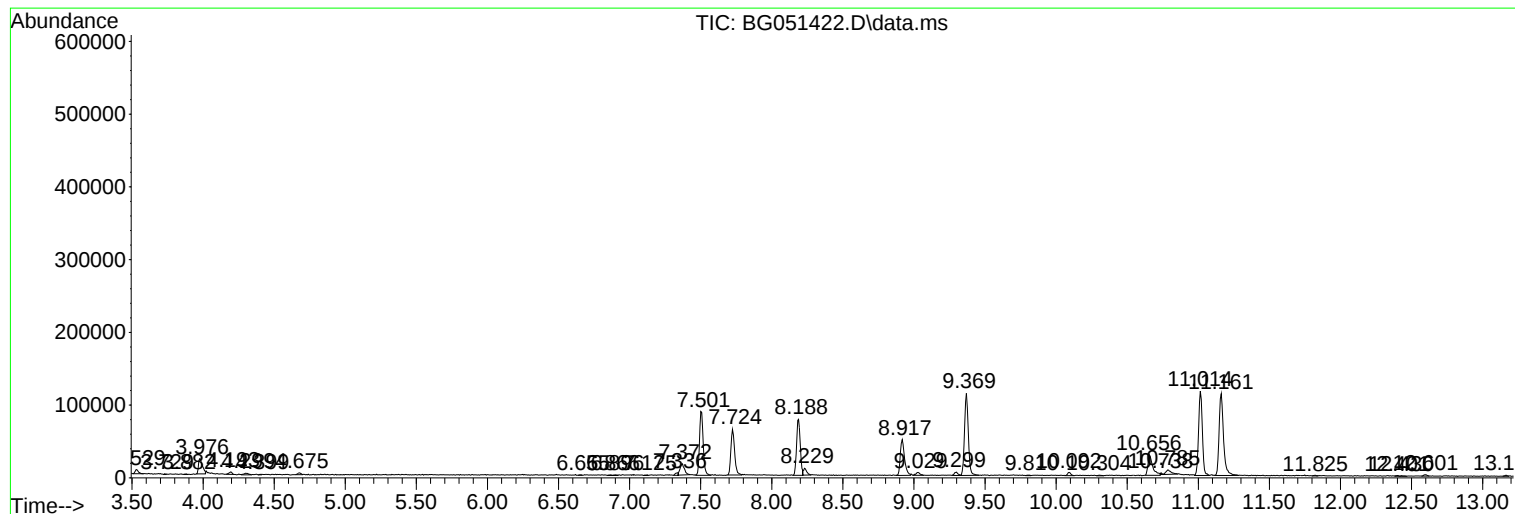

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
Data File : BG051422.D
Acq On : 9 Dec 2021 1:12
Operator : CG/JU
Sample : M4960-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120821\
Data File : BG051422.D
Acq On : 9 Dec 2021 1:12
Operator : CG/JU
Sample : M4960-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGKR6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120821.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc