


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG120915\
 Data File : BG020024.D
 Acq On : 9 Dec 2015 2:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 18:50:01 2015

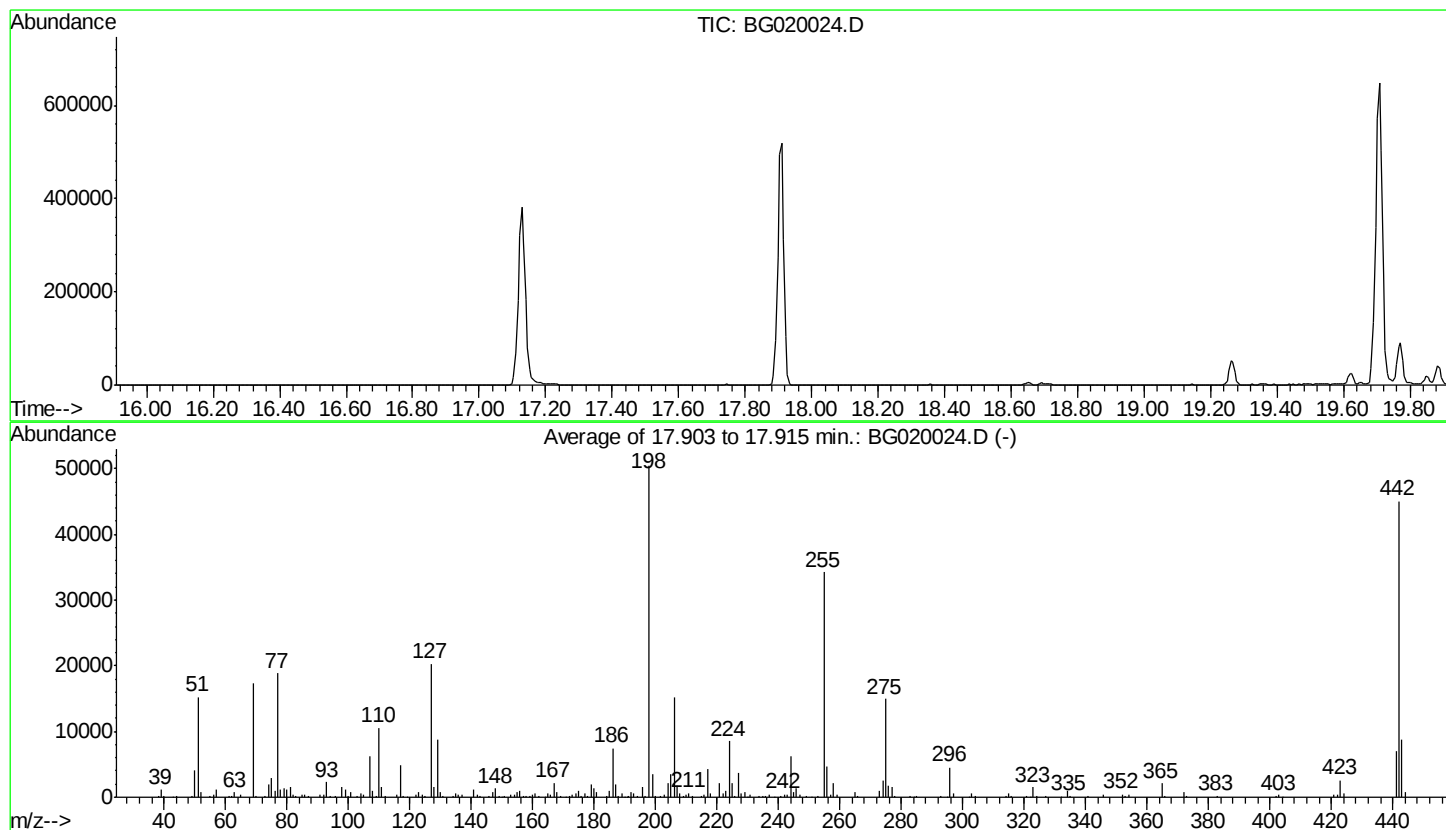

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	15235	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.2	17275	PASS
70	69	0.00	2	0.7	120	PASS
127	198	10	80	40.3	20306	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50448	PASS
199	198	5	9	6.8	3444	PASS
275	198	10	60	29.7	14978	PASS
365	198	1	100	4.1	2083	PASS
441	442	0.01	24	15.4	6953	PASS
442	198	50	100	89.3	45026	PASS
443	442	15	24	19.4	8736	PASS