

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120916\
 Data File : BG025037.D
 Acq On : 9 Dec 2016 13:27
 Operator : UM/SJ
 Sample : H5863-03DL2 30X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DA7Y2DL2

Manual Integrations
 APPROVED

Sohil
 12/12/2016 4:28:11 PM

Quant Time: Dec 12 01:22:31 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 11 23:54:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.25	152	85597	20.00	ng/ul	0.01
18) Naphthalene-d8	11.08	136	359348	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.87	164	285082	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.61	188	572446	20.00	ng/ul	0.00
75) Chrysene-d12	21.91	240	701885	20.00	ng/ul	0.00
83) Perylene-d12	25.32	264	721368	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.60	96	1694	1.02	ng/uL	0.00
5) Phenol-d5	7.40	99	6857	0.93	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.56	67	6991	1.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.77	132	4756	0.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.95	113	6819	1.10	ng/ul	0.01
19) Nitrobenzene-d5	9.43	128	2723	1.07	ng/ul	0.00
22) 2-Nitrophenol-d4	10.15	143	3415	1.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.69	165	8188	1.34	ng/ul	0.01
29) 4-Chloroaniline-d4	11.21	131	48993	8.17	ng/ul	0.00
43) Dimethylphthalate-d6	14.26	166	26508	1.35	ng/ul	0.00
46) Acenaphthylene-d8	14.57	160	31896	1.48	ng/ul	0.01
51) 4-Nitrophenol-d4	15.06	143	7253	2.15	ng/ul	0.01
57) Fluorene-d10	15.85	176	28989	1.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.98	200	5458	1.54	ng/ul	0.01
70) Anthracene-d10	17.71	188	38933	1.61	ng/ul	0.00
76) Pyrene-d10	19.98	212	40695	1.41	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.08	264	40420	1.38	ng/ul	0.01

Target Compounds

						Ovalue
6) Phenol	7.43	94	56746	7.49	ng/ul#	84
11) 2-Methylphenol	8.69	108	141759	25.40	ng/ul	88
14) Acetophenone	9.08	105	67492m	7.19	ng/ul	
16) 4-Methylphenol	9.01	108	260512	41.96	ng/ul	93
24) 2,4-Dimethylphenol	10.23	107	559858m	76.08	ng/ul	
28) Naphthalene	11.13	128	340989	20.41	ng/ul	97
34) 2-Methylnaphthalene	12.72	142	722199	54.79	ng/ul	91
40) 1,1'-Biophenyl	13.70	154	138935	8.04	ng/ul	97
49) Acenaphthene	14.94	153	40435	2.83	ng/ul#	90
53) Dibenzofuran	15.27	168	87334	3.86	ng/ul	93
58) Fluorene	15.91	166	97095	5.27	ng/ul#	97
69) Phenanthrene	17.65	178	39368	1.44	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG120916\
Data File : BG025037.D
Acq On : 9 Dec 2016 13:27
Operator : UM/SJ
Sample : H5863-03DL2 30X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
DA7Y2DL2

Quant Time: Dec 12 01:22:31 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 11 23:54:53 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/12/2016 4:28:11 PM

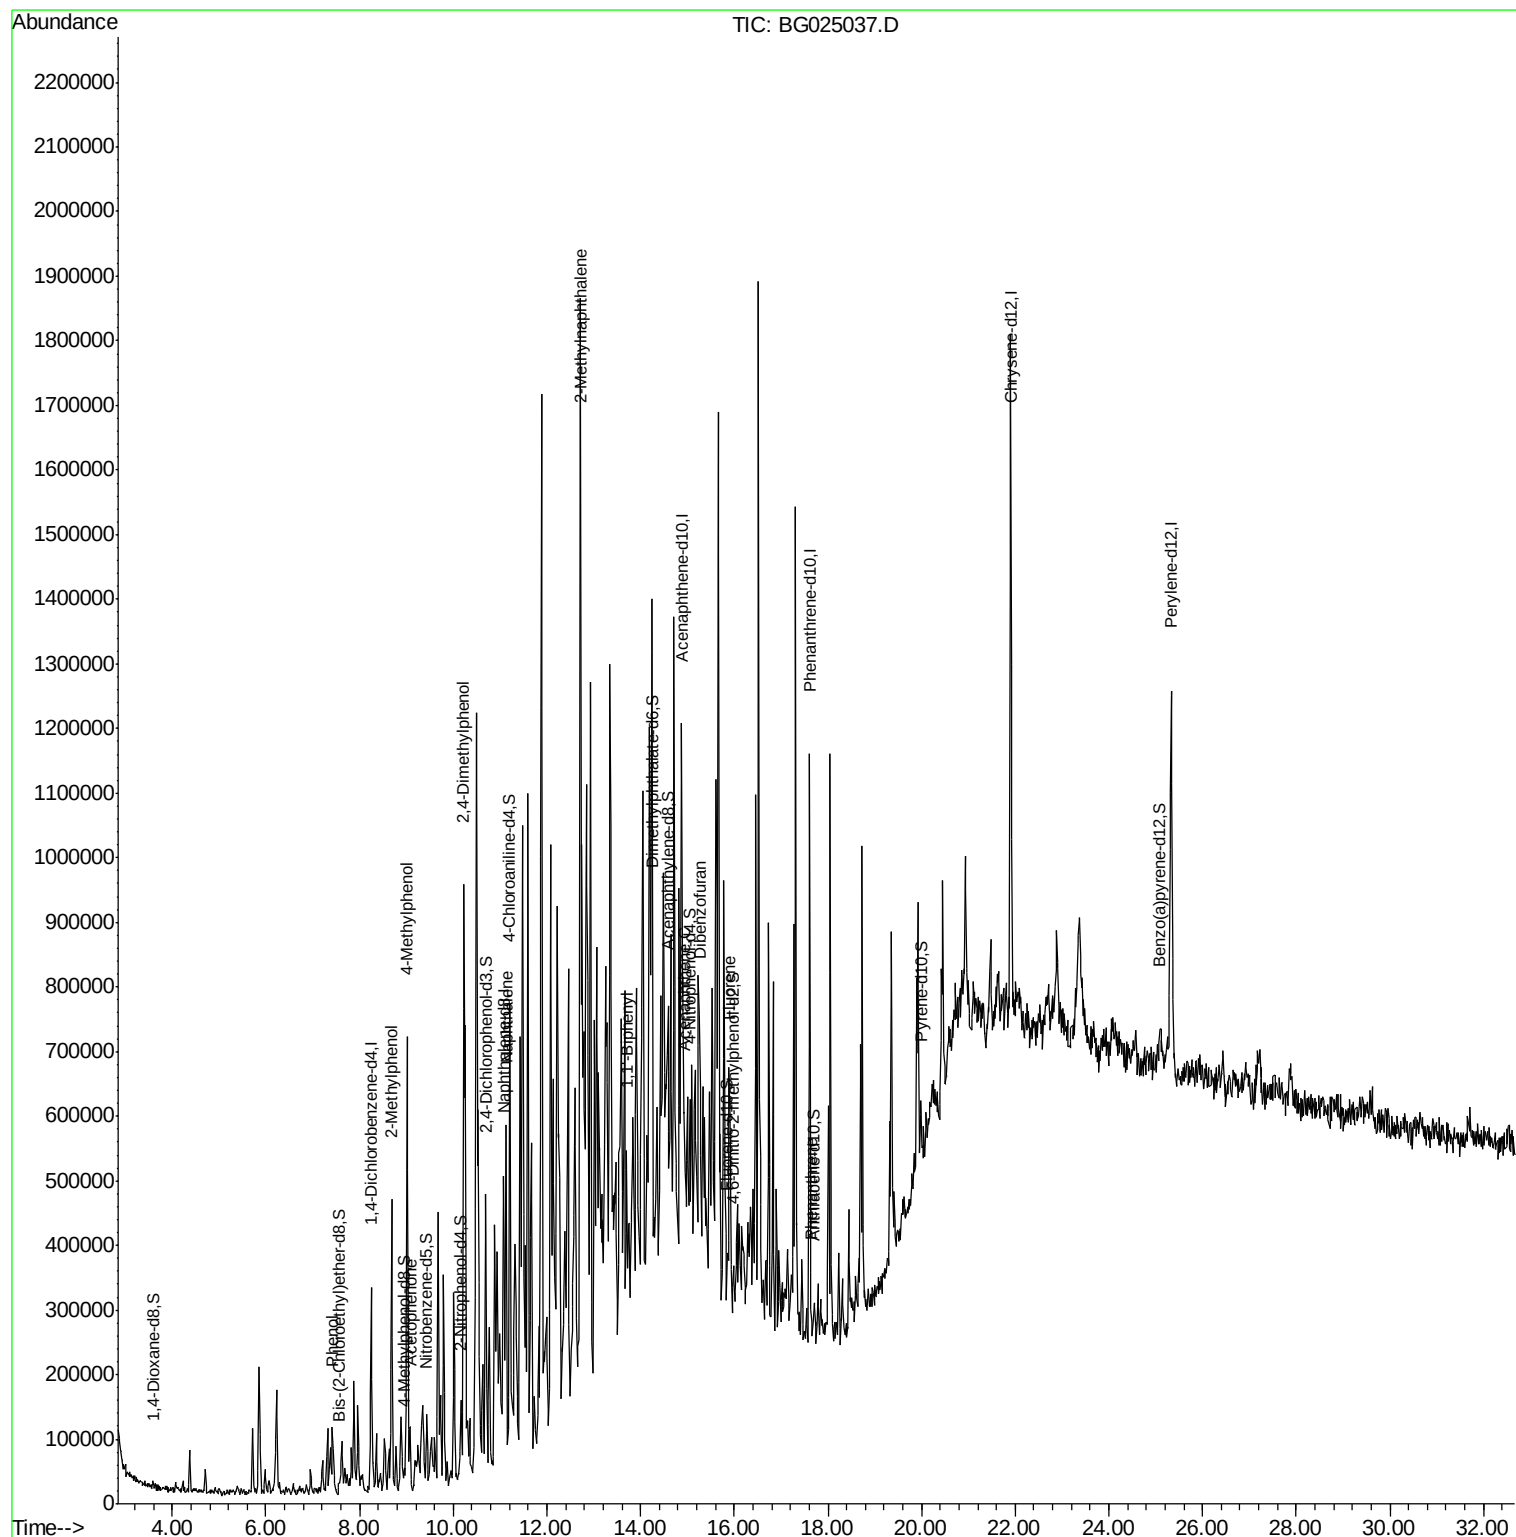

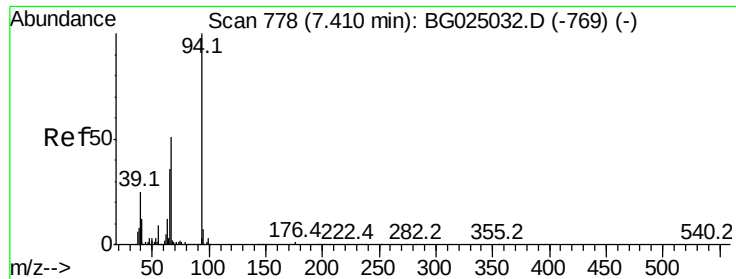

#6

Phenol

Concen: 7.49 ng/ul

RT: 7.43 min Scan# 781

Delta R.T. 0.02 min

Lab File: BG025037.D

Acq: 9 Dec 2016 13:27

Instrument :

BNA_G




ClientSampleId :

DA7Y2DL2

Tot Ion	Ratio	Lower	Upper
94	100		
65	33.9	26.8	40.2
66	36.8	44.4	66.6#

Manual Integrations
APPROVED

Sohil
12/12/2016 4:28:11 PM

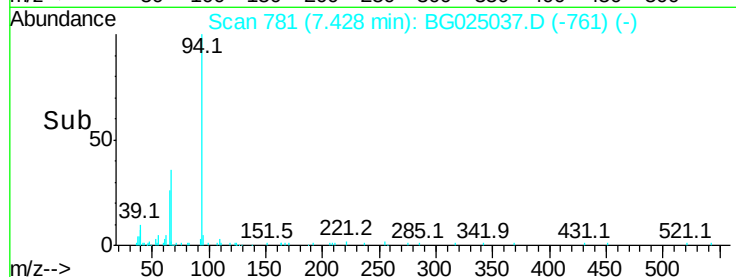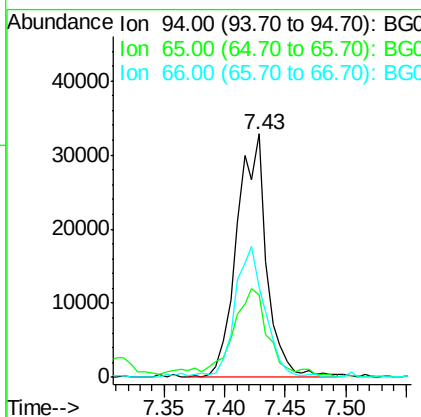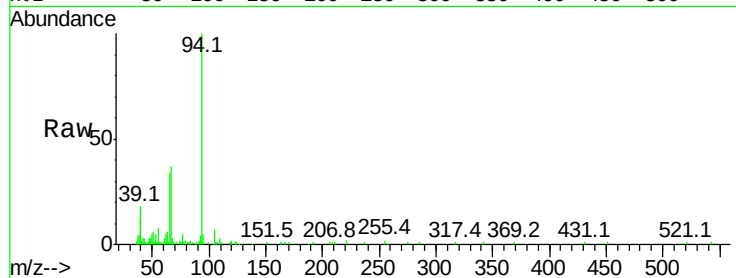

#11

2-Methylphenol

Concen: 25.40 ng/ul





RT: 8.69 min Scan# 995


Delta R.T. 0.01 min

Lab File: BG025037.D

Acq: 9 Dec 2016 13:27

Tgt Ion	Ratio	Lower	Upper
108	100		
107	84.5	76.7	115.1

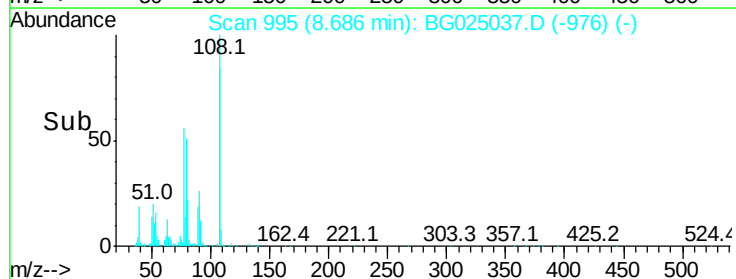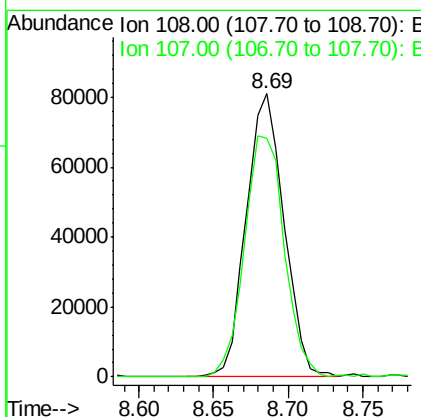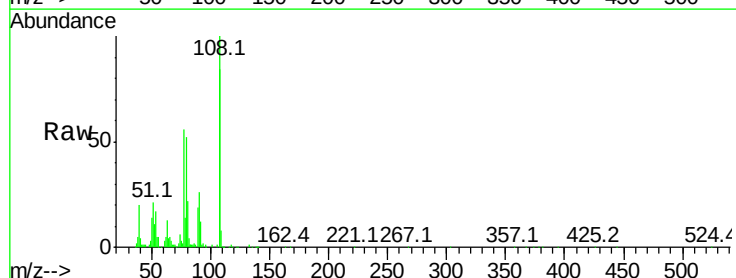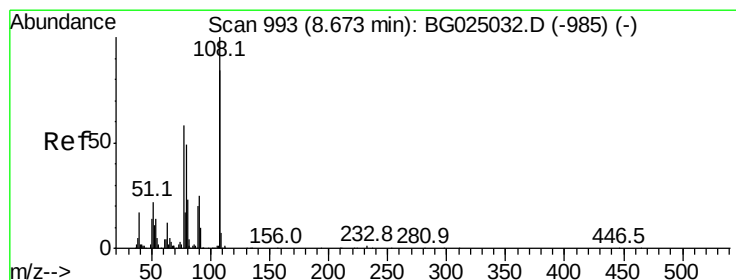

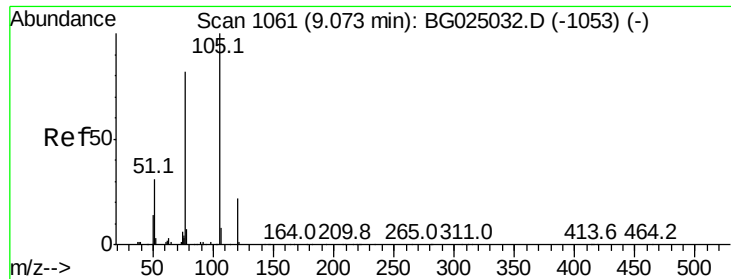





#14
Acetophenone
Concen: 7.19 ng/ul m
RT: 9.08 min Scan# 1062
Delta R.T. 0.01 min
Lab File: BG025037.D
Acq: 9 Dec 2016 13:27

Instrument :
BNA_G
ClientSampleId :
DA7Y2DL2

Tot Ion	Ratio	Lower	Upper
105	100		
77	88.7	76.0	114.0
51	27.8	34.8	52.2#




Manual Integrations
APPROVED


Sohil
12/12/2016 4:28:11 PM

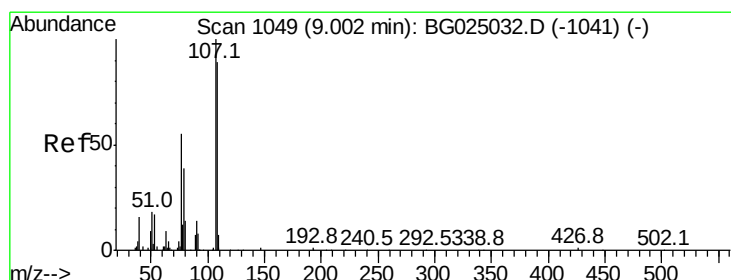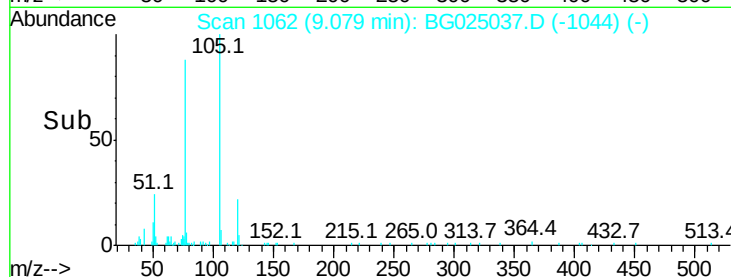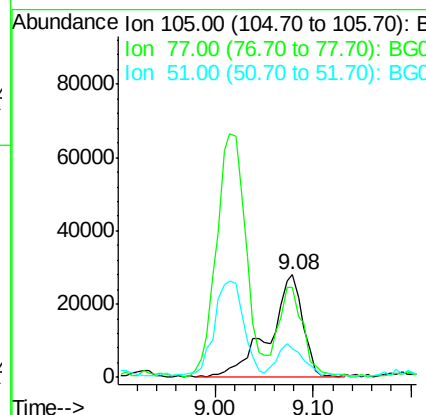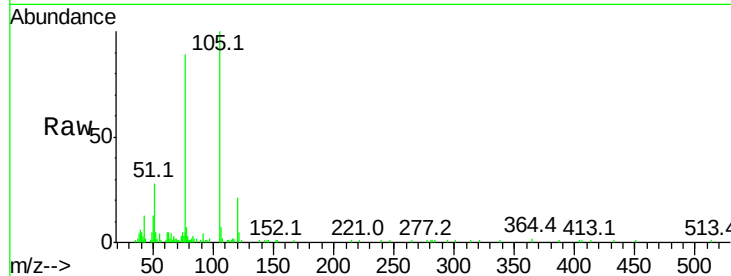

#16
4-Methylphenol
Concen: 41.96 ng/ul
RT: 9.01 min Scan# 1051
Delta R.T. 0.01 min
Lab File: BG025037.D
Acq: 9 Dec 2016 13:27

Tgt Ion	Ratio	Lower	Upper
108	100		
107	107.4	91.7	137.5

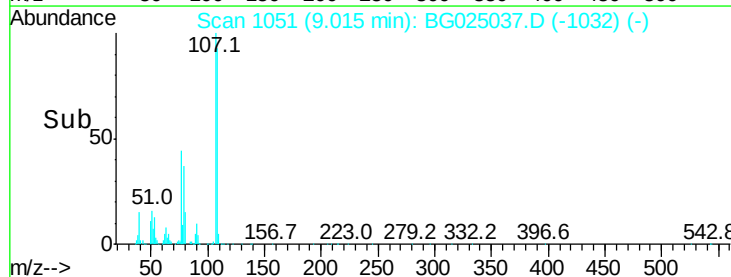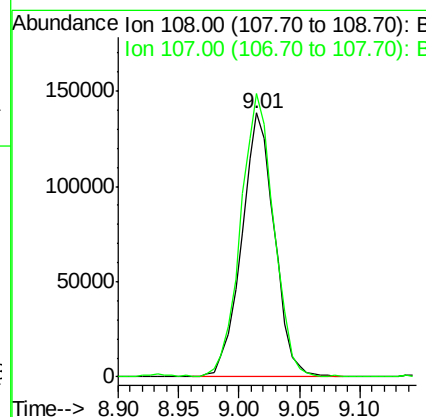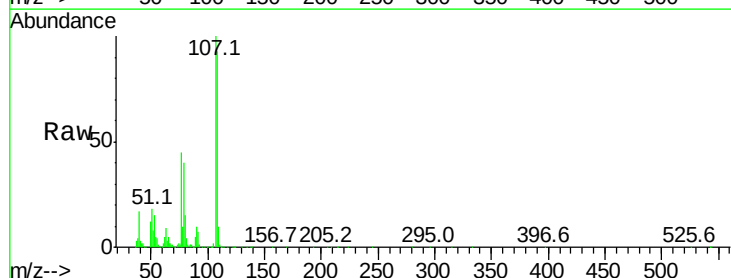

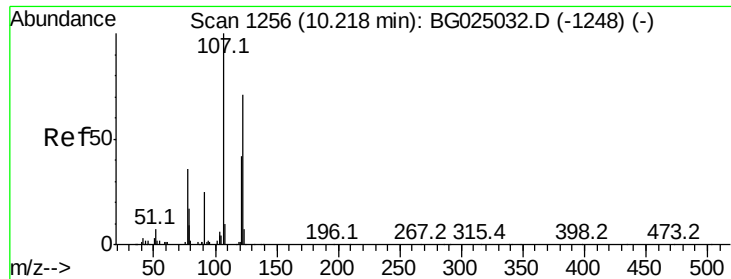





#24
2,4-Dimethylphenol
Concen: 76.08 ng/ul m
RT: 10.23 min Scan# 1258
Delta R.T. 0.01 min
Lab File: BG025037.D
Acq: 9 Dec 2016 13:27

Instrument :
BNA_G
ClientSampleId :
DA7Y2DL2

Tot Ion	Ratio	Resp Lower	Upper
107	100		
121	40.3	32.3	48.5
122	68.1	61.2	91.8




Manual Integrations
APPROVED


Sohil
12/12/2016 4:28:11 PM

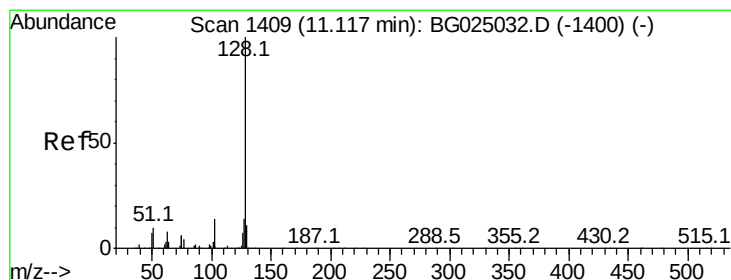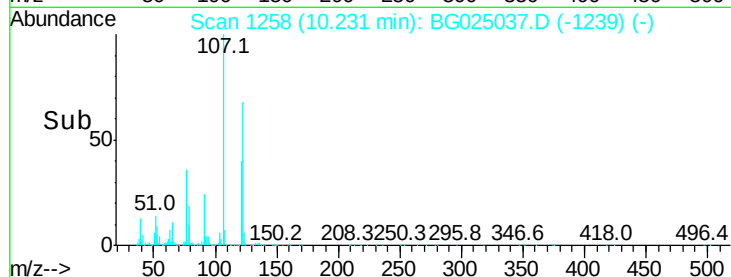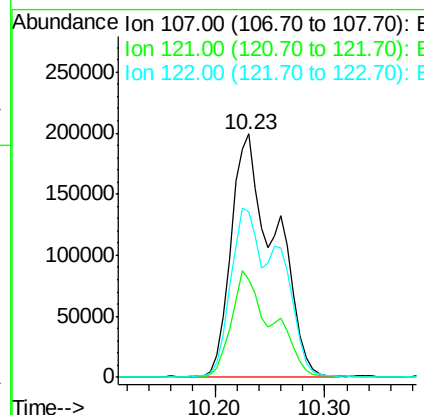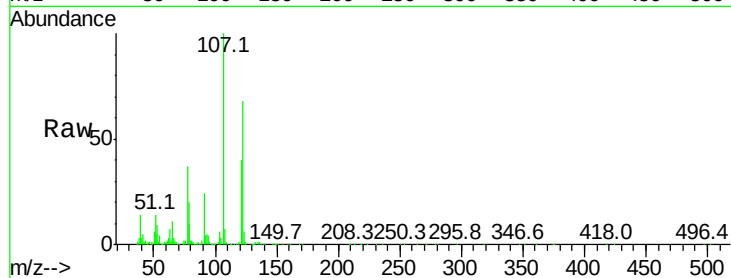

#28
Naphthalene
Concen: 20.41 ng/ul
RT: 11.13 min Scan# 1411
Delta R.T. 0.01 min
Lab File: BG025037.D
Acq: 9 Dec 2016 13:27

Tgt Ion	Ratio	Resp Lower	Upper
128	100		
129	10.3	9.4	14.2
127	14.1	10.3	15.5

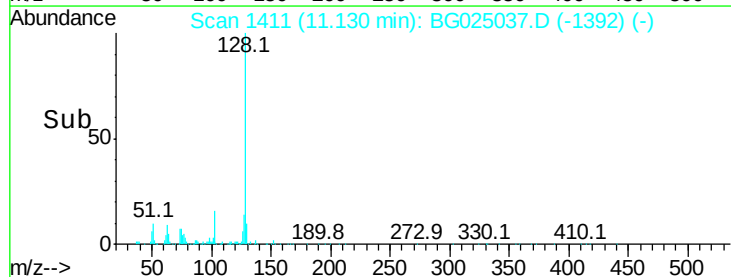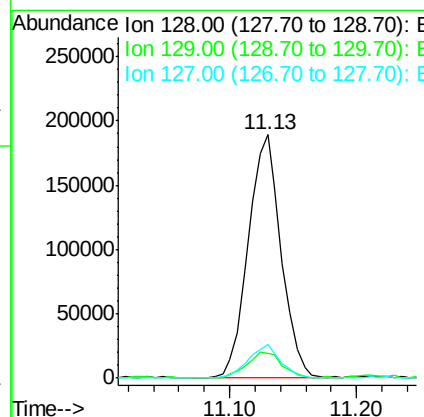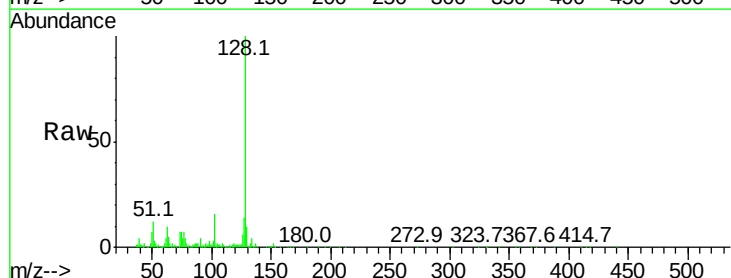

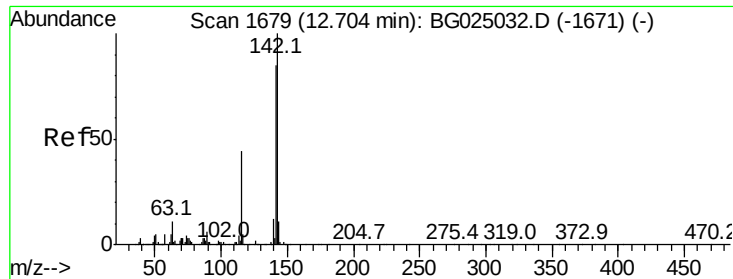





#34
 2-Methylnaphthalene
 Concen: 54.79 ng/ul
 RT: 12.72 min Scan# 1681
 Delta R.T. 0.01 min
 Lab File: BG025037.D
 Acq: 9 Dec 2016 13:27

Instrument :
 BNA_G
 ClientSampleId :
 DA7Y2DL2

Tot Ion	Ratio	Resp	Lower	Upper
142	100	722199		
141	94.1	68.6	102.8	




Manual Integrations
 APPROVED


Sohil
 12/12/2016 4:28:11 PM

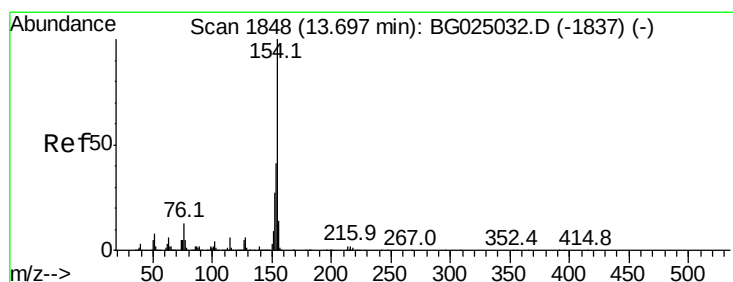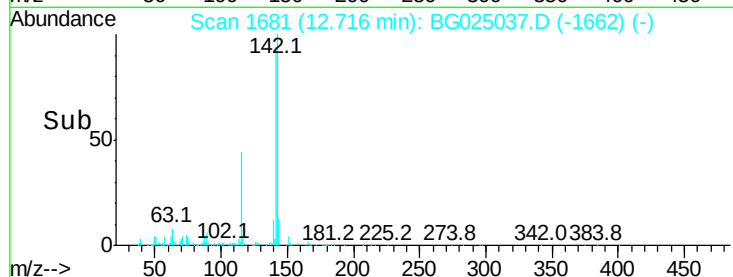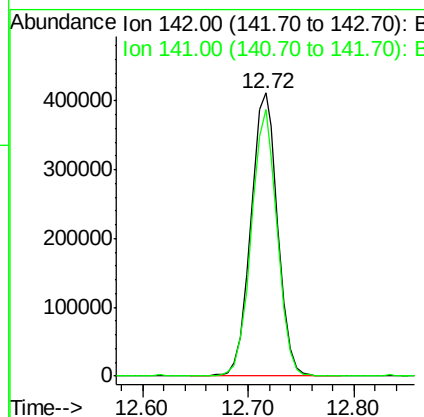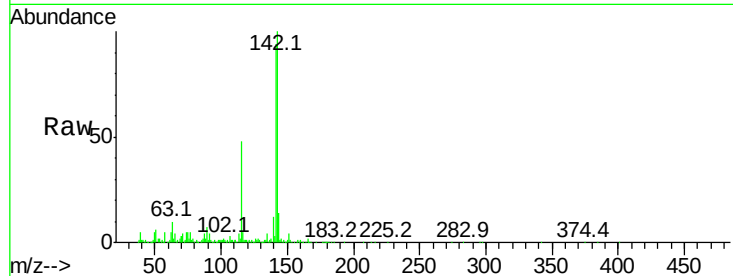

#40
 1,1'-Biphenyl
 Concen: 8.04 ng/ul
 RT: 13.70 min Scan# 1849
 Delta R.T. 0.01 min
 Lab File: BG025037.D
 Acq: 9 Dec 2016 13:27

Tgt Ion	Ratio	Resp	Lower	Upper
154	100	138935		
153	42.4	32.2	48.2	
76	11.1	9.6	14.4	

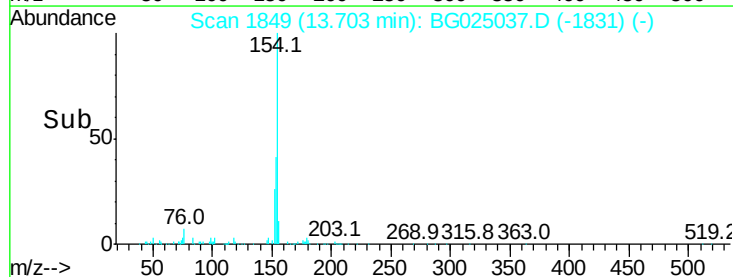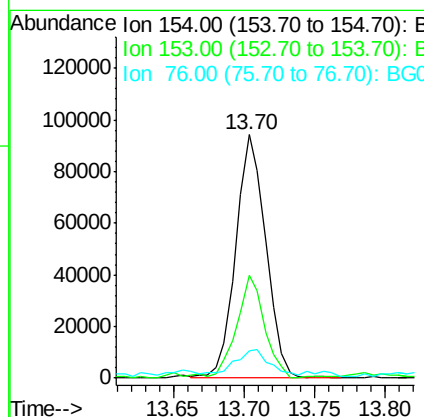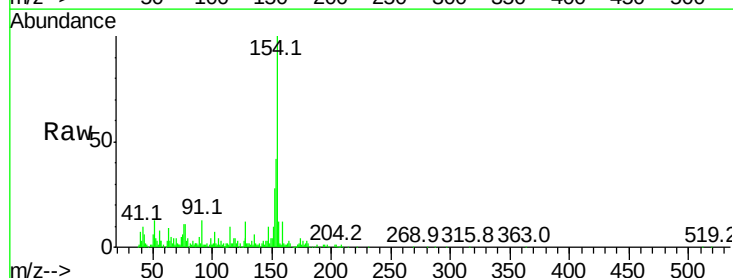

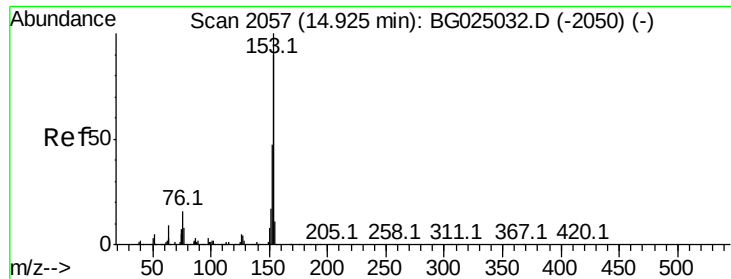

#49

Acenaphthene

Concen: 2.83 ng/ul

RT: 14.94 min Scan# 2059

Delta R.T. 0.01 min

Lab File: BG025037.D

Acq: 9 Dec 2016 13:27

Instrument :

BNA_G





ClientSampleId :

DA7Y2DL2

Tot Ion:	153	Resp:	40435
Ion Ratio	Lower	Upper	
153	100		
152	57.3	36.5	54.7#
154	84.5	72.3	108.5

Manual Integrations
APPROVED

Sohil
12/12/2016 4:28:11 PM

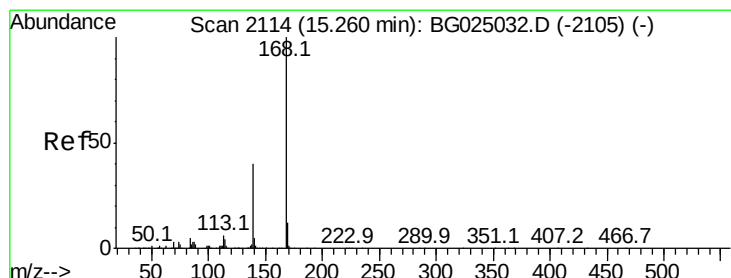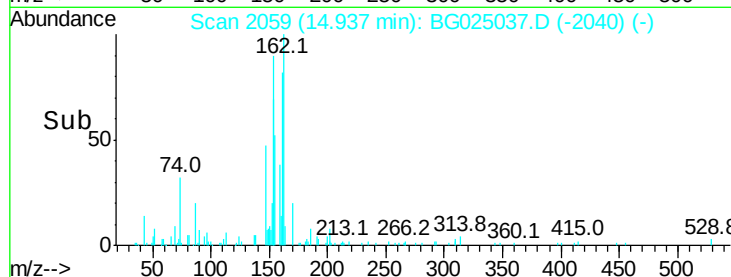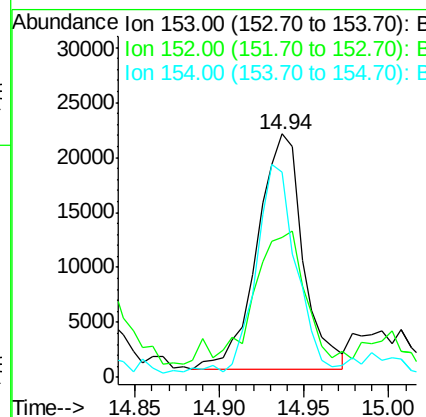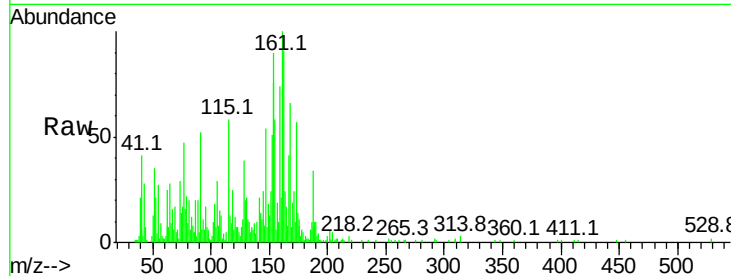

#53

Dibenzofuran

Concen: 3.86 ng/ul




RT: 15.27 min Scan# 2115


Delta R.T. 0.01 min

Lab File: BG025037.D

Acq: 9 Dec 2016 13:27

Tgt Ion:	168	Resp:	87334
Ion Ratio	Lower	Upper	
168	100		
139	46.6	33.8	50.8

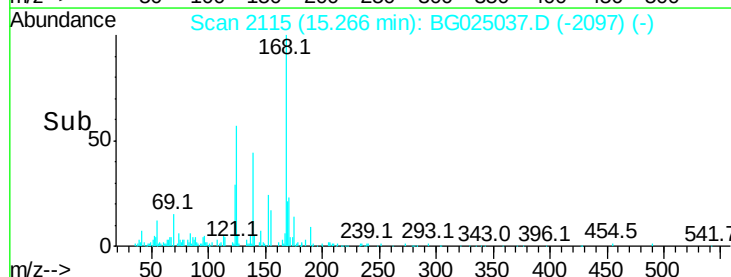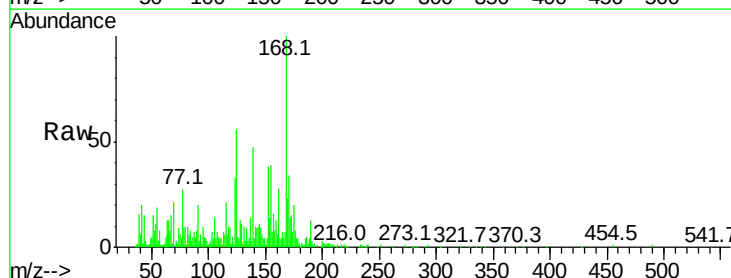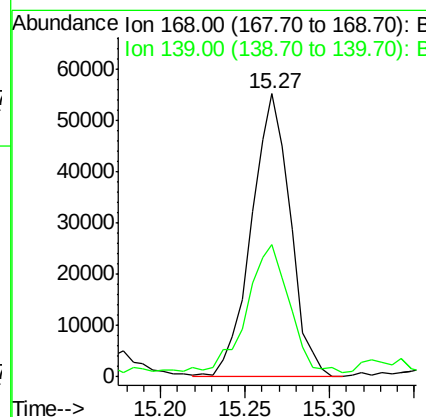

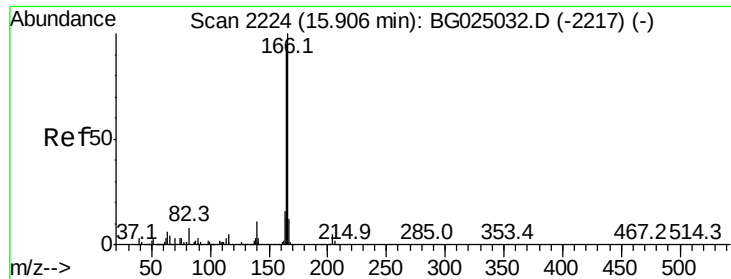





#58
 Fluorene
 Concen: 5.27 ng/ul
 RT: 15.91 min Scan# 2225
 Delta R.T. 0.01 min
 Lab File: BG025037.D
 Acq: 9 Dec 2016 13:27

Instrument :
 BNA_G
 ClientSampleId :
 DA7Y2DL2

Tot Ion	Ratio	Resp	Lower	Upper
166	100	97095		
165	97.1		79.7	119.5
167	17.4		11.4	17.2#

Manual Integrations
 APPROVED

Sohil
 12/12/2016 4:28:11 PM

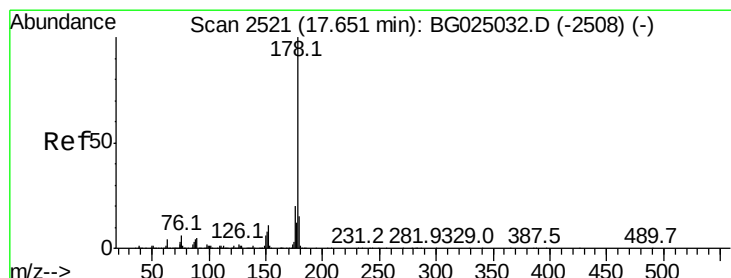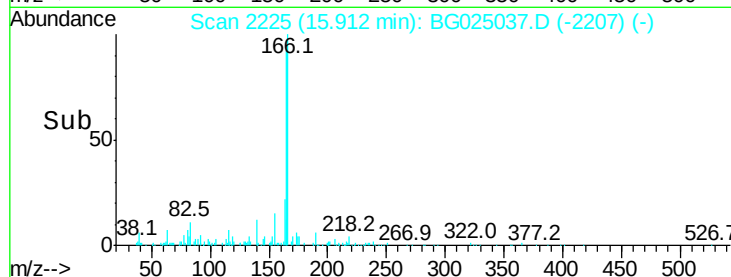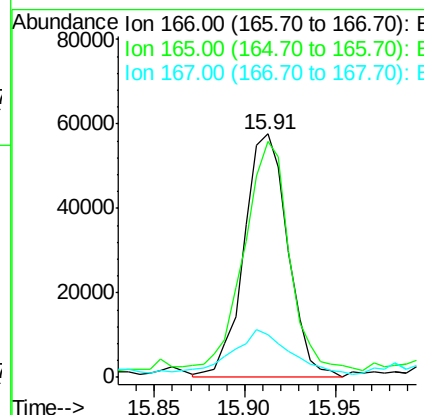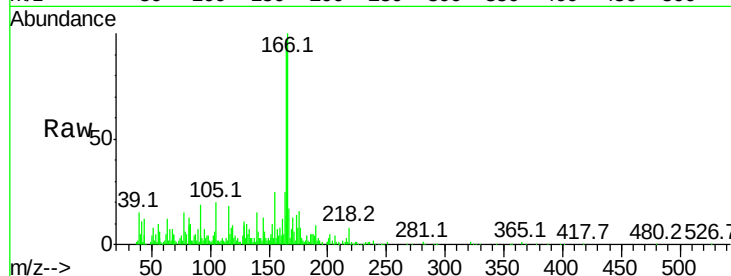

#69
 Phenanthrene
 Concen: 1.44 ng/ul
 RT: 17.65 min Scan# 2521
 Delta R.T. 0.00 min
 Lab File: BG025037.D
 Acq: 9 Dec 2016 13:27

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	39368		
179	18.2		12.4	18.6
176	19.8		16.5	24.7

