

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120916\
 Data File : BG025061.D
 Acq On : 10 Dec 2016 8:24
 Operator : UM/SJ
 Sample : H5863-06DL 20X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DA7Y5DL

Quant Time: Dec 12 04:04:00 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 03:10:41 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	103737	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	460795	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.87	164	366856	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.60	188	759693	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	909739	20.00	ng/ul	0.00
83) Perylene-d12	25.32	264	902207	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.62	96	295	0.15	ng/uL	0.02
5) Phenol-d5	7.39	99	9605	1.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.56	67	6075	1.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.77	132	6758	1.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.94	113	7962	1.06	ng/ul	0.00
19) Nitrobenzene-d5	9.43	128	3409	1.04	ng/ul	0.00
22) 2-Nitrophenol-d4	10.15	143	4436	1.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.69	165	7358	0.94	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	14.25	166	26176	1.04	ng/ul	0.00
46) Acenaphthylene-d8	14.55	160	32995	1.19	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
57) Fluorene-d10	15.85	176	31079	1.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.96	200	2720	0.58	ng/ul	0.00
70) Anthracene-d10	17.70	188	46347	1.45	ng/ul	0.00
76) Pyrene-d10	19.98	212	56026	1.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.07	264	54258	1.48	ng/ul	0.00

Target Compounds


						Ovalue
81) Bis(2-ethylhexyl)phthalate	21.73	149	976096	41.42	ng/ul	100
84) Di-n-octyl phthalate	23.00	149	40354	1.10	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG120916\
Data File : BG025061.D
Acq On : 10 Dec 2016 8:24
Operator : UM/SJ
Sample : H5863-06DL 20X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DA7Y5DL

Quant Time: Dec 12 04:04:00 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 12 03:10:41 2016
Response via : Initial Calibration




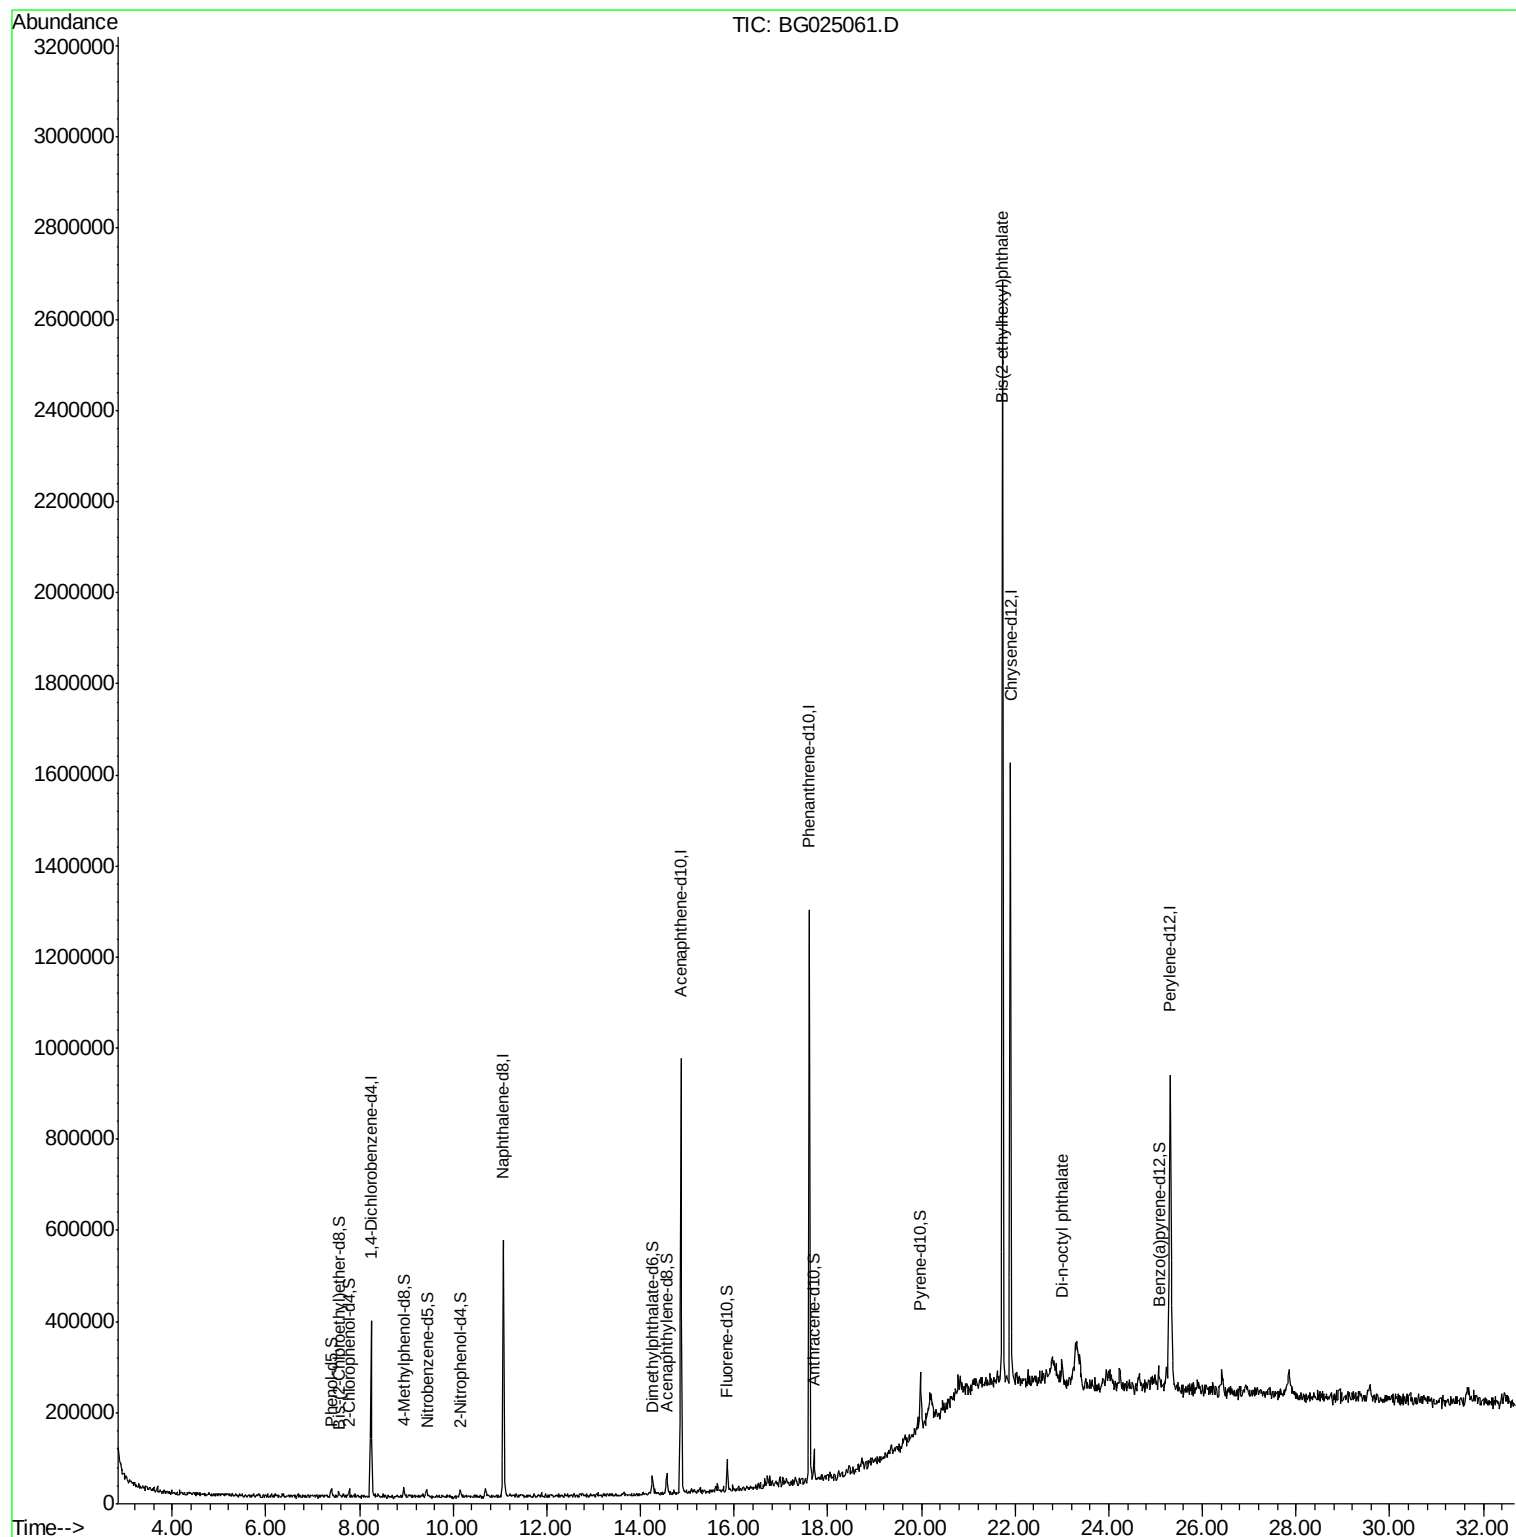


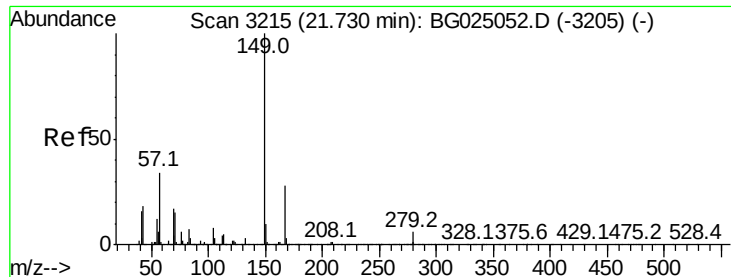

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 41.42 ng/ul
 RT: 21.73 min Scan# 3215
 Delta R.T. -0.00 min
 Lab File: BG025061.D
 Acq: 10 Dec 2016 8:24

Instrument :
 BNA_G
 ClientSampleId :
 DA7Y5DL

Tot Ion	Ratio	Lower	Upper
149	100		
167	27.3	21.8	32.8
279	6.1	4.5	6.7

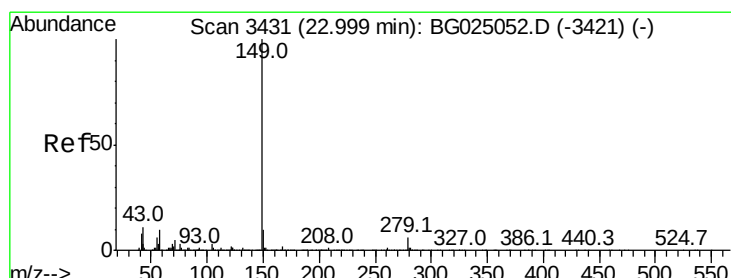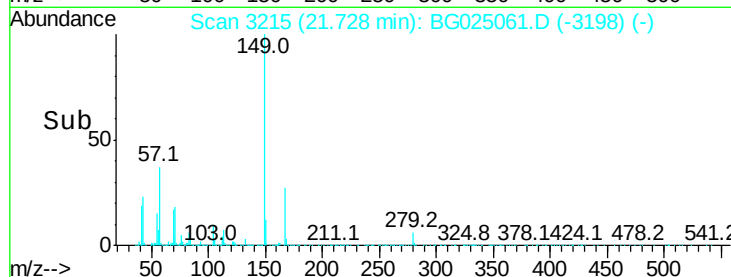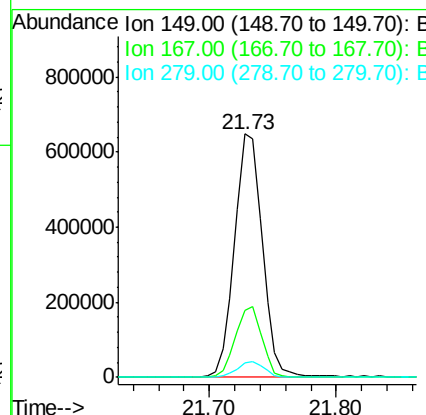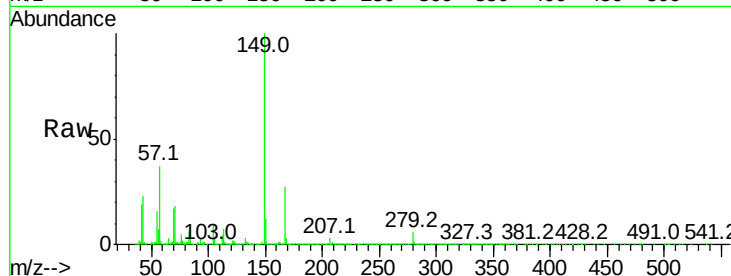

#84
 Di-n-octyl phthalate
 Concen: 1.10 ng/ul
 RT: 23.00 min Scan# 3432
 Delta R.T. 0.00 min
 Lab File: BG025061.D
 Acq: 10 Dec 2016 8:24

Tgt Ion:149 Resp: 40354

