

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
 Data File : BG063602.D
 Acq On : 9 Dec 2024 14:49
 Operator : RC/JU
 Sample : P5066-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E28M3

Quant Time: Dec 10 00:32:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 06 15:14:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.824	152	123203	20.000	ng/ul	0.00
20) Naphthalene-d8	10.615	136	557406	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.469	164	466891	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.219	188	1146313	20.000	ng/ul	0.00
79) Chrysene-d12	21.479	240	956981	20.000	ng/ul	# 0.00
88) Perylene-d12	24.516	264	1075124	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.282	96	11452	4.104	ng/uL	0.00
4) Pyridine-d5	3.688	84	195892	18.975	ng/ul	0.00
7) Phenol-d5	6.996	99	325185	26.808	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.154	67	214473	26.150	ng/ul	0.00
11) 2-Chlorophenol-d4	7.360	132	211804	29.641	ng/ul	0.00
15) 4-Methylphenol-d8	8.535	113	268303	29.832	ng/ul	0.00
21) Nitrobenzene-d5	8.976	128	114191	29.186	ng/ul	0.00
24) 2-Nitrophenol-d4	9.698	143	132332	29.556	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.245	165	265439	27.535	ng/ul	0.01
31) 4-Chloroaniline-d4	10.750	131	336564	28.889	ng/ul	0.00
46) Dimethylphthalate-d6	13.870	166	1033766	30.466	ng/ul	0.00
49) Acenaphthylene-d8	14.158	160	1196214	32.251	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	98918	22.766	ng/ul	0.00
60) Fluorene-d10	15.462	176	1003611	30.005	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.591	200	124603	19.241	ng/ul	0.00
73) Anthracene-d10	17.319	188	1687158	32.233	ng/ul	0.00
81) Pyrene-d10	19.622	212	1855091	34.972	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.305	264	1811679	33.551	ng/ul	0.01
Target Compounds						
					Qvalue	
8) Phenol	7.031	94	14399	1.104	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
Data File : BG063602.D
Acq On : 9 Dec 2024 14:49
Operator : RC/JU
Sample : P5066-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E28M3

Quant Time: Dec 10 00:32:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 06 15:14:46 2024
Response via : Initial Calibration

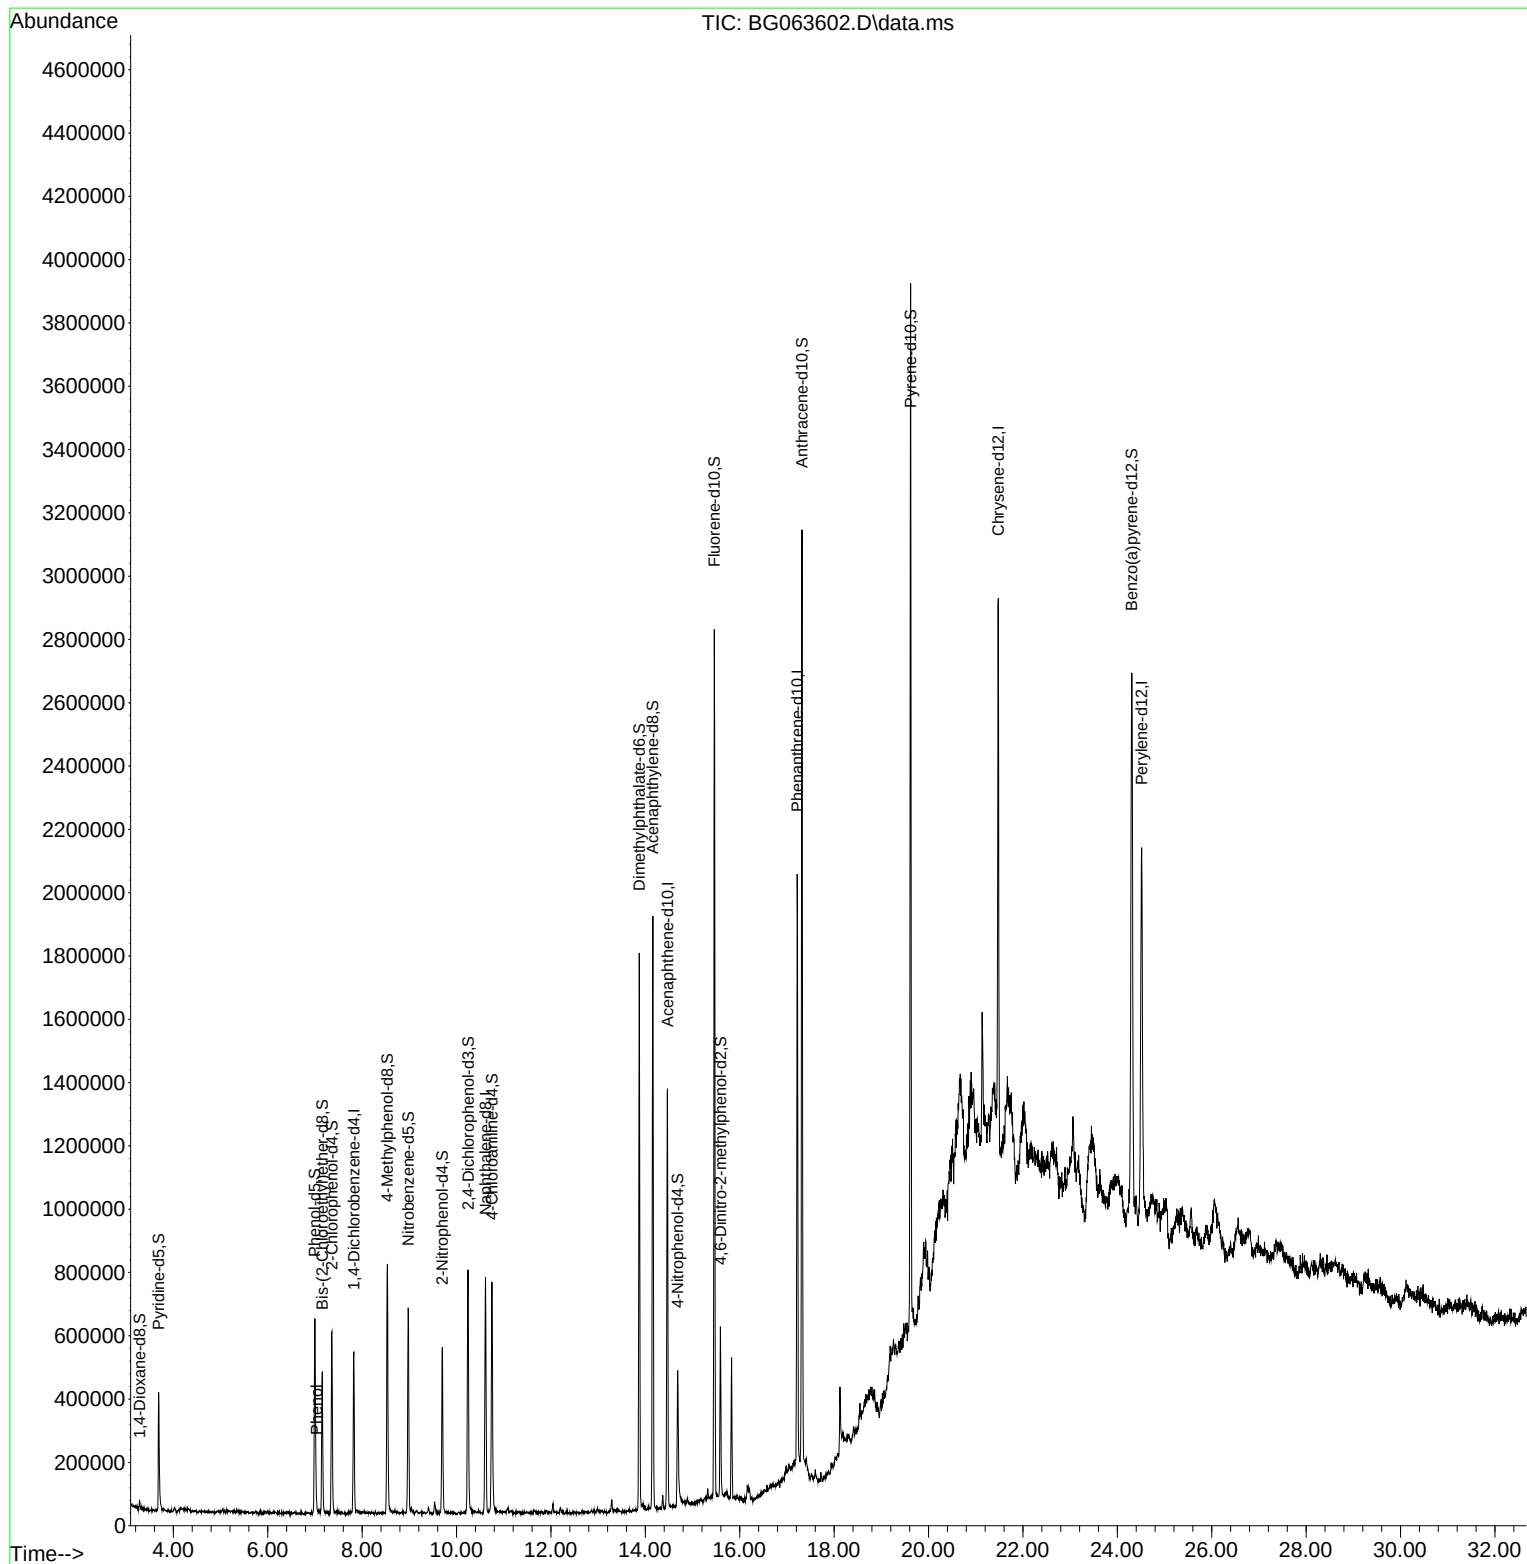

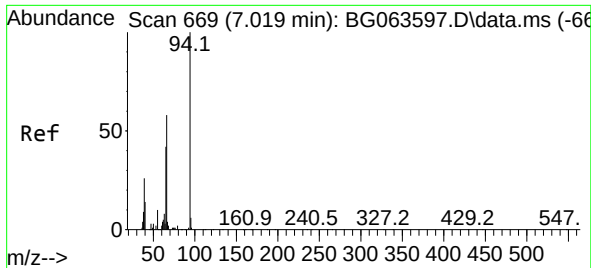

#8
Phenol
Concen: 1.104 ng/ul
RT: 7.031 min Scan# 61
Delta R.T. 0.011 min
Lab File: BG063602.D
Acq: 9 Dec 2024 14:49

Instrument :
BNA_G
ClientSampleId :
E28M3

Tgt Ion: 94 Resp: 14399
Ion Ratio Lower Upper
94 100
65 33.9 31.8 47.8
66 29.8 45.0 67.6#

