

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
 Data File : BG063605.D
 Acq On : 9 Dec 2024 17:01
 Operator : RC/JU
 Sample : PB165440BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK440

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	31	33	38	rVB3	28321	36055	0.81%	0.078%
2	3.686	98	102	116	rBV	404004	685291	15.31%	1.483%
3	3.916	135	141	144	rVB5	9564	19965	0.45%	0.043%
4	4.004	154	156	158	rBV2	8355	9621	0.21%	0.021%
5	4.256	198	199	201	rBV	12361	8501	0.19%	0.018%
6	4.286	201	204	205	rVV3	7593	9310	0.21%	0.020%
7	4.656	265	267	269	rVB	7988	6803	0.15%	0.015%
8	4.762	283	285	288	rVB	11436	6914	0.15%	0.015%
9	4.809	290	293	294	rBV3	6470	7127	0.16%	0.015%
10	5.049	332	334	335	rBV	10334	8661	0.19%	0.019%
11	5.173	353	355	356	rVB2	13881	7590	0.17%	0.016%
12	5.461	402	404	407	rBV4	5983	6675	0.15%	0.014%
13	5.525	413	415	418	rVB2	11408	9605	0.21%	0.021%
14	5.655	435	437	440	rVB3	9036	8506	0.19%	0.018%
15	5.743	448	452	453	rVB3	6353	7616	0.17%	0.016%
16	5.831	465	467	470	rBV3	5843	7219	0.16%	0.016%
17	6.025	497	500	501	rBV	9966	8643	0.19%	0.019%
18	6.142	518	520	523	rVB3	8881	11248	0.25%	0.024%
19	6.471	574	576	579	rVB3	11358	8942	0.20%	0.019%
20	6.495	579	580	584	rBV4	7266	10540	0.24%	0.023%
21	6.565	589	592	594	rBV3	7223	10018	0.22%	0.022%
22	6.747	621	623	628	rVB2	12049	16064	0.36%	0.035%
23	6.789	628	630	632	rBV2	8184	8156	0.18%	0.018%
24	6.865	641	643	646	rBV2	6427	6638	0.15%	0.014%
25	7.000	659	666	674	rBV	621761	1080106	24.13%	2.338%
26	7.153	686	692	700	rBV	418538	692260	15.46%	1.498%
27	7.212	700	702	706	rVB3	8873	10200	0.23%	0.022%
28	7.288	713	715	718	rVB3	8275	10251	0.23%	0.022%
29	7.359	720	727	735	rVV	578675	999868	22.34%	2.164%
30	7.823	798	806	813	rBV	519451	909637	20.32%	1.969%
31	8.534	920	927	939	rBV2	742962	1321532	29.52%	2.860%
32	8.974	994	1002	1011	rBV	543384	984099	21.98%	2.130%
33	9.256	1048	1050	1052	rBV2	8676	8021	0.18%	0.017%
34	9.297	1055	1057	1060	rVV	10754	10820	0.24%	0.023%
35	9.339	1062	1064	1067	rVB3	10023	7847	0.18%	0.017%
36	9.468	1082	1086	1089	rVB2	10542	14920	0.33%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
 Data File : BG063605.D
 Acq On : 9 Dec 2024 17:01
 Operator : RC/JU
 Sample : PB165440BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK440

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Title : SVOA CALIBRATION

37	9.527	1095	1096	1099	rVB2	10934	7919	0.18%	0.017%
38	9.697	1117	1125	1133	rBV2	446102	808688	18.07%	1.750%
39	9.826	1145	1147	1149	rBV	7574	7860	0.18%	0.017%
40	9.861	1152	1153	1156	rBV3	8223	7547	0.17%	0.016%
41	10.243	1209	1218	1229	rBV	682419	1306398	29.18%	2.827%
42	10.614	1274	1281	1290	rVB	808076	1406497	31.42%	3.044%
43	10.749	1295	1304	1314	rBV	621811	1193856	26.67%	2.584%
44	10.860	1321	1323	1326	rBV4	5477	6785	0.15%	0.015%
45	10.919	1331	1333	1336	rVB3	10376	6721	0.15%	0.015%
46	11.189	1377	1379	1382	rVB3	9412	7777	0.17%	0.017%
47	11.213	1382	1383	1387	rVB2	8802	9073	0.20%	0.020%
48	11.313	1397	1400	1402	rBV2	10427	9676	0.22%	0.021%
49	11.383	1409	1412	1415	rBV2	6470	8160	0.18%	0.018%
50	11.583	1444	1446	1451	rBV	7834	11640	0.26%	0.025%
51	11.818	1483	1486	1487	rBV	12049	9463	0.21%	0.020%
52	11.865	1490	1494	1497	rVB2	6832	10460	0.23%	0.023%
53	12.147	1539	1542	1543	rBV2	9075	8551	0.19%	0.019%
54	12.206	1550	1552	1556	rVB3	7956	8064	0.18%	0.017%
55	12.294	1562	1567	1569	rBV3	12046	17132	0.38%	0.037%
56	12.353	1573	1577	1578	rVB2	8413	9675	0.22%	0.021%
57	12.629	1622	1624	1627	rVB	8810	9311	0.21%	0.020%
58	12.652	1627	1628	1631	rBV	8948	9260	0.21%	0.020%
59	12.793	1649	1652	1654	rBV	9113	10262	0.23%	0.022%
60	12.975	1680	1683	1686	rBV3	8202	8608	0.19%	0.019%
61	13.058	1693	1697	1701	rVB3	9995	16814	0.38%	0.036%
62	13.099	1701	1704	1705	rBV2	10195	8551	0.19%	0.019%
63	13.193	1719	1720	1723	rVB2	13902	7856	0.18%	0.017%
64	13.375	1748	1751	1752	rBV	8002	7037	0.16%	0.015%
65	13.528	1773	1777	1780	rBV4	5357	7152	0.16%	0.015%
66	13.622	1790	1793	1795	rBV3	6997	9141	0.20%	0.020%
67	13.663	1798	1800	1802	rBV	7432	7629	0.17%	0.017%
68	13.769	1816	1818	1822	rBV2	5074	6988	0.16%	0.015%
69	13.869	1829	1835	1842	rBV	1342819	2009399	44.89%	4.349%
70	14.156	1877	1884	1895	rBV	1664590	2638576	58.94%	5.711%
71	14.239	1897	1898	1901	rBV2	7278	7890	0.18%	0.017%
72	14.333	1911	1914	1916	rVB	10793	13360	0.30%	0.029%
73	14.356	1916	1918	1919	rBV	9754	8531	0.19%	0.018%
74	14.374	1919	1921	1923	rVB3	9127	7585	0.17%	0.016%
75	14.397	1923	1925	1926	rBV2	7040	6588	0.15%	0.014%
76	14.468	1929	1937	1945	rVV	1603025	2446723	54.66%	5.296%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
 Data File : BG063605.D
 Acq On : 9 Dec 2024 17:01
 Operator : RC/JU
 Sample : PB165440BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK440

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Title : SVOA CALIBRATION

77	14.597	1958	1959	1962	rVB	10042	6935	0.15%	0.015%
78	14.632	1962	1965	1968	rBV3	9747	12811	0.29%	0.028%
79	14.685	1968	1974	1986	rBV	453644	908991	20.31%	1.967%
80	14.797	1991	1993	1994	rBV2	11064	8242	0.18%	0.018%
81	14.891	2005	2009	2010	rVB2	8125	8858	0.20%	0.019%
82	15.261	2070	2072	2074	rVB3	8394	6590	0.15%	0.014%
83	15.461	2100	2106	2115	rBV	2321952	3400538	75.97%	7.360%
84	15.590	2122	2128	2137	rBV2	437860	715179	15.98%	1.548%
85	15.708	2146	2148	2151	rVB4	13818	11520	0.26%	0.025%
86	15.860	2172	2174	2176	rBV2	11416	10363	0.23%	0.022%
87	15.995	2194	2197	2198	rBV2	11395	11727	0.26%	0.025%
88	16.178	2225	2228	2230	rBV	10688	13606	0.30%	0.029%
89	16.272	2243	2244	2248	rVB4	9884	8268	0.18%	0.018%
90	16.366	2259	2260	2264	rBV4	6914	7182	0.16%	0.016%
91	16.889	2346	2349	2350	rBV2	9516	9478	0.21%	0.021%
92	16.971	2361	2363	2366	rBV3	8462	10459	0.23%	0.023%
93	17.218	2399	2405	2412	rBV	2173993	3292936	73.56%	7.127%
94	17.317	2416	2422	2430	rVB	2571191	3841268	85.81%	8.314%
95	17.782	2499	2501	2506	rBV6	9809	15013	0.34%	0.032%
96	17.846	2510	2512	2514	rBV3	10059	12625	0.28%	0.027%
97	19.621	2808	2814	2820	rBV	3242881	4476369	100.00%	9.688%
98	21.477	3125	3130	3141	rVB2	2072722	3253888	72.69%	7.043%
99	24.309	3605	3612	3623	rVB	1457583	3697215	82.59%	8.002%
100	24.515	3640	3647	3661	rVB	1281159	3378836	75.48%	7.313%




Sum of corrected areas: 46203369

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
Data File : BG063605.D
Acq On : 9 Dec 2024 17:01
Operator : RC/JU
Sample : PB165440BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK440

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

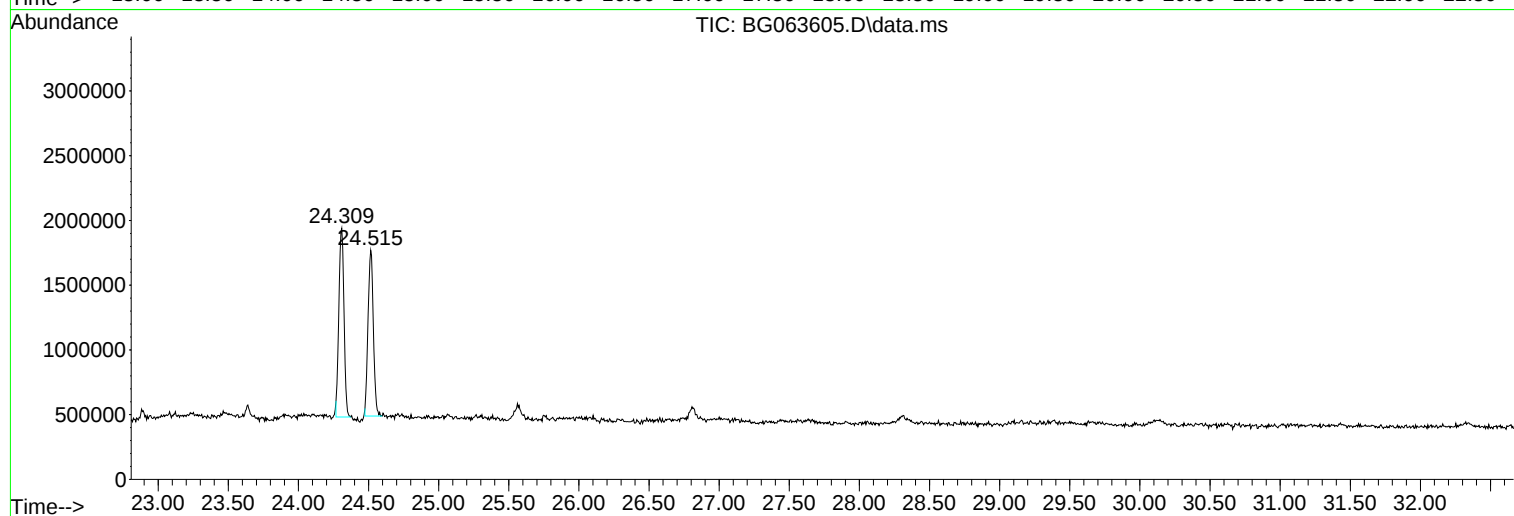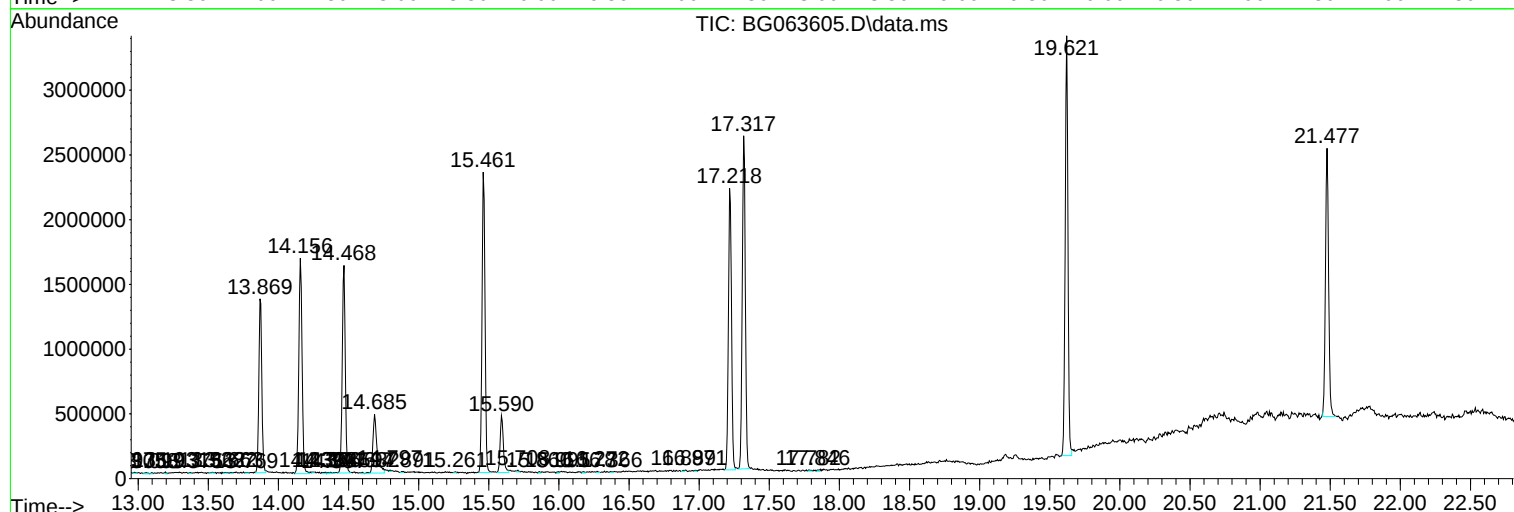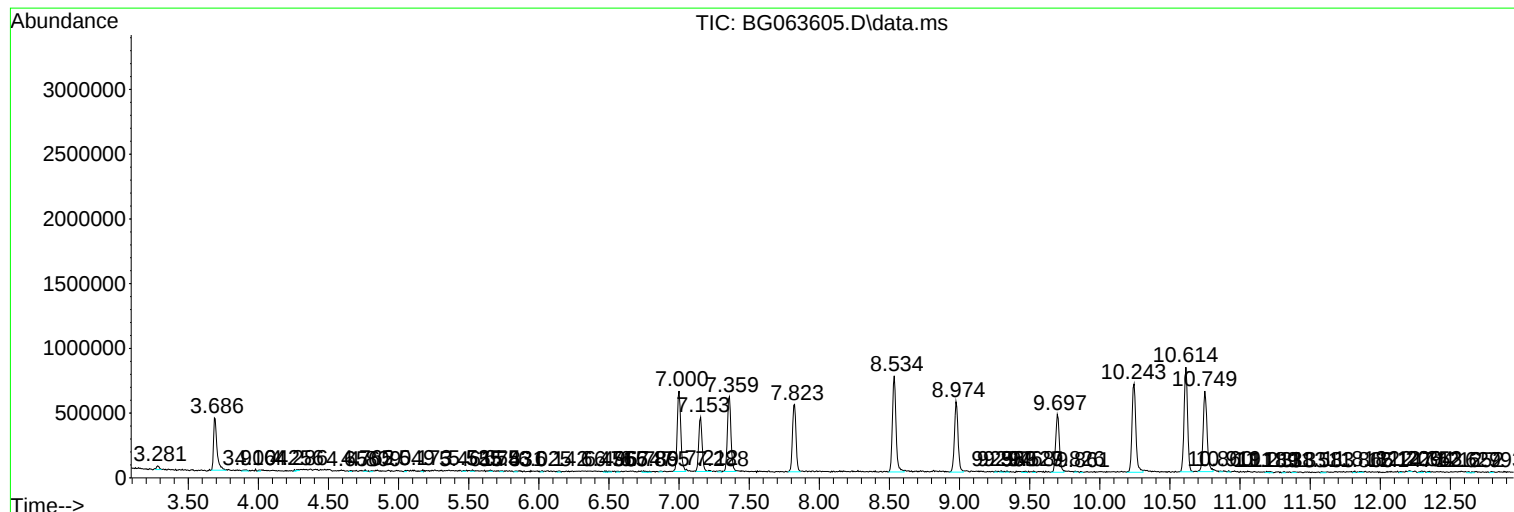

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
Data File : BG063605.D
Acq On : 9 Dec 2024 17:01
Operator : RC/JU
Sample : PB165440BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK440

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG120924\
Data File : BG063605.D
Acq On : 9 Dec 2024 17:01
Operator : RC/JU
Sample : PB165440BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK440

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc