


Data Path : Z:\HPCHEM1\BNA G\DATA\BG121015\
 Data File : BG020062.D
 Acq On : 10 Dec 2015 3:04
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG120215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 02 18:50:01 2015

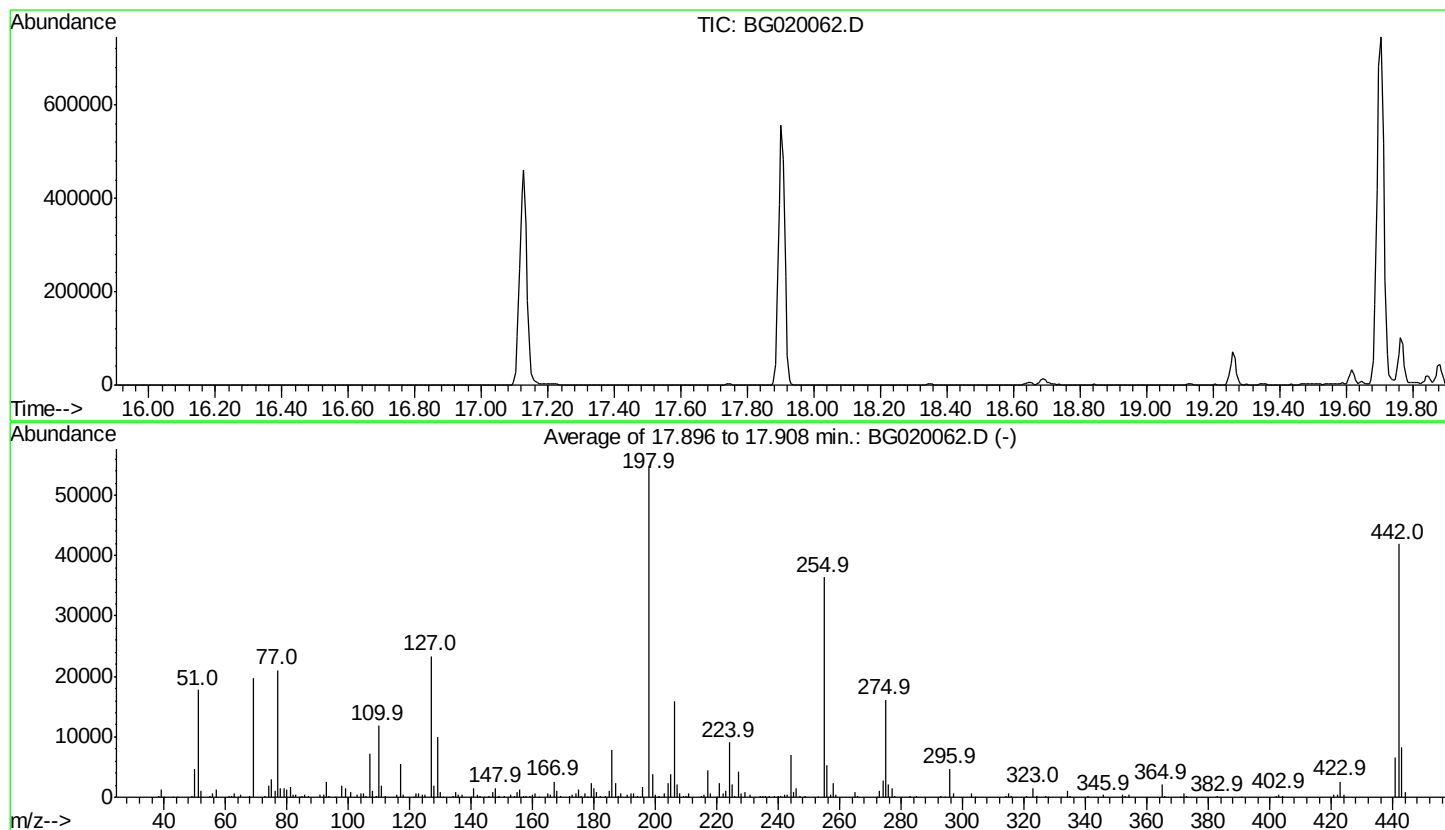

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	17710	PASS
68	69	0.00	2	1.4	271	PASS
69	198	0.00	100	35.7	19616	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.5	23320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54906	PASS
199	198	5	9	6.9	3779	PASS
275	198	10	60	29.5	16221	PASS
365	198	1	100	3.7	2057	PASS
441	442	0.01	24	15.5	6504	PASS
442	198	50	100	76.3	41896	PASS
443	442	15	24	19.5	8174	PASS