

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121016\
 Data File : BG025073.D
 Acq On : 10 Dec 2016 17:58
 Operator : UM/SJ
 Sample : H5861-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 12 02:49:34 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 12 02:45:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	67444	20.00	ng/ul	0.00
18) Naphthalene-d8	11.06	136	277775	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.86	164	225004	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.60	188	562381	20.00	ng/ul	0.00
75) Chrysene-d12	21.89	240	742187	20.00	ng/ul	0.00
83) Perylene-d12	25.31	264	738136	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	2952	2.26	ng/uL	0.00
5) Phenol-d5	7.39	99	50491	8.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	138810	38.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	122400	30.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.94	113	95168	19.57	ng/ul	0.00
19) Nitrobenzene-d5	9.42	128	76248	38.76	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	93729	38.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.68	165	163189	34.60	ng/ul	0.00
29) 4-Chloroaniline-d4	11.20	131	1869	0.40	ng/ul	0.00
43) Dimethylphthalate-d6	14.25	166	681991	44.06	ng/ul	0.00
46) Acenaphthylene-d8	14.55	160	721839	42.58	ng/ul	0.00
51) 4-Nitrophenol-d4	15.05	143	28283	10.63	ng/ul	0.00
57) Fluorene-d10	15.85	176	593331	40.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.96	200	146336	42.08	ng/ul	0.00
70) Anthracene-d10	17.70	188	1053947	44.40	ng/ul	0.00
76) Pyrene-d10	19.97	212	1375183	44.98	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.06	264	1375088	45.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
73) Di-n-butylphthalate	18.53	149	34935	1.20	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG121016\
Data File : BG025073.D
Acq On : 10 Dec 2016 17:58
Operator : UM/SJ
Sample : H5861-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 12 02:49:34 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG113016.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 12 02:45:14 2016
Response via : Initial Calibration

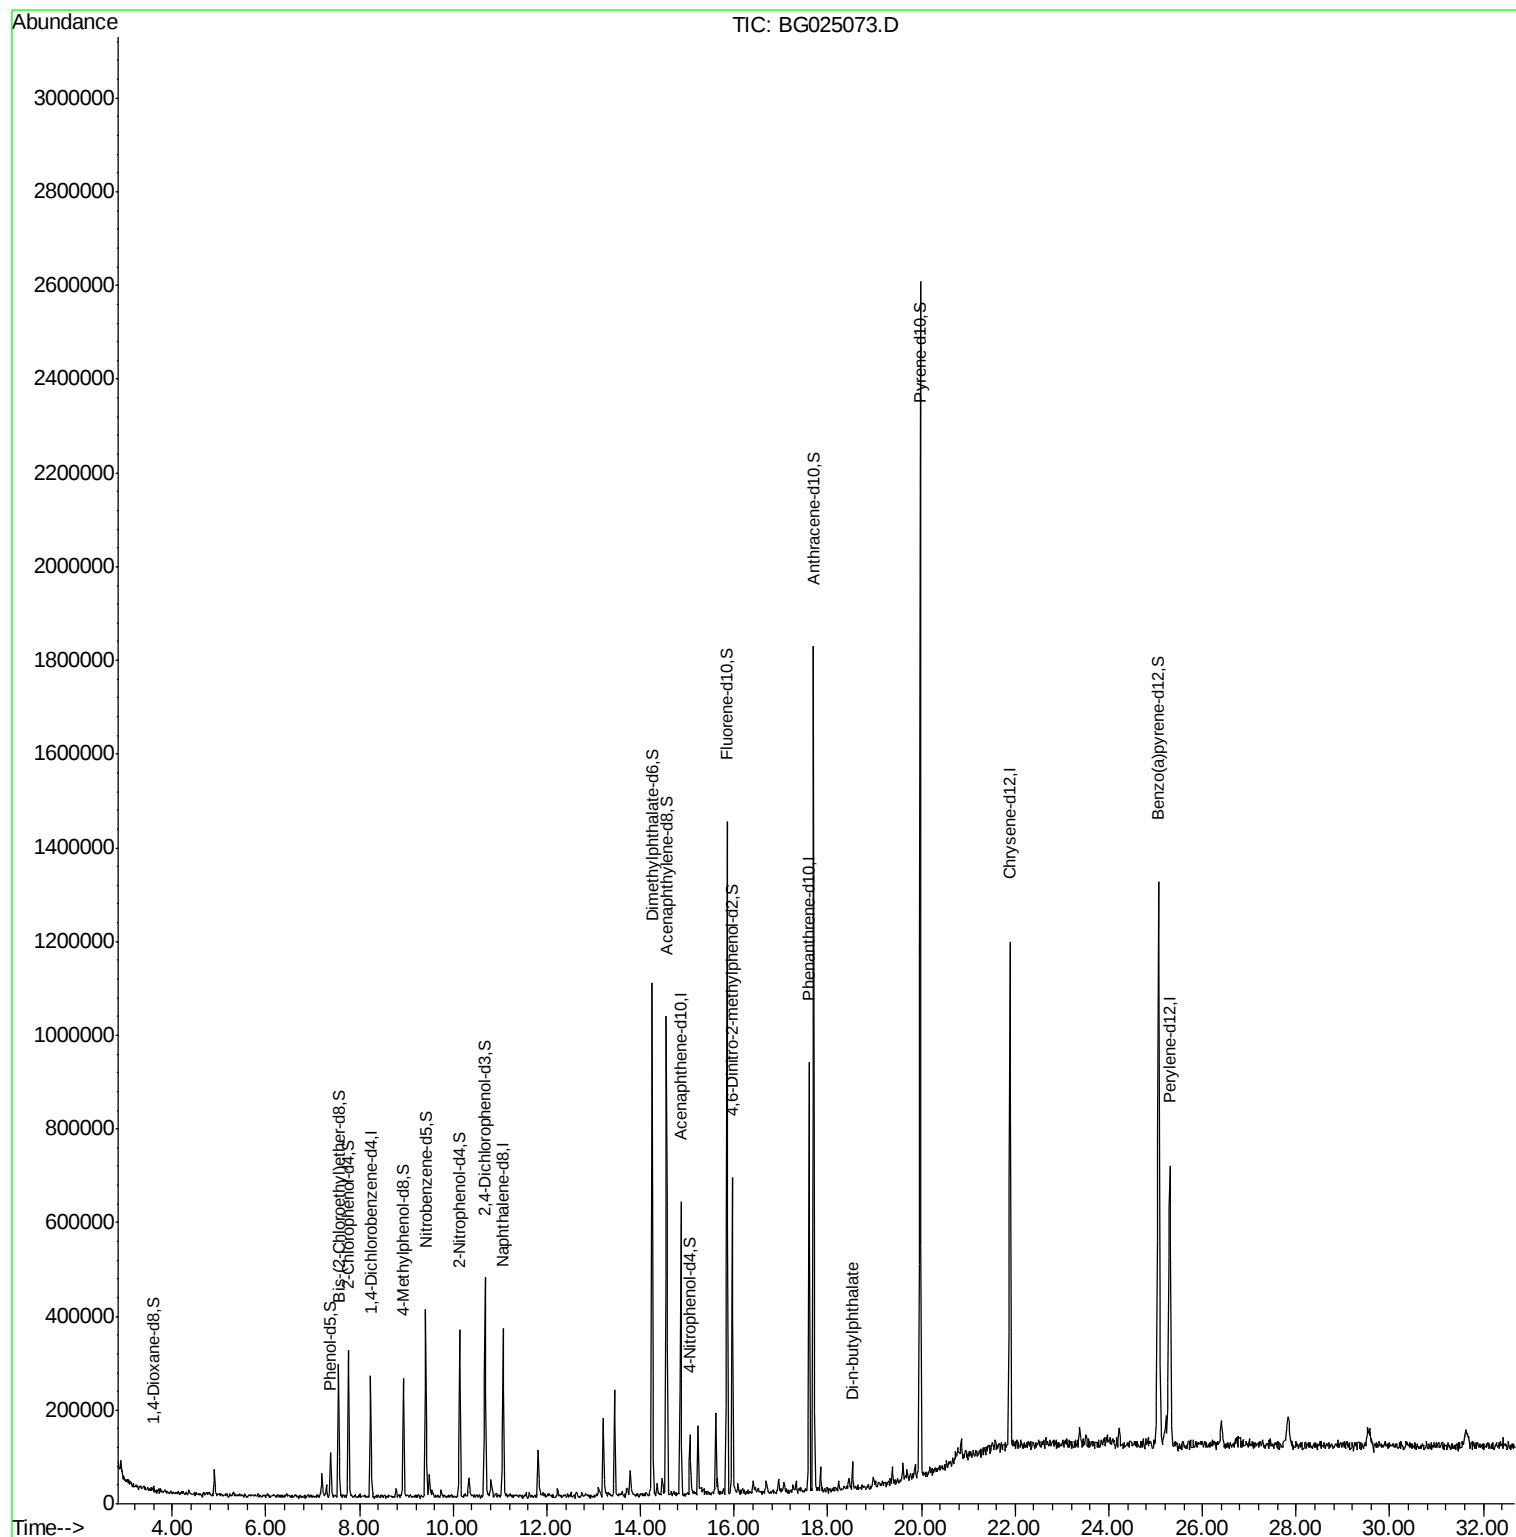


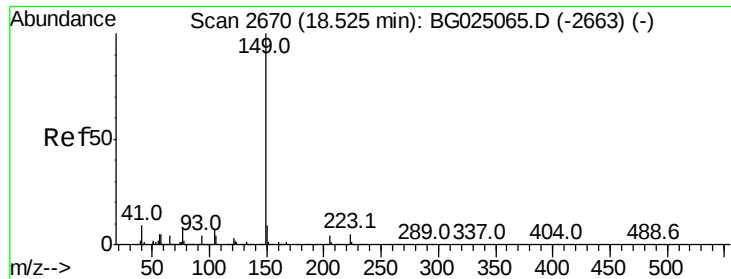

#73
 Di-n-butylphthalate
 Concen: 1.20 ng/ul
 RT: 18.53 min Scan# 2670
 Delta R.T. -0.00 min
 Lab File: BG025073.D
 Acq: 10 Dec 2016 17:58

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
149	100		
150	7.9	7.9	11.9#
104	15.3	5.8	8.8#

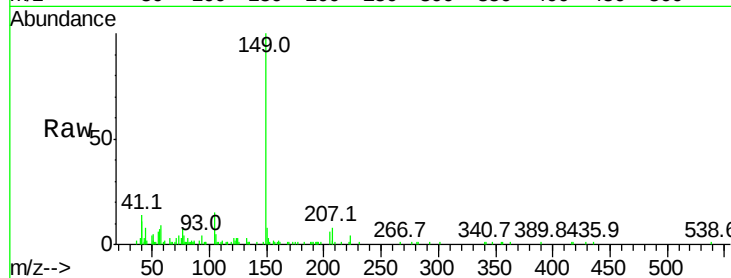

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 104.00 (103.70 to 104.70): E

