
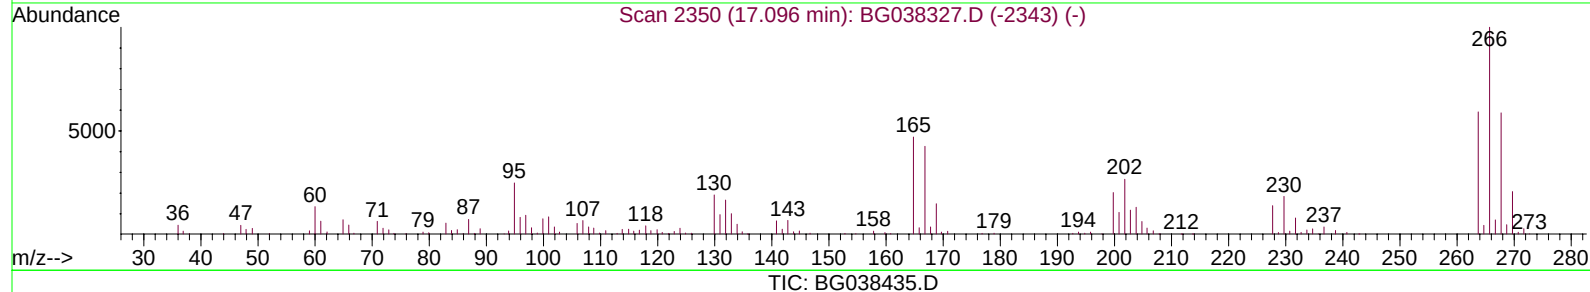
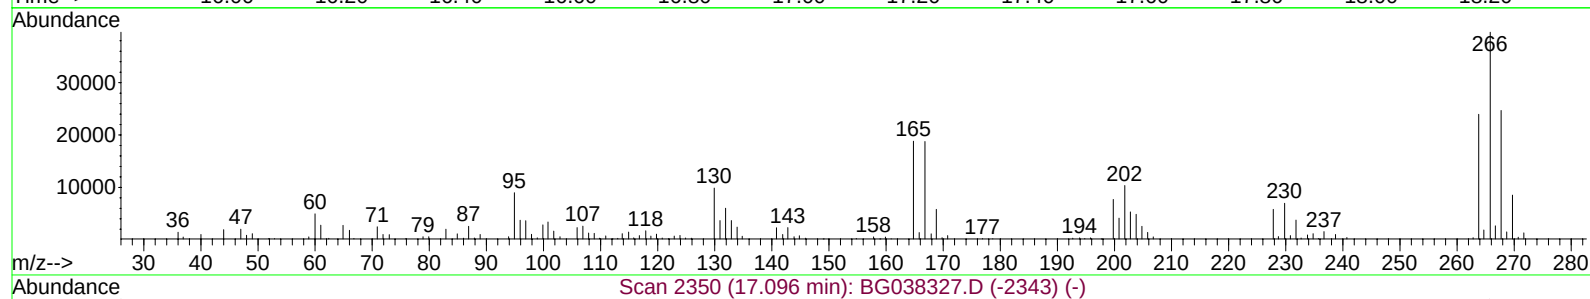


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121018\
Data File : BG038435.D
Acq On : 10 Dec 2018 9:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 13:32:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

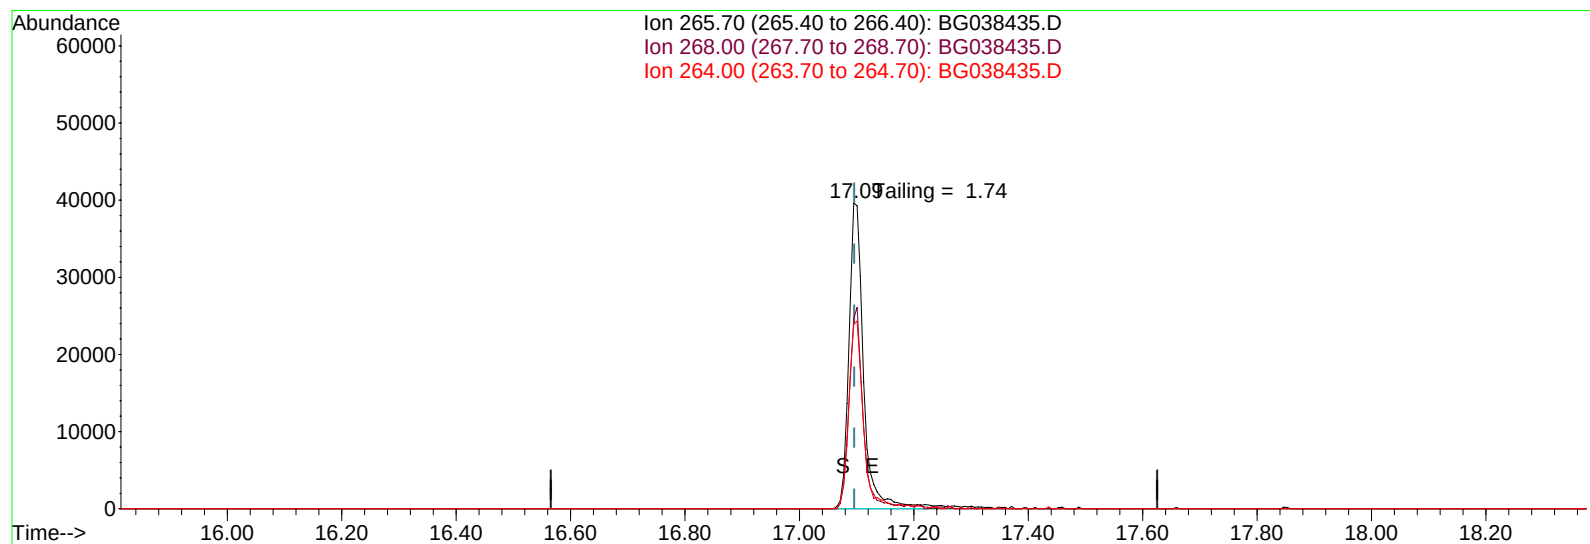

(70) Pentachlorophenol (C)




17.095min (-0.001) 77842.12ng

response 70672

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.07
264.00	73.60	65.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121018\
Data File : BG038435.D
Acq On : 10 Dec 2018 9:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 13:32:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

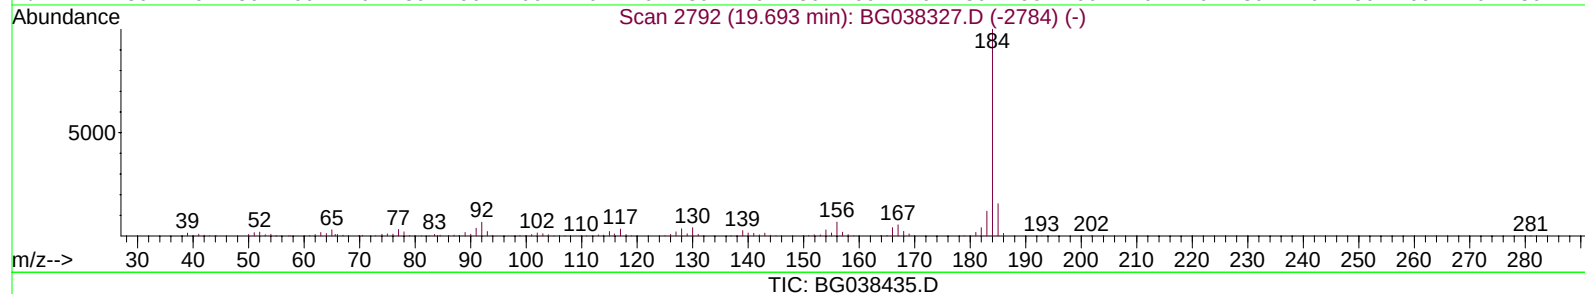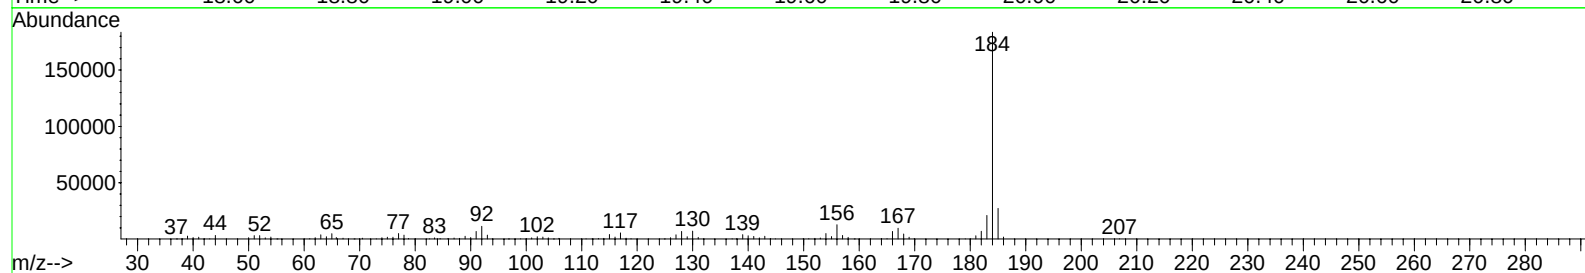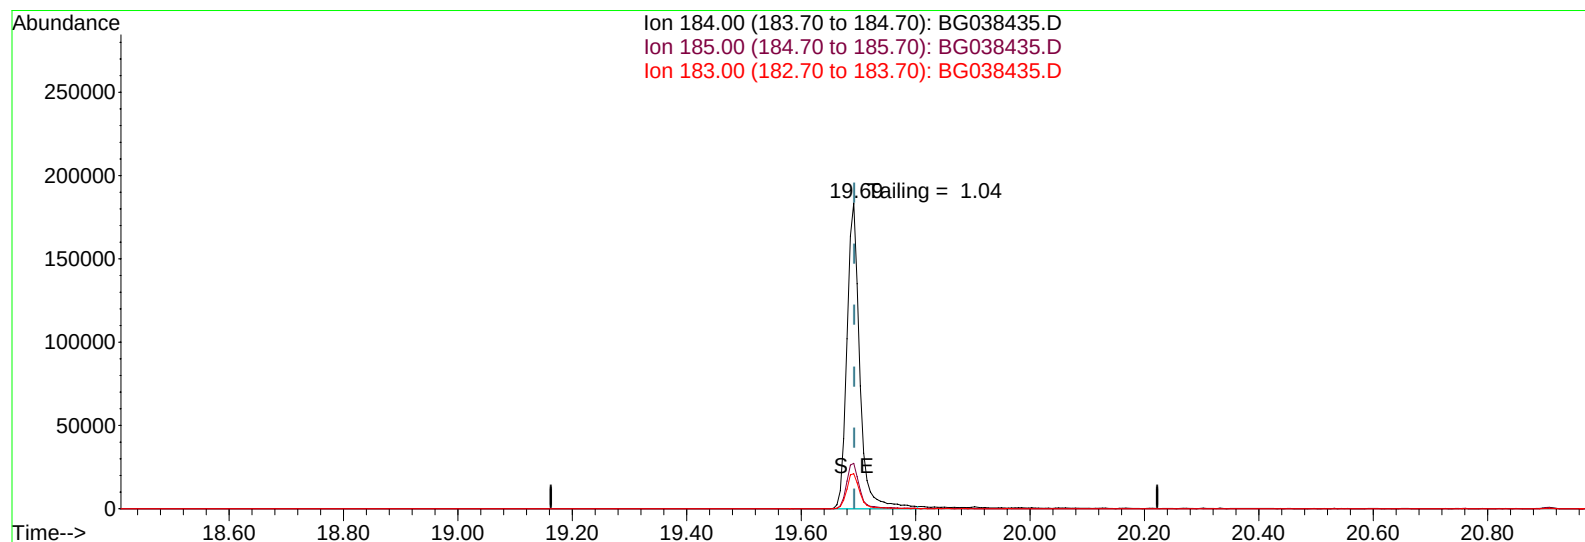

(77) Benzidine

19.692min (-0.001) 12631.45ng

response 289846

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.87
183.00	12.70	11.46
0.00	0.00	0.00