
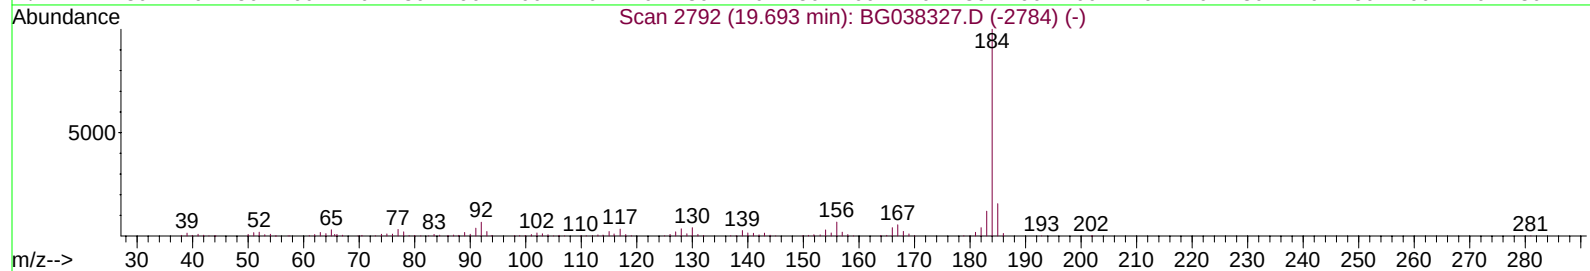
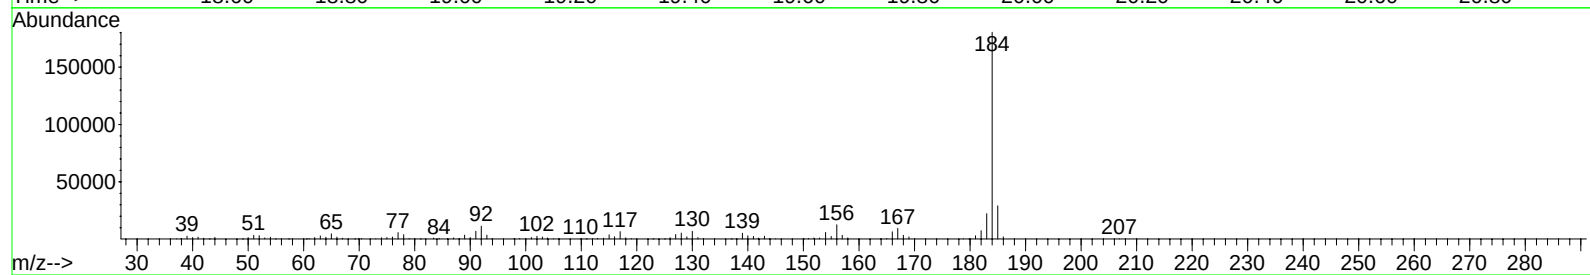


```
Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121018\  
Data File : BG038439.D  
Acq On    : 10 Dec 2018 15:02  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Dec 10 15:32:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

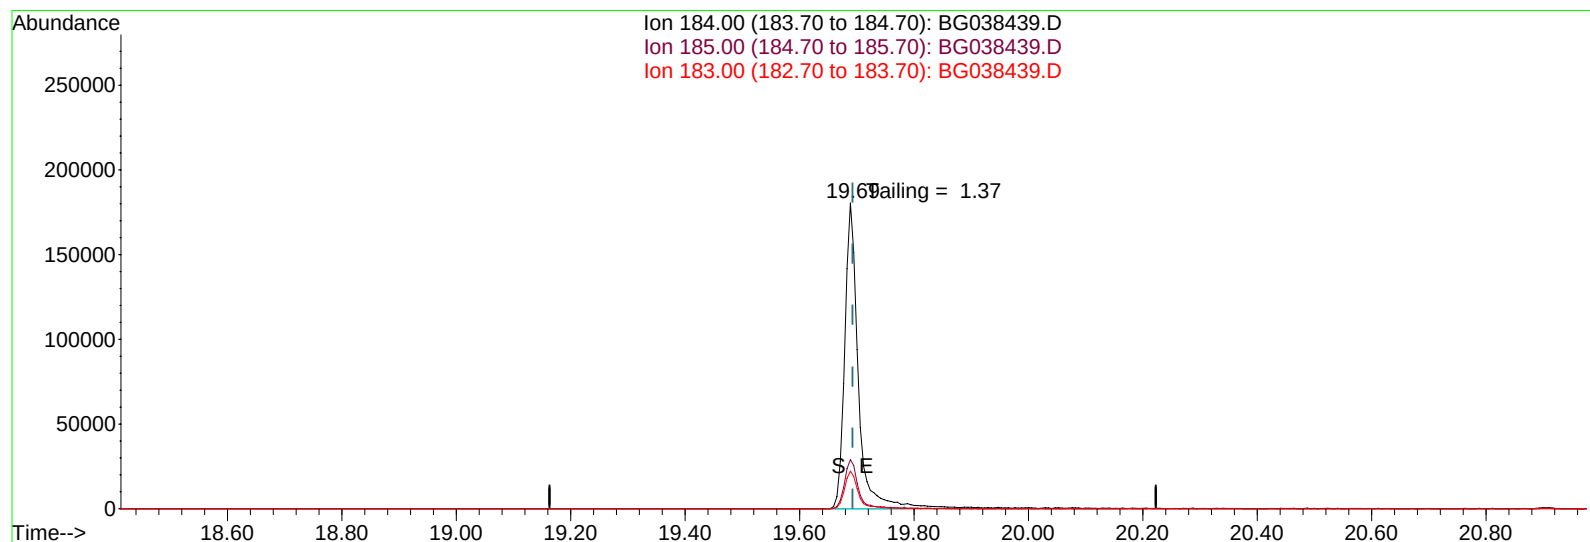

TIC: BG038439.D

(77) Benzidine




19.689min (-0.004) 0.00ng

response 300452

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.08
183.00	12.70	12.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121018\
Data File : BG038439.D
Acq On : 10 Dec 2018 15:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 15:32:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

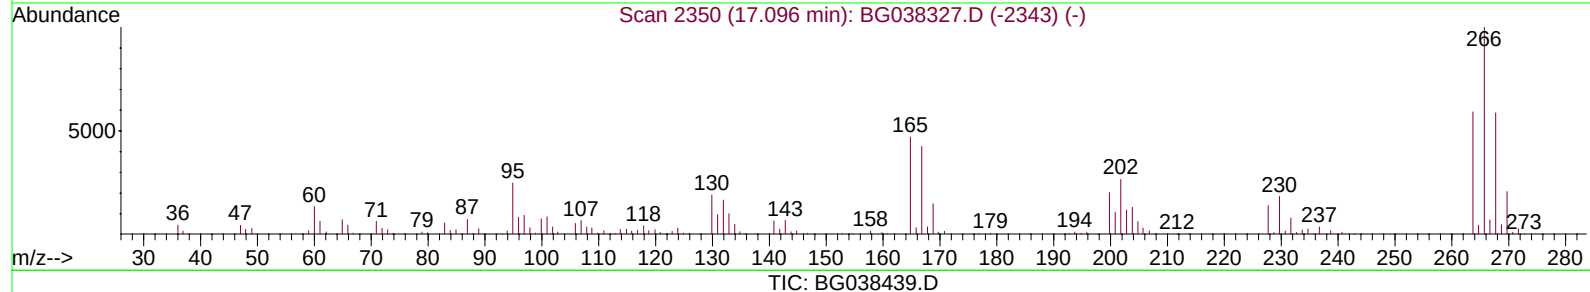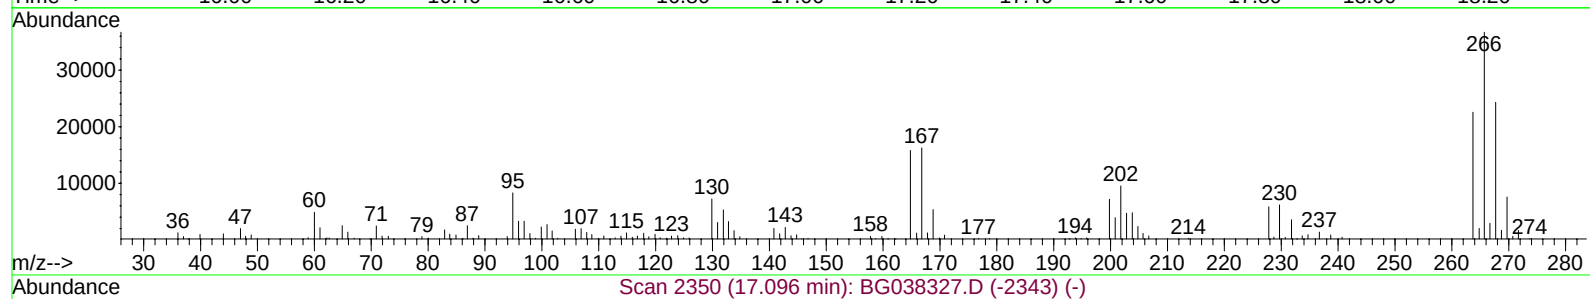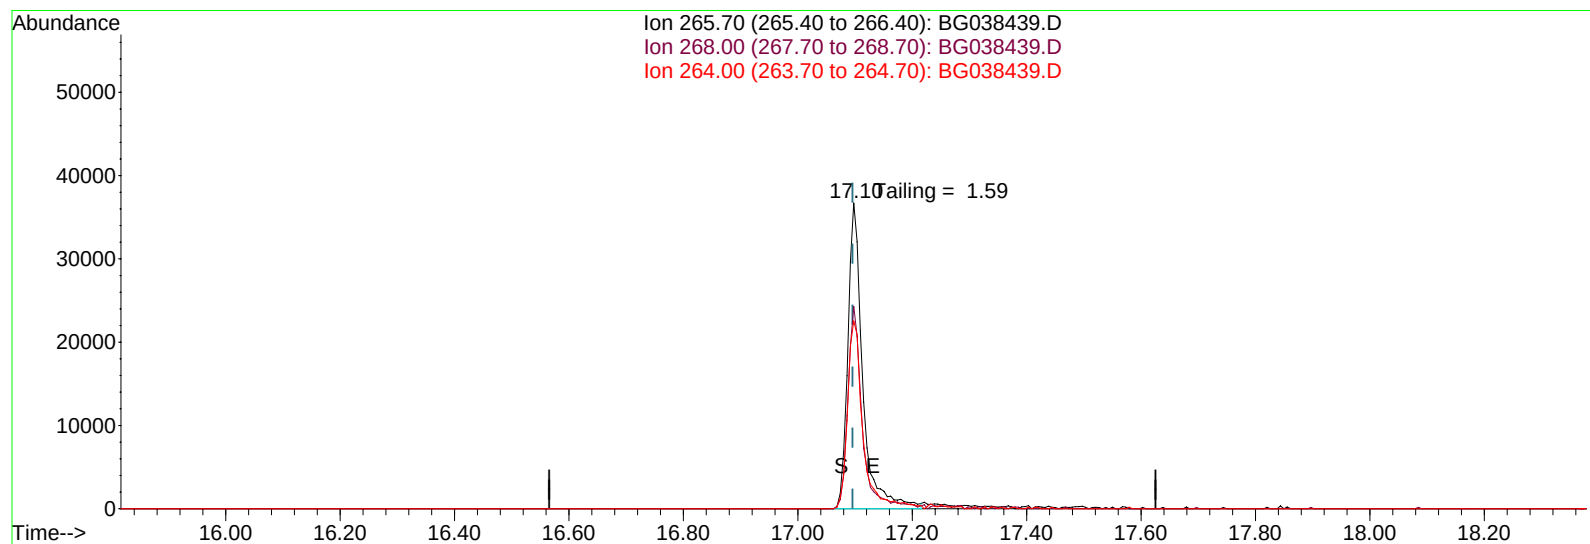

(70) Pentachlorophenol (C)

17.098min (+0.002) 25520.32ng

response 66783

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	70.83
264.00	73.60	61.45
0.00	0.00	0.00