

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121018\
 Data File : BG038452.D
 Acq On : 10 Dec 2018 23:34
 Operator : JU/SJ
 Sample : J6309-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC-20181207-WATER

Quant Time: Dec 11 04:10:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 04 17:15:40 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	25149	20.00	ng	0.00
21) Naphthalene-d8	10.89	136	109552	20.00	ng	0.00
39) Acenaphthene-d10	14.70	164	73823	20.00	ng	0.00
64) Phenanthrene-d10	17.45	188	189435	20.00	ng	0.00
76) Chrysene-d12	21.73	240	184399	20.00	ng	-0.01
87) Perylene-d12	25.04	264	190738	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	179579	126.36	ng	0.00
7) Phenol-d6	7.22	99	229312	111.64	ng	0.00
23) Nitrobenzene-d5	9.25	82	190530	86.35	ng	0.00
42) 2,4,6-Tribromophenol	16.20	330	131976	145.63	ng	0.00
45) 2-Fluorobiphenyl	13.32	172	441716	85.26	ng	0.00
79) Terphenyl-d14	20.06	244	845680	98.25	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG121018\
Data File : BG038452.D
Acq On : 10 Dec 2018 23:34
Operator : JU/SJ
Sample : J6309-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC-20181207-WATER

Quant Time: Dec 11 04:10:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG120418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 04 17:15:40 2018
Response via : Initial Calibration

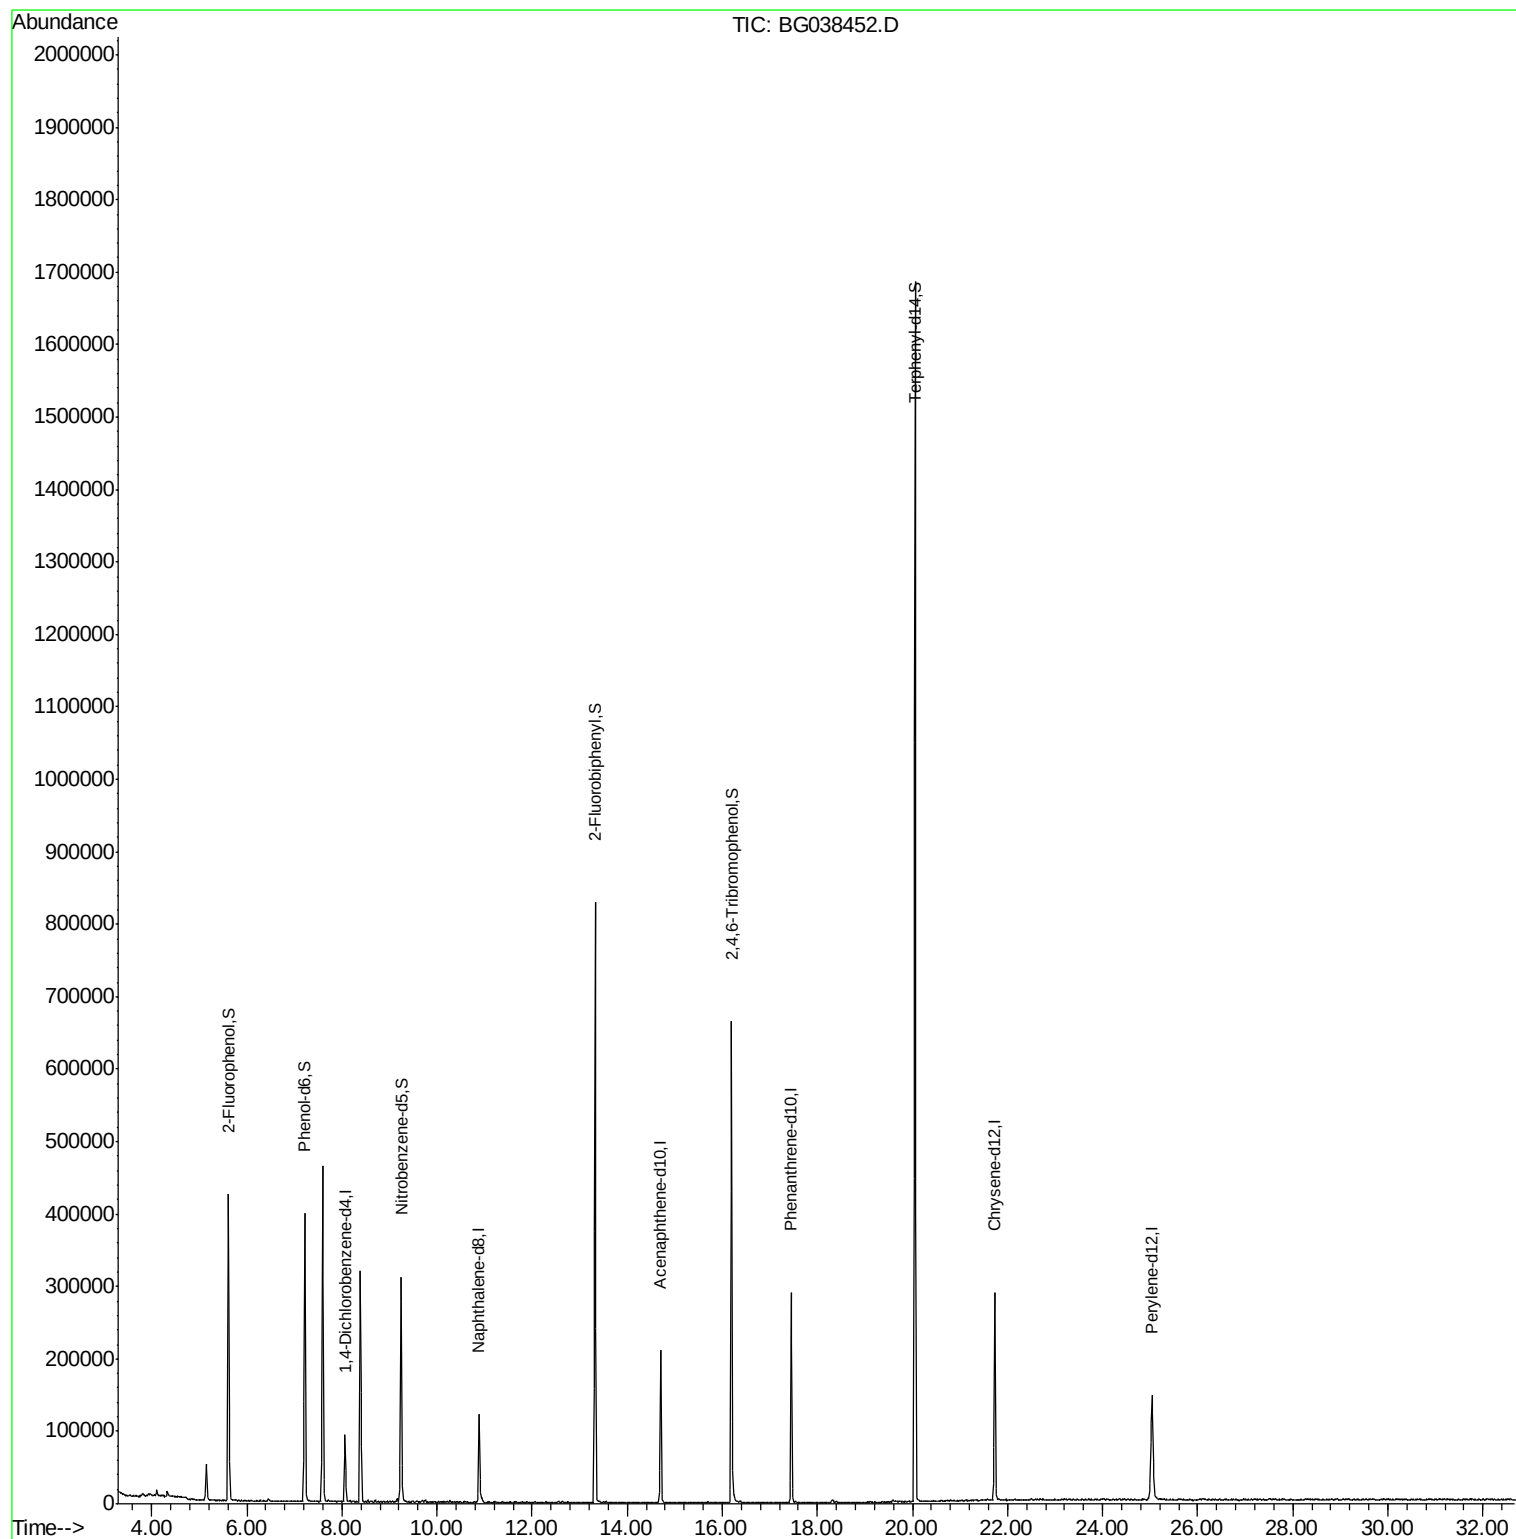

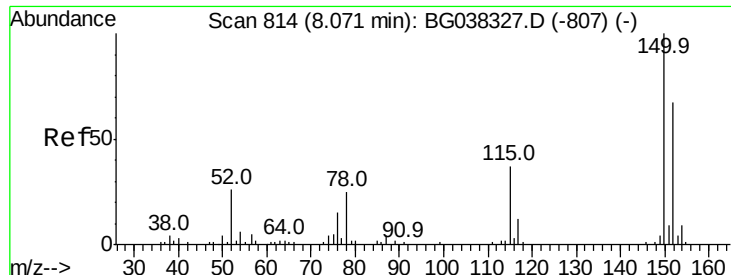


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 814
Delta R.T. -0.00 min
Lab File: BG038452.D
Acq: 10 Dec 2018 23:34

Instrument :
BNA_G
ClientSampleId :
WC-20181207-WATER

Tot Ion:152 Resp: 25149
Ion Ratio Lower Upper
152 100
150 157.0 126.0 189.0
115 63.6 45.5 68.3

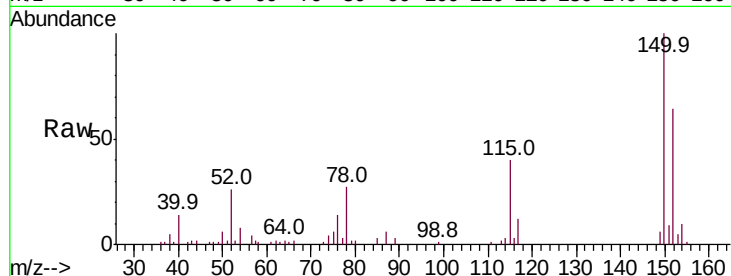


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

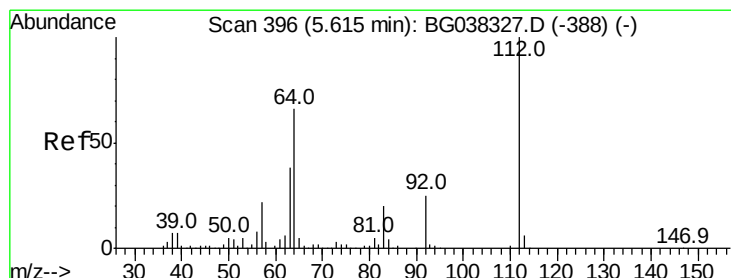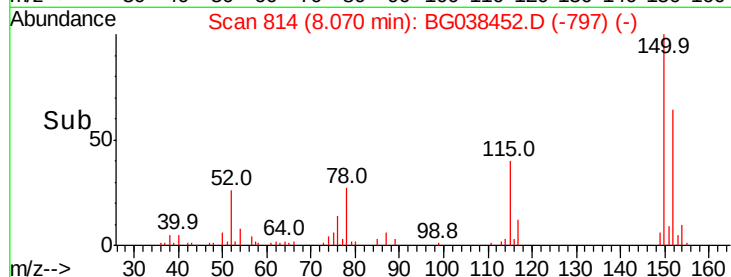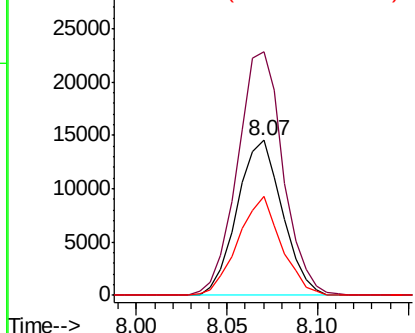



#5


2-Fluorophenol
Concen: 126.363 ng
RT: 5.61 min Scan# 396
Delta R.T. -0.00 min
Lab File: BG038452.D
Acq: 10 Dec 2018 23:34

Tgt Ion:112 Resp: 179579
Ion Ratio Lower Upper
112 100
64 68.2 53.1 79.7
63 37.6 27.3 40.9

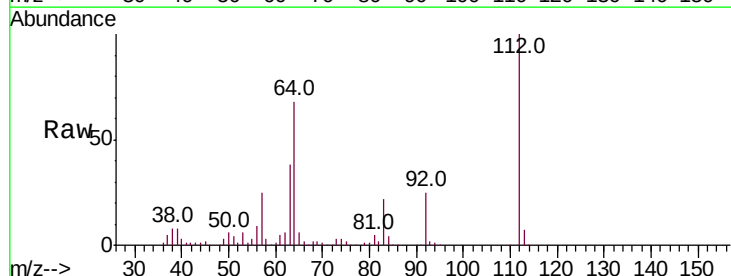

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

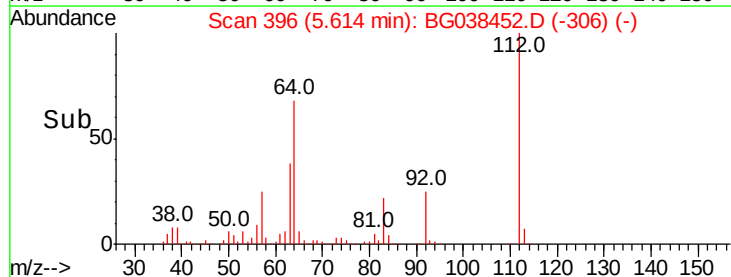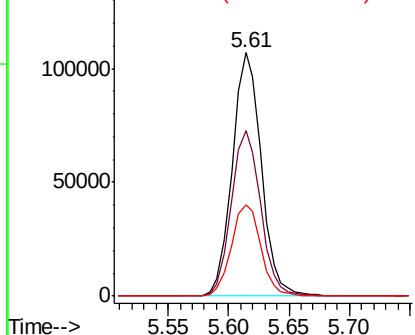

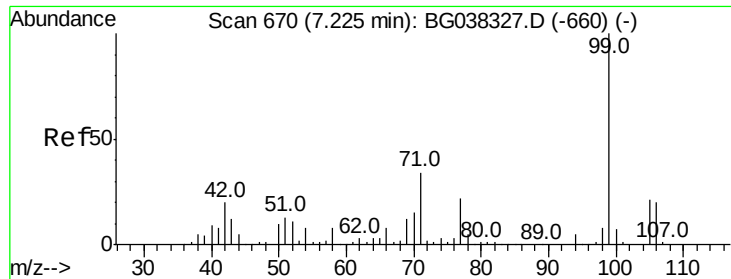

#7

Phenol-d6

Concen: 111.641 ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BG038452.D

Acq: 10 Dec 2018 23:34

Instrument :

BNA_G

ClientSampleId :

WC-20181207-WATER


Tot Ion: 99 Resp: 229312

Ion Ratio Lower Upper




99 100

42 24.7 15.0 22.4#

71 37.1 25.5 38.3

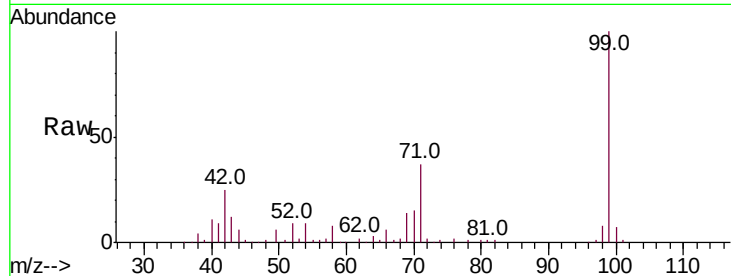

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

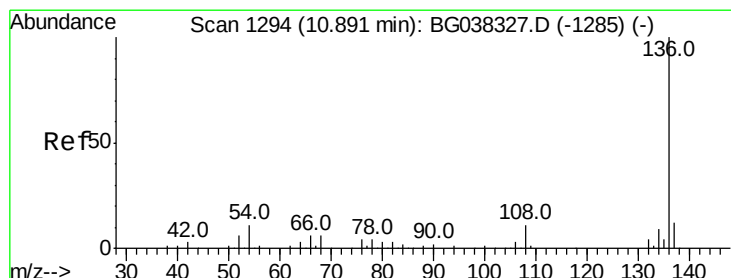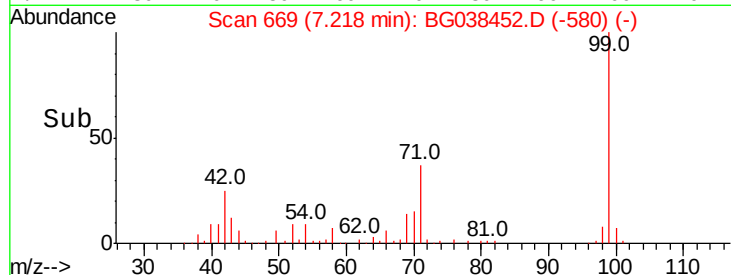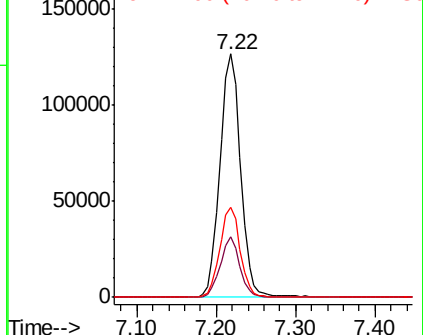

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.89 min Scan# 1294

Delta R.T. -0.00 min

Lab File: BG038452.D

Acq: 10 Dec 2018 23:34

Tgt Ion: 136 Resp: 109552


Ion Ratio Lower Upper

136 100



137 11.6 9.6 14.4


54 11.6 7.9 11.9

68 5.2 4.8 7.2

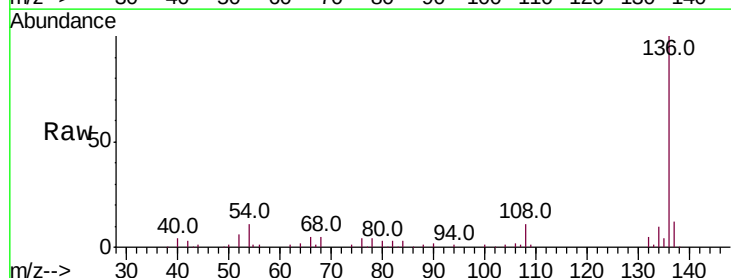

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



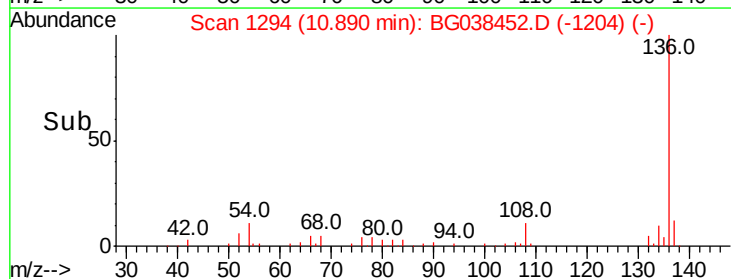
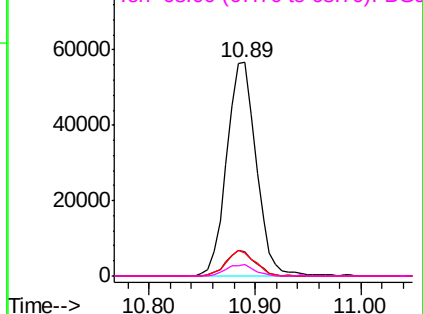


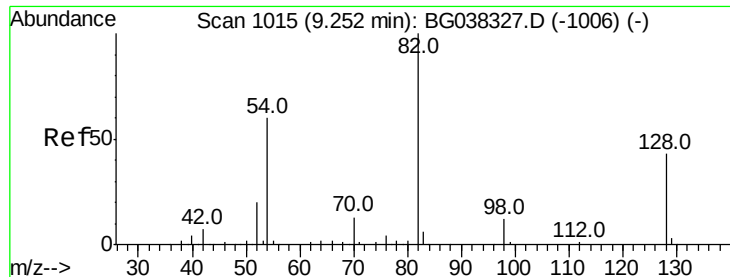

#23
 Nitrobenzene-d5
 Concen: 86.346 ng
 RT: 9.25 min Scan# 1014
 Delta R.T. -0.01 min
 Lab File: BG038452.D
 Acq: 10 Dec 2018 23:34




Instrument :
 BNA_G
 ClientSampleId :
 WC-20181207-WATER


Tot Ion: 82 Resp: 190530
 Ion Ratio Lower Upper
 82 100
 128 43.3 34.6 51.8
 54 64.3 45.3 67.9

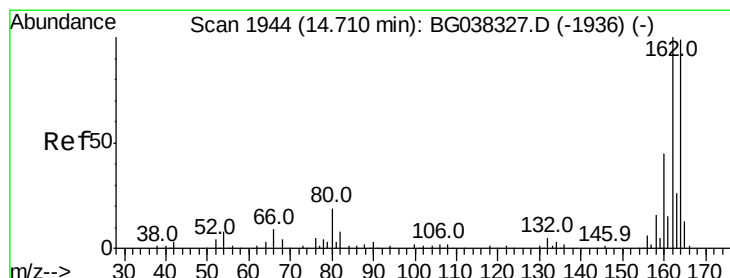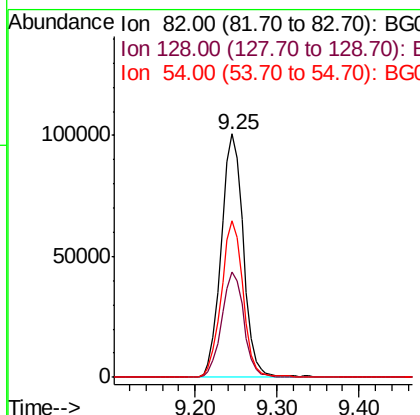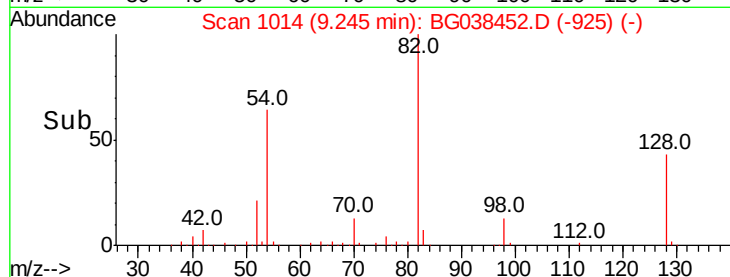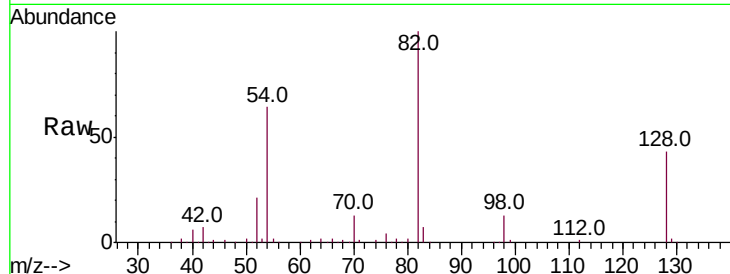

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.70 min Scan# 1943
 Delta R.T. -0.01 min
 Lab File: BG038452.D
 Acq: 10 Dec 2018 23:34

Tgt Ion:164 Resp: 73823
 Ion Ratio Lower Upper
 164 100
 162 107.4 81.3 121.9
 160 45.3 36.3 54.5

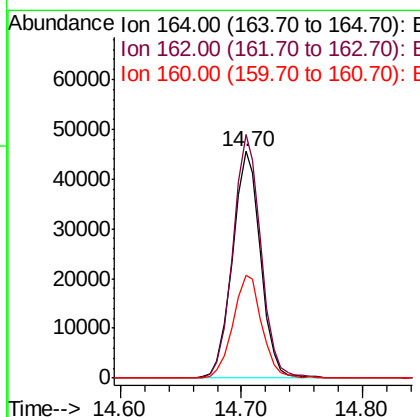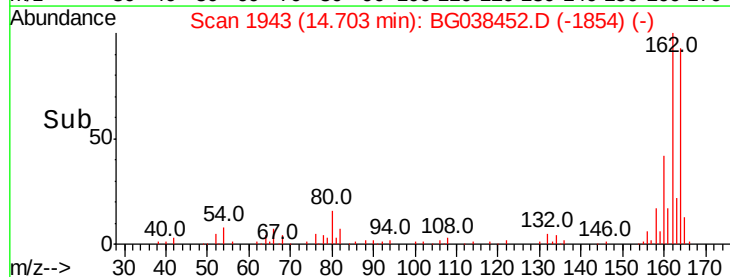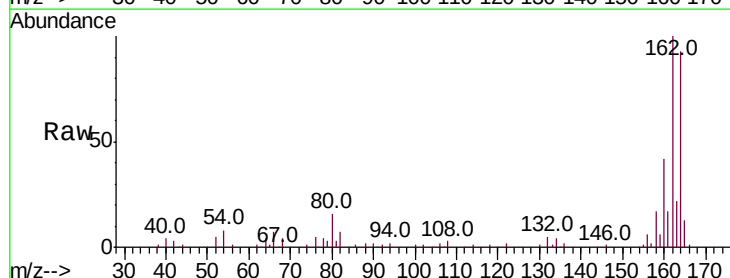


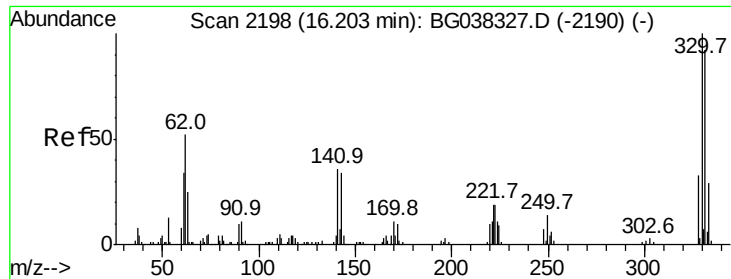




#42
 2,4,6-Tribromophenol
 Concen: 145.626 ng
 RT: 16.20 min Scan# 2197
 Delta R.T. -0.01 min
 Lab File: BG038452.D
 Acq: 10 Dec 2018 23:34

Instrument :
 BNA_G
 ClientSampleId :
 WC-20181207-WATER

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	78.4	117.6
141	37.2	32.2	48.2

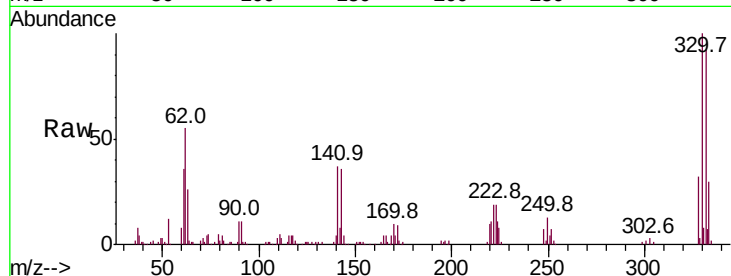


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

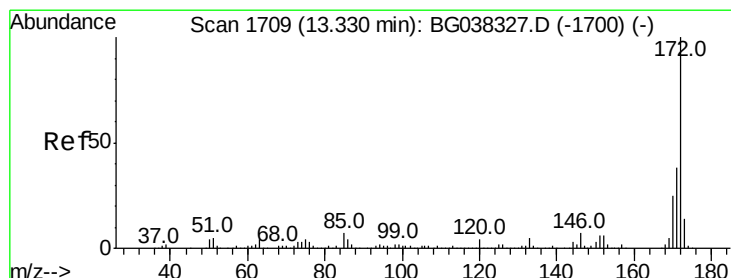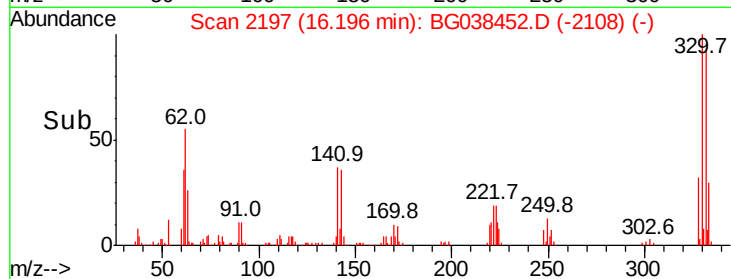
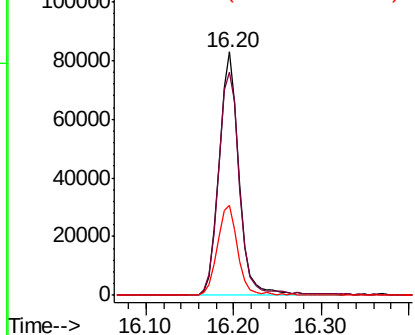



#45
 2-Fluorobiphenyl
 Concen: 85.259 ng
 RT: 13.32 min Scan# 1708
 Delta R.T. -0.01 min
 Lab File: BG038452.D
 Acq: 10 Dec 2018 23:34

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.5	31.0	46.4
170	24.5	20.2	30.2

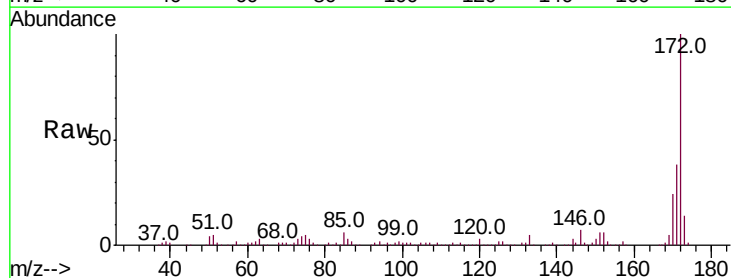

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

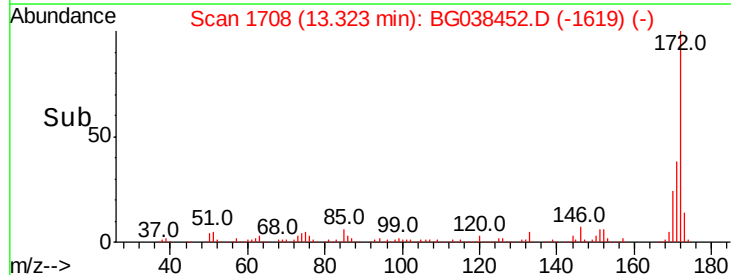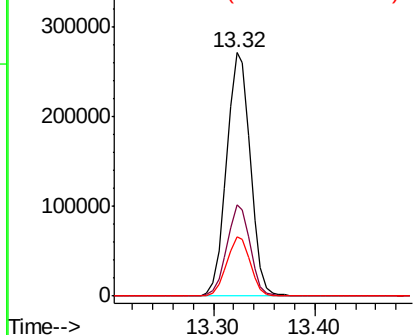


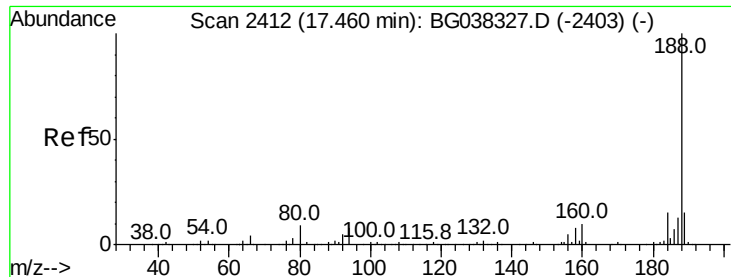




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.45 min Scan# 2411
 Delta R.T. -0.01 min
 Lab File: BG038452.D
 Acq: 10 Dec 2018 23:34

Instrument :
 BNA_G
 ClientSampleId :
 WC-20181207-WATER

Tot Ion:188 Resp: 189435
 Ion Ratio Lower Upper
 188 100
 94 6.7 7.2 10.8#
 80 7.5 7.7 11.5#

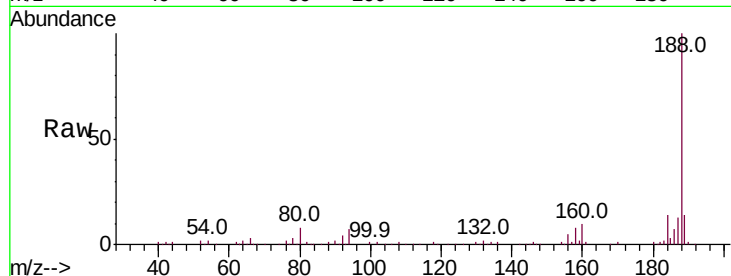


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

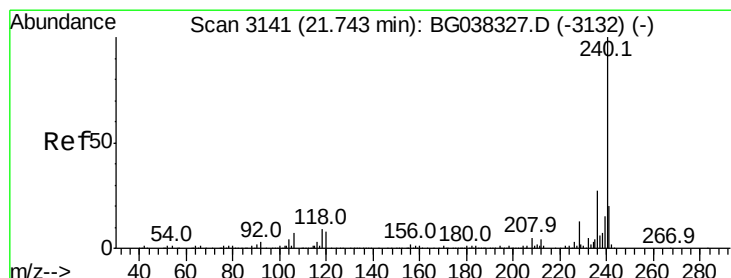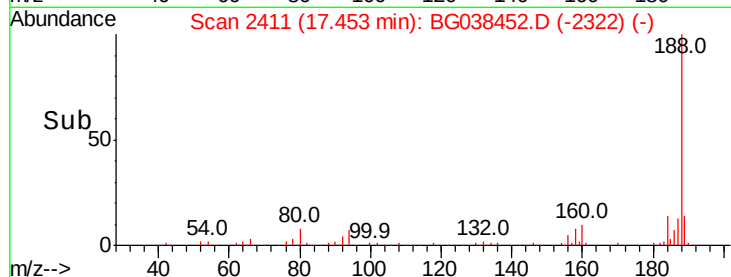
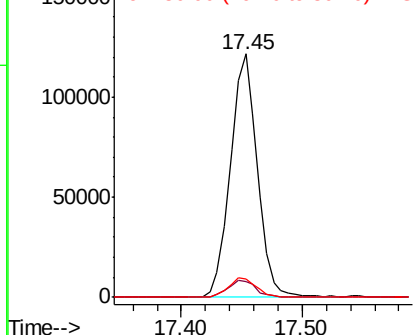



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.73 min Scan# 3139
 Delta R.T. -0.01 min
 Lab File: BG038452.D
 Acq: 10 Dec 2018 23:34

Tgt Ion:240 Resp: 184399
 Ion Ratio Lower Upper
 240 100
 120 7.8 8.1 12.1#
 236 26.4 21.4 32.0

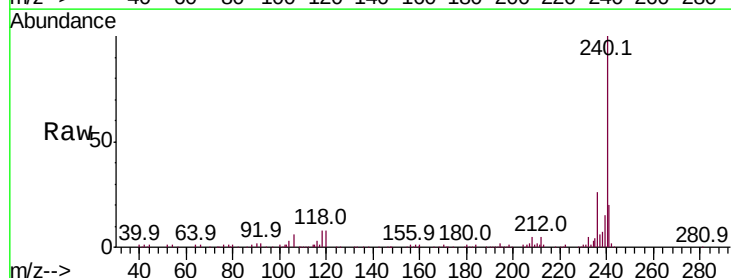

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

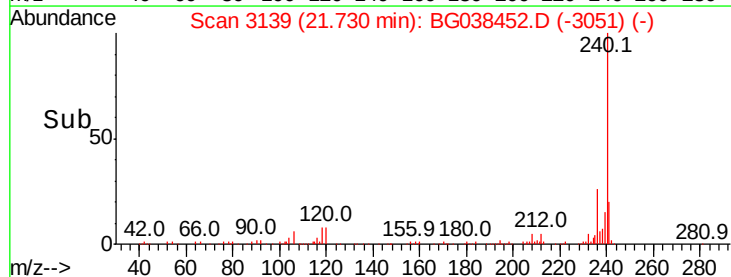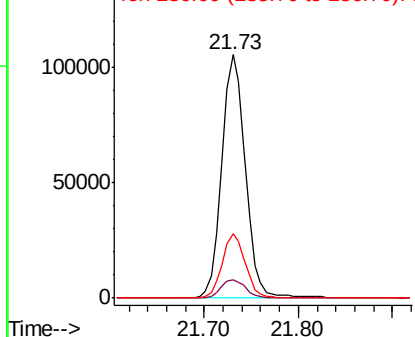

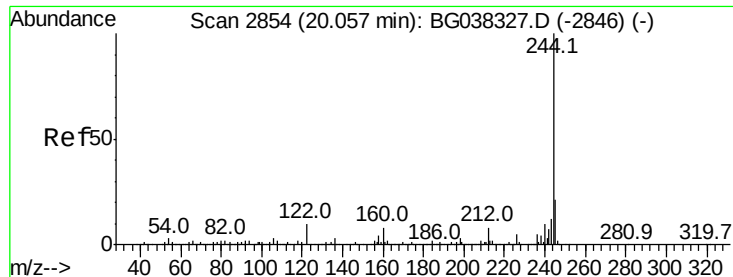

#79

Terphenyl-d14

Concen: 98.247 ng

RT: 20.06 min Scan# 2854

Delta R.T. -0.00 min

Lab File: BG038452.D

Acq: 10 Dec 2018 23:34

Instrument :

BNA_G

ClientSampleId :

WC-20181207-WATER


Tot Ion:244 Resp: 845680

Ion Ratio Lower Upper

244 100

212 7.7 6.5 9.7




122 8.2 9.0 13.4#

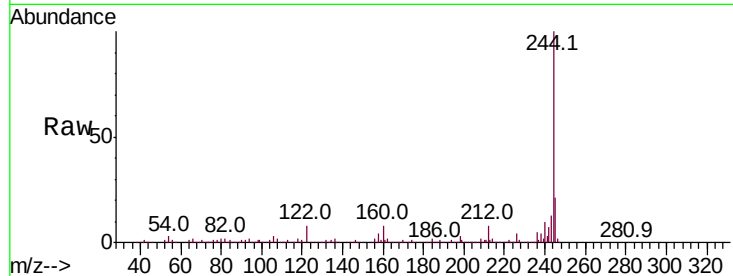

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

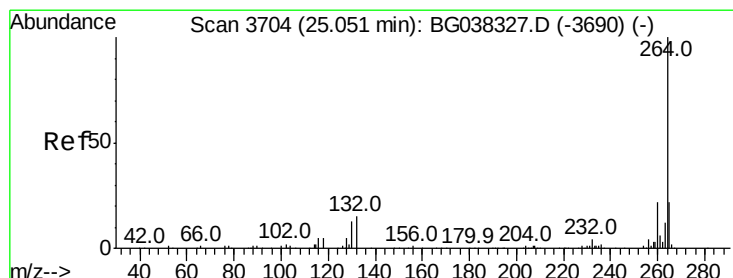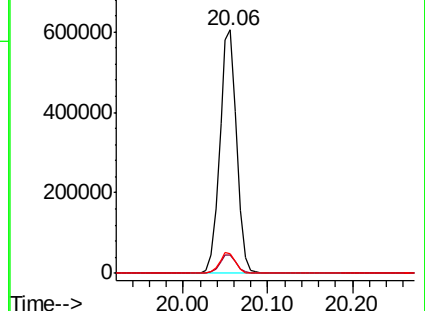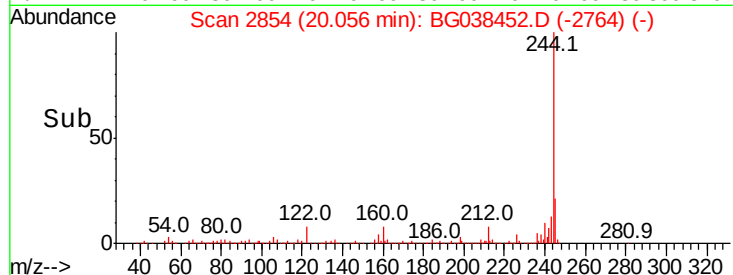

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.04 min Scan# 3702

Delta R.T. -0.01 min

Lab File: BG038452.D

Acq: 10 Dec 2018 23:34


Tgt Ion:264 Resp: 190738

Ion Ratio Lower Upper

264 100

260 21.8 18.2 27.4

265 18.5 17.9 26.9

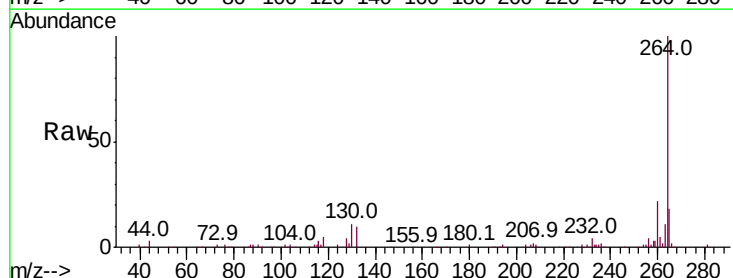

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

