


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121018\
 Data File : BG038435.D
 Acq On : 10 Dec 2018 9:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

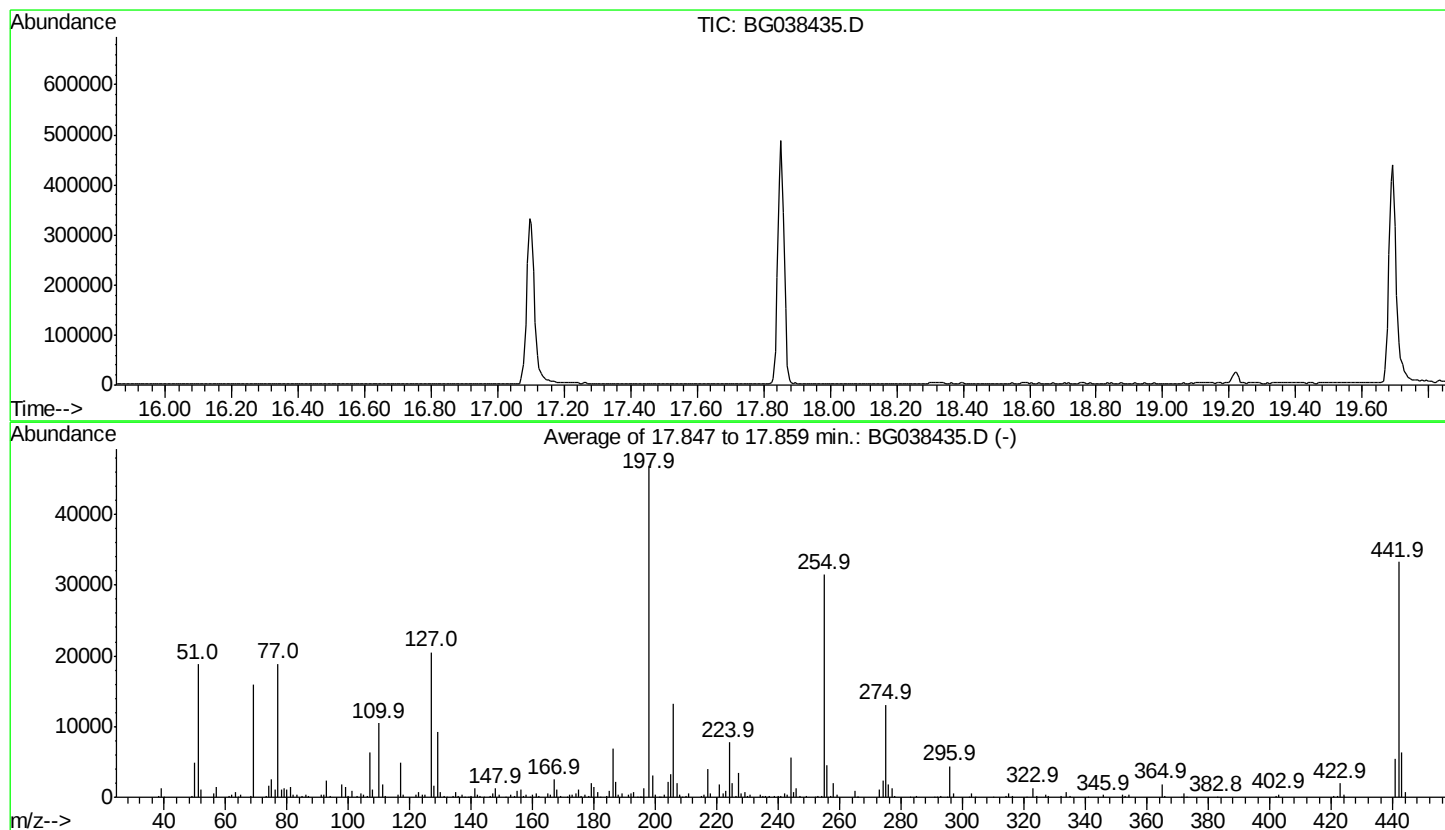

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	18808	PASS
68	69	0.00	2	1.4	217	PASS
69	198	0.00	100	33.8	15856	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.7	20476	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46896	PASS
199	198	5	9	6.5	3063	PASS
275	198	10	60	28.0	13121	PASS
365	198	1	100	4.1	1901	PASS
441	198	0.01	100	11.4	5366	PASS
442	198	50	100	70.9	33253	PASS
443	442	15	24	19.3	6426	PASS