


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG121018\
 Data File : BG038439.D
 Acq On : 10 Dec 2018 15:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG120418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 04 17:15:40 2018

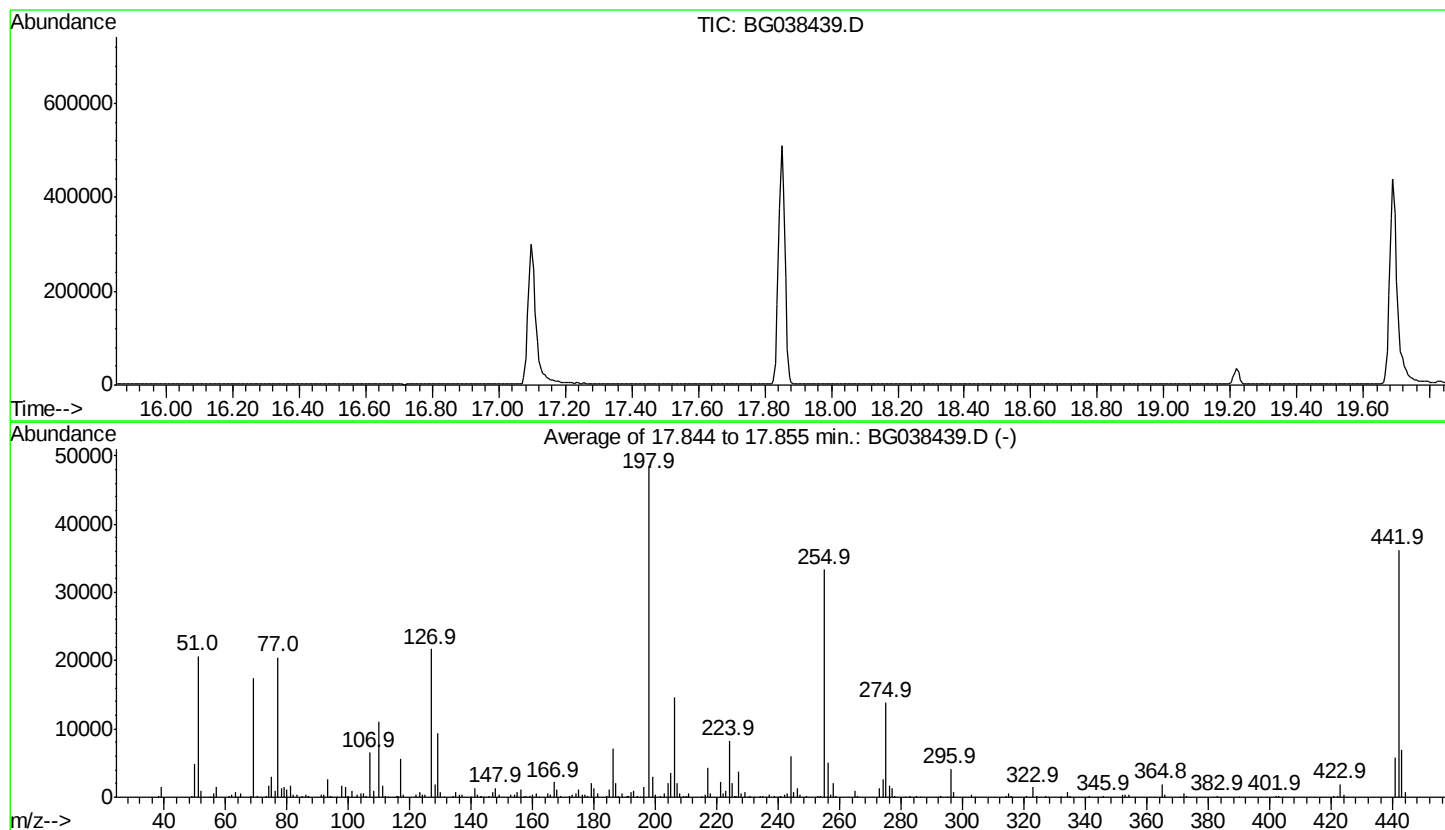

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	20629	PASS
68	69	0.00	2	1.4	241	PASS
69	198	0.00	100	35.9	17428	PASS
70	69	0.00	2	0.8	132	PASS
127	198	10	80	44.7	21725	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48562	PASS
199	198	5	9	6.4	3091	PASS
275	198	10	60	28.5	13834	PASS
365	198	1	100	3.9	1911	PASS
441	198	0.01	100	12.0	5835	PASS
442	198	50	100	74.5	36202	PASS
443	442	15	24	19.0	6892	PASS