

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
 Data File : BG063646.D
 Acq On : 11 Dec 2024 00:14
 Operator : RC/JU
 Sample : PB165508BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS508

Quant Time: Dec 11 00:57:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 06 15:14:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.812	152	145445	20.000	ng/u1	0.00
20) Naphthalene-d8	10.603	136	628458	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	476827	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.201	188	1104192	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.454	240	1063358	20.000	ng/u1	#-0.02
88) Perylene-d12	24.474	264	1137633	20.000	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.282	96	24578m	7.460	ng/uL	0.00
4) Pyridine-d5	3.687	84	422454	34.663	ng/u1	0.00
7) Phenol-d5	6.995	99	543058	37.923	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.148	67	329605	34.042	ng/u1	0.00
11) 2-Chlorophenol-d4	7.353	132	346443	41.069	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	391962	36.917	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	171553	38.890	ng/u1	0.00
24) 2-Nitrophenol-d4	9.686	143	182712	36.195	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.232	165	390689	35.945	ng/u1	0.00
31) 4-Chloroaniline-d4	10.738	131	356687	27.155	ng/u1	0.00
46) Dimethylphthalate-d6	13.858	166	1187751	34.274	ng/u1	0.00
49) Acenaphthylene-d8	14.145	160	1357782	35.845	ng/u1	0.00
54) 4-Nitrophenol-d4	14.674	143	160882	36.256	ng/u1	0.00
60) Fluorene-d10	15.450	176	1040498	30.459	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.579	200	192859	30.918	ng/u1	0.00
73) Anthracene-d10	17.301	188	1768676	35.080	ng/u1	-0.01
81) Pyrene-d10	19.604	212	2002389	33.973	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.269	264	2020948	35.370	ng/u1	-0.03
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.317	88	55477	12.646	ng/uL#	65
5) Pyridine	3.711	79	420370	33.214	ng/u1#	87
6) Benzaldehyde	6.960	77	29755	3.247	ng/u1	98
8) Phenol	7.024	94	571908	37.151	ng/u1#	85
10) Bis(2-Chloroethyl)ether	7.236	93	391480	36.808	ng/u1	88
12) 2-Chlorophenol	7.383	128	358775	42.028	ng/u1	93
13) 2-Methylphenol	8.264	108	400537	37.288	ng/u1	95
14) 2,2'-oxybis(1-Chloropr...	8.329	45	606510	42.407	ng/u1	95
16) Acetophenone	8.634	105	652542	33.385	ng/u1	91
17) N-Nitroso-di-n-propyla...	8.617	70	383000	34.393	ng/u1	98
18) 4-Methylphenol	8.593	108	438176	37.148	ng/u1	99
19) Hexachloroethane	8.887	117	151391	33.188	ng/u1	89
22) Nitrobenzene	9.010	77	571472	32.025	ng/u1#	88
23) Isophorone	9.533	82	1015657	31.569	ng/u1	98
25) 2-Nitrophenol	9.721	139	191036	37.981	ng/u1#	81
26) 2,4-Dimethylphenol	9.786	107	445175	32.479	ng/u1#	82
27) Bis(2-Chloroethoxy)met...	10.015	93	547907	36.449	ng/u1	100
29) 2,4-Dichlorophenol	10.262	162	380385	34.913	ng/u1	97
30) Naphthalene	10.650	128	1144187	35.367	ng/u1	95
32) 4-Chloroaniline	10.761	127	175358	14.093	ng/u1	100
33) Hexachlorobutadiene	10.937	225	288309	25.646	ng/u1	97
34) Caprolactam	11.519	113	118043m	33.096	ng/u1	
35) 4-Chloro-3-methylphenol	11.901	107	445520	32.780	ng/u1#	83
36) 2-Methylnaphthalene	12.265	142	825417	33.094	ng/u1	96


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
 Data File : BG063646.D
 Acq On : 11 Dec 2024 00:14
 Operator : RC/JU
 Sample : PB165508BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS508

Quant Time: Dec 11 00:57:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 06 15:14:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.483	142	824935	32.621	ng/ul#	98
39) 1,2,4,5-Tetrachloroben...	12.635	216	541419	29.206	ng/ul	98
40) Hexachlorocyclopentadiene	12.618	237	157226	20.317	ng/ul#	95
41) 2,4,6-Trichlorophenol	12.882	196	326710	35.736	ng/ul	93
42) 2,4,5-Trichlorophenol	12.964	196	362887	36.791	ng/ul	98
43) 1,1'-Biphenyl	13.282	154	1165123	36.811	ng/ul#	95
44) 2-Chloronaphthalene	13.323	162	921609	35.328	ng/ul	96
45) 2-Nitroaniline	13.528	65	317410	37.246	ng/ul#	81
47) Dimethylphthalate	13.905	163	1176871	33.567	ng/ul	99
48) 2,6-Dinitrotoluene	14.028	165	229029	35.405	ng/ul	90
50) Acenaphthylene	14.175	152	1455242	36.532	ng/ul	99
51) 3-Nitroaniline	14.357	138	144017	26.416	ng/ul	85
52) Acenaphthene	14.516	153	1032721	35.705	ng/ul	96
53) 2,4-Dinitrophenol	14.580	184	100592	31.501	ng/ul	90
55) 4-Nitrophenol	14.686	109	174430	25.585	ng/ul#	81
56) Dibenzofuran	14.850	168	1468176	32.844	ng/ul	99
57) 2,4-Dinitrotoluene	14.827	165	339488	33.276	ng/ul#	84
58) 2,3,4,6-Tetrachlorophenol	15.086	232	288568	31.281	ng/ul#	97
59) Diethylphthalate	15.274	149	1137556	33.296	ng/ul	98
61) Fluorene	15.503	166	1145729	31.467	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.497	204	631613	26.937	ng/ul	97
63) 4-Nitroaniline	15.532	138	219880m	37.505	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.597	198	199185	31.981	ng/ul#	90
67) N-Nitrosodiphenylamine	15.714	169	998370	38.608	ng/ul	98
68) 4-Bromophenyl-phenylether	16.396	248	426555	32.693	ng/ul	92
69) Hexachlorobenzene	16.513	284	458190	32.624	ng/ul	94
70) Atrazine	16.666	200	68296	5.650	ng/ul#	93
71) Pentachlorophenol	16.860	266	191259	38.731	ng/ul#	80
72) Phenanthrene	17.248	178	1985531	36.505	ng/ul	98
74) Anthracene	17.336	178	2000686	35.621	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.246	216	543692	34.889	ng/ul	98
76) Pentachlorobenzene	14.780	250	546625	33.575	ng/ul	98
77) Carbazole	17.612	167	1692911	37.621	ng/ul	96
78) Di-n-butylphthalate	18.170	149	1903695	39.629	ng/ul#	97
80) Fluoranthene	19.269	202	2313510	34.925	ng/ul#	93
82) Pyrene	19.633	202	2489841	35.358	ng/ul#	91
83) Butylbenzylphthalate	20.526	149	731256	49.314	ng/ul#	90
84) 3,3'-Dichlorobenzidine	21.360	252	440583	24.204	ng/ul#	98
85) Benzo(a)anthracene	21.437	228	2445586	34.102	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.349	149	1094800	49.107	ng/ul#	99
87) Chrysene	21.502	228	2311004	34.304	ng/ul	99
89) Di-n-octyl phthalate	22.489	149	1940263	48.802	ng/ul	100
90) Benzo(b)fluoranthene	23.523	252	2431677	34.409	ng/ul#	97
91) Benzo(k)fluoranthene	23.581	252	2447780	34.845	ng/ul#	98
93) Benzo(a)pyrene	24.333	252	2273849	34.306	ng/ul#	96
94) Indeno(1,2,3-cd)pyrene	27.888	276	2804498	35.076	ng/ul#	91
95) Dibenzo(a,h)anthracene	27.929	278	2263883	35.304	ng/ul#	94
96) Benzo(g,h,i)perylene	28.946	276	2196391	36.143	ng/ul#	93





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 12.646 ng/uL
RT: 3.317 min Scan# 39
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion: 88 Resp: 55477
Ion Ratio Lower Upper
88 100
43 30.3 18.3 27.5#
58 87.9 45.2 67.8#

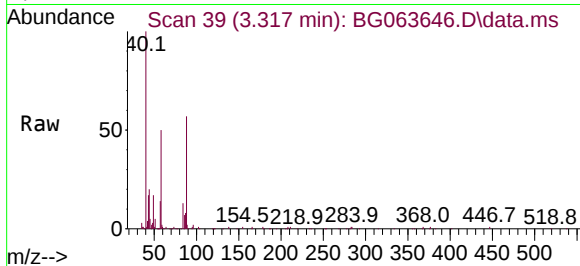

#5
Pyridine
Concen: 33.214 ng/uL
RT: 3.711 min Scan# 106
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion: 79 Resp: 420370
Ion Ratio Lower Upper
79 100
52 76.6 48.6 72.8#
51 37.2 29.8 44.8




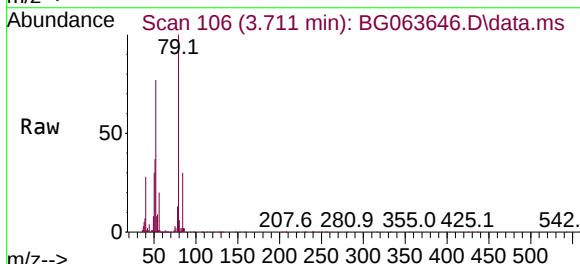




#6
Benzaldehyde
Concen: 3.247 ng/ul
RT: 6.960 min Scan# 61
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion: 77 Resp: 29755
Ion Ratio Lower Upper
77 100
105 82.3 67.3 100.9
106 77.8 60.5 90.7



#8
Phenol
Concen: 37.151 ng/ul
RT: 7.024 min Scan# 670
Delta R.T. 0.004 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion: 94 Resp: 571908
Ion Ratio Lower Upper
94 100
65 32.7 31.8 47.8
66 44.0 45.0 67.6#



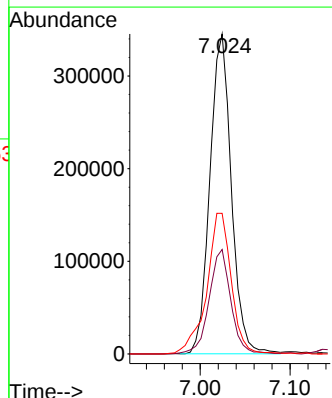





#10
Bis(2-Chloroethyl)ether
Concen: 36.808 ng/ul
RT: 7.236 min Scan# 706
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion: 93 Resp: 391480
Ion Ratio Lower Upper
93 100
63 83.8 77.6 116.4
95 29.9 28.2 42.2



#12
2-Chlorophenol
Concen: 42.028 ng/ul
RT: 7.383 min Scan# 731
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:128 Resp: 358775
Ion Ratio Lower Upper
128 100
64 61.4 54.2 81.2
130 32.2 23.0 34.6









#13
2-Methylphenol
Concen: 37.288 ng/ul
RT: 8.264 min Scan# 881
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:108 Resp: 400537
Ion Ratio Lower Upper
108 100
107 90.0 76.2 114.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 42.407 ng/ul
RT: 8.329 min Scan# 892
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion: 45 Resp: 606510
Ion Ratio Lower Upper
45 100
77 15.0 13.8 20.6
79 11.4 10.8 16.2









#16
Acetophenone
Concen: 33.385 ng/ul
RT: 8.634 min Scan# 944
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:105 Resp: 652542
Ion Ratio Lower Upper
105 100
77 87.1 77.0 115.4
51 29.0 26.2 39.4



#17
N-Nitroso-di-n-propylamine
Concen: 34.393 ng/ul
RT: 8.617 min Scan# 941
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion: 70 Resp: 383000
Ion Ratio Lower Upper
70 100
42 49.4 40.8 61.2
101 7.3 5.1 7.7
130 13.5 11.0 16.6









#18
4-Methylphenol
Concen: 37.148 ng/ul
RT: 8.593 min Scan# 91
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:108 Resp: 438176
Ion Ratio Lower Upper
108 100
107 109.1 88.3 132.5



#19
Hexachloroethane
Concen: 33.188 ng/ul
RT: 8.887 min Scan# 987
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:117 Resp: 151391
Ion Ratio Lower Upper
117 100
201 105.3 97.2 145.8
199 72.0 61.7 92.5









#22
Nitrobenzene
Concen: 32.025 ng/ul
RT: 9.010 min Scan# 1008
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion: 77 Resp: 571472
Ion Ratio Lower Upper
77 100
123 32.4 19.8 29.8#
65 13.0 12.6 18.8

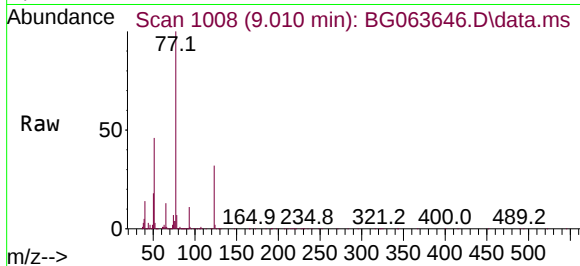

#23
Isophorone
Concen: 31.569 ng/ul
RT: 9.533 min Scan# 1097
Delta R.T. -0.002 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion: 82 Resp: 1015657
Ion Ratio Lower Upper
82 100
95 7.0 6.6 9.8
138 12.0 9.2 13.8




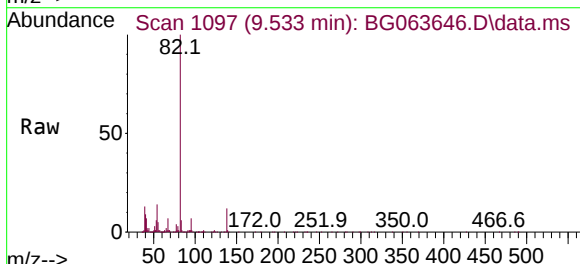




#25
2-Nitrophenol
Concen: 37.981 ng/ul
RT: 9.721 min Scan# 1129
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:139 Resp: 191036
Ion Ratio Lower Upper
139 100
65 73.6 71.2 106.8
109 38.3 43.8 65.6#

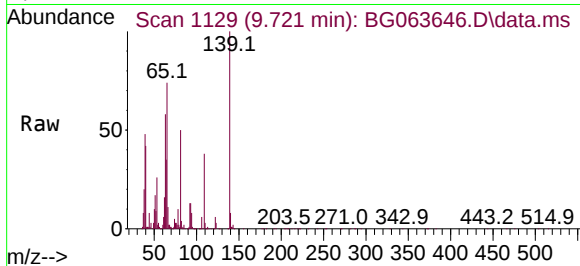

#26
2,4-Dimethylphenol
Concen: 32.479 ng/ul
RT: 9.786 min Scan# 1140
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:107 Resp: 445175
Ion Ratio Lower Upper
107 100
121 45.0 27.1 40.7#
122 79.1 52.0 78.0#

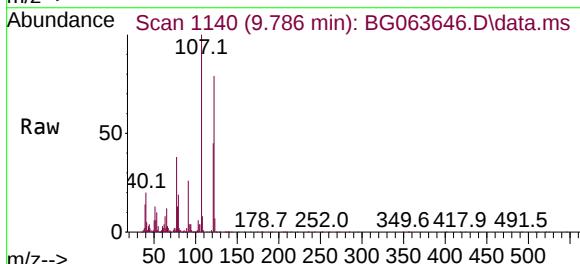







#27
 Bis(2-Chloroethoxy)methane
 Concen: 36.449 ng/ul
 RT: 10.015 min Scan# 1179
 Delta R.T. -0.008 min
 Lab File: BG063646.D
 Acq: 11 Dec 2024 00:14

Instrument :
 BNA_G
 ClientSampleId :
 SLCS508

Tgt Ion: 93 Resp: 547907




Ion	Ratio	Lower	Upper
93	100		
95	31.7	25.6	38.4
123	8.2	6.6	9.8

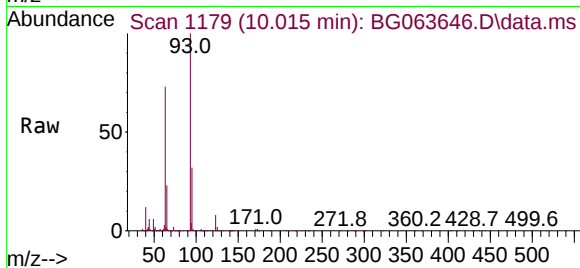


#29
 2,4-Dichlorophenol
 Concen: 34.913 ng/ul
 RT: 10.262 min Scan# 1221
 Delta R.T. -0.002 min
 Lab File: BG063646.D
 Acq: 11 Dec 2024 00:14

Tgt Ion: 162 Resp: 380385

Ion	Ratio	Lower	Upper
162	100		
164	63.2	49.8	74.8
98	36.9	27.2	40.8




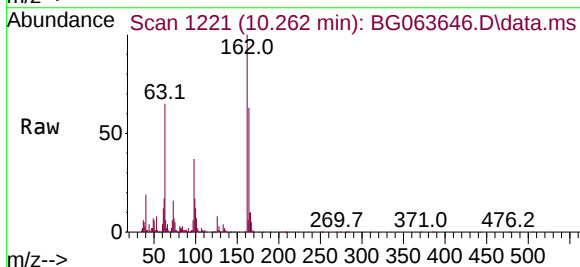




#30
Naphthalene
Concen: 35.367 ng/ul
RT: 10.650 min Scan# 11
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:128 Resp: 1144187
Ion Ratio Lower Upper
128 100
129 11.6 8.4 12.6
127 13.0 12.5 18.7

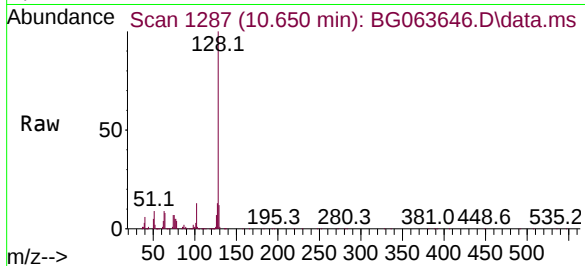

#32
4-Chloroaniline
Concen: 14.093 ng/ul
RT: 10.761 min Scan# 1306
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:127 Resp: 175358
Ion Ratio Lower Upper
127 100
129 30.0 23.8 35.8




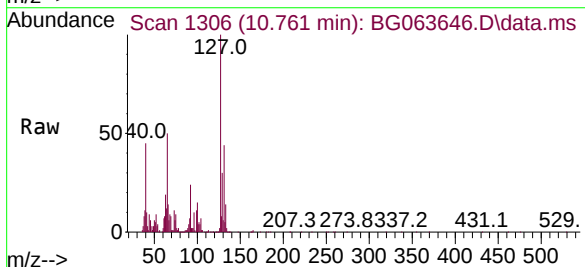




#33
Hexachlorobutadiene
Concen: 25.646 ng/ul
RT: 10.937 min Scan# 11
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:225 Resp: 288309
Ion Ratio Lower Upper
225 100
223 60.0 49.7 74.5
227 66.2 55.2 82.8

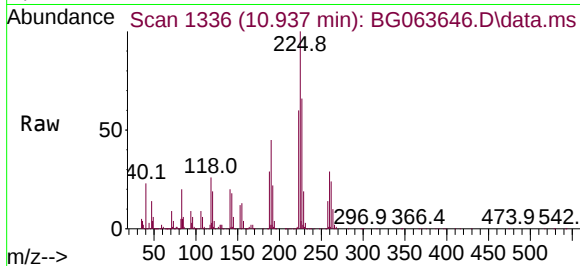

#34
Caprolactam
Concen: 33.096 ng/ul m
RT: 11.519 min Scan# 1435
Delta R.T. 0.010 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:113 Resp: 118043
Ion Ratio Lower Upper
113 100
55 199.3 133.3 199.9
56 149.0 121.6 182.4




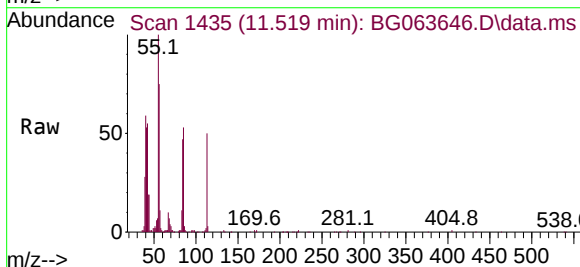




#35
4-Chloro-3-methylphenol
Concen: 32.780 ng/ul
RT: 11.901 min Scan# 1500
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:107 Resp: 445520
Ion Ratio Lower Upper
107 100
144 21.8 14.6 21.8#
142 70.1 44.2 66.4#

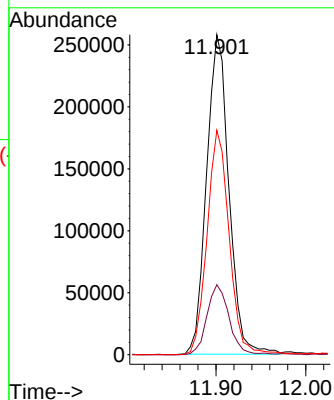

#36
2-Methylnaphthalene
Concen: 33.094 ng/ul
RT: 12.265 min Scan# 1562
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:142 Resp: 825417
Ion Ratio Lower Upper
142 100
141 87.5 73.4 110.0

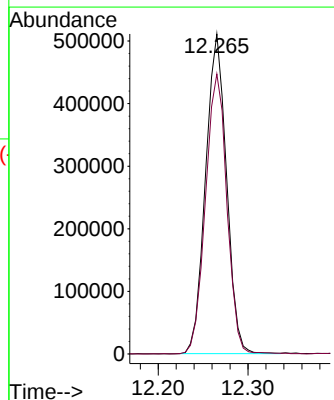



#37

1-Methylnaphthalene

Concen: 32.621 ng/ul

RT: 12.483 min Scan# 1

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Instrument :

BNA_G

ClientSampleId :

SLCS508





Tgt Ion:142 Resp: 824935

Ion Ratio Lower Upper

142 100

141 91.1 74.6 111.8

116 4.9 5.2 7.8#



#39

1,2,4,5-Tetrachlorobenzene

Concen: 29.206 ng/ul

RT: 12.635 min Scan# 1625

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Tgt Ion:216 Resp: 541419




Ion Ratio Lower Upper


216 100

214 78.9 61.8 92.6

179 20.0 16.2 24.4

108 16.7 11.8 17.8









#40
Hexachlorocyclopentadiene
Concen: 20.317 ng/ul
RT: 12.618 min Scan# 1622
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:237 Resp: 157226
Ion Ratio Lower Upper
237 100
235 62.9 53.7 80.5
272 12.0 7.9 11.9#



#41
2,4,6-Trichlorophenol
Concen: 35.736 ng/ul
RT: 12.882 min Scan# 1667
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:196 Resp: 326710
Ion Ratio Lower Upper
196 100
198 99.2 73.9 110.9
200 34.2 24.2 36.4









#42
2,4,5-Trichlorophenol
Concen: 36.791 ng/ul
RT: 12.964 min Scan# 1
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:196 Resp: 362887
Ion Ratio Lower Upper
196 100
198 96.4 78.0 117.0
200 30.4 21.5 32.3



#43
1,1'-Biphenyl
Concen: 36.811 ng/ul
RT: 13.282 min Scan# 1735
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:154 Resp: 1165123
Ion Ratio Lower Upper
154 100
153 40.1 30.6 45.8
76 15.9 9.9 14.9#









#44
2-Chloronaphthalene
Concen: 35.328 ng/ul
RT: 13.323 min Scan# 1742
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:162 Resp: 921609
Ion Ratio Lower Upper
162 100
164 31.9 25.9 38.9
127 37.3 27.0 40.6

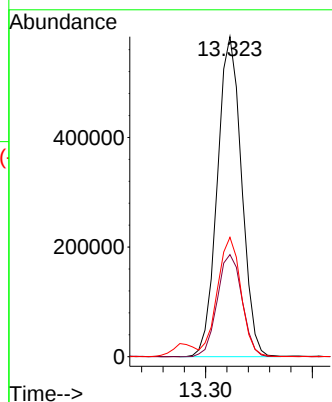

#45
2-Nitroaniline
Concen: 37.246 ng/ul
RT: 13.528 min Scan# 1777
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion: 65 Resp: 317410
Ion Ratio Lower Upper
65 100
92 66.2 44.9 67.3
138 80.1 49.3 73.9#


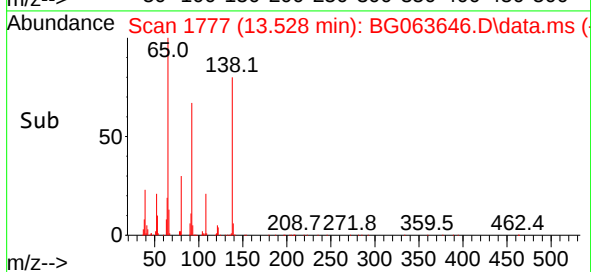
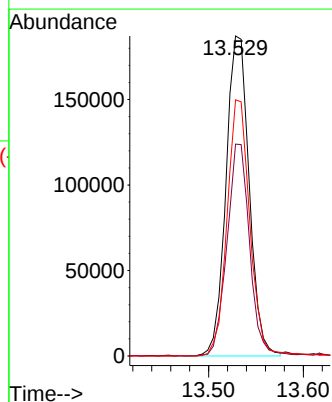





#47
Dimethylphthalate
Concen: 33.567 ng/ul
RT: 13.905 min Scan# 1841
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:163 Resp: 1176871
Ion Ratio Lower Upper
163 100
194 3.6 2.6 3.8
164 9.8 8.3 12.5



#48
2,6-Dinitrotoluene
Concen: 35.405 ng/ul
RT: 14.028 min Scan# 1862
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:165 Resp: 229029
Ion Ratio Lower Upper
165 100
89 80.3 72.9 109.3
121 20.9 18.6 28.0









#50
Acenaphthylene
Concen: 36.532 ng/ul
RT: 14.175 min Scan# 1887
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:152 Resp: 1455242
Ion Ratio Lower Upper
152 100
151 18.4 15.0 22.6
153 12.8 9.9 14.9



#51
3-Nitroaniline
Concen: 26.416 ng/ul
RT: 14.357 min Scan# 1918
Delta R.T. -0.014 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:138 Resp: 144017
Ion Ratio Lower Upper
138 100
108 11.5 9.0 13.4
92 139.0 127.8 191.8









#52
Acenaphthene
Concen: 35.705 ng/ul
RT: 14.516 min Scan# 1945
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:153 Resp: 1032721
Ion Ratio Lower Upper
153 100
152 48.1 37.8 56.8
154 85.2 64.5 96.7



#53
2,4-Dinitrophenol
Concen: 31.501 ng/ul
RT: 14.580 min Scan# 1956
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:184 Resp: 100592
Ion Ratio Lower Upper
184 100
63 74.4 62.9 94.3
154 67.2 65.0 97.4









#55
4-Nitrophenol
Concen: 25.585 ng/ul
RT: 14.686 min Scan# 1974
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:109 Resp: 174430
Ion Ratio Lower Upper
109 100
139 91.9 57.8 86.6#
65 137.0 95.6 143.4

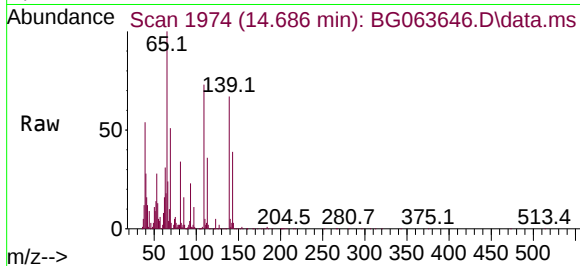

#56
Dibenzofuran
Concen: 32.844 ng/ul
RT: 14.850 min Scan# 2002
Delta R.T. -0.014 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:168 Resp: 1468176
Ion Ratio Lower Upper
168 100
139 35.2 27.9 41.9




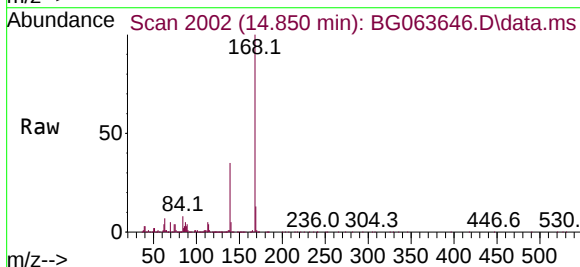




#57
2,4-Dinitrotoluene
Concen: 33.276 ng/ul
RT: 14.827 min Scan# 1998
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:165 Resp: 339488
Ion Ratio Lower Upper
165 100
63 53.1 53.1 79.7#
182 2.2 1.8 2.6



#58
2,3,4,6-Tetrachlorophenol
Concen: 31.281 ng/ul
RT: 15.086 min Scan# 2042
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:232 Resp: 288568
Ion Ratio Lower Upper
232 100
131 34.9 29.3 43.9
130 3.1 1.8 2.8#
166 27.3 20.4 30.6









#59
Diethylphthalate
Concen: 33.296 ng/ul
RT: 15.274 min Scan# 2074
Delta R.T. -0.014 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:149 Resp: 1137556
Ion Ratio Lower Upper
149 100
177 23.3 19.6 29.4
150 12.7 10.2 15.2

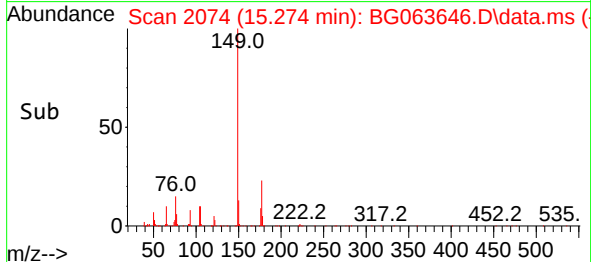

#61
Fluorene
Concen: 31.467 ng/ul
RT: 15.503 min Scan# 2113
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:166 Resp: 1145729
Ion Ratio Lower Upper
166 100
165 101.8 80.6 121.0
167 14.0 10.6 15.8



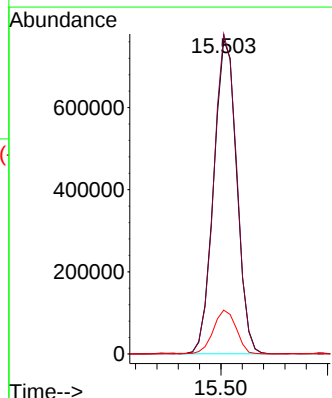





#62
4-Chlorophenyl-phenylether
Concen: 26.937 ng/ul
RT: 15.497 min Scan# 2112
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:204 Resp: 631613
Ion Ratio Lower Upper
204 100
206 34.1 28.2 42.2
141 53.6 40.6 60.8



#63
4-Nitroaniline
Concen: 37.505 ng/ul m
RT: 15.532 min Scan# 2118
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:138 Resp: 219880
Ion Ratio Lower Upper
138 100
92 60.7 56.3 84.5
108 96.0 110.6 165.8#









#66
4,6-Dinitro-2-methylphenol
Concen: 31.981 ng/ul
RT: 15.597 min Scan# 2129
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:198 Resp: 199185
Ion Ratio Lower Upper
198 100
182 4.4 2.6 3.8#
77 25.6 25.0 37.6



#67
N-Nitrosodiphenylamine
Concen: 38.608 ng/ul
RT: 15.714 min Scan# 2149
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:169 Resp: 998370
Ion Ratio Lower Upper
169 100
168 66.3 51.6 77.4
167 36.8 30.7 46.1









#68
4-Bromophenyl-phenylether
Concen: 32.693 ng/ul
RT: 16.396 min Scan# 21
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:248 Resp: 426555
Ion Ratio Lower Upper
248 100
250 93.9 84.5 126.7
141 57.0 46.7 70.1

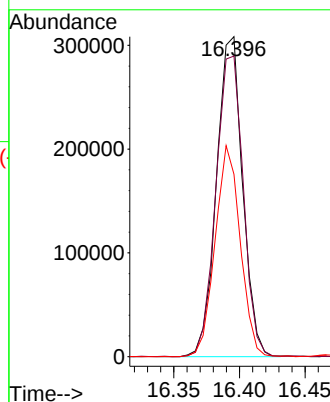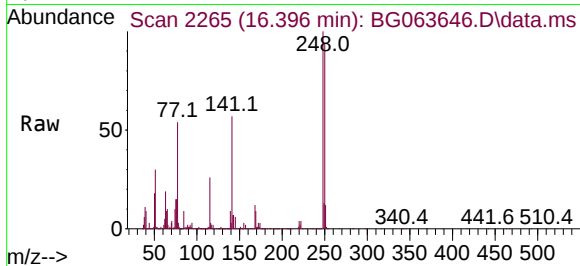

#69
Hexachlorobenzene
Concen: 32.624 ng/ul
RT: 16.513 min Scan# 2285
Delta R.T. -0.014 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:284 Resp: 458190
Ion Ratio Lower Upper
284 100
142 33.4 24.1 36.1
249 37.2 27.4 41.0

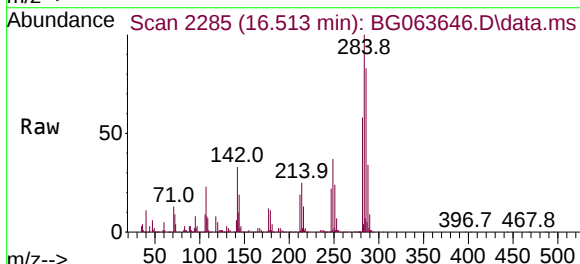



#70

Atrazine

Concen: 5.650 ng/ul

RT: 16.666 min Scan# 21

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Instrument :

BNA_G

ClientSampleId :

SLCS508





Tgt Ion:200 Resp: 68296

Ion Ratio Lower Upper

200 100

173 22.6 14.2 21.2#

215 40.7 35.5 53.3

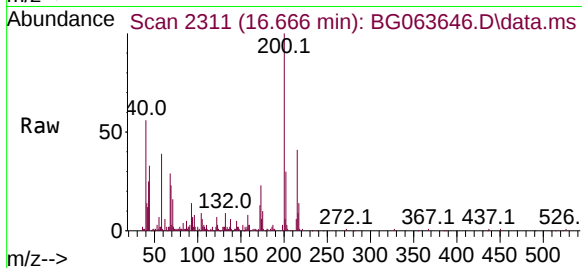

#71

Pentachlorophenol

Concen: 38.731 ng/ul

RT: 16.860 min Scan# 2344

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14




Tgt Ion:266 Resp: 191259


Ion Ratio Lower Upper

266 100

264 62.4 41.8 62.8

268 64.5 37.8 56.8#




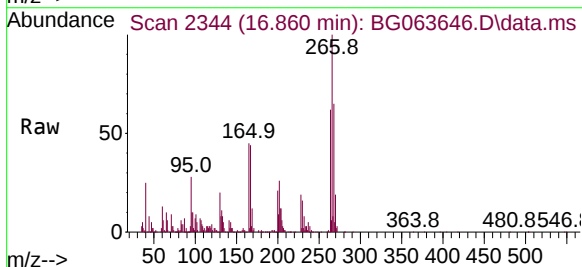




#72
Phenanthrene
Concen: 36.505 ng/uI
RT: 17.248 min Scan# 2410
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:178 Resp: 1985531
Ion Ratio Lower Upper
178 100
179 16.0 13.2 19.8
176 19.9 15.0 22.6

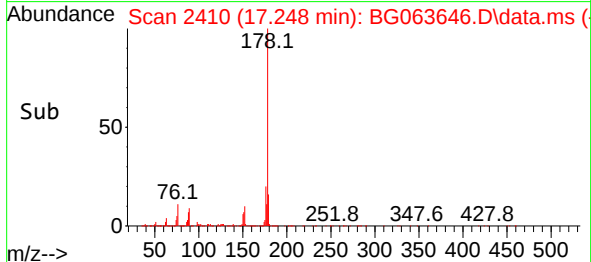

#74
Anthracene
Concen: 35.621 ng/uI
RT: 17.336 min Scan# 2425
Delta R.T. -0.014 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:178 Resp: 2000686
Ion Ratio Lower Upper
178 100
179 16.2 11.8 17.6
176 18.8 14.2 21.2




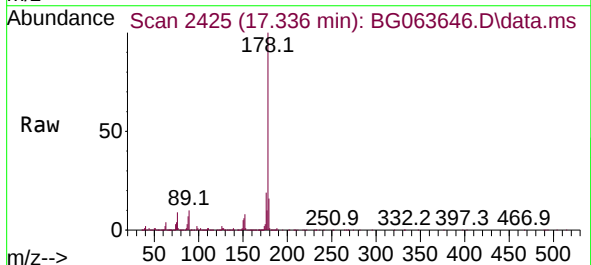




#75
1,2,3,4-Tetrachlorobenzene
Concen: 34.889 ng/ul
RT: 13.246 min Scan# 1730
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:216 Resp: 543692
Ion Ratio Lower Upper
216 100
214 77.4 60.6 90.8
218 46.8 36.2 54.4



#76
Pentachlorobenzene
Concen: 33.575 ng/ul
RT: 14.780 min Scan# 1990
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:250 Resp: 546625
Ion Ratio Lower Upper
250 100
248 63.5 51.3 76.9
252 64.7 50.2 75.4




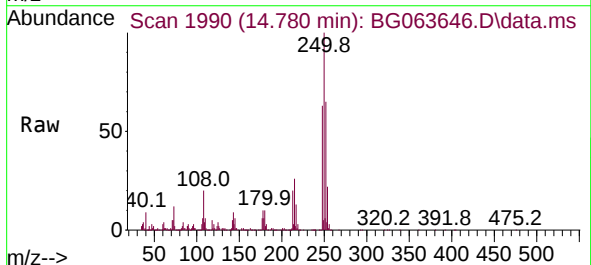




#77
Carbazole
Concen: 37.621 ng/ul
RT: 17.612 min Scan# 2472
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:167 Resp: 1692911
Ion Ratio Lower Upper
167 100
166 23.8 17.2 25.8
139 13.1 9.7 14.5

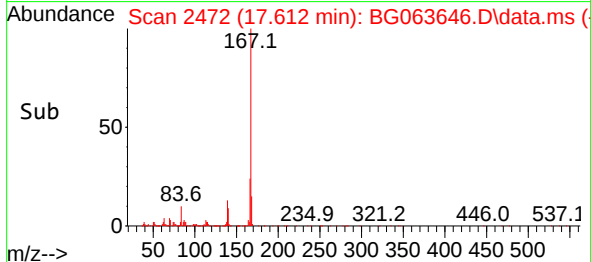

#78
Di-n-butylphthalate
Concen: 39.629 ng/ul
RT: 18.170 min Scan# 2567
Delta R.T. -0.014 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:149 Resp: 1903695
Ion Ratio Lower Upper
149 100
150 9.1 7.0 10.4
104 6.4 6.6 9.8#




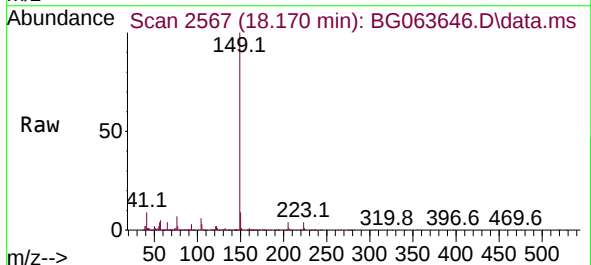




#80
Fluoranthene
Concen: 34.925 ng/ul
RT: 19.269 min Scan# 21
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:202 Resp: 2313510
Ion Ratio Lower Upper
202 100
101 9.8 5.9 8.9#
100 7.9 4.7 7.1#



#82
Pyrene
Concen: 35.358 ng/ul
RT: 19.633 min Scan# 2816
Delta R.T. -0.008 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:202 Resp: 2489841
Ion Ratio Lower Upper
202 100
101 11.9 6.5 9.7#
100 9.8 5.9 8.9#





#83

Butylbenzylphthalate

Concen: 49.314 ng/ul

RT: 20.526 min Scan# 2968

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Instrument :

BNA_G

ClientSampleId :

SLCS508





Tgt Ion:149 Resp: 731256

Ion Ratio Lower Upper

149 100

91 82.9 73.6 110.4

206 24.7 25.2 37.8#

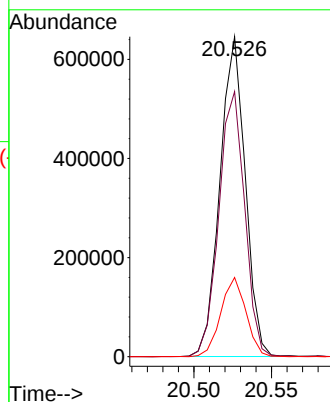

#84

3,3'-Dichlorobenzidine

Concen: 24.204 ng/ul

RT: 21.360 min Scan# 3110

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14




Tgt Ion:252 Resp: 440583


Ion Ratio Lower Upper

252 100

254 64.8 50.8 76.2

126 8.2 4.3 6.5#





#85

Benzo(a)anthracene

Concen: 34.102 ng/ul

RT: 21.437 min Scan# 31

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Instrument :

BNA_G

ClientSampleId :

SLCS508





Tgt Ion:228 Resp: 2445586

Ion Ratio Lower Upper

228 100

229 20.3 16.0 24.0

226 27.9 21.0 31.6

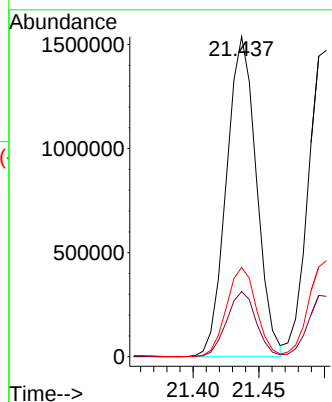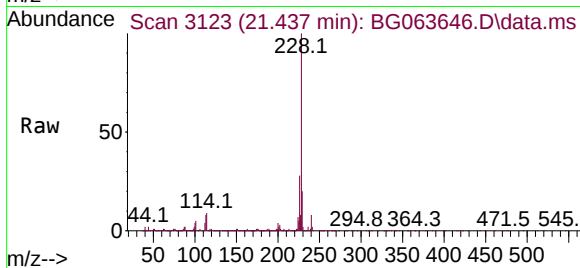

#86

Bis(2-ethylhexyl)phthalate

Concen: 49.107 ng/ul

RT: 21.349 min Scan# 3108

Delta R.T. -0.019 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14




Tgt Ion:149 Resp: 1094800


Ion Ratio Lower Upper

149 100

167 26.2 21.1 31.7

279 3.7 4.1 6.1#

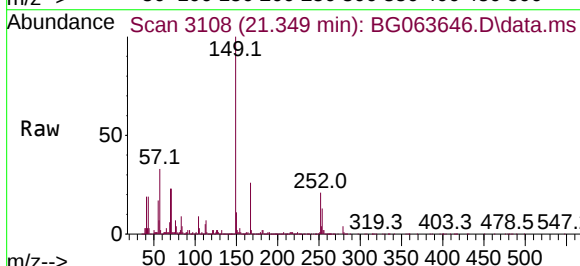



#87

Chrysene

Concen: 34.304 ng/ul

RT: 21.502 min Scan# 31

Delta R.T. -0.014 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Instrument :

BNA_G

ClientSampleId :

SLCS508





Tgt Ion:228 Resp: 2311004

Ion Ratio Lower Upper

228 100

226 31.3 24.6 37.0

229 19.7 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 48.802 ng/ul




RT: 22.489 min Scan# 3302


Delta R.T. -0.019 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Tgt Ion:149 Resp: 1940263









#90
Benzo(b)fluoranthene
Concen: 34.409 ng/ul
RT: 23.523 min Scan# 3479
Delta R.T. -0.019 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14




Instrument :
BNA_G
ClientSampleId :
SLCS508


Tgt Ion:252 Resp: 2431677
Ion Ratio Lower Upper
252 100
253 22.2 18.2 27.4
125 7.9 3.8 5.8#



#91
Benzo(k)fluoranthene
Concen: 34.845 ng/ul
RT: 23.581 min Scan# 3488
Delta R.T. -0.025 min
Lab File: BG063646.D
Acq: 11 Dec 2024 00:14

Tgt Ion:252 Resp: 2447780
Ion Ratio Lower Upper
252 100
253 21.2 17.0 25.6
125 8.4 4.2 6.2#





#93

Benzo(a)pyrene

Concen: 34.306 ng/ul

RT: 24.333 min Scan# 3

Delta R.T. -0.031 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Instrument :

BNA_G

ClientSampleId :

SLCS508





Tgt Ion:252 Resp: 2273849

Ion Ratio Lower Upper

252 100

253 21.8 18.3 27.5

125 9.1 3.6 5.4#



#94

Indeno(1,2,3-cd)pyrene

Concen: 35.076 ng/ul

RT: 27.888 min Scan# 4221

Delta R.T. -0.043 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14




Tgt Ion:276 Resp: 2804498


Ion Ratio Lower Upper

276 100

138 17.4 7.4 11.2#

277 23.7 17.8 26.6





#95

Dibenzo(a,h)anthracene

Concen: 35.304 ng/ul

RT: 27.929 min Scan# 41

Delta R.T. -0.049 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Instrument :

BNA_G

ClientSampleId :

SLCS508





Tgt Ion:278 Resp: 2263883

Ion Ratio Lower Upper

278 100

139 12.7 4.3 6.5#

279 23.0 17.4 26.2



#96

Benzo(g,h,i)perylene

Concen: 36.143 ng/ul

RT: 28.946 min Scan# 4401

Delta R.T. -0.043 min

Lab File: BG063646.D

Acq: 11 Dec 2024 00:14

Tgt Ion:276 Resp: 2196391

Ion Ratio Lower Upper

276 100

138 16.6 7.4 11.0#

277 23.6 18.3 27.5

