

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
 Data File : BG063635.D
 Acq On : 10 Dec 2024 17:19
 Operator : RC/JU
 Sample : PB165510BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	29	32	38	rBV3	37420	62938	1.18%	0.122%
2	3.688	98	102	118	rBV	647900	1157562	21.65%	2.236%
3	5.903	477	479	482	rVB2	11644	7337	0.14%	0.014%
4	6.220	531	533	536	rBV3	7206	7268	0.14%	0.014%
5	6.995	659	665	673	rBV	870745	1502531	28.10%	2.902%
6	7.142	685	690	702	rVV	624402	1055595	19.74%	2.039%
7	7.219	702	703	706	rVB3	15842	11080	0.21%	0.021%
8	7.348	719	725	734	rVB	840880	1413532	26.43%	2.730%
9	7.812	798	804	812	rBV	513947	866391	16.20%	1.673%
10	8.218	871	873	875	rBV2	10354	10497	0.20%	0.020%
11	8.529	919	926	937	rBV	1040558	1823230	34.09%	3.521%
12	8.752	962	964	967	rBV2	11480	10825	0.20%	0.021%
13	8.970	993	1001	1009	rBV	775947	1395162	26.09%	2.694%
14	9.287	1054	1055	1059	rVB2	12192	9995	0.19%	0.019%
15	9.322	1059	1061	1063	rBV2	11673	8243	0.15%	0.016%
16	9.592	1104	1107	1109	rVB	11913	10254	0.19%	0.020%
17	9.616	1109	1111	1112	rBV	9588	8673	0.16%	0.017%
18	9.686	1116	1123	1130	rBV	599567	1077887	20.16%	2.082%
19	10.115	1195	1196	1200	rVB4	9458	10523	0.20%	0.020%
20	10.233	1209	1216	1227	rBV	983075	1794265	33.55%	3.465%
21	10.444	1249	1252	1256	rBV2	8841	15512	0.29%	0.030%
22	10.603	1271	1279	1286	rBV	696185	1250695	23.39%	2.415%
23	10.738	1295	1302	1318	rBV	850831	1635444	30.58%	3.158%
24	10.903	1328	1330	1332	rVB2	11409	8930	0.17%	0.017%
25	10.967	1338	1341	1343	rBV2	8796	9559	0.18%	0.018%
26	11.020	1346	1350	1351	rVB3	8756	10864	0.20%	0.021%
27	11.096	1360	1363	1365	rBV2	10594	13181	0.25%	0.025%
28	11.220	1383	1384	1386	rBV	11835	8164	0.15%	0.016%
29	11.367	1407	1409	1413	rBV4	8507	8920	0.17%	0.017%
30	11.396	1413	1414	1418	rVV2	9059	8854	0.17%	0.017%
31	11.537	1437	1438	1442	rVB2	11159	9673	0.18%	0.019%
32	11.666	1459	1460	1464	rVB	7486	7512	0.14%	0.015%
33	11.772	1476	1478	1480	rBV	8335	7578	0.14%	0.015%
34	11.825	1484	1487	1488	rBV2	9152	9501	0.18%	0.018%
35	12.066	1525	1528	1529	rBV	9819	10227	0.19%	0.020%
36	12.195	1548	1550	1553	rBV3	13672	14074	0.26%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
 Data File : BG063635.D
 Acq On : 10 Dec 2024 17:19
 Operator : RC/JU
 Sample : PB165510BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Title : SVOA CALIBRATION

37	12.595	1614	1618	1621	rVB3	6823	9708	0.18%	0.019%
38	12.677	1631	1632	1636	rVB3	9955	8529	0.16%	0.016%
39	12.736	1640	1642	1646	rVB2	9008	9767	0.18%	0.019%
40	12.789	1649	1651	1653	rVB2	10692	8564	0.16%	0.017%
41	13.129	1707	1709	1713	rVB3	10765	13615	0.25%	0.026%
42	13.176	1716	1717	1719	rBV2	7650	7461	0.14%	0.014%
43	13.423	1757	1759	1761	rVB3	9493	7688	0.14%	0.015%
44	13.541	1777	1779	1782	rBV2	9005	8070	0.15%	0.016%
45	13.676	1799	1802	1804	rBV2	7128	7560	0.14%	0.015%
46	13.711	1806	1808	1809	rBV2	9591	8287	0.15%	0.016%
47	13.770	1815	1818	1820	rBV2	8461	10025	0.19%	0.019%
48	13.858	1825	1833	1843	rBV	1828411	2657903	49.70%	5.133%
49	13.964	1850	1851	1856	rVB4	8569	9624	0.18%	0.019%
50	14.028	1860	1862	1864	rBV2	9661	9205	0.17%	0.018%
51	14.146	1874	1882	1893	rBV	2051001	3198543	59.81%	6.177%
52	14.305	1905	1909	1912	rVB2	11143	16131	0.30%	0.031%
53	14.340	1912	1915	1917	rBV3	9451	9690	0.18%	0.019%
54	14.451	1926	1934	1941	rBV	1231674	1876001	35.08%	3.623%
55	14.575	1953	1955	1956	rBV2	7746	7820	0.15%	0.015%
56	14.587	1956	1957	1961	rVB3	12924	9591	0.18%	0.019%
57	14.675	1967	1972	1985	rBV2	480672	1034900	19.35%	1.999%
58	15.015	2029	2030	2034	rBV2	9726	8370	0.16%	0.016%
59	15.086	2039	2042	2043	rVB3	8678	8086	0.15%	0.016%
60	15.109	2043	2046	2047	rBV3	6003	8048	0.15%	0.016%
61	15.192	2058	2060	2062	rVB2	12704	9124	0.17%	0.018%
62	15.215	2062	2064	2068	rBV2	12777	20485	0.38%	0.040%
63	15.450	2097	2104	2111	rBV	2657007	3953694	73.93%	7.635%
64	15.503	2111	2113	2116	rVB2	8949	8141	0.15%	0.016%
65	15.579	2120	2126	2135	rBV2	408432	658585	12.32%	1.272%
66	15.691	2141	2145	2146	rBV3	11136	12938	0.24%	0.025%
67	15.779	2158	2160	2165	rVB2	12483	11131	0.21%	0.021%
68	15.885	2175	2178	2180	rVB3	6946	7717	0.14%	0.015%
69	15.920	2182	2184	2188	rVB2	15183	12924	0.24%	0.025%
70	15.961	2188	2191	2193	rBV2	7462	7724	0.14%	0.015%
71	16.191	2227	2230	2232	rBV3	8833	10606	0.20%	0.020%
72	16.238	2234	2238	2240	rBV2	14206	17029	0.32%	0.033%
73	16.520	2283	2286	2287	rBV	7327	7857	0.15%	0.015%
74	16.760	2324	2327	2330	rBV	7051	10698	0.20%	0.021%
75	16.990	2365	2366	2369	rVB2	9365	7818	0.15%	0.015%
76	17.207	2396	2403	2411	rVB	1621832	2450560	45.83%	4.733%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
 Data File : BG063635.D
 Acq On : 10 Dec 2024 17:19
 Operator : RC/JU
 Sample : PB165510BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
 Title : SVOA CALIBRATION

77	17.301	2411	2419	2433	rBV	2973960	4636642	86.71%	8.954%
78	17.677	2480	2483	2485	rVB3	12318	11075	0.21%	0.021%
79	17.712	2485	2489	2490	rBV4	11306	9689	0.18%	0.019%
80	17.800	2502	2504	2508	rBV4	9924	11918	0.22%	0.023%
81	17.953	2528	2530	2533	rVB2	9436	7292	0.14%	0.014%
82	17.988	2535	2536	2540	rBV3	7248	7817	0.15%	0.015%
83	18.294	2584	2588	2590	rBV4	10151	9924	0.19%	0.019%
84	18.458	2613	2616	2618	rVB4	10051	10499	0.20%	0.020%
85	18.541	2627	2630	2631	rBV3	8984	8728	0.16%	0.017%
86	18.676	2651	2653	2655	rVB3	12956	12011	0.22%	0.023%
87	18.699	2655	2657	2658	rBV2	9725	8903	0.17%	0.017%
88	18.746	2662	2665	2668	rBV5	7275	10422	0.19%	0.020%
89	18.911	2690	2693	2696	rBV3	9562	10065	0.19%	0.019%
90	18.970	2700	2703	2705	rBV4	10934	9473	0.18%	0.018%
91	19.164	2732	2736	2742	rBV5	49127	82470	1.54%	0.159%
92	19.240	2744	2749	2753	rVV3	44846	73948	1.38%	0.143%
93	19.293	2757	2758	2761	rVB3	11563	9244	0.17%	0.018%
94	19.387	2773	2774	2776	rBV	12226	9254	0.17%	0.018%
95	19.534	2797	2799	2804	rVB6	14228	15537	0.29%	0.030%
96	19.604	2805	2811	2822	rVB	3773875	5347591	100.00%	10.327%
97	21.461	3121	3127	3136	rBV	1574193	2544127	47.58%	4.913%
98	24.275	3597	3606	3617	rBV2	1848932	4818960	90.11%	9.306%
99	24.487	3633	3642	3654	rVB2	973124	2682361	50.16%	5.180%




Sum of corrected areas: 51780643

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
Data File : BG063635.D
Acq On : 10 Dec 2024 17:19
Operator : RC/JU
Sample : PB165510BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

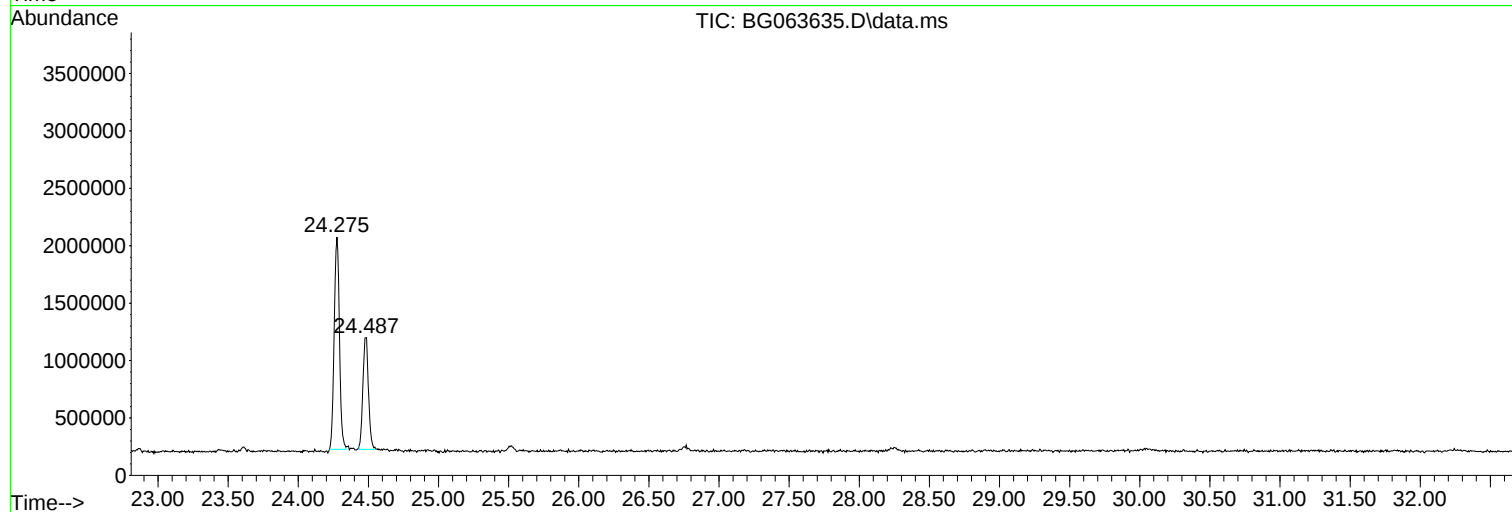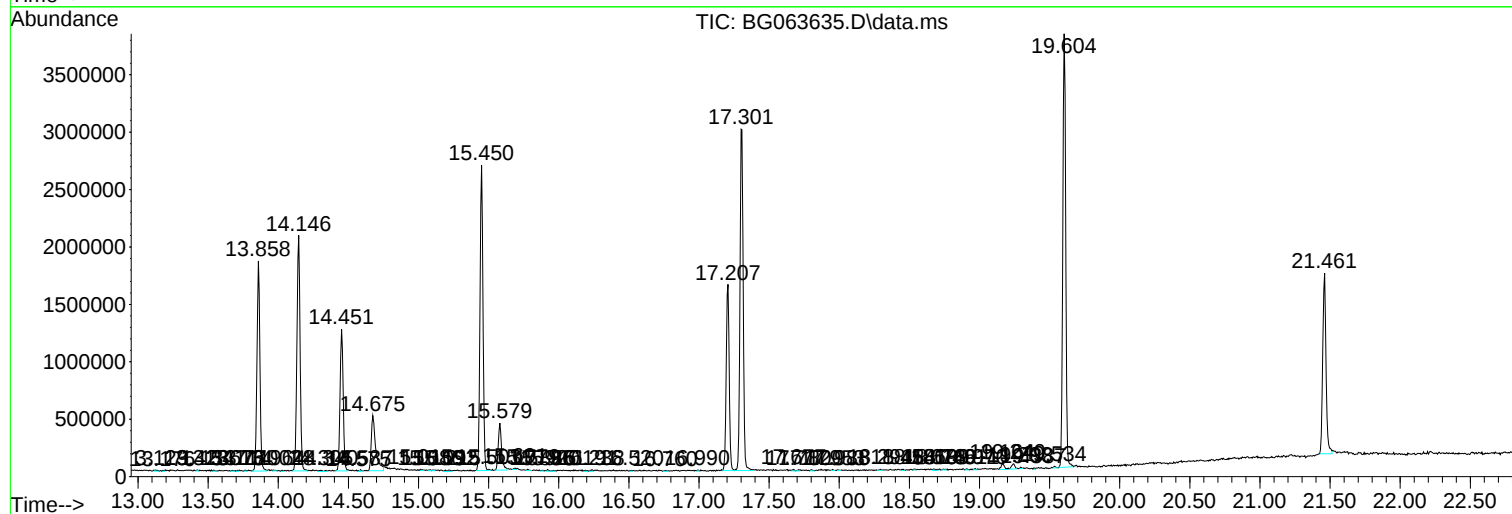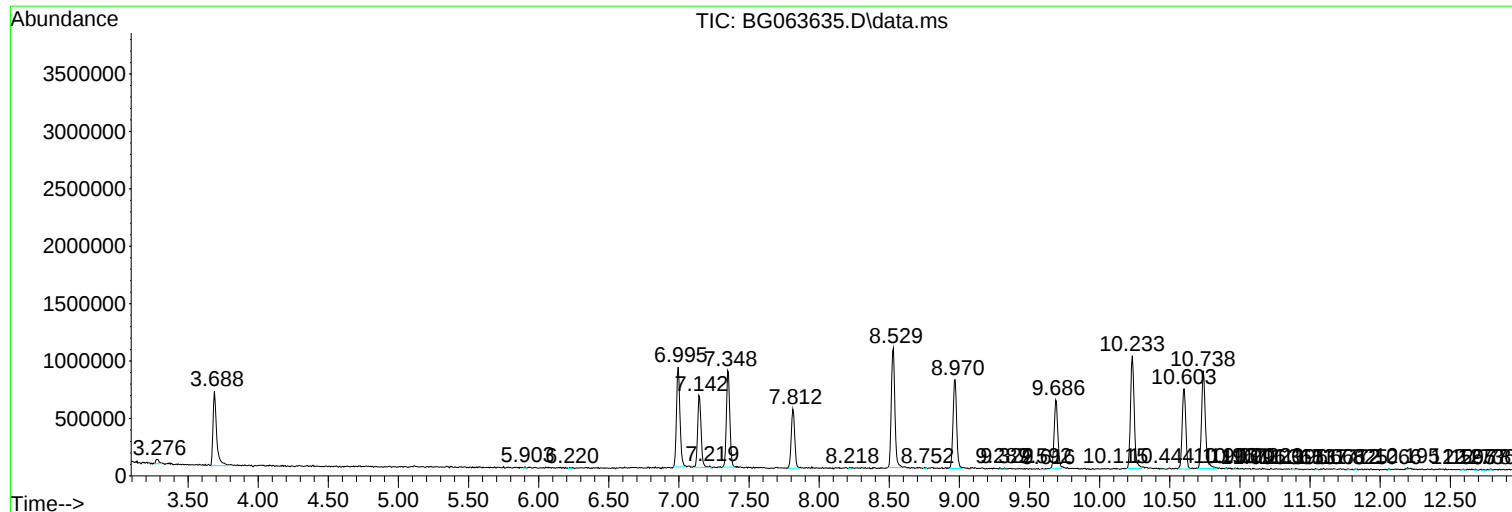

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
Data File : BG063635.D
Acq On : 10 Dec 2024 17:19
Operator : RC/JU
Sample : PB165510BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121024\
Data File : BG063635.D
Acq On : 10 Dec 2024 17:19
Operator : RC/JU
Sample : PB165510BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG120624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc